

**Agilent E5061A/E5062A ENA Series
ENA Series RF Network Analyzers**

Programmer's Guide

Fifth Edition

FIRMWARE REVISIONS

This manual applies directly to instruments that have the firmware revision A.03.00.
For additional information about firmware revisions, see Appendix A.



**Manufacturing No. E5061-90042
October 2008**

Notices

The information contained in this document is subject to change without notice.

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this document may be photocopied, reproduced, or translated to another language without the prior written consent of Agilent Technologies.

Microsoft®, MS-DOS®, Windows®, Visual C++®, Visual Basic®, VBA® and Excel® are registered

UNIX is a registered trademark in U.S. and other countries, licensed exclusively through X/Open Company Limited.

Portions ©Copyright 1996, Microsoft Corporation. All rights reserved.

© Copyright 2004, 2005, 2006, 2007 Agilent Technologies

Manual Printing History

The manual's printing date and part number indicate its current edition. The printing date changes when a new edition is printed. (Minor corrections and updates that are incorporated at reprint do not cause the date to change.) The manual part number changes when extensive technical changes are incorporated.

February 2004	First Edition (part number: E5061-90002)
September 2005	Second Edition (part number: E5061-90012, changes for firmware version A.02.00)
June 2005	Third Edition (part number: E5061-90022, changes for firmware version A.02.10)
February 2007	Fourth Edition (part number: E5061-90032, changes for firmware version A.03.00)
October 2008	Fifth Edition (part number: E5061-90042)

Typeface Conventions

Bold	Boldface type is used when a term is defined. For example: icons are symbols.
<i>Italic</i>	Italic type is used for emphasis and for titles of manuals and other publications.
[Key]	Indicates the hardkey whose key label is Key.
[Key] - Item	Indicates a series of key operations in which you press the [Key] key, select (highlight) the item called Item on the displayed menu using the [↓] key and so on, and then press the [Enter] key.

Sample Program Disk

A sample program disk (Agilent part number: E5061-180x0) is furnished with this manual. The disk contains the sample programs used in this manual.

The customer shall have the personal, non-transferable rights to use, copy, or modify SAMPLE PROGRAMS in this manual for the customer's internal operations. The customer shall use the SAMPLE PROGRAMS solely and exclusively for their own purposes and shall not license, lease, market, or distribute the SAMPLE PROGRAMS or modification of any part thereof.

Agilent Technologies shall not be liable for the quality, performance, or behavior of the SAMPLE PROGRAMS. Agilent Technologies especially disclaims any responsibility for the operation of the SAMPLE PROGRAMS to be uninterrupted or error-free. The SAMPLE PROGRAMS are provided AS IS.

AGILENT TECHNOLOGIES DISCLAIMS ANY IMPLIED WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

Agilent Technologies shall not be liable for any infringement of any patent, trademark, copyright, or other proprietary right by the SAMPLE PROGRAMS or their use. Agilent Technologies does not warrant that the SAMPLE PROGRAMS are free from infringements of such rights of third parties. However, Agilent Technologies will not knowingly infringe or deliver software that infringes the patent, trademark, copyright, or other proprietary right of a third party.

Documentation Map

The following manuals are available for the Agilent E5061A/E5062A.

- ***User's Guide (Part Number E5061-900x0, attached to Option ABA)***

This manual describes most of the basic information needed to use the E5061A/E5062A. It provides a function overview, detailed operation procedure for each function (from preparation for measurement to analysis of measurement results), measurement examples, specifications, and supplemental information. For programming guidance on performing automatic measurement with the E5061A/E5062A, please see the *Programming Manual*.

- ***Installation and Quick Start Guide (Part Number E5061-900x1, attached to Option ABA)***

This manual describes installation of the instrument after it is delivered and the basic procedures for applications and analysis. Refer to this manual when you use the E5061A/E5062A for the first time.

- ***Programmer's Guide (Part Number E5061-900x2, attached to Option ABA)***

This manual provides programming information for performing automatic measurement with the E5061A/E5062A. It includes an outline of remote control, procedures for detecting measurement start (trigger) and end (sweep end), application programming examples, a command reference, and related information.

- ***VBA Programmer's Guide (Part Number E5061-900x3, attached to Option ABA)***

This manual describes programming information for performing automatic measurement with internal controller. It includes an outline of VBA programming, some sample programming examples, a COM object reference, and related information.

- ***Option 100 Fault Location and Structural Return Loss Measurement User's Guide Supplement (Part Number E5061-900x4, attached to Option 100)***

This manual describes information for using the fault location and structural return loss measurement functions.

NOTE

The number position shown by "x" in the part numbers above indicates the edition number. This convention is applied to each manual, CD-ROM (for manuals), and sample programs disk issued.

1. Making Effective Use of This Manual	
Contents of This Manual	18
How To Use This Manual	20
Looking up SCPI commands	20
Using sample programs	21
2. Overview of Remote Control	
Types of remote control system	24
GPIB remote control system	25
What is GPIB?	25
System configuration	25
Device selector	26
LAN remote control system	27
System configuration	27
Control over SICL-LAN server	28
Control over telnet server	33
Sending SCPI command messages	36
Types and structure of commands	36
Grammar of messages	37
Remote mode	38
3. Setting Up the Analyzer	
Selecting the Active Channel/Trace	40
Configuring Measurement Conditions	41
Setting the Number of Traces	41
Selecting Measurement Parameters	41
Setting the Sweep Condition (Stimulus)	41
Configuring Averaging Settings	43
Setting the System Z0	43
Configuring Display Settings	44
Setting the Layout of Windows and Graphs	44
Configuring Trace Display Settings	47
Printing a Message in the Echo Window	49
Turning On or Off Display Update	49
Showing/Hiding Frequencies	49
Showing or Hiding the Title	49
Configuring Date/Time Display	49
Turning On or Off the LCD Backlight	49
Setting display colors	50
Saving and Loading the Settings	51
Sample Program	52
4. Performing a Calibration	
Calibration	60
Performing a Calibration (Obtaining the Calibration Coefficients)	60
Defining Calibration Kits	64
Saving and Loading Calibration Coefficients	66
Sample Program	67

Contents

Calibration	67
ECal	75
 5. Making a Measurement	
Trigger system	80
System-wide state and transition	81
Channel-wide state and transition	82
Starting a Measurement Cycle (Triggering the instrument)	83
Configuring the Instrument to Automatically Perform Continuous Measurement	83
Starting Measurement on Demand	83
Waiting for the End of Measurement	84
Using the Status Register	84
Using the :TRIG:SING Command	87
Using Wait Time	88
 6. Analyzing Data	
Retrieving Measurement Results at Specified Points	90
Showing/Hiding Markers	90
Turning On or Off Reference Marker Mode	90
Setting (Changing) and Retrieving Stimulus Value at Marker Positions	90
Retrieving Measurement Results at Marker Positions	90
Searching for Positions That Match Specified Criteria	91
Using Marker Search	91
Using the Analysis Command	93
Sample Program	95
Bandwidth Search	97
Setting the Bandwidth Definition Value	97
Retrieving Bandwidth Search Results	97
Sample Program	97
Notch search	99
Setting the notch definition value	99
Reading out the notch search result	99
Statistical Analysis	100
Analyzing impedance	101
 7. Reading/Writing Measurement Data	
Data Transfer Format	104
ASCII Transfer Format	105
Binary Transfer Format	106
Internal data processing	108
Data flow	108
Internal data arrays	108
Retrieving Measurement Results	111
Retrieving Internal Data Arrays	111
Entering Data into a Trace	115
 8. Limit Test	
Performing a Limit Test	120

Configuring Limit Lines	120
Showing/Hiding Limit Lines.	120
Turning On or Off the Limit Test Feature.	120
Showing/Hiding “Fail”	120
Obtaining Test Results	121
Test Results at Each Measurement Point	121
Test Results for Each Trace.	121
Test Results for Each Channel	122
Overall Test Result	124
Sample Program	125
9. Saving and Recalling (File Management)	
Saving and Recalling File	132
Specifying file	132
Saving and recalling instrument status	132
Saving measurement data	133
Saving the images on the LCD screen	133
Saving and recalling the segment sweep table	134
Saving and recalling the limit table.	134
Saving/loading (importing) the VBA program	134
Sample program	136
Managing Files	139
Creating directory (folder)	139
Deleting file (directory).	139
Copying file.	139
Transferring files	139
Retrieving data from storage.	139
Sample program	140
10. Communication with External Instruments Using Handler I/O Port	
Handler I/O Port Overview.	148
I/O Signal Pin Layout and Description.	149
Inputting/Outputting Data.	152
Specifying signal direction of port	152
Reading data input to port.	153
Data output to port.	153
Preset states at power-on.	154
Timing Chart.	155
Electrical Characteristics	158
Input signal	158
Output signal	159
Power supply (+5 V).	159
Sample Program	160
11. Working with Automatic Test Systems	
Preventing Erroneous Key Operation on the Front Panel (Key Lock Feature)	162
Improving Command Processing Speed.	163
Measurement results (trace) need not to be updated.	163

Measurement results (trace) need to be updated.	163
Sample program	164
Detecting Occurrence of an Error.	166
Using the status reporting system	166
Using the error queue	166
Sample program	167
 12. Sample Application Programs	
Basic measurement (measuring a band pass filter)	170
Controlling Using SICL-LAN Server	176
Using VBA macro	176
Description of operation in VBA macro.	177
Controlling Using Telnet Server.	184
Using VBA macro	184
Description of operation in VBA macro.	185
 13. SCPI Command Reference	
Notational conventions in this command reference	194
Syntax	194
Description	194
Parameters.	195
Query response	195
Related commands	195
Equivalent key	195
IEEE Common Commands	196
*CLS	196
*ESE	197
*ESR?	197
*IDN?	198
*OPC	198
*OPC?	198
*OPT?	199
*RST	199
*SRE	200
*STB?	201
*TRG	201
*WAI	201
E5061A/E5062A commands	202
:ABOR	202
:CALC{1-4}:BLIM	203
:CALC{1-4}:BLIM:DB	204
:CALC{1-4}:BLIM:DISP:MARK	205
:CALC{1-4}:BLIM:DISP:VAL	206
:CALC{1-4}:BLIM:FAIL?	207
:CALC{1-4}:BLIM:MAX	208
:CALC{1-4}:BLIM:MIN	209
:CALC{1-4}:BLIM:REP?	210
:CALC{1-4}:CONV	211

:CALC{1-4}:CONV:FUNC	212
:CALC{1-4}:CORR:EDEL:TIME	213
:CALC{1-4}:CORR:OFFS:PHAS	214
:CALC{1-4}:DATA:FDAT	215
:CALC{1-4}:DATA:FMEM	216
:CALC{1-4}:DATA:SDAT	217
:CALC{1-4}:DATA:SMEM	218
:CALC{1-4}:FORM	219
:CALC{1-4}:FUNC:DATA?	221
:CALC{1-4}:FUNC:DOM	222
:CALC{1-4}:FUNC:DOM:COUP	223
:CALC{1-4}:FUNC:DOM:STAR	224
:CALC{1-4}:FUNC:DOM:STOP	225
:CALC{1-4}:FUNC:EXEC	225
:CALC{1-4}:FUNC:PEXC	226
:CALC{1-4}:FUNC:POIN?	227
:CALC{1-4}:FUNC:PPOL	228
:CALC{1-4}:FUNC:TARG	229
:CALC{1-4}:FUNC:TTR	230
:CALC{1-4}:FUNC:TYPE	231
:CALC{1-4}:LIM	232
:CALC{1-4}:LIM:DATA	233
:CALC{1-4}:LIM:DISP	235
:CALC{1-4}:LIM:DISP:CLIP	236
:CALC{1-4}:LIM:FAIL?	237
:CALC{1-4}:LIM:OFFS:AMPL	238
:CALC{1-4}:LIM:OFFS:MARK	239
:CALC{1-4}:LIM:OFFS:STIM	240
:CALC{1-4}:LIM:REP:ALL?	241
:CALC{1-4}:LIM:REP?	242
:CALC{1-4}:LIM:REP:POIN?	242
:CALC{1-4}:MARK:BWID	243
:CALC{1-4}:MARK:COUP	244
:CALC{1-4}:MARK:FUNC:DOM	245
:CALC{1-4}:MARK:FUNC:DOM:COUP	246
:CALC{1-4}:MARK:FUNC:DOM:STAR	247
:CALC{1-4}:MARK:FUNC:DOM:STOP	248
:CALC{1-4}:MARK:FUNC:MULT:PEXC	249
:CALC{1-4}:MARK:FUNC:MULT:PPOL	250
:CALC{1-4}:MARK:FUNC:MULT:TARG	251
:CALC{1-4}:MARK:FUNC:MULT:TRAC	252
:CALC{1-4}:MARK:FUNC:MULT:TTR	253
:CALC{1-4}:MARK:FUNC:MULT:TYPE	254
:CALC{1-4}:MARK:MATH:FLAT	255
:CALC{1-4}:MARK:MATH:FLAT:DATA?	256
:CALC{1-4}:MARK:MATH:FST	257
:CALC{1-4}:MARK:MATH:FST:DATA?	258
:CALC{1-4}:MARK:MATH:STAT	259
:CALC{1-4}:MARK:MATH:STAT:DATA?	260

:CALC{1-4}:MARK:NOTC	261
:CALC{1-4}:MARK:REF	262
:CALC{1-4}:MARK{1-10}	263
:CALC{1-4}:MARK{1-10}:ACT	264
:CALC{1-4}:MARK{1-10}:BWID:DATA?	265
:CALC{1-4}:MARK{1-10}:BWID:THR	266
:CALC{1-4}:MARK{1-10}:DISC	267
:CALC{1-4}:MARK{1-10}:FUNC:EXEC	268
:CALC{1-4}:MARK{1-10}:FUNC:PEXC	269
:CALC{1-4}:MARK{1-10}:FUNC:PPOL	270
:CALC{1-4}:MARK{1-10}:FUNC:TARG	271
:CALC{1-4}:MARK{1-10}:FUNC:TRAC	272
:CALC{1-4}:MARK{1-10}:FUNC:TTR	273
:CALC{1-4}:MARK{1-10}:FUNC:TYPE	274
:CALC{1-4}:MARK{1-10}:NOTC:DATA?	276
:CALC{1-4}:MARK{1-10}:NOTC:THR	277
:CALC{1-4}:MARK{1-10}:SET	278
:CALC{1-4}:MARK{1-10}:X	279
:CALC{1-4}:MARK{1-10}:Y?	280
:CALC{1-4}:MATH:FUNC	281
:CALC{1-4}:MATH:MEM	281
:CALC{1-4}:MST	282
:CALC{1-4}:MST:DATA?	283
:CALC{1-4}:PAR:COUN	284
:CALC{1-4}:PAR{1-4}:DEF	285
:CALC{1-4}:PAR{1-4}:SEL	286
:CALC{1-4}:RLIM	286
:CALC{1-4}:RLIM:DATA	287
:CALC{1-4}:RLIM:DISP:LINE	288
:CALC{1-4}:RLIM:DISP:SEL	289
:CALC{1-4}:RLIM:DISP:VAL	290
:CALC{1-4}:RLIM:FAIL?	291
:CALC{1-4}:RLIM:REP?	292
:CALC{1-4}:SMO	293
:CALC{1-4}:SMO:APER	294
:CONT:HAND:A	295
:CONT:HAND:B	295
:CONT:HAND:C	296
:CONT:HAND:C:MODE	297
:CONT:HAND:D	298
:CONT:HAND:D:MODE	299
:CONT:HAND:E	300
:CONT:HAND:F	301
:CONT:HAND:IND:STAT	302
:CONT:HAND:OUTP{1-2}	302
:CONT:HAND:RTR:STAT	303
:DISP:ANN:FREQ	304
:DISP:CCL	304
:DISP:CLOC	305

:DISP:COL{1-2}:BACK.....	306
:DISP:COL{1-2}:GRAT{1-2}	307
:DISP:COL{1-2}:LIM{1-2}	308
:DISP:COL{1-2}:RES	308
:DISP:COL{1-2}:TRAC{1-4}:DATA	309
:DISP:COL{1-2}:TRAC{1-4}:MEM.....	310
:DISP:ECHO.....	311
:DISP:ECHO:CLE	311
:DISP:ENAB.....	312
:DISP:FSIG	313
:DISP:IMAG	313
:DISP:MAX.....	314
:DISP:SKEY	314
:DISP:SPL	315
:DISP:TABL	316
:DISP:TABL:TYPE.....	317
:DISP:UPD	318
:DISP:WIND{1-4}:ACT.....	318
:DISP:WIND{1-4}:ANN:MARK:ALIG	319
:DISP:WIND{1-4}:ANN:MARK:SING.....	320
:DISP:WIND{1-4}:LAB.....	321
:DISP:WIND{1-4}:MAX	322
:DISP:WIND{1-4}:SPL	323
:DISP:WIND{1-4}:TITL	324
:DISP:WIND{1-4}:TITL:DATA.....	324
:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:X	325
:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:Y	326
:DISP:WIND{1-4}:TRAC{1-4}:ANN:YAX:MODE.....	327
:DISP:WIND{1-4}:TRAC{1-4}:MEM	328
:DISP:WIND{1-4}:TRAC{1-4}:STAT	329
:DISP:WIND{1-4}:TRAC{1-4}:Y:AUTO	329
:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV.....	330
:DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV	331
:DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS	332
:DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:FREQ	333
:DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:MODE.....	334
:DISP:WIND{1-4}:X:SPAC	335
:DISP:WIND{1-4}:Y:DIV	336
:FORM:BORD	337
:FORM:DATA.....	338
:HCOP	339
:HCOP:ABOR.....	339
:HCOP:IMAG	339
:INIT{1-4}.....	340
:INIT{1-4}:CONT.....	341
:MMEM:CAT?	342
:MMEM:COPY	343
:MMEM:DEL	344
:MMEM:LOAD	345

:MMEM:LOAD:CHAN	346
:MMEM:LOAD:CHAN:COEF	347
:MMEM:LOAD:LIM	348
:MMEM:LOAD:PROG	349
:MMEM:LOAD:RLIM	350
:MMEM:LOAD:SEGM	351
:MMEM:MDIR	352
:MMEM:STOR	353
:MMEM:STOR:CHAN	354
:MMEM:STOR:CHAN:CLE	354
:MMEM:STOR:CHAN:COEF	355
:MMEM:STOR:FDAT	356
:MMEM:STOR:IMAG	357
:MMEM:STOR:LIM	358
:MMEM:STOR:PROG	359
:MMEM:STOR:RLIM	360
:MMEM:STOR:SALL	361
:MMEM:STOR:SEGM	362
:MMEM:STOR:STYP	363
:MMEM:TRAN	364
:OUTP	365
:PROG:CAT?	365
:PROG:NAME	366
:PROG:STAT	367
:SENS:CORR:COLL:ECAL:PATH?	368
:SENS:CORR:IMP	369
:SENS{1-4}:AVER:CLE	370
:SENS{1-4}:AVER	370
:SENS{1-4}:AVER:COUN	371
:SENS{1-4}:BAND	372
:SENS{1-4}:BWID	373
:SENS{1-4}:CORR:CLE	373
:SENS{1-4}:CORR:COEF?	374
:SENS{1-4}:CORR:COLL:CKIT	375
:SENS{1-4}:CORR:COLL:CKIT:LAB	376
:SENS{1-4}:CORR:COLL:CKIT:ORD:LOAD	377
:SENS{1-4}:CORR:COLL:CKIT:ORD:OPEN	378
:SENS{1-4}:CORR:COLL:CKIT:ORD:SHOR	379
:SENS{1-4}:CORR:COLL:CKIT:ORD:THRU	380
:SENS{1-4}:CORR:COLL:CKIT:RES	380
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:ARB	381
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C0	382
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C1	383
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C2	384
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C3	385
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:DEL	386
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L0	387
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L1	388
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L2	389

:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L3	390
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:LAB	391
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:LOSS	392
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:TYPE	393
:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:Z0	394
:SENS{1-4}:CORR:COLL:ECAL:ERES	395
:SENS{1-4}:CORR:COLL:ECAL:ISOL	395
:SENS{1-4}:CORR:COLL:ECAL:SOLT1	397
:SENS{1-4}:CORR:COLL:ECAL:SOLT2	397
:SENS{1-4}:CORR:COLL:ECAL:THRU	398
:SENS{1-4}:CORR:COLL:ISOL	399
:SENS{1-4}:CORR:COLL:METH:ERES	399
:SENS{1-4}:CORR:COLL:LOAD	401
:SENS{1-4}:CORR:COLL:METH:OPEN	402
:SENS{1-4}:CORR:COLL:METH:SHOR	402
:SENS{1-4}:CORR:COLL:METH:SOLT1	403
:SENS{1-4}:CORR:COLL:METH:SOLT2	403
:SENS{1-4}:CORR:COLL:METH:THRU	404
:SENS{1-4}:CORR:COLL:METH:TYPE?	405
:SENS{1-4}:CORR:COLL:OPEN	406
:SENS{1-4}:CORR:COLL:SAVE	407
:SENS{1-4}:CORR:COLL:SHOR	407
:SENS{1-4}:CORR:COLL:THRU	408
:SENS{1-4}:CORR:EXT	409
:SENS{1-4}:CORR:EXT:PORT{1-2}	410
:SENS{1-4}:CORR:PROP	411
:SENS{1-4}:CORR:RVEL:COAX	411
:SENS{1-4}:CORR:STAT	412
:SENS{1-4}:CORR:TYPE{1-4}?	413
:SENS{1-4}:FREQ	414
:SENS{1-4}:FREQ:CENT	415
:SENS{1-4}:FREQ:DATA?	416
:SENS{1-4}:FREQ:SPAN	417
:SENS{1-4}:FREQ:STAR	418
:SENS{1-4}:FREQ:STOP	419
:SENS{1-4}:ROSC:SOUR?	420
:SENS{1-4}:SEGM:DATA	421
:SENS{1-4}:SEGM:SWE:POIN?	423
:SENS{1-4}:SEGM:SWE:TIME?	423
:SENS{1-4}:SWE:DEL	424
:SENS{1-4}:SWE:POIN	425
:SENS{1-4}:SWE:TIME	426
:SENS{1-4}:SWE:TIME:AUTO	427
:SENS{1-4}:SWE:TYPE	428
:SERV:CHAN:ACT?	428
:SERV:CHAN:COUN?	429
:SERV:CHAN{1-4}:TRAC:ACT?	429
:SERV:CHAN:TRAC:COUN?	429
:SERV:PORT:COUN?	430

:SOUR{1-4}:POW	431
:SOUR{1-4}:POW:ATT	432
:SOUR{1-4}:POW:CENT	433
:SOUR{1-4}:POW:PORT:COUP	434
:SOUR{1-4}:POW:PORT{1-2}	435
:SOUR{1-4}:POW:SLOP	436
:SOUR{1-4}:POW:SLOP:STAT	437
:SOUR{1-4}:POW:SPAN	438
:SOUR{1-4}:POW:STAR	439
:SOUR{1-4}:POW:STOP	440
:STAT:OPER?	441
:STAT:OPER:COND?	441
:STAT:OPER:ENAB	442
:STAT:OPER:NTR	443
:STAT:OPER:PTR	444
:STAT:PRES	445
:STAT:QUES?	445
:STAT:QUES:BLIM?	445
:STAT:QUES:BLIM:CHAN{1-4}?	446
:STAT:QUES:BLIM:CHAN{1-4}:COND?	446
:STAT:QUES:BLIM:CHAN{1-4}:ENAB	447
:STAT:QUES:BLIM:CHAN{1-4}:NTR	448
:STAT:QUES:BLIM:CHAN{1-4}:PTR	449
:STAT:QUES:BLIM:COND?	449
:STAT:QUES:BLIM:ENAB	450
:STAT:QUES:BLIM:NTR	451
:STAT:QUES:BLIM:PTR	452
:STAT:QUES:COND?	453
:STAT:QUES:ENAB	454
:STAT:QUES:LIM?	455
:STAT:QUES:LIM:CHAN{1-4}?	455
:STAT:QUES:LIM:CHAN{1-4}:COND?	455
:STAT:QUES:LIM:CHAN{1-4}:ENAB	456
:STAT:QUES:LIM:CHAN{1-4}:NTR	457
:STAT:QUES:LIM:CHAN{1-4}:PTR	458
:STAT:QUES:LIM:COND?	459
:STAT:QUES:LIM:ENAB	460
:STAT:QUES:LIM:NTR	461
:STAT:QUES:LIM:PTR	462
:STAT:QUES:NTR	463
:STAT:QUES:PTR	464
:STAT:QUES:RLIM?	465
:STAT:QUES:RLIM:CHAN{1-4}?	465
:STAT:QUES:RLIM:CHAN{1-4}:COND?	465
:STAT:QUES:RLIM:CHAN{1-4}:ENAB	466
:STAT:QUES:RLIM:CHAN{1-4}:NTR	467
:STAT:QUES:RLIM:CHAN{1-4}:PTR	468
:STAT:QUES:RLIM:COND?	468
:STAT:QUES:RLIM:ENAB	469

:STAT:QUES:RLIM:NTR	470
:STAT:QUES:RLIM:PTR	471
:SYST:BACK	472
:SYST:BEEP:COMP:IMM	473
:SYST:BEEP:COMP:STAT	473
:SYST:BEEP:WARN:IMM	474
:SYST:BEEP:WARN:STAT	474
:SYST:DATE	475
:SYST:ERR?	476
:SYST:KLOC:KBD	477
:SYST:KLOC:MOUS	478
:SYST:POFF	479
:SYST:PRES	479
:SYST:SEC:LEV	480
:SYST:SERV?	481
:SYST:TIME	482
:SYST:UPR	483
:TRIG	484
:TRIG:SING	484
:TRIG:SOUR	485
Command list	486
Command tree	486

A. Manual Changes

Manual Changes	500
Change 3	501
Change 2	501
Change 1	502

B. Status Reporting System

General Status Register Model	506
Event Register	507
Enable Register	507
Status Byte Register	507
Condition Register and Transition Filter	508
Status Register Structure	509
Using the Status Reporting System	523

C. Error Messages

Error Messages	526
A	526
B	526
C	526
D	527
E	527
F	528
G	529
H	529

I.....	529
L.....	530
M.....	530
N.....	530
O.....	531
P.....	531
Q.....	532
R.....	533
S.....	533
T.....	534
U.....	534
Warning Message	536

1

Making Effective Use of This Manual

This chapter describes the contents of this guide. Using this chapter with the table of contents helps you to retrieve description of a subject you wish to understand as well as to obtain an overview of this guide. Also see the latter part of this chapter for brief description of usage of this guide, focusing on searching commands.

Contents of This Manual

This is a programming guide with Agilent E5061A/E5062A.

This guide describes programming method mainly aiming at learning how to write a program that remotely controls the E5061A/E5062A using SCPI commands, focusing on sample usage with the HTBasic.

Controlling the E5061A/E5062A using the built-in VBA is not covered by this guide; it is described in *VBA Programmer's Guide*. For using the E5061A/E5062A VBA, see *VBA Programmer's Guide*.

Description in this guide assumes that the reader has learned manual operation of the E5061A/E5062A. Thus, this guide does not describe each feature of the E5061A/E5062A in detail. For detailed information on each feature, see *User's Guide*.

The chapter-by-chapter contents of this manual are as follows.

Chapter 1, "Making Effective Use of This Manual."

This chapter describes the contents of this guide. Using this chapter with the table of contents helps you to retrieve description of a subject you wish to understand as well as to obtain an overview of this guide. Also see the latter part of this chapter for brief description of usage of this guide, focusing on searching commands.

Chapter 2, "Overview of Remote Control."

This chapter provides an overview of the remote control system and the SCPI commands.

Chapter 3, "Setting Up the Analyzer."

This chapter describes how to configure measurement conditions and how to configure the way the instrument displays measurement results on the LCD.

Chapter 4, "Performing a Calibration."

This chapter describes how to obtain the calibration coefficients and perform error correction and how to define the calibration kit required to obtain the calibration coefficients.

Chapter 5, "Making a Measurement."

This chapter describes how to trigger the instrument to start a new measurement cycle and how to detect the end of a measurement cycle.

Chapter 6, "Analyzing Data."

This chapter describes how to use markers and analysis command.

Chapter 7, "Reading/Writing Measurement Data."

This chapter provides an overview of the Agilent E5061A/E5062A's internal data processing flow and describes how to read and write measurement results (internal data array).

Chapter 8, "Limit Test."

This chapter describes how to use the Limit Test feature to perform a limit test and determine the pass/fail status of the measured data.

Chapter 9, “Saving and Recalling (File Management).”

This chapter describes how to save and recall instrument status and measurement results onto/from the files. Here also covered is managing files.

Chapter 10, “Communication with External Instruments Using Handler I/O Port.”

This chapter provides necessary information for communicating with external instruments (for example, a handler in a production line) using the handler I/O port equipped with the Agilent E5061A/E5062A.

Chapter 11, “Working with Automatic Test Systems.”

This chapter describes useful features when the Agilent E5061A/E5062A is integrated with the automatic test system.

Chapter 12, “Sample Application Programs.”

This chapter introduces several sample programs for basic measurement, measurement with a system using the handler I/O, and controlling the instrument over LAN.

Chapter 13, “SCPI Command Reference.”

This chapter describes the SCPI command reference for the Agilent E5061A/E5062A. It describes the commands using their abbreviated format in alphabetical order. If you want to look up commands by softkeys, refer to the User's Guide.

Appendix A, “Manual Changes.”

This appendix contains the information required to adapt this manual to earlier versions or configurations of the Agilent E5061A/E5062A than that indicated by the current printing date of this manual. The information in this manual applies directly to the E5061A/E5062A model that has the serial number prefix listed on the title page of this manual.

Appendix B, “Status Reporting System.”

This appendix describes the status reporting system of the Agilent E5061A/E5062A.

Appendix C, “Error Messages.”

The Agilent E5061A/E5062A provides error messages to indicate its operating status. This appendix describes the error messages of the E5061A/E5062A in order of error number.

How To Use This Manual

Chapters 3 to 9 provide task-based descriptions of SCPI commands that are useful for programming and explain how you can use them. These chapters contain explanations and sample program listings that you can use to develop your custom programs. For more information on individual commands, see Chapter 13, “SCPI Command Reference.”

Looking up SCPI commands

Chapter 13 “SCPI Command Reference” contains a complete reference of SCPI commands. You can look up a particular SCPI command in any of the following ways:

Lookup by Abbreviated Command Name

The command reference is organized alphabetically according to the abbreviated name used as the title for each command’s description.

Lookup by Full Command Name

You can use the index at the end of the manual to find full command names along with the page numbers where they appear.

NOTE

Some SCPI commands supported by the E5061A/E5062A have optional syntax elements. In the command reference conventions, these elements are enclosed between square brackets ([]) or printed in lowercase letters. See “Syntax” on page 194 for more information.

Using sample programs

This manual comes with a sample program disk, which contains the source files of the sample programs used in the manual. The disk is DOS-formatted and the files are saved in ASCII format.

Loading a sample program

To load a sample program into the HTBasic interpreter, use the GET command. For example, you can load setup.bas, one of the sample programs, by the following procedure:

In the HTBasic screen, type the following command and press the Return key.

```
GET "setup.bas"
```

Looking up a sample program

To look up the description of a sample program, see the listings under “Sample program” in the index.

2

Overview of Remote Control

This chapter provides an overview of the remote control system and the SCPI commands.

Types of remote control system

Depending on the system controller and the interface, you can configure 4 types of remote control system as shown in the table below.

System controller	Interface	Overview
External controller (external computer such as PC and workstation)	GPIB (talker/listener mode)	System to control the E5061A/E5062A and other devices connected via GPIB from the external controller. For more information, refer to “GPIB remote control system” on page 25.
	LAN	System to control the E5061A/E5062A and other devices connected via LAN from the external controller. For more information, refer to “LAN remote control system” on page 27.
E5061A/E5062A	—	System to control the E5061A/E5062A itself using built-in E5061A/E5062A VBA. For more information, refer to <i>VBA Programmers Guide</i> .
	GPIB (system controller mode)	System to control the E5061A/E5062A itself and external devices connected via GPIB using built-in E5061A/E5062A VBA. For more information, refer to <i>VBA Programmers Guide</i> .

GPIB remote control system

What is GPIB?


GPIB (General Purpose Interface Bus) is an interface standard for connecting computers and peripherals, which supports the following international standards: IEEE 488.1, IEC-625, IEEE 488.2, and JIS-C1901. The GPIB interface allows you to control the Agilent E5061A/E5062A from an external computer. The computer sends commands and instructions to the E5061A/E5062A and receives data sent from the E5061A/E5062A via GPIB.

System configuration

Use GPIB cables to connect between the E5061A/E5062A, the external controller (computer), and peripherals. Figure 2-1 shows the overview of the system configuration of the GPIB remote control system.

Figure 2-1

Configuration of the GPIB remote control system

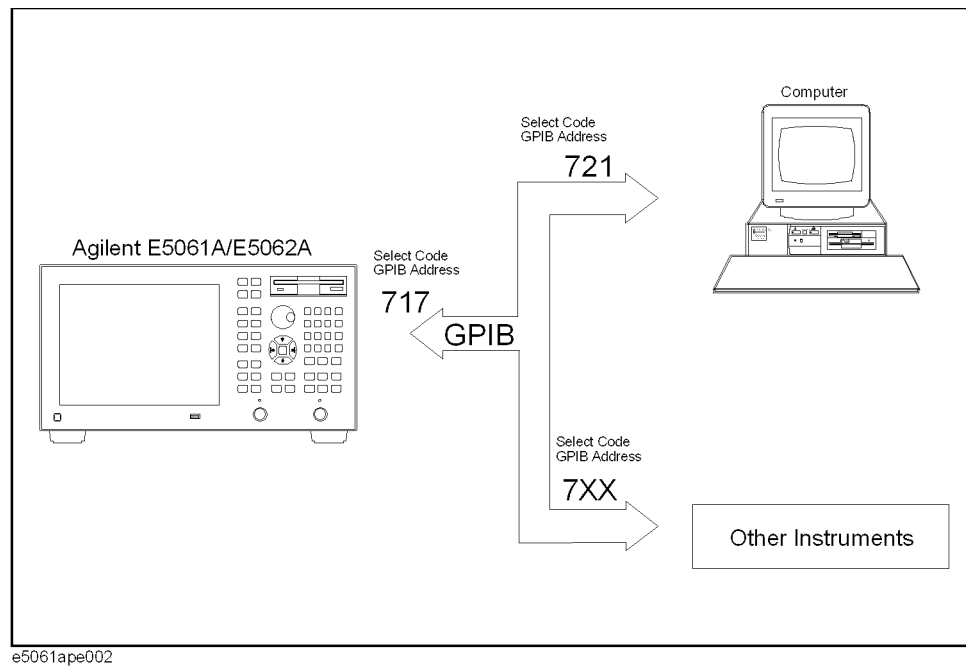

Required Equipment

1. E5061A/E5062A

2. External controller (computer)


Use a personal computer or workstation equipped with the GPIB interface. You need to install software to control this instrument via GPIB into the external controller (for example, HTBasic and Agilent VEE).

3. Other devices (other instruments and/or peripherals that serve your purpose)

4. GPIB cables for connecting the E5061A/E5062A, the external controller, and other devices

Scale of system you can construct

- You can connect up to 15 devices in a single GPIB system.
- The length of cables to connect between devices must be 4 m or less. The total length of connecting cables in a single GPIB system must be $2 \text{ m} \times \text{the number of connected devices (including the controller)}$ or less. You cannot construct the system in which the total cable length exceeds 20 m.
- The number of connectors connected to an individual device must be 4 or less. If you connect 5 or more connectors, excessive force is applied to the connector part, which may result in failure.
- You can choose the device connection topology from star, linear, and combined. Loop connection is not supported.

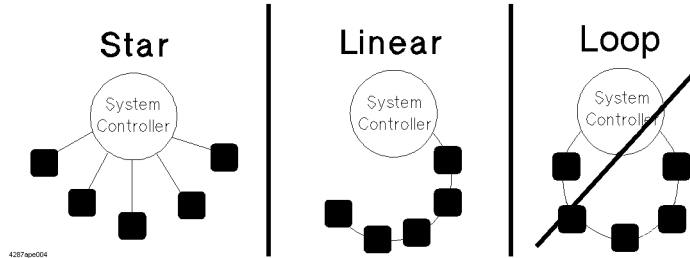

Device selector

The device selector is a unique value assigned to each device that is used by the controller to select the control target (to send/receive messages) among devices connected on the GPIB remote control system.

The device selector consists of a select code (usually, 7) and a GPIB address. For example, when the select code is 7 and the GPIB address is 17, the device selector is 717. The select code must be set for each system. The GPIB address must be set to a unique value for each device, which is used to identify devices on the same system. In the description and sample programs in this manual, it is assumed that the device selector is set to 717.

Setting the GPIB address of the E5061A/E5062A

[System] - GPIB Setup - Talker/Listener Address

LAN remote control system


The LAN (Local Area Network) remote control system provides two methods: controlling the E5061A/E5062A using the SICL-LAN server and controlling the E5061A/E5062A using the telnet server.

System configuration

Use a LAN cable to connect between the E5061A/E5062A and the external controller (computer). Figure 2-2 shows the overview of the system configuration of the LAN remote control system.

Figure 2-2

Configuration of the LAN remote control system

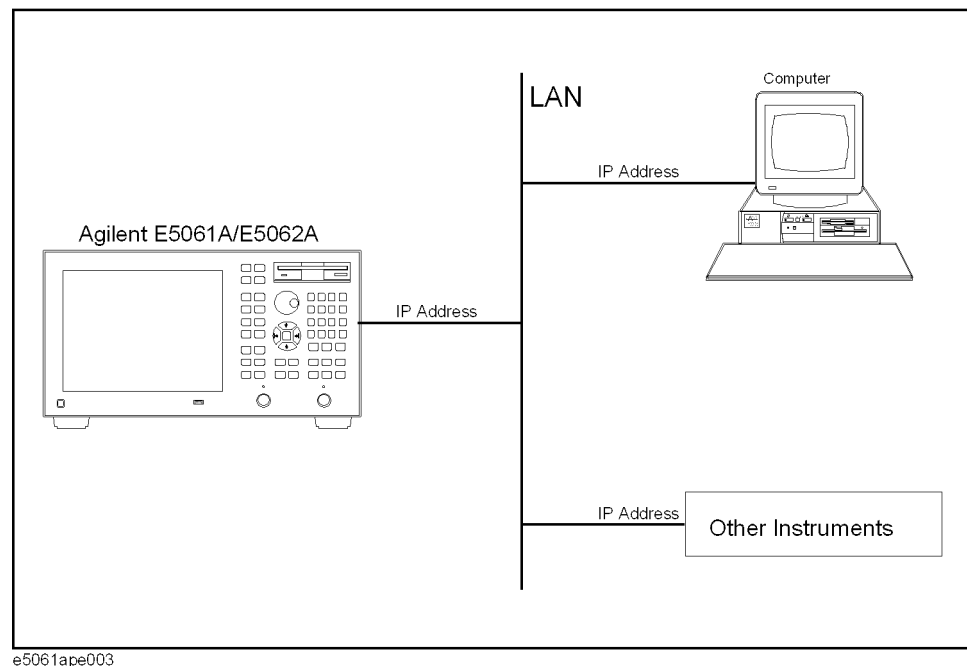

Required Equipment

1. E5061A/E5062A
2. External controller (personal computer or workstation that can be connected to LAN and Agilent I/O Library is installed into)
3. Other devices (other instruments and/or peripherals that serve your purpose)
4. LAN cable for connecting the E5061A/E5062A with the external controller

Preparing the E5061A/E5062A

Before controlling the E5061A/E5062A via LAN, you need to configure the network function. For detailed information on the procedure, refer to *User's Guide*.

Control over SICL-LAN server

In the control system using the SICL-LAN server, communication between the external controller (client) and the E5061A/E5062A (server) is performed using the SICL-LAN protocol. Communication is performed using SICL (Standard Instrument Control Library). You can control the E5061A/E5062A by programming using SICL or VISA with the C language in the UNIX environment, or Visual C++, Visual Basic, or VEE in the Windows environment.

Preparing the E5061A/E5062A

To communicate with the external controller, follow these steps to turn on the SICL-LAN server of the E5061A/E5062A in advance.

Step 1. Turn on the SICL-LAN server of the E5061A/E5062A.

[System] - Misc Setup - Network Setup - SICL-LAN Server [ON]

Step 2. Set the GPIB address of the E5061A/E5062A for control with the SICL-LAN server. “XX” represents an address number.

[System] - Misc Setup - Network Setup - SICL-LAN Address [XX]

NOTE

You need to restart the E5061A/E5062A firmware after changing the on/off setting or address setting of the SICL-LAN server.

Preparing the external controller

In order to establish communication to the E5061A/E5062A using the TCP/IP protocol, you need to set the I/O interface of the external controller in advance. This section shows the setting procedure when using the external controller in the Windows environment.

NOTE


You must install the Agilent I/O Libraries in advance.

Use Agilent I/O Libraries M.01.01 or Agilent I/O Libraries Suite 14 or later.

For further information on the I/O Libraries, see the Agilent I/O Libraries Manual.


The Agilent I/O Libraries may not be available for certain external controllers or OS versions. For further details, refer to the Help guidance for the Agilent I/O Libraries.

- Step 1.** From your PC's Start menu, click Program - Agilent I/O Libraries Suite - Agilent Connection Expert to open the Agilent Connection Expert setting screen.

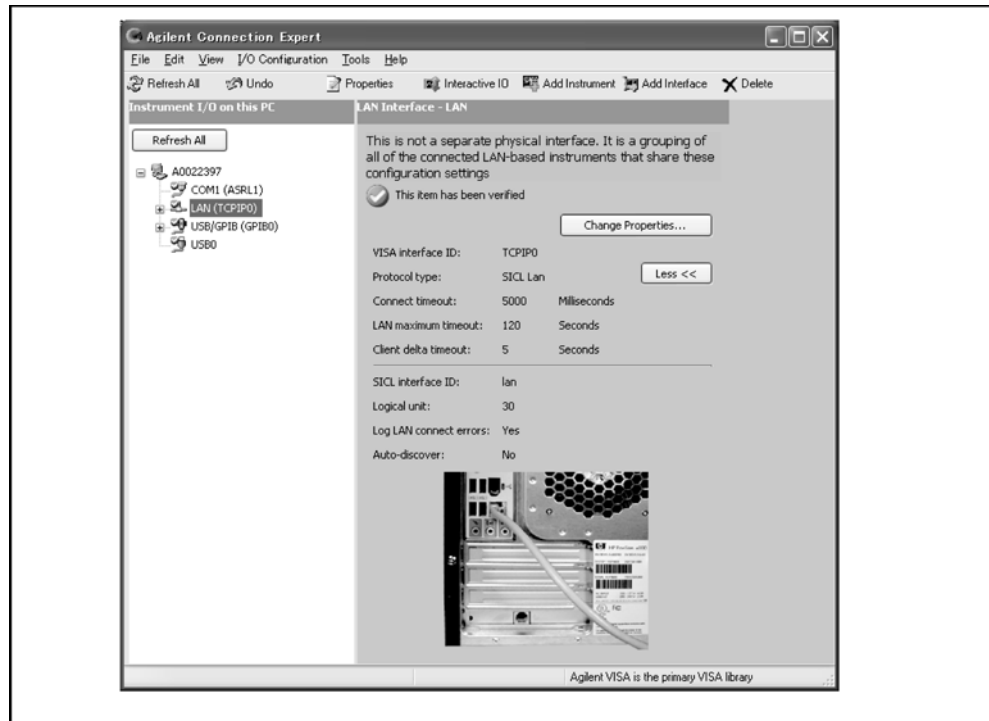

e5061ape4001


- Step 2.** In the Agilent Connection Expert setting screen, select **LAN(TCPIP0)** in the **Instrument I/O on this PC** frame, and then select **I/O Configuration - Add Instrument** on the menu.
- Step 3.** In the Add Instrument screen, press **OK** as LAN has been selected.

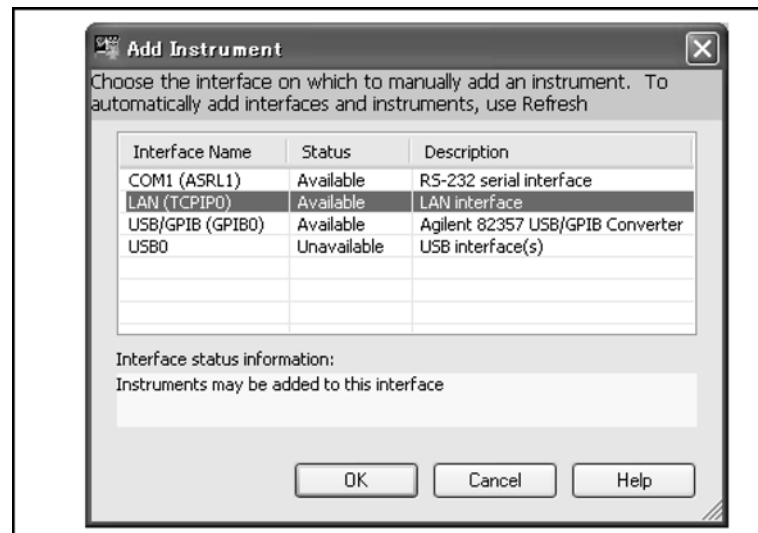

e5061ape4002


Overview of Remote Control LAN remote control system

- Step 4.** In the LAN Instrument Properties screen, set up the IP address of the E5061A/E5062A and click **OK**. You can change settings as necessary. For details, refer to the Agilent I/O Libraries Suite manual.

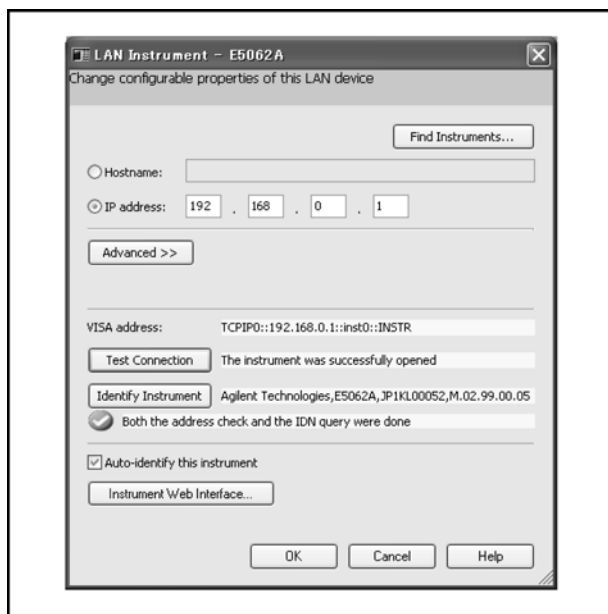

e5061ape4003

- Step 5.** In the Agilent Connection Expert screen, check that the E5061A/E5062A has been added under **LAN(TCPIP0)** in the **Instrument I/O on this PC** frame.

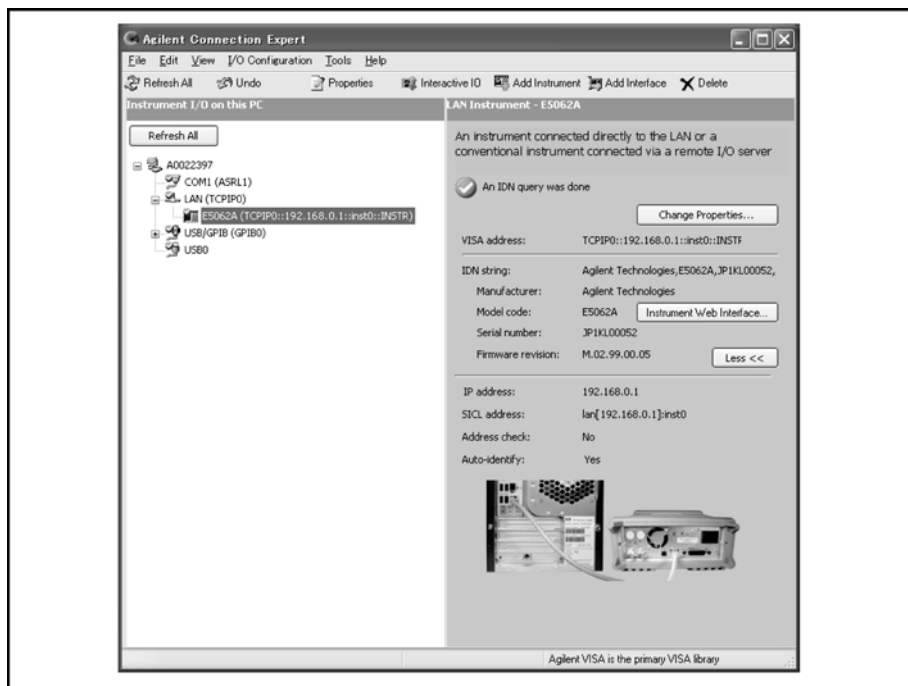

e5061ape4004

Control using C or Visual Basic

You can control the E5061A/E5062A by programming using SICL with the C language in the UNIX environment, or Visual C++ or Visual Basic in the Windows environment.

For more information on the control method, see a sample program using the VBA macro of Microsoft Excel described in “Controlling Using SICL-LAN Server” on page 176.

Control using Agilent VEE


Agilent VEE allows you to control the E5061A/E5062A via the I/O interface. The following example shows how to control the E5061A/E5062A that is set as follows: the address of the SICL-LAN server is 17 and the IP address is 1.10.100.50.

NOTE

When using Agilent VEE for PC, use Agilent VEE Pro 6 for Windows or later.

Step 1. On the Agilent EVE’s I/O menu, click **Instrument Manager...**

Step 2. In the Instrument Manager setting screen, click **Add...**

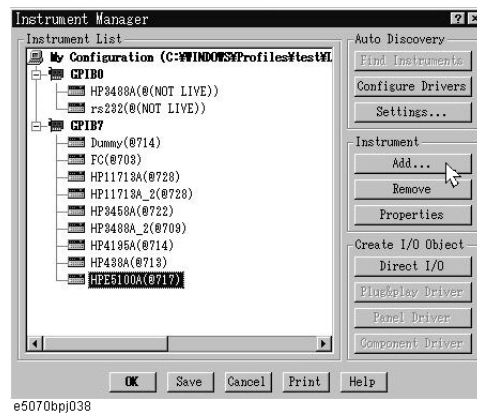

Step 3. The Instrument Properties setting screen appear. Make the settings as follows: Name (1 in the figure below): **SICL_LAN** (you can specify any name), Interface (2 in the figure below): **GP1B**, and Address (3 in the figure below): **917** (for the E5061A/E5062A, fixed to 9. 17 is the address of the SICL-LAN server). Then, click Gateway: **This host**. The Select or Enter Gateway setting screen appears. Enter the IP address or host name of the E5061A/E5062A (4 in the figure below).


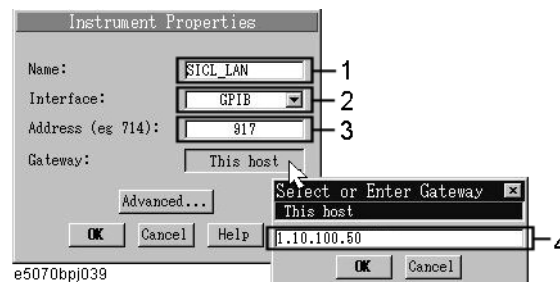


Figure 2-3 shows an example of control using the I/O interface that has been set in the above procedure.

Figure 2-3 Example of control using Agilent VEE

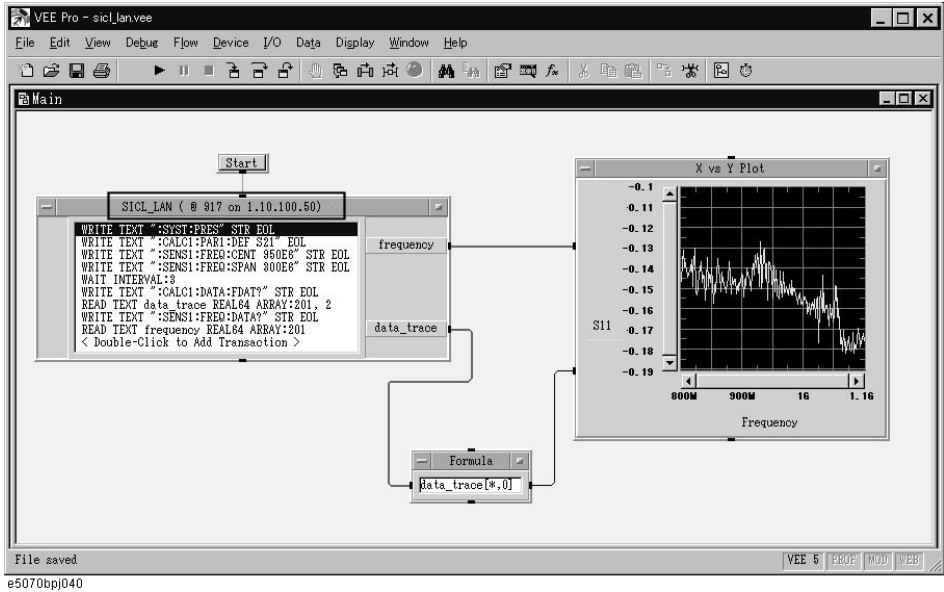

Control over telnet server

In the control system over telnet server, communications are performed through connection between the sockets provided by the processes of the external controller and the E5061A/E5062A to establish a network path between them.

A socket is an endpoint for network connection; port 23 and port 5025 are provided for the sockets for the E5061A/E5062A. Port 23 is provided for conversational control using telnet (user interface program for the TELNET protocol) and port 5025 for control from a program.

Preparing the E5061A/E5062A

To communicate with the external controller, follow these steps to turn on the telnet server of the E5061A/E5062A in advance.

[System] - Misc Setup - Network Setup - Telnet Server [ON]

Conversational control using telnet (using port 23)

You can use telnet to perform conversational control by sending SCPI commands to the E5061A/E5062A on a message-by-message basis. For telnet, the socket of port 23 is used for communications.


In this example, in order to show you the control procedure using telnet, you control the E5061A/E5062A (IP address: 1.10.100.50 and host name: e5061a) from the external controller in the Windows environment.

- Step 1.** Open the MS-DOS command prompt screen.
- Step 2.** At the MS-DOS prompt, type telnet 1.10.100.50 or telnet e5061a and press the return key.
- Step 3.** The telnet screen opens.
- Step 4.** Type a command and press the return key; it is sent to the E5061A/E5062A and executed. If you enter a command that queries some data, the query response is displayed below the line you have entered the command.

Figure 2-4 shows the screen after using the **:SYST:PRES** command on page 479 to reset, the **:SENS{1-4}:FREQ:STAR** command on page 418 and **:SENS{1-4}:FREQ:STOP** command on page 419 commands to set the sweep start value and stop value to 1 GHz and 2 GHz respectively, and checking the settings.

Figure 2-4

Example of control using telnet

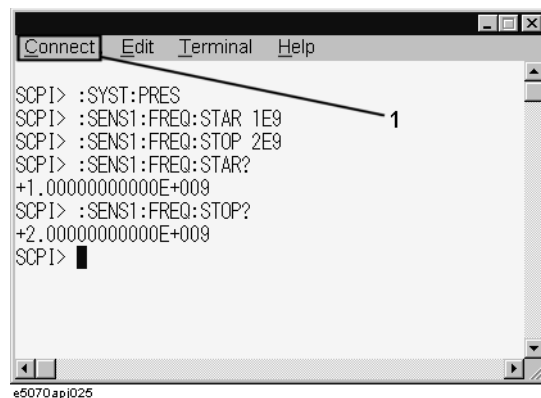

- Step 5.** Select Disconnect from the Connect menu in the telnet screen (1 in Figure 2-4) to break the connection to the E5061A/E5062A and select Exit from the Edit menu to exit the telnet. (In other environment such as the UNIX environment, press] while holding down the control key. The telnet prompt appears. At the telnet prompt, type quit and press the return key. The connection to the E5061A/E5062A breaks and telnet finishes.)

Control from a program (using port 5025)

When controlling the E5061A/E5062A from a program on the external controller, use the socket of port 5025 for connection.

NOTE

Some functions such as service requests that are available in the GPIB remote control system are not available in control over telnet server.

Control using C or Visual Basic

You can control the E5061A/E5062A by socket programming using the C language in the UNIX environment, or Visual C++ or Visual Basic in the Windows environment.

For socket programming, the library for network connection on the TCP/IP protocol is required. For the UNIX environment, BSD (Berkeley Software Distribution) Sockets API is available; for the Windows environment, WinSock (WinSock1.1 and WinSock2.0) created by porting BSD Sockets to Windows and expanding it is available.


For more information on the control method, see a sample program for control using WinSock described in “Controlling Using Telnet Server” on page 184.

Agilent Control using VEE

Agilent VEE allows you to control the E5061A/E5062A through the connection to the socket of port 5025 using To/From Socket. Figure 2-5 shows an example (when the IP address of the E5061A/E5062A is 1.10.100.50). Enter 5025 in the field to specify the port for connection (1 in Figure 2-5) and enter the IP address or host name of the E5061A/E5062A in the field to specify the host name (2 in Figure 2-5).

Figure 2-5

Example of control using Agilent VEE

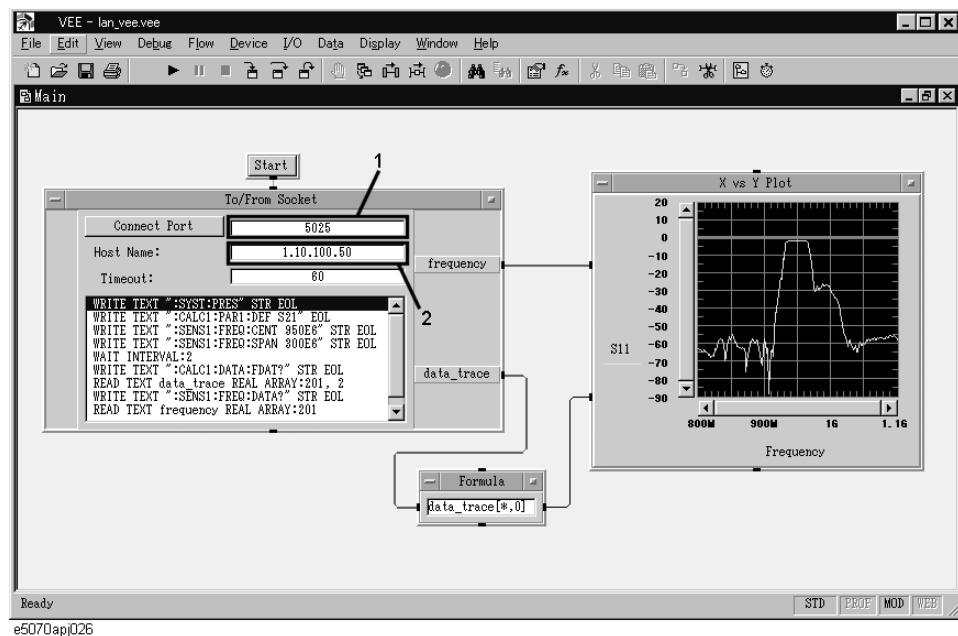

Sending SCPI command messages

Types and structure of commands

The SCPI commands available for the E5061A/E5062A are classified into 2 groups as follows.

E5061A/E5062A commands

Commands specific to the E5061A/E5062A. They cover all measurement functions that the E5061A/E5062A has and some general-purpose functions. The commands in this group are arranged in a hierarchical structure called the command tree (see “Command tree” on page 486). Each command consists of character strings (mnemonics) indicating each hierarchical level and colon (:) separators between hierarchical levels.

IEEE common commands

Commands to cover general-purpose functions defined in IEEE488.2 that are available commonly to instruments that support this standard. The commands in this group have an asterisk (*) at the beginning. For the commands in this group, there is no hierarchical structure.

Concepts of the command tree


The commands at the top of the command tree are called “root command” or simply “root.” To access lower level commands in the tree, you need to specify a specific path like a directory path in the DOS file system. After power-on or reset, the current path is set to the root. Special characters in messages change the path setting as described below.

- | | |
|--------------------|---|
| Message terminator | A message terminator such as the
<new line> character sets the current path to the root. |
| Colon (:) | A colon between 2 command mnemonics lowers the level of the current path in the command tree. A colon used as the first character of a command specifies the command mnemonic that follows as the root-level command. |
| Semicolon (;) | A semicolon does not change the current path and separates 2 commands in the same message. |

Figure 2-6 shows an example of how to use colons and semicolons to efficiently access commands in the command tree.

Figure 2-6

Using colons and semicolons

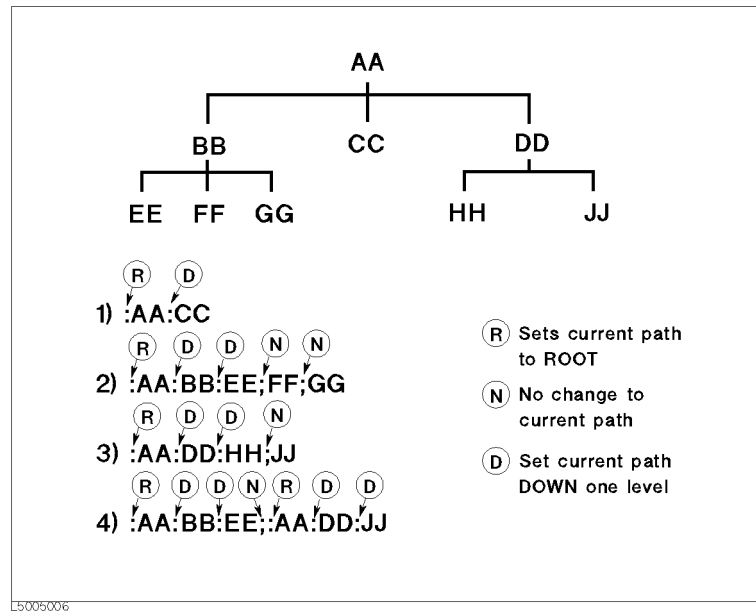

Grammar of messages

This section describes the grammar to send program messages via GPIB. Program messages are messages that the user sends to the instrument from the external controller to control the instrument. A program message consists of 1 or more commands and their necessary parameters.

Upper/lower case sensitivity

Upper/lower case insensitive.

Program message terminator

A program message must be terminated with one of the 3 program message terminators: <new line>, <^END>, or <new line><^END>. <^END> indicates that EOI on the GPIB interface becomes active at the instant when the immediately previous data byte is sent. For example, the OUTPUT command of HTBasic automatically sends the message terminator after the last data byte.

Parameters

A space (ASCII code: 32) is required between a command and its first parameter. When sending several parameters in a single command, separate each parameter with a comma (.).

Message including several commands

When sending 2 or more commands in a single message, separate each command with a semicolon (;). The following example shows how to send the ***CLS** command and the **:STAT:PRES** command in a single message using HTBasic.

OUTPUT 717; "*CLS; :STAT:PRES"

Remote mode

The E5061A/E5062A does not provide remote mode. Therefore, even if you send a GPIB command, it never enters into remote mode automatically. There is no local key to release remote mode.

If you need to prevent misoperation during remote control due to entry from the front panel or mouse, lock the input devices using the following commands.

- **:SYST:KLOC:KBD** command on page 477
- **:SYST:KLOC:MOUS** command on page 478

3

Setting Up the Analyzer

This chapter describes how to configure measurement conditions and how to configure the way the instrument displays measurement results on the LCD.

Selecting the Active Channel/Trace

You can configure the E5061A/E5062A using various commands. Some commands require you to specify, and deal only with, a particular channel or trace while other commands do not require you to do so.

Those commands that do not require you to specify a particular channel or trace apply to currently active channels and traces. Before issuing such a command, therefore, you must make the appropriate channels and traces active.

To make a channel active, use the following command:

- :DISP:WIND{1-4}:ACT on page 318

NOTE

Only the currently displayed channels can be an active channel. Therefore, you must display the desired channels using :DISP:SPL command on page 315 before you can make them active.

To make a trace active, use the following command:

- :CALC{1-4}:PAR{1-4}:SEL on page 286

NOTE

Only the currently displayed traces can be an active trace. Therefore, you must display the desired traces using :CALC{1-4}:PAR:COUN command on page 284 before you can make them active.

Configuring Measurement Conditions

Setting the Number of Traces

When you set the number of traces, that setting determines the upper limit trace number; for example, if the setting is 3, traces 1 through 3 will be displayed. To set the number of traces, use the following command:

- `:CALC{1-4}:PAR:COUN` on page 284

NOTE

Only the currently displayed traces can be an active trace. Therefore, you must set the number of traces appropriately before you can make them active.

Selecting Measurement Parameters

To select the measurement parameter (S parameter) for each trace, use the following command:

- `:CALC{1-4}:PAR{1-4}:DEF` on page 285

Setting the Sweep Condition (Stimulus)

How you can set the sweep condition depends on the sweep type. You can choose between the following four sweep types:

- Liner sweep
- Log sweep
- Segment sweep
- Power sweep

To select one of the above sweep types, use the following command:

- `:SENS{1-4}:SWE:TYPE` on page 428

Turning On/Off of Stimulus Signal Output

To turn on/off the stimulus signal output, use the following commands. For example, if the power output is automatically turned off due to the power trip feature, remove the cause of the overinput and turn on the stimulus signal output by executing the following command. You cannot perform measurement until you turn on the stimulus signal output.

- `:OUTP` on page 365

Configuring Linear Sweep Settings

To set the sweep range, use the following commands:

Start value	<code>:SENS{1-4}:FREQ:STAR</code> on page 418
Stop value	<code>:SENS{1-4}:FREQ:STOP</code> on page 419
Center value	<code>:SENS{1-4}:FREQ:CEN</code> on page 415

Setting Up the Analyzer

Configuring Measurement Conditions

Span value	:SENS{1-4}:FREQ:SPAN on page 417
------------	----------------------------------

To set the number of measurement points, use the following command:

- :SENS{1-4}:SWE:POIN on page 425

To set the measurement time, use the following commands:

Measurement time	:SENS{1-4}:SWE:TIME on page 426
Turning on/off auto setting	:SENS{1-4}:SWE:TIME:AUTO on page 427

To set the sweep delay time, use the following command:

- :SENS{1-4}:SWE:DEL on page 424

To set the IF bandwidth, use the one of the following commands (both provide the same function):

- :SENS{1-4}:BAND on page 372
- :SENS{1-4}:BWID on page 373

Setting Power Level

When the instrument is equipped with the power range expansion function (Option 250, 275, 1E1), you select the power range using the following command:

- :SOUR{1-4}:POW:ATT on page 432

To set the power level, use the following command:

- :SOUR{1-4}:POW on page 431

To select whether to output the same power level (the set value for port 1) or different power level for each port, use the following command:

- :SOUR{1-4}:POW:PORT:COUP on page 434
- :SOUR{1-4}:POW:PORT{1-2} on page 435

To set the correction of power level attenuation proportional to the frequency (power slope feature), use the following command:

- :SOUR{1-4}:POW:SLOP:STAT on page 437
- :SOUR{1-4}:POW:SLOP on page 436

Configuring Segment Sweep Settings

When you opt to use segment sweep, you can set all items (in the segment sweep table) using a single command:

- :SENS{1-4}:SEGM:DATA on page 421

Alternatively, you can configure the segment sweep settings based on the data contained in a CSV file by issuing the following command:

- :MMEM:LOAD:SEGM on page 351

Also, you can save the contents of the current segment sweep table to a file by issuing the following command:

- :MMEM:STOR:SEGM on page 362

For more information on how to save and load the segment sweep table, refer to “Saving and recalling the segment sweep table.”

Configuring Power Sweep Settings

To set the sweep range, use the following commands:

Start value	:SOUR{1-4}:POW:STAR on page 439
Stop value	:SOUR{1-4}:POW:STOP on page 440
Center value	:SOUR{1-4}:POW:CENT on page 433
Span value	:SOUR{1-4}:POW:SPAN on page 438

To set the fixed frequency (CW frequency), use the following command:

- :SENS{1-4}:FREQ on page 414

To set the number of points, the sweep time, the sweep delay time, and the IF bandwidth, use the same commands as for the linear/log sweep.

Configuring Averaging Settings

To configure the smoothing settings, use the following commands:

On/off	:SENS{1-4}:AVER on page 370
Averaging factor	:SENS{1-4}:AVER:COUN on page 371
Clear (Restart)	:SENS{1-4}:AVER:CLE on page 370

Setting the System Z0

NOTE

This function is available with the firmware version 3.01 or greater.

To set the system characteristic impedance (Z0), use the following command:

- :SENS:CORR:IMP on page 369

Configuring Display Settings

Setting the Layout of Windows and Graphs

You can split the E5061A/E5062A's LCD screen into multiple windows that display channel-specific result information, and can select the window layout from a number of variations. In addition, you can place on screen a segment sweep table or echo window (which you can use to display messages from your custom program).

Selecting the Window Layout (Channel Display Mode)

One window displays the results for a single channel. You cannot have a single window display the results from more than one channel. This means that setting the window layout determines the number of channels displayed on screen.

To select one of the 14 different window layouts shown in Figure 3-1, use the following command:

- :DISP:SPL on page 315

Selecting the Graph Layout (Trace Display Mode)

You can place a number of trace graphs in each window, and can select one of the pre-defined graph layouts. The number of graphs differ depending on your selected graph layout. If the number of graphs is equal to or larger than the number of traces (set by the :CALC{1-4}:PAR:COUN command on page 284 command), each graph always displays one trace. On the other hand, if the number of graphs is smaller than the number of traces, some of the graphs display two or more traces. Graph 1 is populated with trace 1, graph 2 with trace 2, and so on. Traces whose numbers exceed the last graph's number will populate graph 1, graph 2, and so on.

To select one of the 14 different graph layouts shown in Figure 3-1, use the following command:

- :DISP:WIND{1-4}:SPL on page 323

Maximizing a Window and Graphs

When you have multiple windows displayed, you can maximize the active channel window so that it covers the entire screen area. To maximize a window, use the following command:


- :DISP:MAX on page 314

Similarly, when you have multiple traces displayed, you can maximize the active trace so that it extends throughout the entire window. To maximize a trace, use the following command:

- :DISP:WIND{1-4}:MAX on page 322

Figure 3-1

Window/graph layouts and command parameters

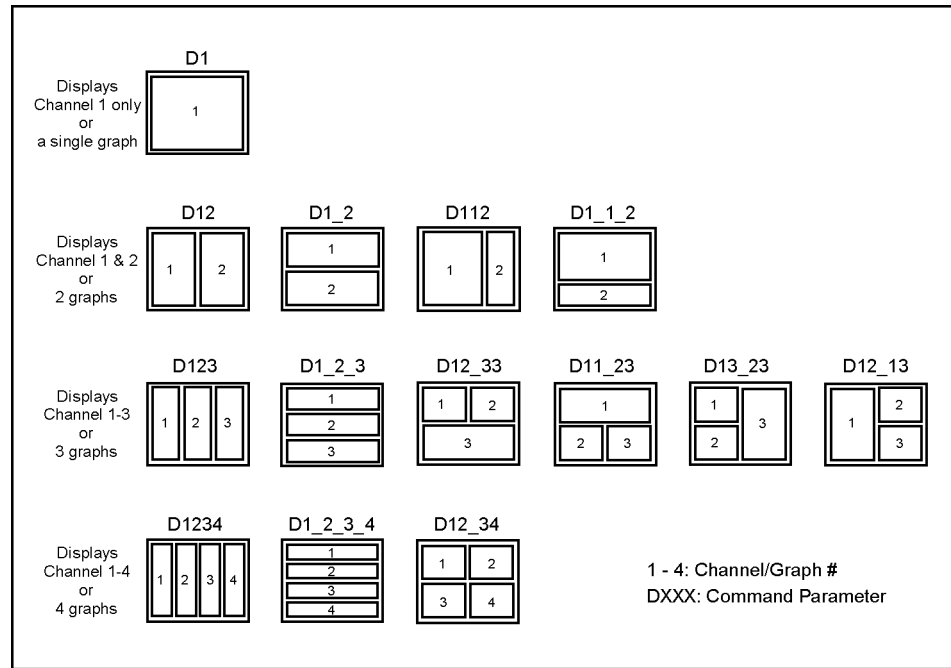

e5061ape001

Showing/Hiding a Table or Echo Window

You can have the following items displayed at the bottom of the LCD screen.

- Segment sweep table
- Limit table
- Marker list table
- Echo window (a window you can use to display messages from your custom program)

To show or hide each of the above items, use the following command:

- :DISP:TABL on page 316

You can have two or more of the above items displayed at a time. The screen displays only the item selected using the following command:

- :DISP:TABL:TYPE on page 317

Showing/Hiding Softkey Labels

You can show or hide the softkey labels placed alongside the right-hand edge of the LCD screen. To show or hide the softkey labels, use the following command:

- :DISP:SKEY on page 314

Configuring Trace Display Settings

Selecting Which Traces to Display

Each trace has two different representations: data and memory traces. You can show or hide the data and memory traces independently of each other. To show or hide the data or memory traces, use the following commands:

Data trace	:DISP:WIND{1-4}:TRAC{1-4}:STAT on page 329
Memory trace	:DISP:WIND{1-4}:TRAC{1-4}:MEM on page 328

To copy the data trace to the memory trace, use the following command:

- :CALC{1-4}:MATH:MEM on page 281

Configuring Cross-Trace Math Operations

You can perform math operations performed between the data and memory traces and have the results displayed as the data trace. To perform cross-trace math operations, use the following command:

- :CALC{1-4}:MATH:FUNC on page 281

Configuring Smoothing Settings

To turn on or off smoothing, use the following command:

- :CALC{1-4}:SMO on page 293

The smoothing aperture is expressed as a percentage with respect to the sweep range. To set the smoothing aperture, use the following command:

- :CALC{1-4}:SMO:APER on page 294

Selecting the Data Format

You can select the following data format:

- ☐ Rectangular display formats
 - Log magnitude format
 - Phase format
 - Group delay format
 - Linear magnitude format
 - SWR format
 - Real format
 - Imaginary format
 - Expanded phase format
 - Positive phase format
- ☐ Imaginary format
- ☐ Expanded phase format

To select the measurement parameter data format, use the following command:

- :CALC{1-4}:FORM on page 219

Configuring the Display Scale

Depending on the measurement parameter data format, you can configure the display scale in one of the following two ways:

Rectangular display formats:

When you are using one of rectangular display formats (Logarithmic magnitude/Phase/Group delay/Linear magnitude/SWR/Real/Imaginary/Expanded phase/Positive phase), you can configure the display scale by setting the following four items:

Number of divisions	:DISP:WIND{1-4}:Y:DIV on page 336
Scale per division	:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV on page 330
Reference graticule line	:DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS on page 332
Reference graticule line value	:DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV on page 331

NOTE

The number of divisions is a channel-wide setting (shared among all traces) while the remaining three settings are trace-specific.

You can show or hide graticule label (the label on the left-hand side of the graticule lines) by issuing the following command:

- :DISP:WIND{1-4}:LAB on page 321

Smith Chart/Polar formats:

When you are using one of Smith chart/Polar formats, you can only set the full scale value (the outermost circle's value) using the following command:

- :DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV on page 330

Auto Scale

You can use Auto Scale to automatically set the display scale. This feature works by automatically adjusting the reference division line value and the scale value per division when you are using one of rectangular display formats; or the full scale value when you are using one of Smith chart/Polar formats.

To perform Auto Scale, use the following command:

- :DISP:WIND{1-4}:TRAC{1-4}:Y:AUTO on page 329

Printing a Message in the Echo Window

You can print a message in the echo window by issuing the following command:

- :DISP:ECHO on page 311

You can clear any message displayed in the echo window by issuing the following command:

- :DISP:ECHO:CLE on page 311

Turning On or Off Display Update

To turn on or off the update of the LCD screen, use the following command:

- :DISP:ENAB on page 312

Showing/Hiding Frequencies

To show or hide frequencies on the LCD screen, use the following command:

- :DISP:ANN:FREQ on page 304

Showing or Hiding the Title

To show or hide the title, use the following command:

- :DISP:WIND{1-4}:TITL on page 324

To define the title string that appears in the title display area, use the following command:

- :DISP:WIND{1-4}:TITL:DATA on page 324

Configuring Date/Time Display

To show or hide the current date and time on the left-hand side of the instrument status bar, use the following command:

- :DISP:CLOC on page 305

To set the date and time, use the following command:

- :SYST:DATE on page 475
- :SYST:TIME on page 482

Turning On or Off the LCD Backlight

To turn on or off the LCD backlight, use the following command (note that turning off the backlight makes the screen unreadable):

- :SYST:BACK on page 472

Setting display colors

Selecting display mode

You can select the display mode of the LCD display from 2 modes: normal display (background: black) or inverted display (background: white).

To select the display mode, use the following command:

- :DISP:IMAG on page 313

Setting display color for each item

To set the display colors, use the following commands:

Data trace	:DISP:COL{1-2}:TRAC{1-4}:DATA on page 309
Memory trace	:DISP:COL{1-2}:TRAC{1-4}:MEM on page 310
Graph	:DISP:COL{1-2}:GRAT{1-2} on page 307
Limit test	:DISP:COL{1-2}:LIM{1-2} on page 308
Background	:DISP:COL{1-2}:BACK on page 306

Resetting display colors to factory state

You can reset the display colors in normal display and inverted display to the preset factory state.

To reset the display colors, use the following command:

- :DISP:COL{1-2}:RES on page 308

Saving and Loading the Settings

You can save the settings for measurement conditions and screen display to a file along with other instrument settings, and can later load them from the file.

Once you have saved the measurement condition and screen display settings to a file, you can later load them whenever necessary; you can quickly modify the settings loaded from a file to create new settings without having to issue many commands.

To save the current settings to a file, use the following command:

- :MMEM:STOR on page 353

To load the settings from a file, use the following command:

- :MMEM:LOAD on page 345

For more information on how to save and load the settings, refer to “Saving and recalling instrument status.”

Sample Program

Example 3-1 is a sample program that demonstrates how to configure measurement conditions. You can find the source file of this program, named setup.htb, on the sample program disk.

The sample program puts the instrument into the preset state, configures it as shown in Table 3-1, and saves the settings to a file named “Ex_3_1.sta”.

Table 3-1

Target settings in Example 3-1

Item			Setting
Window Layout			Channel 1 in the upper window (2/3 of the screen height) and channel 2 in the lower window (1/3 of the screen height)
Channel 1	Sweep type		Segment
	Sweep range		See Table 3-2.
	Number of measurement points		
	IF bandwidth		
	Power		
	Number of traces		4
	Graph Layout		Four graphs at upper left, upper right, lower left, and lower right.
	Trace 1	Measurement parameter	S11
		Data format	Smith chart (Lin)
		Full-scale value	2
	Trace 2	Measurement parameter	S21
		Data format	Log magnitude
		Reference division line number	9
		Reference division line value	2
		Scale per division	10 dBm
	Trace 3	Measurement parameter	S12
		Data format	Log magnitude
		Reference division line number	9
		Reference division line value	2
		Scale per division	10 dBm
	Trace 4	Measurement parameter	S22
		Data format	Smith chart (Lin)
		Full-scale value	2

Table 3-1 Target settings in Example 3-1

Item			Setting
Channel 2	Sweep type		Linear
	Sweep range	Center value	1.9 GHz
		Span value	500 MHz
	Number of measurement points		101
	IF bandwidth		30 kHz
	Power		0 dBm
	Number of traces		4
	Graph Layout		Two graphs at left and right
	Trace 1	Measurement parameter	S21
		Data format	Log magnitude
		Reference division line number	9
		Reference division line value	2
		Scale per division	10 dBm
	Trace 2	Measurement parameter	S22
		Data format	Smith chart (Lin)
		Full-scale value	2

Table 3-2 Segment table for channel 1

Segment Number	Start value	Stop value	Number of measurement points	IF bandwidth	Power
1	1.7 GHz	1.9 GHz	21	30 kHz	0 dBm
2	1.9 GHz	2 GHz	101	10 kHz	-10 dBm
3	2 GHz	2.2 GHz	21	30 kHz	0 dBm

Setting Up the Analyzer

Sample Program

The program is described in detail below:

Line 70	Assigns a GPIB address to the I/O pass.
Line 90	Stores the number of channel 1's sweep segments into the Segm variable.
Lines 100 to 150	These lines store the start and stop values for channel 1's segments 1 through 3 into the Star1(*) and Stop1(*) variables, respectively.
Lines 160 to 170	These lines store channel 2's center and span values into the Star2 and Stop2 variables, respectively.
Lines 180 to 210	These lines store the number of points for channel 1's segments 1 through 3 into the Nop1(*) variable, and the number of measurement points for channel 2 into the Nop2 variable.
Lines 220 to 250	These lines store the IF bandwidth for channel 1's segments 1 through 3 into the If_bw1(*) variable, and the IF bandwidth for channel 2 into the If_bw2 variable.
Lines 260 to 290	These lines store the power for channel 1's segments 1 through 3 into the Pow1(*) variable, and the power for channel 2 into the Pow2 variable.
Lines 300 to 310	These lines store the number of channel 1's traces into the Num_of_tr1 variable, and the number of channel 2's traces into the Num_of_tr2 variable.
Lines 320 to 330	These lines store channel 1's graph layout into the Allocate1\$ variable, and channel 2's graph layout into the Allocate2\$ variable.
Lines 340 to 390	These lines store the measurement parameters for channel 1's traces 1 through 4 into the Para1\$(*) variable, and the measurement parameters for channel 2's traces 1 through 2 into the Para2\$(*) variable.
Lines 400 to 450	These lines store the data formats for channel 1's traces 1 through 4 into the Fmt1\$(*) variable, and the data formats for channel 2's traces 1 through 2 into the Fmt2\$(*) variable.
Lines 460 to 480	These lines store the reference division line numbers for channel 1's traces 2 through 3 into the Ref_pos1(*) variable, and the reference division line numbers for channel 2's trace 1 into the Ref_pos2(*) variable.
Lines 490 to 510	These lines store the reference division line values for channel 1's traces 2 through 3 into the Ref_lev1(*) variable, and the reference division line values for channel 2's trace 1 into the Ref_lev2(*) variable.
Lines 520 to 570	These lines store the data formats for channel 1's traces 1 through 4 into the Fmt1\$(*) variable, and the data formats for channel 2's traces 1 through 2 into the Fmt2\$(*) variable.
Line 580	Stores the name of the file into the File\$ variable.
Line 600	Puts the instrument into preset state.
Line 620	Places the window for channel 1 in the upper part of the LCD screen, and the window for channel 2 in the lower part.
Lines 630 to 640	These lines turn on Continuous Activation mode for channels 1 and 2.

Line 680	Sets channel 1's sweep type to "segment".
Lines 690 to 730	These lines set up the segment table for channel 1. Line 600: Sends the command that sets up the segment table along with the parameter header ("5,0,1,1,0,0" causes the IF bandwidth and power to be set on a segment by segment basis; Segm represents the number of segments). Lines 700 to 730: Send the data for the start and stop values, number of points, IF bandwidth, and power (Star1, Stop1, Nop1, If_bw1, Pow1) on a segment by segment basis.
Lines 750 to 760	For channel 1, these lines set the number of traces to Num_of_tr1 and the graph layout to Allocate1\$.
Lines 770 to 890	For channel 1, the program iterates the following loop while incrementing i from 1 to Num_of_tr1 for each trace. Line 780: Sets the measurement parameter to Para1\$(i). Line 790: Makes trace(i) active. Line 800: Sets the data format to Fmt1\$(i). Line 830: If the data format is Smith chart or polar, this line sets the full-scale value to Scale1(i). Lines 850 to 870: If the data format is neither Smith chart nor polar, these lines set the reference division line number to Ref_pos1(i), the reference division line value to Ref_lev1(i), and the scale per division to Scale1(i).
Line 930	Sets channel 2's sweep type to "linear".
Lines 940 to 980	For channel 2, these lines set the center value to Cent2, the span value to Span2, the number of measurement points to Nop2, the IF bandwidth to If_bw2, and the power to Pow2.
Lines 1000 to 1010	For channel 2, these lines set the number of traces to Num_of_tr2 and the graph layout to Allocate2\$.
Lines 1020 to 1140	For channel 2, the program iterates the following loop while incrementing i from 1 to Num_of_tr2 for each trace. Line 1030: Sets the measurement parameter to Para2\$(i). Line 1040: Makes trace(i) active. Line 1050: Sets the data format to Fmt2\$(i). Line 1080: If the data format is Smith chart or polar, this line sets the full-scale value to Scale2(i). Lines 1100 to 1120: If the data format is neither Smith chart nor polar, these lines set the reference division line number to Ref_pos2(i), the reference division line value to Ref_lev2(i), and the scale per division to Scale2(i).
Line 1160	Saves the settings of the E5061A/E5062A under the file name File\$.

Example 3-1

Configuring Measurement Conditions (setup.htb)

```

10  DIM Allocate1$(9),Allocate2$(9),File$(20)
20  DIM Para1$(1:4)[9],Para2$(1:2)[9],Fmt1$(1:4)[9],Fmt2$(1:2)[9]
30  REAL Star1(1:3),Stop1(1:3),Pow1(1:3),Cent2,Span2,Pow2
40  REAL Ref_rev1(1:4),Ref_rev2(1:2),Scale1(1:4),Scale2(1:2)
50  INTEGER Segm,Nop1(1:3),Nop2,Num_of_tr1,Num_of_tr2
60  INTEGER Ref_pos1(1:4),Ref_pos2(1:2),I
70  ASSIGN @Agte507x TO 717
80  !
90  Segm=3                ! Number of Segment Ch.1      : 3
100 Star1(1)=1.7E+9       ! Start Frequency Ch.1 Segm.1: 1.7 GHz
110 Star1(2)=1.9E+9       !                      Segm.2: 1.9 GHz
120 Star1(3)=2.E+9        !                      Segm.3: 2 GHz
130 Stop1(1)=1.9E+9       ! Stop Frequency Ch.1 Segm.1: 1.9 GHz
140 Stop1(2)=2.E+9        !                      Segm.2: 2 GHz
150 Stop1(3)=2.2E+9       !                      Segm.3: 2.2 GHz
160 Cent2=1.9E+9          ! Center Frequency Ch.2      : 1.9 GHz
170 Span2=5.00E+8         ! Span Ch.2                  : 500 MHz
180 Nop1(1)=21            ! Number Ch.1 Segm.1: 21
190 Nop1(2)=101          ! of Points Segm.2: 101
200 Nop1(3)=21           !                      Segm.3: 21
210 Nop2=101             !                      Ch.2      : 101
220 If_bw1(1)=5.0E+4      ! IF Bandwidth Ch.1 Segm.1: 50 kHz
230 If_bw1(2)=1.0E+4      !                      Segm.2: 10 kHz
240 If_bw1(3)=5.0E+4      !                      Segm.3: 50 kHz
250 If_bw2=7.0E+4         !                      Ch.2      : 70 kHz
260 Pow1(1)=0             ! Power Ch.1 Segm.1: 0 dBm
270 Pow1(2)=-10           !                      Segm.2: -10 dBm
280 Pow1(3)=0             !                      Segm.3: 0 dBm
290 Pow2=0                !                      Ch.2      : 0 dBm
300 Num_of_tr1=4          ! Number Ch.1              : 4
310 Num_of_tr2=2          ! of Traces Ch.2           : 2
320 Allocate1$="D12_34"   ! Allocate Traces Ch.1     : D12_34
330 Allocate2$="D12"      !                      Ch.2     : D12
340 Para1$(1)="S11"        ! Measurement Ch.1 Trace1: S11
350 Para1$(2)="S21"        ! Parameter Trace2: S21
360 Para1$(3)="S12"        !                      Trace3: S12
370 Para1$(4)="S22"        !                      Trace4: S22
380 Para2$(1)="S21"        !                      Ch.2 Trace1: S21
390 Para2$(2)="S22"        !                      Trace2: S22
400 Fmt1$(1)="SLIN"       ! Data Format Ch.1 Trace1:
    Smith(Lin/Phase)
410 Fmt1$(2)="MLOG"       !                      Trace2: Log Mag
420 Fmt1$(3)="MLOG"       !                      Trace3: Log Mag
430 Fmt1$(4)="SLIN"       !                      Trace4: Smith(Lin/Phase)
440 Fmt2$(1)="MLOG"       !                      Ch.2 Trace1: Log Mag
450 Fmt2$(2)="SLIN"       !                      Trace2: Smith(Lin/Phase)
460 Ref_pos1(2)=9         ! Reference Ch.1 Trace2: 9
470 Ref_pos1(3)=9         ! Position Trace3: 9
480 Ref_pos2(1)=9         !                      Ch.2 Trace1: 9
490 Ref_lev1(2)=0         ! Reference Level Ch.1 Trace2: 0 dBm
500 Ref_lev1(3)=0         !                      Trace3: 0 dBm
510 Ref_lev2(1)=0         !                      Ch.2 Trace1: 0 dBm
520 Scale1(1)=2           ! Scale Ch.1 Trace1: 2
530 Scale1(2)=10          !                      Trace2: 10 dBm
540 Scale1(3)=10          !                      Trace3: 10 dBm

```

```

550 Scale1(4)=2          !                      Trace4: 2
560 Scale2(1)=10         !                      Ch.2 Trace1: 10 dBm
570 Scale2(2)=2          !                      Trace2: 2
580 File$="Ex_3_1.sta"   ! Save File Name      : Ex_3_1.sta
590 !
600 OUTPUT @Agte507x;":SYST:PRES"
610 !
620 OUTPUT @Agte507x;":DISP:SPL D1_1_2"
630 OUTPUT @Agte507x;":INIT1:CONT ON"
640 OUTPUT @Agte507x;":INIT2:CONT ON"
650 !
660 ! Channel 1
670 !
680 OUTPUT @Agte507x;":SENS1:SWE:TYPE SEGM"
690 OUTPUT @Agte507x;":SENS1:SEGM:DATA 5,0,1,1,0,0,";Segm;",";
700 FOR I=1 TO Segm-1
710     OUTPUT
@Agte507x;Star1(I);",";Stop1(I);",";Nop1(I);",";If_bw1(I);",";Pow1(I);",
";
720 NEXT I
730 OUTPUT
@Agte507x;Star1(Segm);",";Stop1(Segm);",";Nop1(Segm);",";If_bw1(Segm);",
";Pow(Segm)
740 !
750 OUTPUT @Agte507x;":CALC1:PAR:COUN ";Num_of_tr1
760 OUTPUT @Agte507x;":DISP:WIND1:SPL "&Allocate1$
770 FOR I=1 TO Num_of_tr1
780     OUTPUT @Agte507x;":CALC1:PAR"&VAL$(I)&":DEF "&Para1$(I)
790     OUTPUT @Agte507x;":CALC1:PAR"&VAL$(I)&":SEL "
800     OUTPUT @Agte507x;":CALC1:FORM "&Fmt1$(I)
810     SELECT Fmt1$(I)
820         CASE "SLIN","SLOG","SCOM","SMIT","SADM","PLIN","PLOG","POL"
830             OUTPUT @Agte507x;":DISP:WIND1:TRAC"&VAL$(I)&":Y:PDIV
";Scale1(I)
840         CASE ELSE
850             OUTPUT @Agte507x;":DISP:WIND1:TRAC"&VAL$(I)&":Y:RPOS
";Ref_pos1(I)
860             OUTPUT @Agte507x;":DISP:WIND1:TRAC"&VAL$(I)&":Y:RLEV
";Ref_rev1(I)
870             OUTPUT @Agte507x;":DISP:WIND1:TRAC"&VAL$(I)&":Y:PDIV
";Scale1(I)
880         END SELECT
890     NEXT I
900 !
910 ! Channel 2
920 !
921 PAUSE
930 OUTPUT @Agte507x;":SENS2:SWE:TYPE LIN"
940 OUTPUT @Agte507x;":SENS2:FREQ:CENT ";Cent2
950 OUTPUT @Agte507x;":SENS2:FREQ:SPAN ";Span2
960 OUTPUT @Agte507x;":SENS2:SWE:POIN ";Nop2
970 OUTPUT @Agte507x;":SENS2:BAND ";If_bw2
980 OUTPUT @Agte507x;":SOUR2:POW ";Pow2
990 !
1000 OUTPUT @Agte507x;":CALC2:PAR:COUN ";Num_of_tr2
1010 OUTPUT @Agte507x;":DISP:WIND2:SPL "&Allocate2$
1020 FOR I=1 TO Num_of_tr2
1030     OUTPUT @Agte507x;":CALC2:PAR"&VAL$(I)&":DEF "&Para2$(I)

```

Setting Up the Analyzer

Sample Program

```
1040      OUTPUT @Agte507x;":CALC2:PAR"&VAL$(I)&":SEL"
1050      OUTPUT @Agte507x;":CALC2:FORM "&Fmt2$(I)
1060      SELECT Fmt2$(I)
1070          CASE "SLIN", "SLOG", "SCOM", "SMIT", "SADM", "PLIN", "PLOG", "POL"
1080              OUTPUT @Agte507x;":DISP:WIND2:TRAC"&VAL$(I)&":Y:PDIV
";Scale2(I)
1090          CASE ELSE
1100              OUTPUT @Agte507x;":DISP:WIND2:TRAC"&VAL$(I)&":Y:RPOS
";Ref_pos2(I)
1110              OUTPUT @Agte507x;":DISP:WIND2:TRAC"&VAL$(I)&":Y:RLEV
";Ref_rev2(I)
1120              OUTPUT @Agte507x;":DISP:WIND2:TRAC"&VAL$(I)&":Y:PDIV
";Scale2(I)
1130          END SELECT
1140      NEXT I
1150      !
1160      OUTPUT @Agte507x;":MMEM:STOR ""&File$&""
1170      END
```

4

Performing a Calibration

This chapter describes how to obtain the calibration coefficients and perform error correction and how to define the calibration kit required to obtain the calibration coefficients.

Calibration

You need to execute calibration to eliminate error elements related to measurement and perform accurate measurement.

Performing a Calibration (Obtaining the Calibration Coefficients)

Selecting a Calibration Kit

To select a calibration kit, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT** on page 375

Selecting a Calibration Type

The calibration coefficients are calculated based on the selected calibration type. Before you can calculate the calibration coefficients, therefore, you must select the appropriate calibration type using the following command.

Calibration type		Command
Response	OPEN	:SENS{1-4}:CORR:COLL:METH:OPEN on page 402
	SHORT	:SENS{1-4}:CORR:COLL:METH:SHOR on page 402
	THRU	:SENS{1-4}:CORR:COLL:METH:THRU on page 404
Enhanced Response		:SENS{1-4}:CORR:COLL:METH:ERES on page 399
Full 1-Port		:SENS{1-4}:CORR:COLL:METH:SOLT1 on page 403
Full 2-Port		:SENS{1-4}:CORR:COLL:METH:SOLT2 on page 403

To check the currently selected calibration type, use the following command:

- **:SENS{1-4}:CORR:COLL:METH:TYPE?** on page 405

Measuring the Calibration Data

To measure the calibration data, use the following command:

Calibration data items	Command
OPEN	:SENS{1-4}:CORR:COLL:OPEN on page 406
SHORT	:SENS{1-4}:CORR:COLL:SHOR on page 407
LOAD	:SENS{1-4}:CORR:COLL:LOAD on page 401
THRU	:SENS{1-4}:CORR:COLL:THRU on page 408
Isolation	:SENS{1-4}:CORR:COLL:ISOL on page 399

NOTE

You cannot run more than one of the commands listed above at a time; if you issue another command before the currently running command completes successfully, the current command will be aborted. When you write a program that issues multiple calibration commands in series, therefore, you should use the ***OPC?** command on page 198 command or some other means to ensure that no command is executed before the

_____ preceding command completes.

As shown in Table 4-1, the data required to calculate the calibration coefficients differs depending on the selected calibration type.

Table 4-1 Calibration Types and Required Data

Calibration type Selected ports are enclosed in parentheses.		Data				
		OPEN	SHORT	LOAD	THRU	Isolation
Response	OPEN (a)	a	Not required	[a]	Not required	Not required
	SHORT (a)	Not required	a	[a]	Not required	Not required
	THRU (a-b)	Not required	Not required	Not required	a-b	[a-b]
Enhanced Response (a-b)		b	b	b	a-b	[a-b]
Full 1-Port (a)		a	a	a	Not required	Not required
Full 2-Port (a-b)		a, b	a, b	a, b	a-b, b-a	[a-b], [b-a]

In the data section in the table, the letter m (for example, 1, a) represents the measurement data at port m; m-n (for example, 1-2, a-b) represents the measurement data between response port m and stimulus port n. You can omit data enclosed in brackets.

Performing a Calibration

Calibration

Calculating the Calibration Coefficients

To calculate the calibration coefficients, use the following command:

Calibration type	Command
All calibration types	:SENS{1-4}:CORR:COLL:SAVE on page 407

Before issuing the above command, you must measure all the required calibration data items according to your selected calibration types (see Table 4-1).

Calculating the calibration coefficients clears all calibration data regardless it is used for the calculation. The calibration type selection is also cleared, which results in the state when no calibration type is selected.

Turning On or Off Error Correction

To turn on or off Error Correction, use the following command:

- **:SENS{1-4}:CORR:STAT** on page 412

Also, once you have calculated the calibration coefficient using the **:SENS{1-4}:CORR:COLL:SAVE** command, Error Correction is automatically turned on.

Using ECal

An ECal (Electronic Calibration) module allows you to perform full 1/2-port calibration and response (THRU) calibration without having to replacing the standard device.

ECal works by using the calibration kit data contained in the ECal module, instead of the calibration kit data selected on the part of the E5061A/E5062A. This means that you do not have to define or select a calibration kit when using ECal.

NOTE

When two or more ECal modules are connected through the USB port, the system uses the calibration kit data contained in the first ECal module.

To perform ECal, use the following command:

Calibration type	Command
Full 1-Port Calibration	:SENS{1-4}:CORR:COLL:ECAL:SOLT1 on page 397
Full 2-Port Calibration	:SENS{1-4}:CORR:COLL:ECAL:SOLT2 on page 397
Enhanced Response Calibration	:SENS{1-4}:CORR:COLL:ECAL:ERES on page 395
Response Calibration (THRU)	:SENS{1-4}:CORR:COLL:ECAL:THRU on page 398

Simply issuing one of the above commands completes all the tasks necessary for error correction, including measuring the calibration data, calculating the calibration coefficients, and running on the Error Correction feature.

You can control whether to perform isolation measurement during ECal. To turn on or off isolation measurement, use the following command:

- :SENS{1-4}:CORR:COLL:ECAL:ISOL on page 395

NOTE

If the ECal module does not support isolation measurement, the system never performs isolation measurement.

Checking the Applied Calibration Type

When you turn on Error Correction, you can check the calibration type actually applied to each trace. To check the calibration type, use the following command:

- :SENS{1-4}:CORR:TYPE{1-4}? on page 413

NOTE

The above command reads out the same parameter (SOLT3) for both the full 3 port and the simplified full 3-port and therefore they cannot be discriminated. For the same reason, the full 4 port and the simplified full 4 port cannot be discriminated.

Defining Calibration Kits

Selecting a Calibration Kit

To select a calibration kit, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT** on page 375

Setting the Calibration Kit Name

To set the name of a calibration kit, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:LAB** on page 376

Standard Definitions

Selecting a Standard Type To select a standard type, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:TYPE** on page 393

Setting the Standard Name To set the standard name, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:LAB** on page 391

Setting the Standard Value To set the standard value, use the following command:

Item	Command
C0	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C0 on page 382
C1	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C1 on page 383
C2	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C2 on page 384
C3	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C3 on page 385
L0	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L0 on page 387
L1	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L1 on page 388
L2	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L2 on page 389
L3	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L3 on page 390
Offset Delay	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:DEL on page 386
Offset Loss	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:LOSS on page 392
Offset Z0	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:Z0 on page 394
Arbitrary Impedance	:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:ARB on page 381

As shown in Table 4-2, you need to set different items depending on the standard type.

Table 4-2

Settings Specific to Each Standard Type

Standard Types	C0 to C3	L0 to L3	Offset Delay	Offset Loss	Offset Z0	Arbitrary Impedance
OPEN	√		√	√	√	
SHORT		√	√	√	√	
LOAD			√	√	√	
THRU			√	√	√	
Arbitrary Impedance			√	√	√	√

You need to set the items identified by √ marks in the table above.

Defining a Standard Class Assignment

To select the standard to be applied to the OPEN measurement for each port, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:ORD:OPEN** on page 378

To select the standard to be applied to the SHORT measurement for each port, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:ORD:SHOR** on page 379

To select the standard to be applied to the LOAD measurement for each port, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:ORD:LOAD** on page 377

To select the standard to be applied to the THRU measurement between each pair of ports, use the following command:

- **:SENS{1-4}:CORR:COLL:CKIT:ORD:THRU** on page 380

Saving and Loading Calibration Coefficients

You can save calibration coefficients to a file along with other instrument settings, and can later load them from the file.

NOTE

You cannot save, load, read, or write calibration coefficients independently of the other instrument settings.

By default, the system does not save calibration coefficients when it saves instrument settings. To save calibration coefficients, therefore, you must explicitly configure the system to save calibration coefficients by issuing the following command:

- **:MMEM:STOR:STYP** on page 363

To save calibration coefficients to a file, use the following command:

- **:MMEM:STOR** on page 353

To load calibration coefficients from a file, use the following command:

- **:MMEM:LOAD** on page 345

For more information on how to save and load calibration coefficients, refer to “Saving and recalling instrument status.”

Sample Program

Calibration

Example 4-1 shows a sample program that demonstrates how to calibrate the instrument. You can find the source file of this program, named `cal.htb`, on the sample program disk.

The sample program performs calibration with the specified calibration type, and saves the results to a file named “`Ex_4_1.sta`.”

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Line 50	Stores the name of the file (<code>Ex_4_1.sta</code>) into the <code>File\$</code> variable.
Line 60	Stores the channel number (1) into the <code>Ch\$</code> variable.
Line 80	Calls a subprogram named <code>Select_cal_kit</code> to select the calibration kit.
Line 110	Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while selecting the calibration type number.
Lines 130 to 210	These lines display the list of supported calibration types, and prompts the user to choose one of the items by typing in the appropriate number.
Line 220	Converts the entered value into an integer and stores it into the <code>Cal_type</code> variable.
Line 230	Returns to the entry start line if an invalid value is contained in <code>Cal_type</code> .
Lines 260 to 420	These lines call a subprogram named <code>Select_port</code> to select the appropriate port based on the value of <code>Cal_type</code> , and then perform calibration. - Lines 280 to 290: If <code>Cal_type</code> = 1, the program calls a subprogram named <code>Cal_resp</code> to perform response calibration (OPEN) after selecting the port. - Lines 310 to 320: If <code>Cal_type</code> = 2, the program calls the subprogram <code>Cal_resp</code> to perform response calibration (SHORT) after selecting the port. - Lines 340 to 350: If <code>Cal_type</code> = 3, the program calls a subprogram named <code>Cal_resp_thru</code> to perform response calibration (THRU) after selecting the port. - Lines 370 to 380: If <code>Cal_type</code> = 4, the program calls a subprogram named <code>Cal_solt</code> to perform full 1-port calibration after selecting the port. - Lines 400 to 410: If <code>Cal_type</code> = 5, the program calls the subprogram <code>Cal_solt</code> to perform full 2-port calibration after selecting the port.
Lines 440 to 450	These lines configure the system to save calibration coefficients along

Performing a Calibration

Sample Program

with instrument settings, and then save the instrument settings under the file name contained in the File\$ variable.

The Select_cal_kit subprogram in lines 500 to 740, which selects the calibration kit, is described below.

Lines 550 to 590	These lines retrieve the names of all the calibration kits and stores them into the Cal_kit_lbl\$(*) variable.
Line 600	Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while entering the number that identifies the calibration kit.
Lines 620 to 680	Displays the list of supported calibration kits, and prompts the user to choose one of the items by typing in the appropriate number.
Line 690	Converts the entered value into an integer and stores it into the Cal_kit variable.
Line 700	Returns to the entry start line if an invalid value is contained in Cal_kit.
Line 730	Selects the calibration kit that matches the number contained in the Cal_kit variable.

The Select_port subprogram in lines 780 to 1010, which allows the user to select a port, is described below.

Lines 830 to 840	If the value of Num_of_ports is 2 (2-port), the subprogram determines the port numbers (1, 2) without prompting the user to enter port numbers, and then store the port numbers into the Port(*) variable.
Lines 860 to 990	If the value of Num_of_ports is not 2, the subprogram prompts the user to select as many ports as Num_of_ports.

Line 870: Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while entering the port number.

Lines 890 to 910: These lines print the index of the current port and prompt the user to enter the port number.

Lines 920: Converts the entered value into an integer and stores it into the Port(*) variable.

Lines 930 to 960: Return to the entry start line if the port number is beyond the range of 1 to 2 or conflicts with an already selected number.

The Cal_resp subprogram in lines 1050 to 1170, which performs response calibration (OPEN/SHORT), is described below.

- Line 1080 Displays the calibration type.
- Line 1090 Configures the instrument to perform response calibration (Type\$) on the port identified by the Port variable.
- Lines 1100 to 1110 These lines prompt the user to connect a Type\$ to port Port, and wait for a press of the [Enter] key after the connection.
- Lines 1120 to 1140 These lines execute the calibration data measurement command identified by Type\$ on port Port, and wait until the measurement completes successfully.
- Line 1150 Calculates the calibration coefficients and turns on error correction.
- Line 1160 Displays a closing message.

The Cal_resp_thru subprogram in lines 1210 to 1330, which performs response calibration (THRU), is described below.

- Line 1240 Displays the calibration type.
- Line 1250 Configures the instrument to perform response calibration (THRU) on response port Port 1 and stimulus port Port 2.
- Lines 1260 to 1270 These lines prompt the user to connect a THRU standard between the ports identified by Port1 and Port2, and wait for a press of the [Enter] key after the connection.
- Lines 1280 to 1300 These lines execute the THRU calibration data measurement command on response port Port1 and stimulus port 2, and wait until the measurement completes successfully.
- Line 1310 Calculates the calibration coefficients and turns on error correction.
- Line 1320 Displays a closing message.

Performing a Calibration

Sample Program

The Cal_solt subprogram in lines 1370 to 1900, which performs full n-port calibration, is described below.

- Line 1410 Displays the calibration type.
- Lines 1450 to 1490 These lines configure the instrument to perform full Num_of_ports port calibration on the ports identified by Port(1) through Port(Num_of_ports).
- Lines 1630 to 1690 These lines make up a loop that iterates while incrementing i from 1 to Num_of_ports.
- Lines 1540 to 1550: Prompt the user to connect an OPEN standard to port Port(i), and wait for a press of the [Enter] key after the connection.
- Lines 1560 to 1580: Execute the OPEN calibration data measurement command on port Port(i), and wait until the measurement completes successfully.
- Lines 1590 to 1600: Prompt the user to connect a SHORT standard to port Port(i), and wait for a press of the [Enter] key after the connection.
- Lines 1610 to 1630: Execute the SHORT calibration data measurement command on port Port(i), and wait until the measurement completes successfully.
- Lines 1640 to 1650: Prompt the user to connect a LOAD standard to port Port(i), and wait for a press of the [Enter] key after the connection.
- Lines 1660 to 1680: Execute the LOAD calibration data measurement command on port Port(i), and wait until the measurement completes successfully.
- Lines 1730 to 1840 These lines make up a loop that iterates while incrementing i from 1 to Num_of_ports-1 and j from i+1 to Num_of_ports.
- Lines 1750 to 1760: Prompt the user to connect a THRU standard between port Port(i) and port Port(j), and wait for a press of the [Enter] key after the connection.
- Lines 1770 to 1790: Execute the THRU calibration data measurement command on response port Port(i) and stimulus port Port(j), and wait until the measurement completes successfully.
- Lines 1800 to 1820: Execute the THRU calibration data measurement command on response port Port(j) and stimulus port Port(i), and wait until the measurement completes successfully.
- Line 1880 Calculates the calibration coefficients and turns on error correction.
- Line 1890 Displays a closing message.

Example 4-1

Calibration (cal.htb)

```

10    DIM File$[20],Ch$[9],Inp_char$[9]
20    INTEGER Cal_kit,Cal_type,Port(1:2)
30    !
40    ASSIGN @Agte507x TO 717
50    File$="Ex_4_1.sta"
60    Ch$="1"
70    !
80    Select_cal_kit(@Agte507x,Ch$)
90    !
100   CLEAR SCREEN
110   ON ERROR GOTO Type_select
120  Type_select: !
130   PRINT "## Calibration Type Selection ##"
140   PRINT " 1: Response (Open)"
150   PRINT " 2: Response (Short)"
160   PRINT " 3: Response (Thru)"
170   PRINT " 4: Full 1 Port"
180   PRINT " 5: Full 2 Port"
190   PRINT ""
200   PRINT "Input 1 to 5"
210   INPUT "Input number? (1 to 5)",Inp_char$
220   Cal_type=IVAL(Inp_char$,10)
230   IF Cal_type<1 OR Cal_type>5 THEN Type_select
240   OFF ERROR
250   !
260   SELECT Cal_type
270     CASE 1
280       Select_port(1,Port(*))
290       Cal_resp(@Agte507x,Ch$,"OPEN",Port(1))
300     CASE 2
310       Select_port(1,Port(*))
320       Cal_resp(@Agte507x,Ch$,"SHOR",Port(1))
330     CASE 3
340       Select_port(2,Port(*))
350       Cal_resp_thru(@Agte507x,Ch$,Port(1),Port(2))
360     CASE 4
370       Select_port(1,Port(*))
380       Cal_solt(@Agte507x,Ch$,1,Port(*))
390     CASE 5
400       Select_port(2,Port(*))
410       Cal_solt(@Agte507x,Ch$,2,Port(*))
420   END SELECT
430   !
440   OUTPUT @Agte507x;":MMEM:STOR:STYP CST"
450   OUTPUT @Agte507x;":MMEM:STOR ""&File$&""""
460   END
470   !=====
480   ! Calibration Kit Selection Function
490   !=====
500  SUB Select_cal_kit(@Agte507x,Ch$)
510    DIM Cal_kit_lbl$(1:10)[20],Inp_char$[9]
520    INTEGER Cal_kit,I
530    CLEAR SCREEN
540    !
550    FOR I=1 TO 10
560      OUTPUT @Agte507x;":SENS1:CORR:COLL:CKIT ";I
570      OUTPUT @Agte507x;":SENS1:CORR:COLL:CKIT:LAB?"
580      ENTER @Agte507x;Cal_kit_lbl$(I)
590    NEXT I
600    ON ERROR GOTO Kit_select
610  Kit_select: !

```

Performing a Calibration

Sample Program

```
620 PRINT "## Calibration Kit Selection ##"
630 FOR I=1 TO 10
640 PRINT USING "X,2D,A,X,20A";I,":",Cal_kit_lbl$(I)
650 NEXT I
660 PRINT ""
670 PRINT "Input 1 to 10"
680 INPUT "Input number? (1 to 10)",Inp_char$
690 Cal_kit=IVAL(Inp_char$,10)
700 IF Cal_kit<1 OR Cal_kit>10 THEN Kit_select
710 OFF ERROR
720 !
730 OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:CKIT ";Cal_kit
740 SUBEND
750 !=====
760 ! Port Selection Function
770 !=====
780 SUB Select_port(INTEGER Num_of_ports,INTEGER Port(*))
790 DIM Inp_char$(9)
800 !
810 CLEAR SCREEN
820 IF Num_of_ports=2 THEN
830 Port(1)=1
840 Port(2)=2
850 ELSE
860 PRINT "## Test Ports Selection ##"
870 ON ERROR GOTO Port_select
880 FOR I=1 TO Num_of_ports
890 PRINT "Port("&VAL$(I)&"):";
900 Port_select: !
910 INPUT "Number?",Inp_char$
920 Port(I)=IVAL(Inp_char$,10)
930 IF Port(I)<1 OR Port(I)>2 THEN Port_select
940 FOR J=1 TO I-1
950 IF Port(I)=Port(J) THEN Port_select
960 NEXT J
970 PRINT Port(I)
980 NEXT I
990 OFF ERROR
1000 END IF
1010 SUBEND
1020 !=====
1030 ! Response (Open/Short) Calibration Function
1040 !=====
1050 SUB Cal_resp(@Agte507x,Ch$,Type$,INTEGER Port)
1060 DIM Buff$(9)
1070 !
1080 PRINT "## Response ("&Type$&") Calibration ##"
1090 OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:METH:"&Type$& " ;Port
1100 PRINT "Set "&Type$& " to Port "&VAL$(Port)& ". Then push [Enter]
key."
1110 INPUT "",Buff$
1120 OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:"&Type$& " ;Port
1130 OUTPUT @Agte507x;"*OPC?"
1140 ENTER @Agte507x;Buff$
1150 OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:SAVE"
1160 PRINT "Done"
1170 SUBEND
1180 !=====
1190 ! Response (Thru) Calibration Function
1200 !=====
1210 SUB Cal_resp_thru(@Agte507x,Ch$,INTEGER Port1,Port2)
1220 DIM Buff$(9)
1230 !
1240 PRINT "## Response (Thru) Calibration ##"
```

```

1250  OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:METH:THRU
";Port1;",";Port2
1260  PRINT "Set THRU between Port "&VAL$(Port1)&" and Port
"&VAL$(Port2)&". Then push [Enter] key."
1270  INPUT "",Buff$
1280  OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:THRU ";Port1;",";Port2
1290  OUTPUT @Agte507x;":*OPC?"
1300  ENTER @Agte507x;Buff$
1310  OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:SAVE"
1320  PRINT "Done"
1330  SUBEND
1340  !=====
1350  ! Full n Port Calibration Function
1360  !=====
1370  SUB Cal_solt(@Agte507x,Ch$,INTEGER Num_of_ports,INTEGER Port(*))
1380  DIM Buff$[9]
1390  INTEGER I,J
1400  !
1410  PRINT "## Full "&VAL$(Num_of_ports)&" Port Calibration ##"
1420  !
1430  ! Calibration Type Selection
1440  !
1450  OUTPUT
@Agte507x;":SENS"&Ch$&":CORR:COLL:METH:SOLT"&VAL$(Num_of_ports)&" ";
1460  FOR I=1 TO Num_of_ports-1
1470      OUTPUT @Agte507x;Port(I);",";
1480  NEXT I
1490  OUTPUT @Agte507x;Port(Num_of_ports)
1500  !
1510  ! Reflection Measurement
1520  !
1530  FOR I=1 TO Num_of_ports
1540      PRINT "Set OPEN to Port "&VAL$(Port(I))&". Then push [Enter]
key."
1550      INPUT "",Buff$
1560      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:OPEN ";Port(I)
1570      OUTPUT @Agte507x;":*OPC?"
1580      ENTER @Agte507x;Buff$
1590      PRINT "Set SHORT to Port "&VAL$(Port(I))&". Then push [Enter]
key."
1600      INPUT "",Buff$
1610      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:SHOR ";Port(I)
1620      OUTPUT @Agte507x;":*OPC?"
1630      ENTER @Agte507x;Buff$
1640      PRINT "Set LOAD to Port "&VAL$(Port(I))&". Then push [Enter]
key."
1650      INPUT "",Buff$
1660      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:LOAD ";Port(I)
1670      OUTPUT @Agte507x;":*OPC?"
1680      ENTER @Agte507x;Buff$
1690  NEXT I
1700  !
1710  ! Transmission Measurement
1720  !
1730  FOR I=1 TO Num_of_ports-1
1740      FOR J=I+1 TO Num_of_ports
1750          PRINT "Set THRU between Port "&VAL$(Port(I))&" and Port
"&VAL$(Port(J))&". Then push [Enter] key."
1760          INPUT "",Buff$
1770          OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:THRU
";Port(I);",";Port(J)
1780          OUTPUT @Agte507x;":*OPC?"
1790          ENTER @Agte507x;Buff$
1800          OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:THRU

```

Performing a Calibration

Sample Program

```
" ;Port(J);"," ;Port(I)
1810      OUTPUT @Agte507x;"*0PC?"
1820      ENTER @Agte507x;Buff$
1830      NEXT J
1840      NEXT I
1850      !
1860      ! Done
1870      !
1880      OUTPUT @Agte507x;" :SENS"&Ch$&" :CORR:COLL:SAVE"
1890      PRINT "Done"
1900 SUBEND
```

ECal

Example 4-2 shows a sample program that demonstrates how to use ECal. You can find the source file of this program, named `ecal.hrb`, on the sample program disk.

The sample program performs full 1-port or 2-port calibration using ECal, and saves the results to a file named “`Ex_4_2.sta`.”

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Line 50	Stores the name of the file (<code>Ex_4_2.sta</code>) into the <code>File\$</code> variable.
Line 60	Stores the channel number (1) into the <code>Ch\$</code> variable.
Line 90	Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while selecting the calibration type number.
Lines 110 to 160	These lines display the list of supported calibration types, and prompt the user to choose one of the items by typing in the appropriate number.
Line 170	Converts the entered value into an integer and stores it into the <code>Cal_type</code> variable.
Line 180	Returns to the entry start line if an invalid value is contained in <code>Cal_type</code> .
Lines 210 to 220	These lines call a subprogram named <code>Select_port</code> to select the appropriate port based on the value of <code>Cal_type</code> , and then perform ECal.
Lines 240 to 250	These lines configure the system to save calibration coefficients along with instrument settings, and then save the instrument settings under the file name contained in the <code>File\$</code> variable.

For more information on the `Select_port` subprogram (lines 300 to lines 530), refer to the description in Example 4-1.

Performing a Calibration

Sample Program

The ECal subprogram in lines 570 to 870, which performs ECal, is described below.

Line 610	Displays the calibration type.
Line 630	Clears the error queue.
Lines 660 to 680	If Num_of_ports = 1, the subprogram prompts the user to connect the E5061A/E5062A's port Port(1) with the ECal module, and waits for a press of the [Enter] key after the connection.
Line 690	If Num_of_ports = 1, the subprogram executes the ECal command that performs full 1-port calibration on port Port(1).
Lines 710 to 740	If Num_of_ports = 2, the subprogram prompts the user to connect the E5061A/E5062A's ports Port(1) and Port(2) with the ECal module, and waits for a press of the [Enter] key after the connection.
Line 750	If Num_of_ports = 2, the subprogram executes the ECal command that performs full 2-port calibration on ports Port(1) and Port(2).
Lines 780 to 790	These lines retrieve the error number and error message from the error queue, and then store them into the variables Err_no and Err_msg\$, respectively.

NOTE

The ECal command can be combined with the ***OPC?** command to make the program wait until the measurement completes successfully. The sample program executes the **:SYST:ERR?** for the purposes of waiting for the completion of ECal and checking for any errors.

Lines 810 to 830	If Err_no returns a non-zero value (an error value), the program displays the corresponding error message.
Line 850	If Err_no returns 0 (no error), the program displays a closing message.

Example 4-2

ECal (ecal.htb)

```

10    DIM File$[20],Ch$[9],Inp_char$[9]
20    INTEGER Cal_kit,Cal_type,Port(1:2)
30    !
40    ASSIGN @Agte507x TO 717
50    File$="Ex_4_2.sta"
60    Ch$="1"
70    !
80    CLEAR SCREEN
90    ON ERROR GOTO Type_select
100  Type_select: !
110  PRINT "## Calibration Type Selection ##"
120  PRINT " 1: Full 1 Port"
130  PRINT " 2: Full 2 Port"
140  PRINT ""
150  PRINT "Input 1 to 2"
160  INPUT "Input number? (1 to 2)",Inp_char$
170  Cal_type=IVAL(Inp_char$,10)
180  IF Cal_type<1 OR Cal_type>2 THEN Type_select
190  OFF ERROR
200  !
210  Select_port(Cal_type,Port(*))
220  Ecal(@Agte507x,Ch$,Cal_type,Port(*))
230  !
240  OUTPUT @Agte507x;":MMEM:STOR:STYP CST"
250  OUTPUT @Agte507x;":MMEM:STOR ""&File$&""""
260  END
270  !=====
280  ! Port Selection Function
290  !=====
300  SUB Select_port(INTEGER Num_of_ports,INTEGER Port(*))
310  DIM Inp_char$[9]
320  !
330  CLEAR SCREEN
340  IF Num_of_ports=2 THEN
350    Port(1)=1
360    Port(2)=2
370  ELSE
380    PRINT "## Test Ports Selection ##"
390    ON ERROR GOTO Port_select
400    FOR I=1 TO Num_of_ports
410      PRINT "Port("&VAL$(I)&"):";
420  Port_select: !
430    INPUT "Number?",Inp_char$
440    Port(I)=IVAL(Inp_char$,10)
450    IF Port(I)<1 OR Port(I)>2 THEN Port_select
460    FOR J=1 TO I-1
470      IF Port(I)=Port(J) THEN Port_select
480    NEXT J
490    PRINT Port(I)
500  NEXT I
510  OFF ERROR
520  END IF
530  SUBEND
540  !=====
550  ! Electronic Calibration Function
560  !=====
570  SUB Ecal(@Agte507x,Ch$,INTEGER Num_of_ports,INTEGER Port(*))
580  DIM Buff$[9],Err_msg$[100]
590  INTEGER Err_no,Port1
600  !
610  PRINT "## Full "&VAL$(Num_of_ports)&" Port ECal ##"

```

Performing a Calibration

Sample Program

```
620      !
630      OUTPUT @Agte507x;"*CLS"
640      SELECT Num_of_ports
650          CASE 1
660              PRINT "Connect Port "&VAL$(Port(1))&" to ECal Module."
670              PRINT "Then push [Enter] key."
680              INPUT "",Buff$
690              OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:ECAL:SOLT1 ";Port(1)
700          CASE 2
710              PRINT "Connect Port "&VAL$(Port(1));
720              PRINT " and Port "&VAL$(Port(2))&" to ECal Module."
730              PRINT "Then push [Enter] key."
740              INPUT "",Buff$
750              OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:ECAL:SOLT2
";Port(1);",";Port(2)
760      END SELECT
770      PRINT "Executing ..."
780      OUTPUT @Agte507x;":SYST:ERR?"
790      ENTER @Agte507x;Err_no,Err_msg$
800      IF Err_no<>0 THEN
810          PRINT "Error occurred!!"
820          PRINT "  No: ";Err_no,"Description: "&Err_msg$
830          PRINT "ECAL INTERRUPT!!"
840      ELSE
850          PRINT "Done"
860      END IF
870  SUBEND
```


Making a Measurement

5. Making a Measurement

Trigger system

The trigger system is responsible for such tasks as detecting the start of a measurement cycle (triggering) and enabling/disabling measurement on each channel. As shown in Figure 5-1, the trigger system has two types of state: system-wide and channel-wide. The system-wide state can be “Hold”, “Waiting for Trigger”, or “Measurement” while the channel-wide state can be “Idle” or “Initiate”.

Figure 5-1 Trigger system

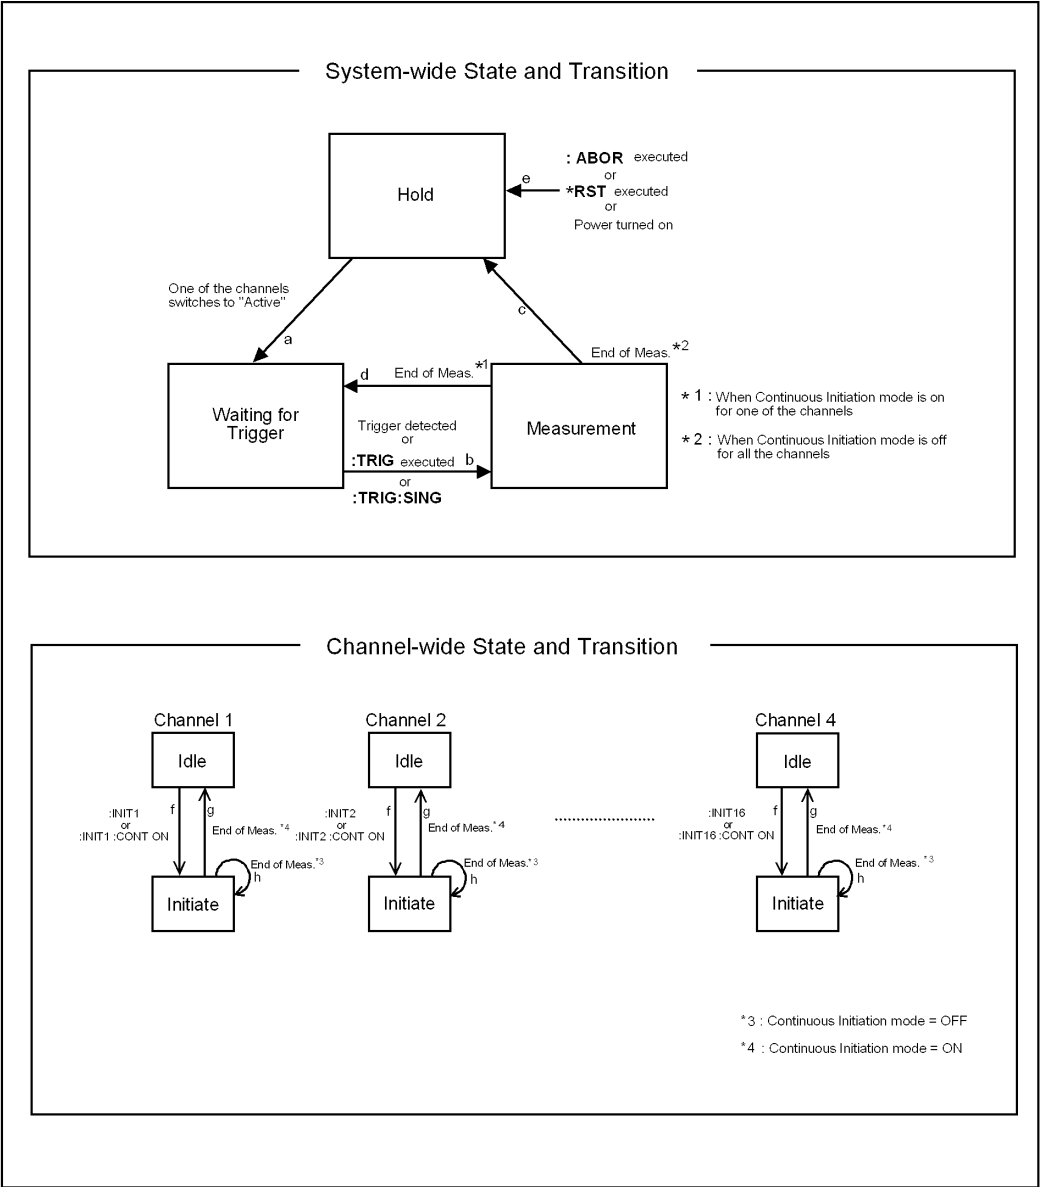

The following subsections describe each state and how the trigger system switches among the states.

System-wide state and transition

“Hold” State

The trigger system switches to “Hold” state when one of the following commands has been executed (arrow “e” in Figure 5-1). Also, turning on the power to the instrument puts the trigger system into “Hold” state. When the power is turned on, however, continuous initiation mode is on for channel 1 and the trigger source is set to “Internal”; therefore, the trigger system immediately switches to “Waiting for Trigger” state and subsequently repeats transitions between “Measurement” and “Waiting for Trigger” states.

- **:ABOR** on page 202
- ***RST** on page 199

When the trigger system is in “Hold” state and one of the channels switches to “Initiate” state (arrow “f” in Figure 5-1), then the trigger system switches to “Waiting for Trigger” state (arrow “a” in Figure 5-1).

“Waiting for Trigger” State

When the trigger system is in “Waiting for Trigger” state and either the instrument is triggered (i.e., a trigger is detected) or one of the commands is executed, then the trigger system switches to “Measurement” state (arrow “B” in Figure 5-1).

- **:TRIG** on page 484
- **:TRIG:SING** on page 484

As shown in the table below, how the instrument is triggered differs depending on which trigger source is specified. To specify the trigger source, use the **:TRIG:SOUR** command on page 485 command.

Trigger Source	How the instrument is triggered
Internal trigger	The instrument is automatically triggered within itself.
External trigger	The instrument is triggered when a trigger signal is input through the Ext Trig terminal or handler interface.
Bus trigger	The instrument is triggered when the *TRG command on page 201 command is issued.
Manual trigger	The instrument is triggered when you press [Trigger] - Trigger on the front panel.

“Measurement” State

In “Measurement” state, the instrument waits for the elapse of the sweep delay time (set by the **:SENS{1-4}:SWE:DEL** command on page 424) and then starts a measurement cycle; this process is performed sequentially on each of those channels that were in “Initiate” state immediately before the transition to this state, in the ascending order of the channel numbers.

When the instrument has finished measuring all the active channels, the trigger system behaves in one of the following ways depending on the setting of continuous initiation mode.

If continuous initiation mode is off for all the channels:

The trigger system switches to “Hold” state (arrow “c” in Figure 5-1).

If continuous initiation mode is on for one of the channels:

The trigger system switches to “Waiting for Trigger” state (arrow “d” in Figure 5-1).

Channel-wide state and transition

“Idle” State

A channel switches to “Initiate” state when one of the following commands has been executed (arrow “f” in Figure 5-1).

- **:INIT{1-4}** on page 340
- **:INIT{1-4}:CONT** on page 341 (“ON” specified)

“Initiate” State

A channel in this state is measured just before the entire system switches to “Measurement” state.

When the instrument has finished measuring a channel, the channel behaves in one of the following ways depending on the setting of continuous initiation mode (set by the **:INIT{1-4}:CONT** command on page 341 command).

If continuous initiation mode is off: The channel switches to “Idle” state (arrow “g” in Figure 5-1).

If continuous initiation mode is on: The channel remains in “Initiate” state (arrow “h” in Figure 5-1).

Starting a Measurement Cycle (Triggering the instrument)

Configuring the Instrument to Automatically Perform Continuous Measurement

- Step 1.** Use the **:INIT{1-4}:CONT** command on page 341 to turn on continuous initiation mode for the channels you want to measure and turn the mode off for any other channels.
- Step 2.** Issue the **:TRIG:SOUR** command on page 485 to set the trigger source to Internal trigger.

Starting Measurement on Demand

- Step 1.** Use the **:INIT{1-4}:CONT** command to turn on continuous initiation mode for the channels you want to measure and turn the mode off for any other channels.
- Step 2.** Issue the **:TRIG:SOUR** command to set the trigger source to “Bus Trigger”.
- Step 3.** Trigger the instrument at any time you want to perform measurement. An external controller can trigger the instrument using one of the following three commands:

Command	Can the *OPC? command on page 198 command be used to wait for the end of sweep?	Applicable trigger source
*TRG on page 201	No	Bus trigger only
:TRIG on page 484		External trigger
:TRIG:SING on page 484	Yes	Bus trigger Manual trigger

- Step 4.** To start the next measurement cycle, repeat step 3.

Waiting for the End of Measurement

Using the Status Register

The status of the E5061A/E5062A can be detected through the status registers. This section describes how to detect the end of measurement using the status registers. For the complete description of the status report mechanism, including the specifications of each bit, see Appendix B, “Status Reporting System.”

Measurement status is reported by the operation status condition register (see Table B-3 on page 518). An SRQ (service request) is useful when you create a program that uses the information reported by this register to detect the end of measurement.

To detect the end of measurement via an SRQ, use one of the following commands:


- ***SRE** on page 200
- **:STAT:OPER:ENAB** on page 442
- **:STAT:OPER:PTR** on page 444
- **:STAT:OPER:NTR** on page 443

Follow these steps:

- Step 1.** Configure the E5061A/E5062A so that it generates an SRQ when the operation status condition register's bit 4 (a bit that is set to 1 during measurement) is changed from 1 to 0.
- Step 2.** Trigger the instrument to start a measurement cycle.
- Step 3.** When an SRQ is generated, the program interrupts the measurement cycle.

Figure 5-2

SRQ generation sequence (at the end of measurement)

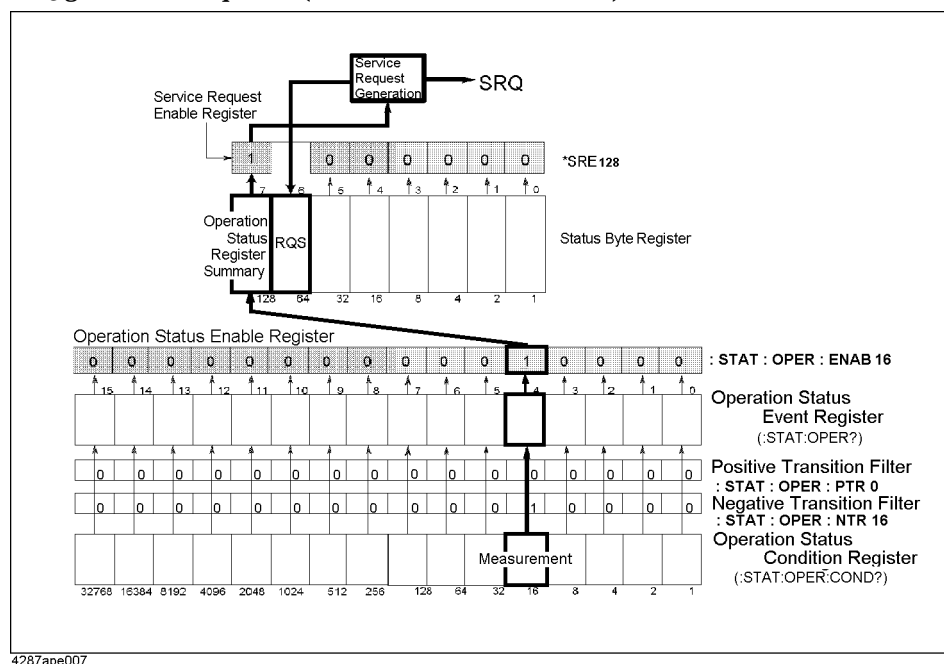

Sample Program

Example 5-2 is a sample program that demonstrates how to use an SRQ to detect the end of measurement. You can find the source file of this program, named `srq_meas.htb`, on the sample program disk.

NOTE

This sample program correctly runs when the maximum number of channels/traces is set 9 channels/9 traces.

The sample program sets up the trigger system, configures the instrument to properly generate an SRQ, and then triggers the instrument. When the instrument has generated an SRQ that indicates the end of measurement, the program exits after printing a measurement completion message.

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Lines 60 to 90	These lines store the settings of continuous initiation mode for each channel (on for channels 1 and 2; off for channels 3 through 4) into the array variable <code>Cont_mode\$(*)</code> .
Lines 110 to 130	These lines turn on or off continuous initiation mode for each channel depending on the value of <code>Cont_mode\$(*)</code> .
Line 140	Sets the trigger source to “Bus Trigger”.
Lines 160 to 170	These lines configure the instrument so that operation status event register's bit 4 is set to 1 only when operation status condition register's bit 4 is changed from 1 to 0 (negative transition).
Lines 180 to 190	These lines enable the operation status event register's bit 4 and status byte register's bit 7.
Lines 200 to 220	These lines clear the status byte register and operation status event register.
Lines 240 to 250	These lines set the branch target for an SRQ interrupt to enable SRQ interrupts.
Lines 260 to 290	These lines trigger the instrument, and waits until the measurement cycle finishes.
Line 300	Displays a measurement completion message.

Example 5-1

Using an SRQ to Detect the End of Measurement (srq_meas.htb)

```
10    DIM Cont_mode$(1:4)[9], Buff$[9]
20    INTEGER I
30    !
40    ASSIGN @Agte507x TO 717
50    !
60    Cont_mode$(1)="ON"
70    Cont_mode$(2)="ON"
80    Cont_mode$(3)="OFF"
90    Cont_mode$(4)="OFF"
100   !
110   FOR I=1 TO 4
120       OUTPUT @Agte507x;":INIT"&VAL$(I):":CONT "&Cont_mode$(I)
130   NEXT I
140   OUTPUT @Agte507x;":TRIG:SOUR BUS"
150   !
160   OUTPUT @Agte507x;":STAT:OPER:PTR 0"
170   OUTPUT @Agte507x;":STAT:OPER:NTR 16"
180   OUTPUT @Agte507x;":STAT:OPER:ENAB 16"
190   OUTPUT @Agte507x;":*SRE 128"
200   OUTPUT @Agte507x;":*CLS"
210   OUTPUT @Agte507x;":*OPC?"
220   ENTER @Agte507x;Buff$
230   !
240   ON INTR 7 GOTO Meas_end
250   ENABLE INTR 7;2
260   OUTPUT @Agte507x;":*TRG"
270   PRINT "Waiting..."
280 Meas_wait:  GOTO Meas_wait
290 Meas_end:  OFF INTR 7
300   PRINT "Measurement Complete"
310   END
```

Using the :TRIG:SING Command

When you trigger the instrument by issuing the **:TRIG:SING** command on page 484 command, you can use the ***OPC?** command to wait until the measurement cycle completes.

Sample Program

Example 5-2 is a sample program that demonstrates how to use the **:TRIG:SING** command to wait until the measurement cycle completes. You can find the source file of this program, named `trg_sing.htb`, on the sample program disk.

The sample program uses the **:TRIG:SING** command to start a sweep (measurement) cycle, uses the ***OPC?** command to wait until the measurement cycle completes, then prints a message and exits.

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Lines 60 to 90	These lines store the settings of continuous initiation mode for each channel (on for channels 1 and 2; off for channels 3 through 4) into the array variable <code>Cont_mode\$(*)</code> .
Lines 110 to 130	These lines turn on or off continuous initiation mode for each channel depending on the value of <code>Cont_mode\$(*)</code> .
Line 140	Sets the trigger source to “Bus Trigger”.
Line 160	Triggers the instrument to start a sweep cycle.
Lines 170 to 180	These lines execute the *OPC? command and wait until the command returns 1 (i.e., the measurement cycle completes).
Line 200	Displays a measurement completion message.

Example 5-2

**Using the :TRIG:SING Command to Wait until the End of Measurement
(trg_sing.htb)**

```
10    DIM Cont_mode$(1:4)[9], Buff$[9]
20    INTEGER I
30    !
40    ASSIGN @Agte507x TO 717
50    !
60    Cont_mode$(1)="ON"
70    Cont_mode$(2)="ON"
80    Cont_mode$(3)="OFF"
90    Cont_mode$(4)="OFF"
100   !
110   FOR I=1 TO 4
120       OUTPUT @Agte507x; ":INIT"&VAL$(I)& ":CONT "&Cont_mode$(I)
130   NEXT I
140   OUTPUT @Agte507x; ":TRIG:SOUR BUS"
150   !
160   OUTPUT @Agte507x; ":TRIG:SING"
170   OUTPUT @Agte507x; "*OPC?"
180   ENTER @Agte507x; Buff$
190   !
200   PRINT "Measurement complete"
210   END
```

Using Wait Time

Before creating your program, actually measure the time between the start and end of the measurement cycle. Then code your program so that the controller waits for the actually measured time using the appropriate command (for example, the WAIT command for HTBasic). This is a straightforward method, but care must be taken: an incorrect wait time could result in an unexpected error.

6

Analyzing Data

This chapter describes how to use markers and analysis command.

Retrieving Measurement Results at Specified Points

Markers allow you to retrieve measurement results at your specified points. You can use up to eight markers for each trace, and you can move them to any point on the trace. In addition to the regular markers, you can use a reference marker.

Showing/Hiding Markers

To show or hide markers including the reference marker, use the following command:

- **:CALC{1-4}:MARK{1-10}** on page 263

NOTE

You can move markers or retrieve the data at a marker even when the markers are hidden.

NOTE

The display of the reference marker is turned on or off when you turn on or off Reference Marker mode.

Turning On or Off Reference Marker Mode

Turning on Reference Marker mode provides relative marker values with respect to the reference marker (by deducting the value at the reference marker from the value at a particular marker).

To turn on or off Reference Marker mode, use the following command:

- **:CALC{1-4}:MARK:REF** on page 262

Setting (Changing) and Retrieving Stimulus Value at Marker Positions

To set (or change along the frequency axis) the stimulus value at a particular marker or the reference marker or retrieve the current stimulus value, use the following command:

- **:CALC{1-4}:MARK{1-10}:X** on page 279

When Reference Marker mode is on, the stimulus value at a regular marker is a relative stimulus value obtained by deducting the stimulus value at the reference marker from the actual stimulus value at that particular marker.

Retrieving Measurement Results at Marker Positions

To retrieve the measurement results (response values) at a particular marker or the reference marker, use the following command:

- **:CALC{1-4}:MARK{1-10}:Y?** on page 280

When Reference Marker mode is on, the response value at a regular marker is a relative value obtained by deducting the response value at the reference marker from the actual response value at that particular marker.

Searching for Positions That Match Specified Criteria

You can search for a position that matches your specified criteria using the Marker Search feature or analysis command.

Using Marker Search

NOTE

Marker Search is available whether the markers are shown or hidden.

Setting the Search Range

You can use either the entire sweep range or a user-defined range for the marker search range, using the following command:

- **:CALC{1-4}:MARK:FUNC:DOM** on page 245

When you opt to use a user-defined range, use the following command to set the range:

Start value (lower limit value)	:CALC{1-4}:MARK:FUNC:DOM:STAR on page 247
Stop value (upper limit value)	:CALC{1-4}:MARK:FUNC:DOM:STOP on page 248

You can also select whether to specify the marker search range independently for each trace, using the following command.

- **:CALC{1-4}:FUNC:DOM:COUP** on page 223

Selecting a Search Type

Marker Search allows you to choose from the following eight search types:

- ☐ Maximum value
- ☐ Minimum value
- ☐ Peak (3 types)
 - Maximum peak (for a positive peak), minimum peak (for a negative peak)
 - Peak nearest to the left-hand side of the marker position
 - Peak nearest to the right-hand side of the marker position
- ☐ Target (3 types)
 - Peak nearest to the marker position
 - Target nearest to the left-hand side of the marker position
 - Target nearest to the right-hand side of the marker position

To select a search type, use the following command:

- **:CALC{1-4}:MARK{1-10}:FUNC:TYPE** on page 274

Defining a Peak

You can define a peak by specifying the lower limit for the peak excursion value and polarity (positive or negative peak). The peak excursion value is the difference between the positive peak and the minimum value on either side (or between the negative peak and the maximum value on either side). For more information about the peak excursion value, see *User's Guide*.

To define a peak, use the following command:

lower limit for the peak excursion value	:CALC{1-4}:MARK{1-10}:FUNC:PEXC on page 269
polarity	:CALC{1-4}:MARK{1-10}:FUNC:PPOL on page 270

Defining a Target

You can define a target by specifying the target value (response value) and transitional direction (positive or negative value change).

To define a target, use the following command:

Target value	:CALC{1-4}:MARK{1-10}:FUNC:TARG on page 271
Transitional direction	:CALC{1-4}:MARK{1-10}:FUNC:TTR on page 273

Performing Marker Search

To perform Marker Search, use the following command:

- :CALC{1-4}:MARK{1-10}:FUNC:EXEC on page 268

To turn on or off the Search Tracking feature, which performs Marker Search every time the trace is updated, use the following command:

- :CALC{1-4}:MARK{1-10}:FUNC:TRAC on page 272

Retrieving Search Results

Performing Marker Search moves the marker to the points that matches the search criteria, so you can obtain the search results by retrieving the marker value. For information on how to retrieve marker values, refer to “Setting (Changing) and Retrieving Stimulus Value at Marker Positions” on page 90 and “Retrieving Measurement Results at Marker Positions” on page 90.

Using the Analysis Command

You can use the analysis command to perform search and analysis.

Setting the Search (Analysis) Range

You can use either the entire sweep range or a user-defined range as the search (analysis) range, using the following command:

- **:CALC{1-4}:FUNC:DOM** on page 222

When you opt to use a user-defined range, use the following command to set the range:

Start value (lower limit value)	:CALC{1-4}:FUNC:DOM:STAR on page 224
Stop value (upper limit value)	:CALC{1-4}:FUNC:DOM:STOP on page 225

You can also select whether to specify the marker search (analysis) range independently for each trace, using the following command.

- **:CALC{1-4}:FUNC:DOM:COUP** on page 223

Selecting the Search (Analysis) Type

The analysis command allows you to choose from the following five search types:

- ☐ Maximum value
- ☐ Minimum value
- ☐ Maximum peak (for a positive peak), minimum peak (for a negative peak)
- ☐ All peaks
- ☐ All targets

In addition, you can choose from the following three analysis types:

- ☐ Difference between the maximum and minimum values
- ☐ Standard deviation
- ☐ Average

To select the search (analysis) type, use the following command:

- **:CALC{1-4}:FUNC:TYPE** on page 231

Defining a Peak

You can define a peak by specifying the lower limit for the peak excursion value and polarity (positive or negative peak). The peak excursion value is the difference between the positive peak and the minimum value on either side (or between the negative peak and the maximum value on either side). For more information about the peak excursion value, see *User's Guide*.

To define a peak, use the following command:

lower limit for the peak excursion value	:CALC{1-4}:FUNC:PEXC on page 226
Polarity	:CALC{1-4}:FUNC:PPOL on page 228

Defining a Target

You can define a target by specifying the target value (response value) and transitional direction (positive or negative value change).

To define a target, use the following command:

Target value	:CALC{1-4}:FUNC:TARG on page 229
Transitional direction	:CALC{1-4}:FUNC:TTR on page 230

Performing Search (Analysis)

To perform search (analysis), use the following command:

- :CALC{1-4}:FUNC:EXEC on page 225

Retrieving Search (Analysis) Results

To retrieve search (analysis) results, use the following command:

- :CALC{1-4}:FUNC:DATA? on page 221

The number of the data items contained in search (analysis) results differ depending on the search (analysis) type and the number of points found by the search operation. To retrieve the number of data items, use the following command:

- :CALC{1-4}:FUNC:POIN? on page 227

Sample Program

Example 6-2 is a sample program that demonstrates how to search for peaks using the Marker Search feature and analysis command. You can find the source file of this program, named `search.htb`, on the sample program disk.

This program works in two steps: it uses Marker Search to search for the maximum positive peak and displays the results; it then uses analysis command to search for all positive peaks and displays the results.

The program is described in detail below:

Line 50	Assigns a GPIB address to the I/O pass.
Line 60	Stores a peak excursion value of 0.5 into the Excursion variable.
Lines 80 to 120	These lines configure the system to generate an SRQ when it cannot perform Bandwidth Search due to an error.
Lines 130 to 140	These lines set the branch target for an SRQ interrupt to enable SRQ interrupts.
Line 180	Sets the active trace to trace 1.
Line 190	Sets the search type for marker 1 to Peak.
Lines 200 to 210	These lines set the Excursion variable to the peak excursion value for the peak search of marker 1 and set the polarity to Positive Peak.
Line 220	Performs Peak Search, and moves marker 1 to the maximum positive peak.
Lines 230 to 240	These lines retrieve the frequency at marker 1.
Lines 250 to 260	These lines retrieve the response value at marker 1.
Lines 270 to 290	These lines display the results of searching for the maximum positive peak.
Line 330	Sets the analysis range to the entire sweep range.
Line 340	Sets the search type of the analysis command to All Peaks.
Lines 350 to 360	These lines set the Excursion variable to the peak excursion value for the peak search of the analysis command and set the polarity to Positive Peak.
Line 370	Searches for all peaks.
Lines 380 to 390	These lines retrieve the number of data pairs contained in the search results, and stores that number into the Point variable.
Line 400	Resizes the Result array based on the value of the Point variable.
Lines 380 to 390	These lines retrieve the response values and frequencies for all peaks.
Lines 430 to 470	These lines display the results of searching for all peaks.
Lines 490 to 530	These lines define an error handler that retrieves and displays the number and message of an error that has occurred.

Example 6-1

Peak Search (search.htb)

```
10    DIM Buff$[9],Img$[50],Err_msg$[100]
20    REAL Excursion,Freq,Resp,Result(1:100,1:2)
30    INTEGER Poin,Err_no
40    !
50    ASSIGN @Agte507x TO 717
60    Excursion=.5
70    !
80    OUTPUT @Agte507x;"*ESE 60"
90    OUTPUT @Agte507x;"*SRE 32"
100   OUTPUT @Agte507x;"*CLS"
110   OUTPUT @Agte507x;"*OPC?"
120   ENTER @Agte507x;Buff$
130   ON INTR 7 GOTO Err
140   ENABLE INTR 7;2
150   !
160   PRINT "Maximum Peak Search using Marker 1"
170   !
180   OUTPUT @Agte507x;":CALC1:PAR1:SEL"
190   OUTPUT @Agte507x;":CALC1:MARK1:FUNC:TYPE PEAK"
200   OUTPUT @Agte507x;":CALC1:MARK1:FUNC:PEXC ";Excursion
210   OUTPUT @Agte507x;":CALC1:MARK1:FUNC:PPOL POS"
220   OUTPUT @Agte507x;":CALC1:MARK1:FUNC:EXEC"
230   OUTPUT @Agte507x;":CALC1:MARK1:X?"
240   ENTER @Agte507x;Freq
250   OUTPUT @Agte507x;":CALC1:MARK1:Y?"
260   ENTER @Agte507x;Resp
270   Img$="8A,MD.4DE,2X,MD.6DE"
280   PRINT "          Frequency          Response"
290   PRINT USING Img$;"Peak:  ",Freq,Resp
300   !
310   PRINT "All Peaks Search using Command"
320   !
330   OUTPUT @Agte507x;":CALC1:FUNC:DOM OFF"
340   OUTPUT @Agte507x;":CALC1:FUNC:TYPE APE"
350   OUTPUT @Agte507x;":CALC1:FUNC:PEXC ";Excursion
360   OUTPUT @Agte507x;":CALC1:FUNC:PPOL POS"
370   OUTPUT @Agte507x;":CALC1:FUNC:EXEC"
380   OUTPUT @Agte507x;":CALC1:FUNC:POIN?"
390   ENTER @Agte507x;Poin
400   REDIM Result(1:Poin,1:2)
410   OUTPUT @Agte507x;":CALC1:FUNC:DATA?"
420   ENTER @Agte507x;Result(*)
430   Img$="4A,2D,2A,MD.4DE,2X,MD.6DE"
440   PRINT "          Frequency          Response"
450   FOR I=1 TO Poin
460     PRINT USING Img$;"Peak",I," ": ",Result(I,2),Result(I,1)
470   NEXT I
480   GOTO No_err
490 Err: OFF INTR 7
500   OUTPUT @Agte507x;";:SYST:ERR?"
510   ENTER @Agte507x;Err_no,Err_msg$
520   PRINT "Error occurred!!"
530   PRINT "  No: ";Err_no,"Description: "&Err_msg$
540 No_err: OFF INTR 7
550   END
```

Bandwidth Search

The E5061A/E5062A has a feature called Bandwidth Search. This feature searches for the cutoff points on both right- and left-hand sides of the marker position on the trace.

- ☐ Bandwidth ($BW = high - low$)
- ☐ Center frequency ($cent = \frac{high + low}{2}$)
- ☐ Q value ($Q = \frac{cent}{BW}$)
- ☐ Loss (response value at the marker position)

Where *high* is the right-hand cutoff point frequency; *low* is the left-hand cutoff point frequency.

Setting the Bandwidth Definition Value

Bandwidth Search finds a point whose response value is different, by the amount defined as the bandwidth definition value, than the response value at the marker position, and identifies that point as the cutoff point.

To set the bandwidth definition value, use the following command:

- **:CALC{1-4}:MARK{1-10}:BWID:THR** on page 266

Retrieving Bandwidth Search Results

Once you have moved the marker to the appropriate position using Marker Search or some other feature, you can retrieve the results of Bandwidth Search using the following command:

- **:CALC{1-4}:MARK{1-10}:BWID:DATA?** on page 265

Also, you can use the following command to control whether to display the results of Bandwidth Search on the LCD:

- **:CALC{1-4}:MARK:BWID** on page 243

NOTE

You can retrieve the results of Bandwidth Search even after you have turned off the display of markers or the results of Bandwidth Search.

Sample Program

Example 6-2 shows a sample program that demonstrates how to perform Bandwidth Search. You can find the source file of this program, named `bandwid.htb`, on the sample program disk.

The sample program moves the marker to the maximum value position, then retrieves and displays the results of Bandwidth Search.

The program is described in detail below:

- Line 50 Assigns a GPIB address to the I/O pass.
- Line 60 Stores a bandwidth definition value of 3 into the Threshold variable.

Analyzing Data

Bandwidth Search

Lines 80 to 120	These lines configure the system to generate an SRQ when it cannot perform Bandwidth Search due to an error.
Lines 130 to 140	These lines set the branch target for an SRQ interrupt to enable SRQ interrupts.
Line 160	Sets the search type for marker 1 to Peak.
Lines 170 to 180	These lines use the Marker Search feature to move the marker to the maximum value position.
Line 190	Sets the bandwidth definition value to Threshold.
Lines 200	Sends the command to retrieve the results of Bandwidth Search.
Lines 210	Waits 0.5 seconds to prevent the retrieve before an SRQ is generated if an error occurs on Bandwidth Search.
Lines 220	Retrieves the results of Bandwidth Search.
Lines 240 to 280	These lines display the results of Bandwidth Search.
Lines 310 to 350	These lines define an error handler that retrieves and displays the number and message of an error that has occurred.

Example 6-2

Bandwidth Search (bandwid.htb)

```
10    DIM Buff$(9),Err_msg$(100)
20    REAL Threshold,Bwid,Cent,Q, Loss
30    INTEGER Err_no
40    !
50    ASSIGN @Agte507x TO 717
60    Threshold=-3
70    !
80    OUTPUT @Agte507x;"*ESE 60"
90    OUTPUT @Agte507x;"*SRE 32"
100   OUTPUT @Agte507x;"*CLS"
110   OUTPUT @Agte507x;"*OPC?"
120   ENTER @Agte507x;Buff$
130   ON INTR 7 GOTO Err
140   ENABLE INTR 7;2
150   !
160   OUTPUT @Agte507x;":CALC1:PAR1:SEL"
170   OUTPUT @Agte507x;":CALC1:MARK1:FUNC:TYPE MAX"
180   OUTPUT @Agte507x;":CALC1:MARK1:FUNC:EXEC"
190   OUTPUT @Agte507x;":CALC1:MARK1:BWID:THR ";Threshold
200   OUTPUT @Agte507x;":CALC1:MARK1:BWID:DATA?"
210   WAIT .5
220   ENTER @Agte507x;Bwid,Cent,Q, Loss
230   !
240   PRINT "## Bandwidth Search ##"
250   PRINT "Bandwidth      : ",Bwid
260   PRINT "Center Frequency: ",Cent
270   PRINT "Q                  : ",Q
280   PRINT "Loss                 : ",Loss
290   !
300   GOTO No_err
310 Err: OFF INTR 7
320   OUTPUT @Agte507x;":SYST:ERR?"
330   ENTER @Agte507x;Err_no,Err_msg$
340   PRINT "Error occurred!!"
350   PRINT "  No: ";Err_no,"Description: "&Err_msg$
360 No_err: OFF INTR 7
370   END
```

Notch search

The E5061A/E5062A provides the notch search function. This function searches for points that meet the conditions on the trace, initiated at the marker position and sweeping the trace rightward, and calculates the following items.

- ❑ Bandwidth($BW = high - low$)
- ❑ Center frequency ($cent = \frac{high + low}{2}$)
- ❑ Q value ($Q = \frac{cent}{BW}$)
- ❑ Loss (response value at the marker position)

Where, *high* is the right-hand cutoff point frequency, and *low* is the left-hand cutoff point frequency.

Setting the notch definition value

The notch search function finds a point whose response value is different, by the amount defined as the notch definition value, than the response value at the marker position, and identifies that point as the cutoff point.

To set the notch definition value, use the following command:

- **:CALC{1-4}:MARK{1-10}:NOTC:THR** on page 277

Reading out the notch search result

Once you have moved the marker to the appropriate position using the marker search function or some other function, you can retrieve the notch search result using the following command:

- **:CALC{1-4}:MARK{1-10}:NOTC:DATA?** on page 276

Also, you can use the following command to control whether to display the notch search result on the LCD:

- **:CALC{1-4}:MARK:NOTC** on page 261

NOTE

You can retrieve the notch search result regardless of whether the marker display and the notch search result display is on/off.

Statistical Analysis

The E5061A/E5062A provides a mechanism that analyzes trace statistics. You can analyze the following statistics:

- ☐ Average
- ☐ Standard deviation
- ☐ Difference between the maximum and minimum values

To retrieve the results of statistical analysis, use the following command:

- **:CALC{1-4}:MARK:MATH:STAT:DATA?** on page 260

Also, you can use the following command to control whether to display the results of statistical analysis on the LCD:

- **:CALC{1-4}:MARK:MATH:STAT** on page 259

NOTE

You can retrieve the results of statistical analysis even after you have turned off the display of the results of statistical analysis.

Alternatively, you can use the analysis command to analyze the trace statistics. When you use the analysis command, you can analyze the trace data in a specific range as well as the trace data throughout the entire sweep range. For information how to use the analysis command, refer to “Using the Analysis Command” on page 93.

Analyzing impedance

By turning on the parameter conversion function, you can convert the measurement result of the S parameter to the following parameters.

- ☐ Equivalent impedance in reflection measurement
- ☐ Equivalent impedance in transmission measurement
- ☐ Equivalent admittance in reflection measurement
- ☐ Equivalent admittance in transmission measurement
- ☐ Inverse of S-parameter ($1/S$)

To turn ON/OFF the parameter conversion function, use the following command:

- **:CALC{1-4}:CONV** on page 211

To select the parameter to which you want to convert the measurement result, use the following command:

- **:CALC{1-4}:CONV:FUNC** on page 212

7

Reading/Writing Measurement Data

This chapter provides an overview of the Agilent E5061A/E5062A's internal data processing flow and describes how to read and write measurement results (internal data array).

Data Transfer Format

When you transfer data using the one of the following commands, you can choose among ASCII transfer format, IEEE 64-bit floating point binary transfer format and IEEE 32-bit floating point binary transfer format.

NOTE

The instrument always uses the ASCII transfer format when you transfer data without using any of the following commands.

- **:CALC{1-4}:DATA:FDAT** on page 215
- **:CALC{1-4}:DATA:FMEM** on page 216
- **:CALC{1-4}:DATA:SDAT** on page 217
- **:CALC{1-4}:DATA:SMEM** on page 218
- **:CALC{1-4}:FUNC:DATA?** on page 221
- **:CALC{1-4}:LIM:DATA** on page 233
- **:CALC{1-4}:LIM:REP?** on page 242
- **:SENS{1-4}:FREQ:DATA?** on page 416
- **:SENS{1-4}:SEGM:DATA** on page 421

To set the data transfer format, use the following command:

- **:FORM:DATA** on page 338

NOTE

Executing the **:SYST:PRES** command on page 479 or ***RST** command on page 199 does not affect the current setting of the data transfer format.


ASCII Transfer Format

When you select the ASCII transfer format as the data transfer format, numbers are transferred as ASCII bytes, each of which corresponds to one of the formats shown below. Note that numbers are separated from one another with a comma (,) in accordance with the IEEE 488.2 specification.

NOTE Numeric data strings vary in length. Keep this in mind when you extract some data from retrieved numeric data strings in your program.


- Integer format
- Figure 7-1 shows this format. Numbers are expressed as integers. For example, 201 is expressed as “+201” or “201.”

Figure 7-1 Integer format

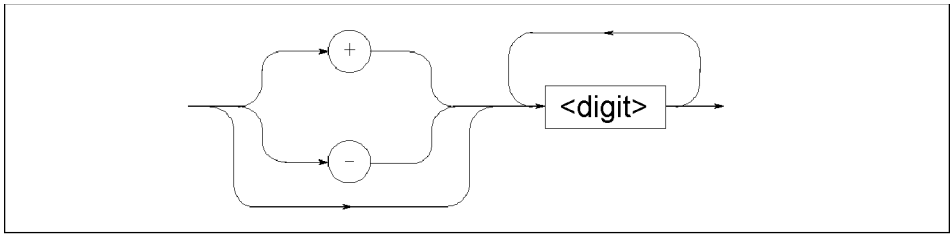

- Floating-point number format
- Figure 7-2 shows this format. Numbers are expressed with floating points. For example, 1000 is expressed as “+1.0000000000+003”.

Figure 7-2 Floating-point number format

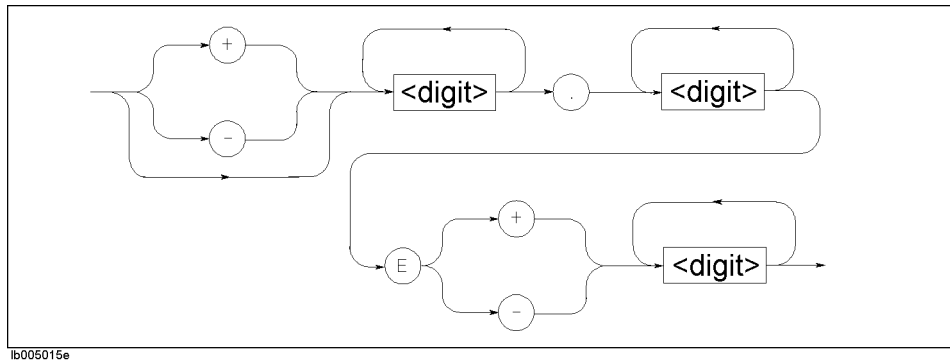

Binary Transfer Format


You can select the binary transfer format from the IEEE 64-bit floating point format or the IEEE 32-bit floating point format depending on the controller you use.

IEEE 64-bit floating point format

When you select the IEEE 64-bit floating point binary transfer format as the data transfer format, numbers are transferred in the format shown in Figure 7-3.

Figure 7-3

Binary transfer format

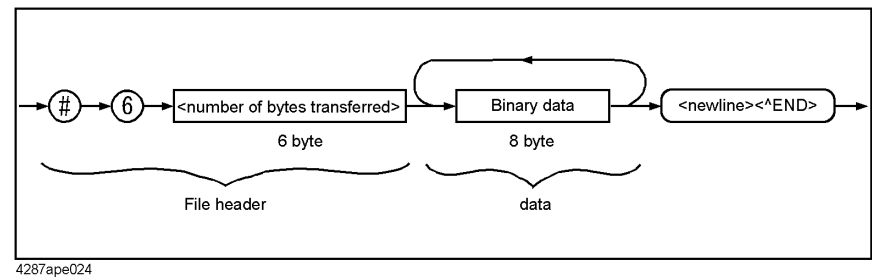


This data transfer format uses a header that consists of a sharp character (#), a number of 6 (which indicates the byte size of the <number of bytes transferred> part), and the <number of bytes transferred> part in this order. The header is followed by the binary data (each number consists of 8 bytes and the total is the byte size indicated by <number of bytes transferred>) and the message terminator <new line>^END.

The binary data is expressed in the IEEE 754 64-bit floating-point number format shown in Figure 7-4.

Figure 7-4

64-bit floating point format

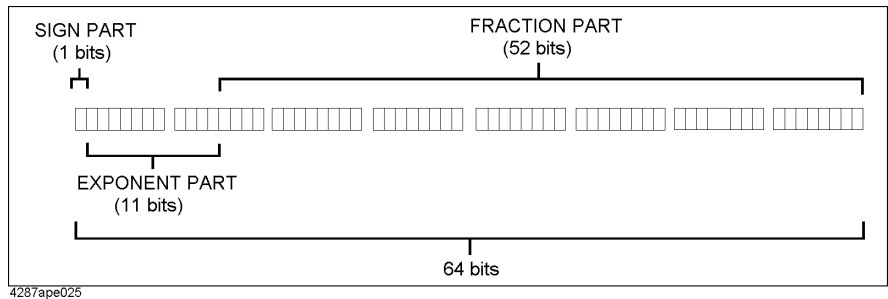


IEEE 32-bit floating point format

When you select the IEEE 32-bit floating point binary transfer format as the data transfer format, numbers are transferred in the format shown in Figure 7-5.

Figure 7-5

IEEE 32-bit floating point binary transfer format

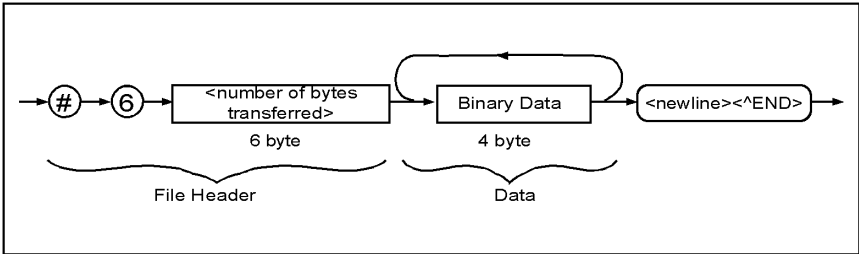


This data transfer format uses a header that consists of a sharp character (#), a number of 6 (which indicates the byte size of the <number of bytes transferred> part), and the <number of bytes transferred> part in this order. The header is followed by the binary data (each number consists of 4 bytes and the total is the byte size indicated by <number of bytes transferred>) and the message terminator <new line>^END.

The binary data is expressed in the IEEE 754 32-bit floating-point number format shown in Figure 7-6.

Figure 7-6

32-bit floating point data

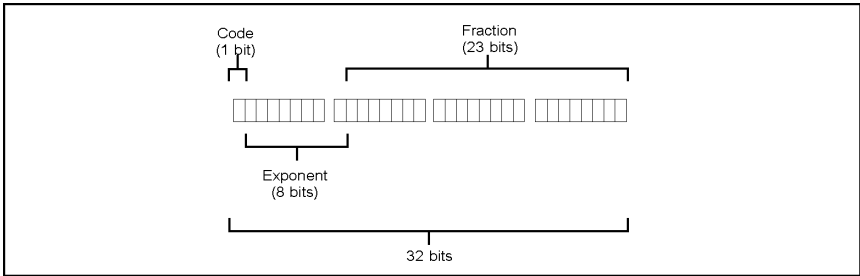

Byte order

When you opt to perform binary transfer, you can configure the instrument to transfer the bytes of the data in one of the following two byte orders:

- | | |
|---------|--|
| NORMAL | Transfer begins with the byte that contains the MSB (most significant bit); that is, the leftmost byte in Figure 7-4 and Figure 7-6. |
| SWAPped | Transfer begins with the byte that contains the LSB (least significant bit); that is, the rightmost byte in Figure 7-4 and Figure 7-6. |

To set the byte order, use the following command:

- **:FORM:BORD** on page 337

NOTE

Executing the **:SYST:PRES** command on page 479 or ***RST** command on page 199 does not affect the current setting of the byte order.


Internal data processing

Data flow

Figure 7-7 provides an overview of the E5061A/E5062A's internal data processing flow. For more information on the data processing flow, refer to "User's Guide."

Figure 7-7

E5061A/E5062A's data processing flow

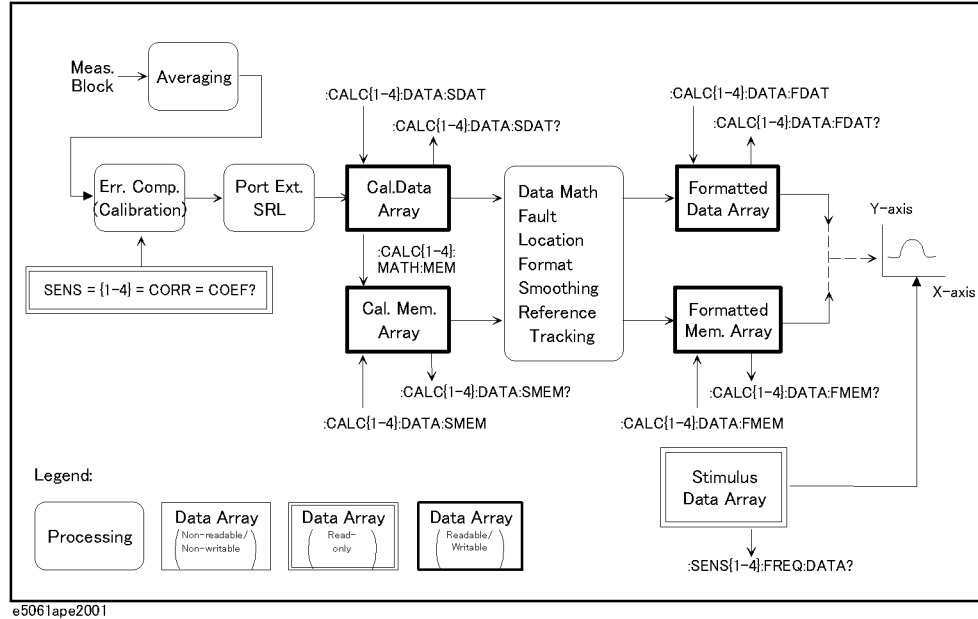

Internal data arrays

Corrected data arrays

A corrected data array contains the corrected data obtained by performing error correction, port extension compensation (calibration), Fixture Simulator operations on the raw measured data of S parameter specified for each trace of each channel. Each data element is stored as a complex number (Re/Im).

The instrument retains 16 corrected data arrays at maximum, each of which is associated with one of the 4 traces contained in one of the 4 channels $4 \times 4 = 16$). To read/write one of the corrected data arrays, use the following command:

- **:CALC{1-4}:DATA:SDAT** on page 217

Corrected memory arrays

When the **:CALC{1-4}:MATH:MEM** command on page 281 command is executed on a particular corrected data array, its copy is stored into the corrected memory array corresponding to that corrected data array.

The instrument retains 16 corrected memory arrays at maximum, each of which is

associated with one of the 4 traces contained in one of the 4 channels $4 \times 4 = 16$). To read/write one of the corrected data arrays, use the following command:

- **:CALC{1-4}:DATA:SMEM** on page 218

Formatted data array

A formatted data array contains the formatted data (values to be displayed) obtained by performing data math operations, measurement parameter conversion, and smoothing on a particular corrected data array. Regardless of the data format, it contains two data elements per measurement point as shown in the following table:

Table 7-1

Data elements and data formats

Data format*1	Data element (primary value)	Data element (secondary value)
log magnitude	log magnitude	Always 0
Phase	Phase	Always 0
Group delay	Group delay	Always 0
Smith chart (Lin)	Liner magnitude	Phase
Smith chart (Log)	log magnitude	Phase
Smith chart (Re/Im)	Real part of a complex number	Imaginary part of a complex number
Smith chart (R+jX)	Resistance	Reactance
Smith chart (G+jB)	Conductance	Susceptance
Polar (Lin)	Liner magnitude	Phase
Polar (Log)	log magnitude	Phase
Polar (Re/Im)	Real part of a complex number	Imaginary part of a complex number
Liner magnitude	Liner magnitude	Always 0
SWR	SWR	Always 0
Real number	Real part of a complex number	Always 0
Imaginary number	Imaginary part of a complex number	Always 0
Expanded phase	Expanded phase	Always 0
Positive phase	Positive phase	Always 0

*1. To set this, use the **:CALC{1-4}:FORM** command on page 219 command.

The instrument retains 16 formatted data arrays at maximum, each of which is associated with one of the 4 traces contained in one of the 4 channels $4 \times 4 = 16$). To read/write one of the formatted data arrays, use the following command:

- **:CALC{1-4}:DATA:FDAT** on page 215

Formatted memory arrays

A formatted memory array contains the formatted data (values to be displayed) obtained by performing data math operations, measurement parameter conversion, and smoothing on a particular corrected memory array.

The instrument retains 16 formatted memory arrays at maximum, each of which is associated with one of the 4 traces contained in one of the 4 channels $4 \times 4 = 16$). To read/write one of the formatted memory arrays, use the following command:

- **:CALC{1-4}:DATA:FMEM** on page 216

Stimulus data arrays

A stimulus data array contains the stimulus values for all measurement points.

The instrument retains 4 stimulus data arrays at maximum, each of which is associated with one of the 4 channels. Stimulus data arrays are read-only. To retrieve one of the stimulus data arrays, use the following command:

- **:SENS{1-4}:FREQ:DATA?** on page 416

Calibration coefficient arrays

A calibration coefficient array contains the calibration coefficients calculated based on the results of measurement performed with standard devices.

The instrument retains 4 calibration coefficient arrays at maximum, each of which is associated with one of the 4 channels. No commands are available that read or write calibration coefficient arrays.

Retrieving Measurement Results

“Internal data arrays” on page 108 allow you to retrieve all measurement results throughout a particular trace. Alternatively, markers allow you to retrieve measurement results at your specified points. For information on how to retrieve marker values, refer to “Retrieving Measurement Results at Marker Positions” on page 90.

Retrieving Internal Data Arrays

You can choose between the ASCII and binary data transfer formats when you retrieve internal data arrays. For more information, refer to “Data Transfer Format” on page 104.

Example 7-1 and Example 7-2 show sample programs that demonstrate how to retrieve formatted data arrays. The sample program in Example 7-1 uses the ASCII transfer format while the sample in Example 7-2 uses the binary transfer format. You can find the source files of these programs, named `read_asc.htb` and `read_bin.htb`, on the sample program disk.

Each of the sample programs holds the sweep on channel 1, then retrieves and displays the stimulus array for channel 1 and the formatted data array for trace 1.

The program in Example 7-1 is described in detail below:

Line 50	Assigns a GPIB address to the I/O pass.
Lines 70 to 90	These lines set channel 1's active trace to trace 1 and hold the sweep.
Lines 100 to 110	These lines retrieve the number of points in channel 1 and stores that number into the Nop variable.
Line 120	Resizes the Fdata and Freq arrays based on the value of the Nop variable (the number of points).
Line 160	Sets the data transfer format to ASCII.
Lines 180 to 190	These lines retrieve the formatted data array for the active trace (trace 1) in channel 1, and store the data into the Fdata array.
Lines 200 to 210	These lines retrieve the stimulus array for channel 1 and stores the data into the Freq variable.
Lines 250 to 260	These lines retrieve the data format for the active trace (trace 1) in channel 1, and store it into the Fmt\$ array.
Lines 270 to 400	The lines display each point along with one measured value and a frequency if the Fmt\$ is “MLOG”, “PHAS”, “GDEL”, “MLIN”, “SWR”, “REAL”, “IMAG”, or “UPH”; or along with two measured values and a frequency if Fmt\$ returns any other string.

Example 7-1

Using the ASCII Transfer Format to Retrieve Internal Data Arrays (read_asc.htb)

```
10    REAL Fdata(1:1601,1:2),Freq(1:1601)
20    DIM Img$[30]
30    INTEGER Nop,I
40    !
50    ASSIGN @Agte507x TO 717
60    !
70    OUTPUT @Agte507x;":CALC1:PAR1:SEL"
80    OUTPUT @Agte507x;":INIT1:CONT OFF"
90    OUTPUT @Agte507x;":ABOR"
100   OUTPUT @Agte507x;":SENS1:SWE:POIN?"
110   ENTER @Agte507x;Nop
120   REDIM Fdata(1:Nop,1:2),Freq(1:Nop)
130   !
140   ! Reading out in ASCII transfer format
150   !
160   OUTPUT @Agte507x;":FORM:DATA ASC"
170   !
180   OUTPUT @Agte507x;":CALC1:DATA:FDAT?"
190   ENTER @Agte507x;Fdata(*)
200   OUTPUT @Agte507x;":SENS1:FREQ:DATA?"
210   ENTER @Agte507x;Freq(*)
220   !
230   ! Displaying
240   !
250   OUTPUT @Agte507x;":CALC1:FORM?"
260   ENTER @Agte507x;Fmt$
270   SELECT Fmt$
280       CASE "MLOG","PHAS","GDEL","MLIN","SWR","REAL","IMAG","UPH"
290           Img$="MD.4DE,2X,MD.6DE"
300           PRINT " Frequency      Data"
310           FOR I=1 TO Nop
320               PRINT USING Img$;Freq(I),Fdata(I,1)
330           NEXT I
340       CASE ELSE
350           Img$="MD.4DE,2X,MD.6DE,2X,MD.6DE"
360           PRINT " Frequency      Data1      Data2"
370           FOR I=1 TO Nop
380               PRINT USING Img$;Freq(I),Fdata(I,1),Fdata(I,2)
390           NEXT I
400   END SELECT
410   !
420   END
```

The program in Example 7-2 is described in detail below:

Lines 50 to 60	Assigns a GPIB address to the I/O pass.
Lines 80 to 100	These lines set channel 1's active trace to trace 1 and hold the sweep.
Lines 110 to 120	These lines retrieve the number of points in channel 1 and store that number into the Nop variable.
Line 130	Resizes the Fdata and Freq arrays based on the value of the Nop variable (the number of points).
Line 170	Sets the data transfer format to binary.
Lines 190 to 200	These lines retrieve the data header.
Line 210	Retrieves the formatted data array for the active trace (trace 1) in channel 1, and stores the data into the Fdata array.

NOTE

Because binary data must be read without being formatted, the program uses an I/O path (@Binary) that is configured to support the retrieval of unformatted data. This applies to line 250 as well.

Line 220	Reads the message terminator at the end of the data.
Lines 230 to 240	These lines retrieve the data header.
Line 250	Retrieves the stimulus array for channel 1 and stores the data into the Freq variable.
Line 260	Reads the message terminator at the end of the data.
Lines 300 to 310	These lines retrieve the data format for the active trace (trace 1) in channel 1, and store it into the Fmt\$ array.
Lines 320 to 450	The lines display each point along with one measured value and a frequency if the Fmt\$ is "MLOG", "PHAS", "GDEL", "MLIN", "SWR", "REAL", "IMAG", or "UPH"; or along with two measured values and a frequency if Fmt\$ returns any other string.

Example 7-2

Using the Binary Transfer Format to Retrieve Internal Data Arrays (read_bin.htb)

```
10    REAL Fdata(1:1601,1:2),Freq(1:1601)
20    DIM Buff$(9),Img$(30)
30    INTEGER Nop,I
40    !
50    ASSIGN @Agte507x TO 717
60    ASSIGN @Binary TO 717;FORMAT OFF
70    !
80    OUTPUT @Agte507x;":CALC1:PAR1:SEL"
90    OUTPUT @Agte507x;":INIT1:CONT OFF"
100   OUTPUT @Agte507x;":ABOR"
110   OUTPUT @Agte507x;":SENS1:SWE:POIN?"
120   ENTER @Agte507x;Nop
130   REDIM Fdata(1:Nop,1:2),Freq(1:Nop)
140   !
150   ! Reading out in binary transfer format
160   !
170   OUTPUT @Agte507x;":FORM:DATA REAL"
180   !
190   OUTPUT @Agte507x;":CALC1:DATA:FDAT?"
200   ENTER @Agte507x USING "#,8A";Buff$
210   ENTER @Binary;Fdata(*)
220   ENTER @Agte507x USING "#,1A";Buff$
230   OUTPUT @Agte507x;":SENS1:FREQ:DATA?"
240   ENTER @Agte507x USING "#,8A";Buff$
250   ENTER @Binary;Freq(*)
260   ENTER @Agte507x USING "#,1A";Buff$
270   !
280   ! Displaying
290   !
300   OUTPUT @Agte507x;":CALC1:FORM?"
310   ENTER @Agte507x;Fmt$
320   SELECT Fmt$
330       CASE "MLOG","PHAS","GDEL","MLIN","SWR","REAL","IMAG","UPH"
340           Img$="MD.4DE,2X,MD.6DE"
350           PRINT " Frequency      Data"
360           FOR I=1 TO Nop
370               PRINT USING Img$;Freq(I),Fdata(I,1)
380           NEXT I
390       CASE ELSE
400           Img$="MD.4DE,2X,MD.6DE,2X,MD.6DE"
410           PRINT " Frequency      Data1      Data2"
420           FOR I=1 TO Nop
430               PRINT USING Img$;Freq(I),Fdata(I,1),Fdata(I,2)
440           NEXT I
450   END SELECT
460   !
470   END
```

Entering Data into a Trace

You can change the data/memory trace on the LCD by writing the new data into the “Formatted data array” on page 109/“Formatted memory arrays” on page 110.

When you write data into formatted data/memory array, you can choose either the ASCII or binary transfer format (see “Data Transfer Format” on page 104).

Example 7-3 and Example 7-4 show sample programs that demonstrate how to write data into formatted data arrays. The sample program in Example 7-3 uses the ASCII transfer format while the sample in Example 7-4 uses the binary transfer format. You can find the source files of these programs, named write_a.htb and write_b.htb, on the sample program disk.

Each of the sample programs holds the sweep on channel 1, retrieves the data from a specified file (a file saved measurement data using the **:MMEM:STOR:FDAT** command on page 356 command), and populates trace 1 for channel 1 with the retrieved data.

The program in Example 7-3 is described in detail below:

Line 50	Assigns a GPIB address to the I/O pass.
Line 70	Passes control to a subprogram named Inp_file_name, which lets the user input a file name, and then stores the returned file name into the File\$ variable. For more information on the Inp_file_name subprogram, refer to the description in Example 7-4.
Lines 90 to 110	These lines set channel 1's active trace to trace 1 and hold the sweep.
Lines 130 to 140	These lines retrieve the number of points in channel 1 and stores that number into the Nop variable.
Line 150	Resizes the Fdata array based on the value of the Nop variable (the number of points).
Line 170	This line points to the statement block to be executed if an error occurs in retrieving data from the file (for example, if no file matches File\$).
Lines 180 to 260	These lines retrieve the formatted data from the file identified by File\$, and store the data into the Fdata array.
Line 280	Sets the data transfer format to ASCII.
Line 300	Writes Fdata into the formatted data array for the active trace (trace 1) in channel 1.
Lines 340 to 380	This statement block is executed if an error occurs in retrieving data from the file.

Example 7-3

Using the ASCII Transfer Format to Write Formatted Data Arrays (write_a.htb)

```
10 REAL Freq,Fdata(1:1601,1:2)
20 DIM File$[300]
30 INTEGER Nop
40 !
50 ASSIGN @Agte507x TO 717
60 !
70 CALL Inp_file_name(File$)
80 !
90 OUTPUT @Agte507x;":CALC1:PAR1:SEL"
100 OUTPUT @Agte507x;":INIT1:CONT OFF"
110 OUTPUT @Agte507x;":ABOR"
120 !
130 OUTPUT @Agte507x;":SENS1:SWE:POIN?"
140 ENTER @Agte507x;Nop
150 REDIM Fdata(1:Nop,1:2)
160 !
170 ON ERROR GOTO File_error
180 ASSIGN @File TO File$
190 ENTER @File USING "K";Buff$
200 ENTER @File USING "K";Buff$
210 ENTER @File USING "K";Buff$
220 FOR I=1 TO Nop
230 ENTER @File USING "19D,2X,19D,2X,19D";Freq,Fdata(I,1),Fdata
(I,2)
240 NEXT I
250 ASSIGN @File TO *
260 OFF ERROR
270 !
280 OUTPUT @Agte507x;":FORM:DATA ASC"
290 !
300 OUTPUT @Agte507x;":CALC1:DATA:FDAT ";Fdata(*)
310 !
320 GOTO Prog_end
330 !
340 File_error: OFF ERROR
350 PRINT "##### ERROR #####"
360 PRINT File$&" is NOT exist."
370 PRINT " or"
380 PRINT File$&" has UNSUITABLE data."
390 !
400 Prog_end: END
410 !=====
420 ! File Name Input Function
430 !=====
440 SUB Inp_file_name(Inp_name$)
450 DIM Inp_char$[9]
460 ON ERROR GOTO Inp_start
470 Inp_start: !
480 PRINT "Input File Name!"
490 INPUT "Name?",Inp_name$
500 PRINT "Input Name: "&Inp_name$
510 INPUT "OK? [Y/N]",Inp_char$
520 IF UPC$(Inp_char$)<>"Y" THEN Inp_start
530 OFF ERROR
540 SUBEND
```

The program in Example 7-4 is described in detail below:

Lines 50 to 60	Assigns a GPIB address to the I/O pass.
Line 70	Passes control to a subprogram named <code>Inp_file_name</code> , which lets the user input a file name, and then stores the returned file name into the <code>File\$</code> variable.
Lines 90 to 110	These lines set channel 1's active trace to trace 1 and hold the sweep.
Lines 130 to 140	These lines retrieve the number of points in channel 1 and stores that number into the <code>Nop</code> variable.
Line 150	Resizes the <code>Fdata</code> array based on the value of the <code>Nop</code> variable (the number of points).
Line 170	This line points to the statement block to be executed if an error occurs in retrieving data from the file (for example, if no file matches <code>File\$</code>).
Lines 180 to 260	These lines retrieve the formatted data from the file identified by <code>File\$</code> , and store the data into the <code>Fdata</code> array.
Line 280	Sets the data transfer format to binary.
Line 290	Creates the data header and stores it into the <code>Header\$</code> variable.
Line 300	Sends the command that writes data into the formatted data array for the active trace (trace 1) in channel 1, following it with the data header (<code>Header\$</code>).
Line 310	Sends the data itself (<code>Fdata</code>), following it with a message terminator.

NOTE

Because binary data must be written without being formatted, the program uses an I/O path (`@Binary`) that is configured to support writing unformatted data.

Lines 340 to 380 This statement block is executed if an error occurs in retrieving data from the file.

The `Inp_file_name` subprogram in lines 440 to 540, which is used to enter a save filename, is described below.

Line 460	Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while entering the target file name.
Lines 480 to 490	These lines prompt the user to enter the target file name. The program does not continue till the user actually enters the file name.
Lines 500 to 510	These lines display the entered file name and waits for a confirmation entry (y/n key).
Line 520	Returns to the entry start line if the key the user pressed in line 870 is not the y key.

Example 7-4

Using the Binary Transfer Format to Write Formatted Data Arrays (write_b.htb)

```
10     REAL Freq,Fdata(1:1601,1:2)
20     DIM File$[300],Header$[10]
30     INTEGER Nop
40     !
50     ASSIGN @Agte507x TO 717
60     ASSIGN @Binary TO 717;FORMAT OFF
70     CALL Inp_file_name(File$)
80     !
90     OUTPUT @Agte507x;":CALC1:PAR1:SEL"
100    OUTPUT @Agte507x;":INIT1:CONT OFF"
110    OUTPUT @Agte507x;":ABOR"
120    !
130    OUTPUT @Agte507x;":SENS1:SWE:POIN?"
140    ENTER @Agte507x;Nop
150    REDIM Fdata(1:Nop,1:2)
160    !
170    ON ERROR GOTO File_error
180    ASSIGN @File TO File$
190    ENTER @File USING "K";Buff$
200    ENTER @File USING "K";Buff$
210    ENTER @File USING "K";Buff$
220    FOR I=1 TO Nop
230        ENTER @File USING "19D,2X,19D,2X,19D";Freq,Fdata(I,1),Fdata
(I,2)
240    NEXT I
250    ASSIGN @File TO *
260    OFF ERROR
270    !
280    OUTPUT @Agte507x;":FORM:DATA REAL"
290    Header$="#6"&IVAL$(8*2*Nop,10)
300    OUTPUT @Agte507x;":CALC1:DATA:FDAT ";Header$;
310    OUTPUT @Binary;Fdata(*),END
320    GOTO Prog_end
330    !
340 File_error: OFF ERROR
350    PRINT "##### ERROR #####"
360    PRINT File$&" is NOT exist."
370    PRINT "          or"
380    PRINT File$&" has UNSUITABLE data."
390    !
400 Prog_end: END
410    !=====
420    ! File Name Input Function
430    !=====
440 SUB Inp_file_name(Inp_name$)
450     DIM Inp_char$[9]
460     ON ERROR GOTO Inp_start
470 Inp_start: !
480     PRINT "Input File Name!"
490     INPUT "Name?",Inp_name$
500     PRINT "Input Name: "&Inp_name$
510     INPUT "OK? [Y/N]",Inp_char$
520     IF UPC$(Inp_char$)<>"Y" THEN Inp_start
530     OFF ERROR
540 SUBEND
```

8 Limit Test

This chapter describes how to use the Limit Test feature to perform a limit test and determine the pass/fail status of the measured data.

Performing a Limit Test

Configuring Limit Lines

The Limit Test feature of the E5061A/E5062A allows you to create up to 100 upper/lower limit lines on each trace and then determine the pass/fail status of the measured data.

When you manually configure limit lines, you must add each segment (limit line) to the limit table, and define various conditions that apply to the specific segment. On the other hand, when you use an external controller to configure limit lines, you can use the following command to define all the segment conditions (all limit lines) in the active table trace at once.

- **:CALC{1-4}:LIM:DATA** on page 233

Alternatively, you can configure limit lines based on the data contained in a CSV file by issuing the following command:

- **:MMEM:LOAD:LIM** on page 348

Also, you can save the contents of the current limit table to a file by issuing the following command:

- **:MMEM:STOR:LIM** on page 358

Showing/Hiding Limit Lines

To turn on or off limit lines, use the following command:

- **:CALC{1-4}:LIM:DISP** on page 235

Even when limit lines are hidden, the system performs limit test if the Limit Test feature is on.

To show or hide the part that is not used for evaluation, use the following command:

- **:CALC{1-4}:LIM:DISP:CLIP** on page 236

Turning On or Off the Limit Test Feature

To turn on or off the Limit Test feature, use the following command:

- **:CALC{1-4}:LIM** on page 232

Showing/Hiding “Fail”

To turn on or off the “Fail” which is displayed at the center of the window when the test result for the channel is “fail,” use the following command:

- **:DISP:FSIG** on page 313

Obtaining Test Results

You can obtain the test results by issuing a result retrieval command or through the status register. For detailed information on the status register, see Appendix B, “Status Reporting System.”

Test Results at Each Measurement Point

Using Commands That Retrieve Test Results

You can obtain the test results at each measurement point by retrieving the stimulus value at failed measurement points. To retrieve failed measurement points, use the following command:

Stimulus value	:CALC{1-4}:LIM:REP? on page 242
Number of measurement points	:CALC{1-4}:LIM:REP:POIN? on page 242

Using the Status Register

You cannot use the status register to obtain the test results at each measurement point.

Test Results for Each Trace

Using Commands That Retrieve Test Results

You can retrieve the test result for each trace (i.e., the trace-wide result that combines the results for all measurement points in a particular trace) by issuing the following command:

- :CALC{1-4}:LIM:FAIL? on page 237

Using the Status Register

The condition register and event register under the questionable limit channel {1-4} status register provide fourteen bits that correspond to traces 1 to 4 and contain the test results (0:Pass, 1:Fail) for the respective traces; for example, you can obtain the test result for trace 1 from bit 1, and that for trace 4 from bit 4.

Every bit of the condition register is set to 0 when a measurement cycle is started. Upon completion of measurement, those bits that correspond to failed traces are set to 1.

If the corresponding bit of the positive transition filter sets to 1 (preset value), each bit of the event register is set to 1 when the corresponding bit of the condition register changes from 0 to 1 (indicating that the corresponding trace failed the test).

Limit Test

Obtaining Test Results

To retrieve the registers, use the following command:

Questionable limit channel{1-16} status register	
Condition register	:STAT:QUES:LIM:CHAN{1-4}:COND? on page 455
Event register	:STAT:QUES:LIM:CHAN{1-4}? on page 455

Test Results for Each Channel

Using Commands That Retrieve Test Results

No commands are available that allow you to directly retrieve the test result for each channel (i.e., the channel-wide result that combines the results for all traces in a particular channel).

Using the Status Register

The questionable limit status event register provides fourteen bits that correspond to channels 1 to 4 and contain the test results (0:Pass, 1:Fail) for the respective channels; for example, you can obtain the test result for channel 1 from bit 1, and that for channel 4 from bit 4. .

Every bit of the condition register is set to 0 after the event registers are cleared by ***CLS** command on page 196. Upon completion of measurement, if the channel-wide test result that combines the results for all traces^{*1} in a channel is “fail”, the corresponding bit of the condition register is set to 1.

If the corresponding bit of the positive transition filter sets to 1 (preset value), every bit of the event register is set to 1 when the corresponding bit of the condition register changes from 0 to 1.


To retrieve the registers, use the following command:

Questionable limit status register	
Condition register	:STAT:QUES:LIM:COND? on page 459
Event register	:STAT:QUES:LIM? on page 455

^{*1}. This is when the registers are set as preset values. You can configure the enable registers and transition filters under the questionable limit channel {1-16} status register so that the condition register's bits reflect the result that combines the results for a limited set of traces, rather than for all the traces.

Figure 8-1

Obtaining the test results for a channel (channel 1 in this example) using the status register

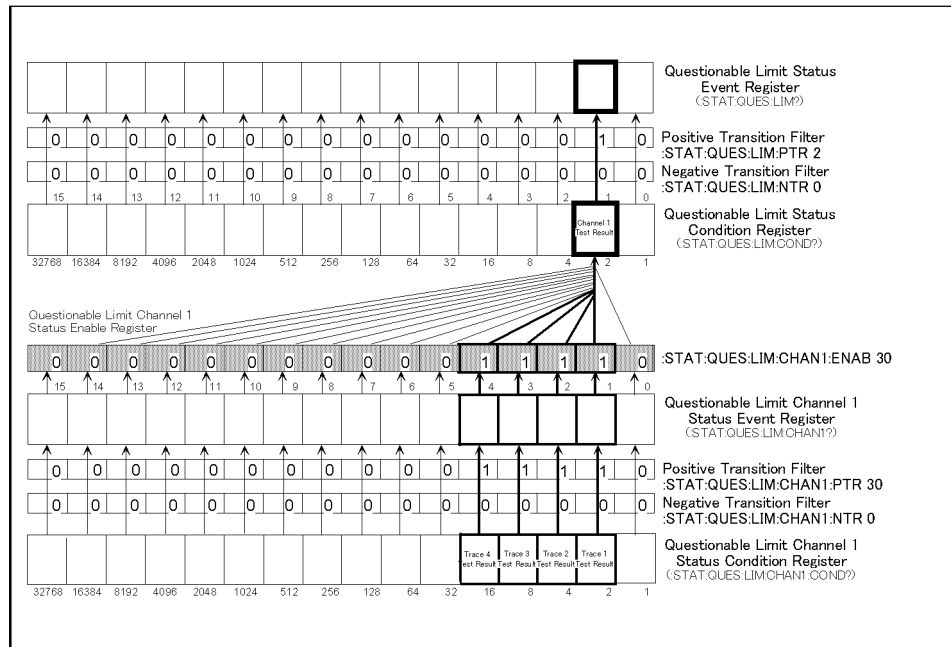

e5061ape0403

Overall Test Result

Using Commands That Retrieve Test Results

No commands are available that allow you to directly retrieve the overall test result that combine the test results for all channels.

Using the Status Register

Each of the condition register and event register under the questionable status event register provides bit 10, from which you can obtain the overall test result (0:Pass, 1:Fail).
The condition register's bit 10 is set to 0 after the event registers are cleared by ***CLS** command on page 196. Upon completion of measurement, this bit is set to 1 if the overall test result that combines the results for all channels^{*1} is "fail".


If the positive transition filter's bit 10 sets to 1 (preset value), the event register's bit 10 is set to 1 when the condition register's bit 10 changes from 0 to 1.

To retrieve the condition register and event register under the questionable status register, use the following command:

Condition register	:STAT:QUES:COND? on page 453
Event register	:STAT:QUES? on page 445

Figure 8-2

Obtaining the overall test result using the status register

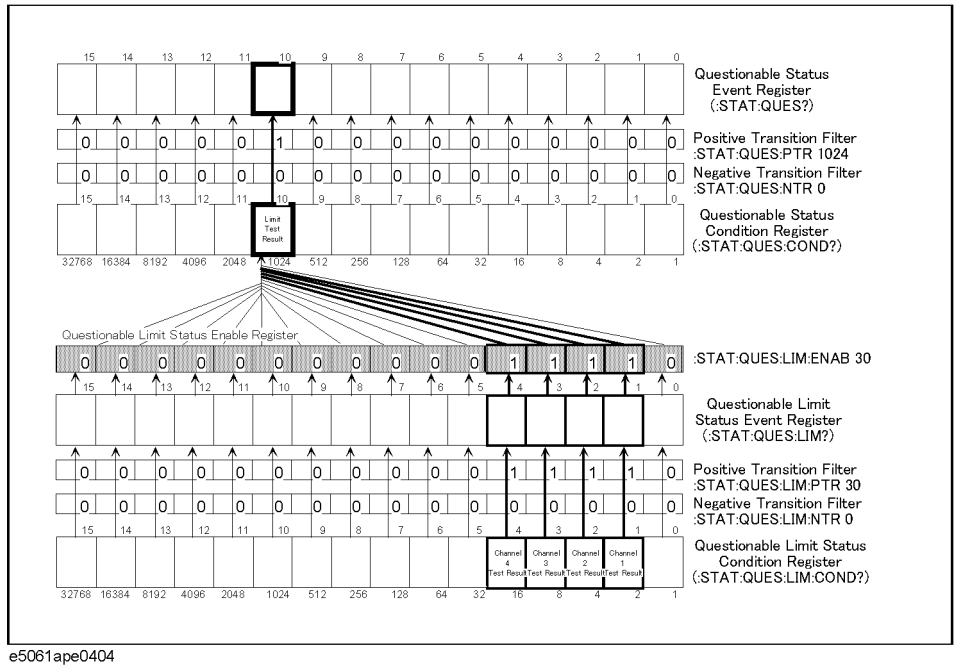

^{*1}. This is when the registers are set as preset values. You can configure the enable registers and transition filters under the questionable limit status register so that the condition register's bit 10 reflects the result that combines the results for a limited set of channels, rather than for all the channels.

Sample Program

Example 8-1 shows a sample program that demonstrates how to perform limit tests. You can find the source file of this program, named `lim_test.htb`, on the sample program disk.

The sample program creates a limit table as shown in Table 8-1 and Table 8-2; turns on the Limit Test feature; performs one cycle of measurement; then displays the test results.

Table 8-1

Limit table for trace 1

No.	Type	Begin Stimulus	End Stimulus	Begin Response	End Response
1	MAX	847.5 MHz	905.0 MHz	-55.0 dB	-55.0 dB
2	MIN	935.0 MHz	960.0 MHz	-3.5 dB	-3.5 dB
3	MAX	935.0 MHz	960.0 MHz	0 dB	0 dB
4	MAX	980.0 MHz	1047.5 MHz	-25.0 dB	-25.0 dB

Table 8-2

Limit table for trace 2

No.	Type	Begin Stimulus	End Stimulus	Begin Response	End Response
1	MAX	847.5 MHz	925.0 MHz	0 dB	0 dB
2	MIN	935.0 MHz	960.0 MHz	-9.5 dB	-9.5 dB
3	MAX	970.0 MHz	1047.5 MHz	0 dB	0 dB

The program is described in detail below:

Line 50	Assigns a GPIB address to the I/O pass.
Lines 70 to 120	These lines store the sweep center value, sweep span value, trace 1 measurement parameter, trace 2 measurement parameter, trace 1 data format, and trace 2 data format into the variables Cent, Span, Param1\$, Param2\$, Fmt1\$, and Fmt2\$, respectively.
Line 150	Stores the number of segments in trace 1 limit table into the Num_of_seg1 variable.
Lines 160 to 390	These lines store the settings in trace 1 limit table into the Lim1(*) variable.
Line 410	Stores the number of segments in trace 2 limit table into the Num_of_seg2 variable.
Lines 420 to 590	These lines store the settings in trace 2 limit table into the Lim2(*) variable.
Lines 610 to 620	These lines configure the sweep range for channel 1's sweep range using the center and span values contained in the Cent and Span values.
Lines 630 to 660	These lines configure channel 1 so that it contains 2 traces, displays graphs in two windows tiled horizontally (i.e., with the screen split into the upper and lower halves), uses a bus trigger source, and works in continuous activation mode.

Limit Test Sample Program

Line 700	Sets channel 1's active trace to trace 1.
Lines 720 to 730	These lines store trace 1's measurement parameter and data format into the variables Param1\$ and Fmt1\$, respectively.
Lines 750 to 810	These lines set up the limit table for trace 1. Line 750: Sends the command that sets up a limit table along with the Num_of_seg1 variable that contains the number of segments. Lines 770 to 790: Sends five data items (type, start point stimulus value, end point stimulus value, start point response value, and end point response value) for each segment.
Lines 820 to 830	These lines turns on the display of limit lines and the Limit Test feature for trace 1.
Line 870	Sets channel 1's active trace to trace 2.
Lines 890 to 900	These lines set trace 2's measurement parameter and data format to Param2\$ and Fmt2\$, respectively.
Lines 920 to 980	These lines set up the limit table for trace 2.
Lines 990 to 1000	These lines turns on the display of limit lines and the Limit Test feature for trace 2.
Lines 1040 to 1060	These lines set, under the questionable limit channel 1 status register, the enable register and positive transition filter to 6 (000000000000110 in binary notation) while setting the negative transition filter to 0 so that the questionable limit status condition register's bit 1 is set to 1 when the test result that combines the results for trace 1 and trace 2 is "fail".

NOTE

The sample program provides an example of explicitly configuring the register bits so that they reflect the test result that only covers trace 1 and trace 2. However, because the results for traces 3 to 9 will never be "fail" as long as the Limit Test feature is disabled for those traces, the register bits would reflect the test result that is limited to traces 1 and 2 even if you did not change the default setting.

Lines 1070 to 1080	These lines set transition filters so that the questionable limit status event register's bit 1 is set to 1 when the questionable limit status condition register's bit 1 changes from 0 to 1.
Line 1090	Clears the questionable limit status event register and questionable limit channel 1 status event register.
Lines 1110 to 1130	These lines trigger the instrument, and waits until the sweep cycle completes.
Lines 1170 to 1190	These lines retrieve the value of the questionable limit status event register, and store the setting of bit 1 of the value into Ch1_judge.
Lines 1200 to 1230	These lines retrieve the value of the questionable limit channel 1 status event register, and store the settings of bit 1 and bit 2 of the value into Tr1_judge and Tr2_judge, respectively.
Line 1280	Displays a message indicating that the DUT has passed the limit test if the test result for channel 1 is "Pass" (i.e., if Ch1_judge returns 0).
Lines 1300 to 1660	These lines are executed if the test result for channel 1 is "Fail" (i.e., if

Ch1_judge returns 1).

Line 1300: Notifies the user that the limit test result is “Fail”.

Line 1320: Displays a message indicating that trace 1 has passed the limit test if the test result for trace 1 is “Pass” (i.e., if Tr1_judge returns 0).

Lines 1340 to 1470: These lines are executed if the test result for trace 1 is “Fail” (i.e., if Tr1_judge returns 1). The lines notify the user that the test result for trace 1 is “Fail”, then retrieve and display the frequencies at the failed measurement points on trace 1.

Line 1340: Notifies the user that the limit test result for trace 1 is “Pass”.

Line 1380: Sets channel 1's active trace to trace 2.

Lines 1390 to 1410: These lines retrieve the number of failed measurement points on trace 1 and, based on that number, resize the array that will contain retrieved frequencies.

Lines 1420 to 1470: These lines retrieve and display the frequencies at the failed measurement points on trace 1.

Line 1500: Displays a message indicating that trace 2 has passed the limit test if the test result for trace 2 is “Pass” (i.e., if Tr2_judge returns 0).

Lines 1520 to 1650: If the test result for trace 2 is “Fail” (i.e., if Tr2_judge returns 1), these lines notify the user that trace 2 has failed to pass the limit test, and then retrieve and display the frequencies at the failed measurement points on trace 2.

Limit Test Sample Program

Example 8-1

Limit Test (lim_test.hbt)

```
10    DIM Param1$(9),Param2$(9),Fmt1$(9),Fmt2$(9),Buff$(9)
20    REAL Cent,Span,Lim1(1:4,1:5),Lim2(1:3,1:5),Fail_data(1:1601)
30    INTEGER Num_of_seg1,Num_of_seg2,Segment,Column,Fail_point
40    !
50    ASSIGN @Agte507x TO 717
60    !
70    Cent=9.475E+8
80    Span=2.00E+8
90    Param1$="S21"
100   Param2$="S11"
110   Fmt1$="MLOG"
120   Fmt2$="MLOG"
130   !
140   ! == Trace 1 Limit Line ==
150   Num_of_seg1=4           ! Number of segments: 4
160   ! -- Segment 1 --
170   Lim1(1,1)=1             ! Type           : Maximum
180   Lim1(1,2)=8.475E+8      ! Frequency Start: 847.5 MHz
190   Lim1(1,3)=9.050E+8      !           Stop : 905.0 MHz
200   Lim1(1,4)=-55           ! Response Start: -55 dBm
210   Lim1(1,5)=-55           !           Stop : -55 dBm
220   ! -- Segment 2 --
230   Lim1(2,1)=2             ! Type           : Minimum
240   Lim1(2,2)=9.350E+8      ! Frequency Start: 935.0 MHz
250   Lim1(2,3)=9.600E+8      !           Stop : 960.0 MHz
260   Lim1(2,4)=-3.5          ! Response Start: -3.5 dBm
270   Lim1(2,5)=-3.5          !           Stop : -3.5 dBm
280   ! -- Segment 3 --
290   Lim1(3,1)=1             ! Type           : Maximum
300   Lim1(3,2)=9.350E+8      ! Frequency Start: 935.0 MHz
310   Lim1(3,3)=9.600E+8      !           Stop : 960.0 MHz
320   Lim1(3,4)=0             ! Response Start: 0 dBm
330   Lim1(3,5)=0             !           Stop : 0 dBm
340   ! -- Segment 4 --
350   Lim1(4,1)=1             ! Type           : Maximum
360   Lim1(4,2)=9.800E+8      ! Frequency Start: 980.0 MHz
370   Lim1(4,3)=1.0475E+9     !           Stop : 1047.5 MHz
380   Lim1(4,4)=-25           ! Response Start: -25 dBm
390   Lim1(4,5)=-25           !           Stop : -25 dBm
400   ! == Trace 2 Limit Line ==
410   Num_of_seg2=3           ! Number of segments: 3
420   ! -- Segment 1 --
430   Lim2(1,1)=1             ! Type           : Maximum
440   Lim2(1,2)=8.475E+8      ! Frequency Start: 847.5 MHz
450   Lim2(1,3)=9.250E+8      !           Stop : 925.0 MHz
460   Lim2(1,4)=0             ! Response Start: 0 dBm
470   Lim2(1,5)=0             !           Stop : 0 dBm
480   ! -- Segment 2 --
490   Lim2(2,1)=1             ! Type           : Maximum
500   Lim2(2,2)=9.350E+8      ! Frequency Start: 935.0 MHz
510   Lim2(2,3)=9.600E+8      !           Stop : 960.0 MHz
520   Lim2(2,4)=-9.5          ! Response Start: -9.5 dBm
530   Lim2(2,5)=-9.5          !           Stop : -9.5 dBm
540   ! -- Segment 3 --
550   Lim2(3,1)=1             ! Type           : Maximum
```

```

560 Lim2(3,2)=9.700E+8      ! Frequency Start: 970.0 MHz
570 Lim2(3,3)=1.0475E+9    !           Stop : 1047.5 MHz
580 Lim2(3,4)=0            ! Response  Start: 0 dBm
590 Lim2(3,5)=0            !           Stop : 0 dBm
600 !
610 OUTPUT @Agte507x;":SENS1:FREQ:CENT ";Cent
620 OUTPUT @Agte507x;":SENS1:FREQ:SPAN ";Span
630 OUTPUT @Agte507x;":CALC1:PAR1:COUN 2"
640 OUTPUT @Agte507x;":DISP:WIND1:SPL D1_2"
650 OUTPUT @Agte507x;":TRIG:SOUR BUS"
660 OUTPUT @Agte507x;":INIT1:CONT ON"
670 !
680 ! Trace 1
690 !
700 OUTPUT @Agte507x;":CALC1:PAR1:SEL"
710 !
720 OUTPUT @Agte507x;":CALC1:PAR1:DEF "&Param1$
730 OUTPUT @Agte507x;":CALC1:FORM "&Fmt1$
740 !
750 OUTPUT @Agte507x;":CALC1:LIM:DATA ";Num_of_seg1;
760 FOR Segment=1 TO Num_of_seg1
770     FOR Column=1 TO 5
780         OUTPUT @Agte507x;",";Lim1(Segment,Column);
790     NEXT Column
800 NEXT Segment
810 OUTPUT @Agte507x;""
820 OUTPUT @Agte507x;":CALC1:LIM:DISP ON"
830 OUTPUT @Agte507x;":CALC1:LIM ON"
840 !
850 ! Trace 2
860 !
870 OUTPUT @Agte507x;":CALC1:PAR2:SEL"
880 !
890 OUTPUT @Agte507x;":CALC1:PAR2:DEF "&Param2$
900 OUTPUT @Agte507x;":CALC1:FORM "&Fmt2$
910 !
920 OUTPUT @Agte507x;":CALC1:LIM:DATA ";Num_of_seg2;
930 FOR Segment=1 TO Num_of_seg2
940     FOR Column=1 TO 5
950         OUTPUT @Agte507x;",";Lim2(Segment,Column);
960     NEXT Column
970 NEXT Segment
980 OUTPUT @Agte507x;""
990 OUTPUT @Agte507x;":CALC1:LIM:DISP ON"
1000 OUTPUT @Agte507x;":CALC1:LIM ON"
1010 !
1020 ! Setting status registers
1030 !
1040 OUTPUT @Agte507x;":STAT:QUES:LIM:CHAN1:ENAB 6"
1050 OUTPUT @Agte507x;":STAT:QUES:LIM:CHAN1:PTR 6"
1060 OUTPUT @Agte507x;":STAT:QUES:LIM:CHAN1:NTR 0"
1070 OUTPUT @Agte507x;":STAT:QUES:LIM:PTR 2"
1080 OUTPUT @Agte507x;":STAT:QUES:LIM:NTR 0"
1090 OUTPUT @Agte507x;"*CLS"
1100 !
1110 OUTPUT @Agte507x;":TRIG:SING"
1120 OUTPUT @Agte507x;"*OPC?"
1130 ENTER @Agte507x;Buff$

```

Limit Test

Sample Program

```
1140      !
1150      ! Checking test results
1160      !
1170      OUTPUT @Agte507x;":STAT:QUES:LIM?"
1180      ENTER @Agte507x;Reg_val
1190      Ch1_judge=BIT(Reg_val,1)
1200      OUTPUT @Agte507x;":STAT:QUES:LIM:CHAN1?"
1210      ENTER @Agte507x;Reg_val
1220      Tr1_judge=BIT(Reg_val,1)
1230      Tr2_judge=BIT(Reg_val,2)
1240      !
1250      ! Displaying test results
1260      !
1270      IF Ch1_judge=0 THEN
1280          PRINT "## PASS! ##"
1290      ELSE
1300          PRINT "## FAIL! ##"
1310          IF Tr1_judge=0 THEN
1320              PRINT " Trace1(S21): PASS"
1330          ELSE
1340              PRINT " Trace1(S21): FAIL"
1350              !
1360              ! Reading and displaying frequency at failed points
1370              !
1380              OUTPUT @Agte507x;":CALC1:PAR1:SEL"
1390              OUTPUT @Agte507x;":CALC1:LIM:REP:POIN?"
1400              ENTER @Agte507x;Fail_point
1410              REDIM Fail_data(1:Fail_point)
1420              OUTPUT @Agte507x;":CALC1:LIM:REP?"
1430              ENTER @Agte507x;Fail_data(*)
1440              PRINT "  Frequency:"
1450              FOR I=1 TO Fail_point
1460                  PRINT USING "3X,MD.4DE";Fail_data(I)
1470              NEXT I
1480          END IF
1490          IF Tr2_judge=0 THEN
1500              PRINT " Trace2(S11): PASS"
1510          ELSE
1520              PRINT " Trace2(S11): FAIL"
1530              !
1540              ! Reading and displaying frequency at failed points
1550              !
1560              OUTPUT @Agte507x;":CALC1:PAR2:SEL"
1570              OUTPUT @Agte507x;":CALC1:LIM:REP:POIN?"
1580              ENTER @Agte507x;Fail_point
1590              REDIM Fail_data(1:Fail_point)
1600              OUTPUT @Agte507x;":CALC1:LIM:REP?"
1610              ENTER @Agte507x;Fail_data(*)
1620              PRINT "  Frequency:"
1630              FOR I=1 TO Fail_point
1640                  PRINT USING "3X,MD.4DE";Fail_data(I)
1650              NEXT I
1660          END IF
1670      END IF
1680      END
```

9

Saving and Recalling (File Management)

This chapter describes how to save and recall instrument status and measurement results onto/from the files. Here also covered is managing files.

Saving and Recalling File

Specifying file

When running a command for saving, recalling, and managing files, use a filename with extension to specify a particular file. Specify “A:” in the beginning of the file name, when specifying a file on the flexible disk. Also, when specifying a file name with directory, use “/” (slash) or “\” (backslash) as a delimiter.

Saving and recalling instrument status

You can save the instrument state using one of the following 2 methods:

- ☐ Saving the entire instrument state into a file
- ☐ Saving the state for each channel into registers A to D (volatile memory)

Selecting content to be saved

When saving the instrument status into a file or register, the content to be saved can be selected among the following 4 options:

- ☐ Instrument status only (see *Users Guide* for setting items to be saved)
- ☐ Instrument status and calibration coefficient array.
- ☐ Instrument status, corrected data/memory array (measurement data)
- ☐ Instrument status, calibration coefficient array, and corrected data/memory array (measurement data)

To select a content to be saved, use the following command:

- :MMEM:STOR:STYP on page 363

Selecting Content to be Saved

To select whether to save the setting of all channels/traces or that of the displayed channels/traces, use the following command:

- :MMEM:STOR:SALL on page 361

Saving and recalling entire instrument status

To save the entire instrument status into a file, use the following command:

- :MMEM:STOR on page 353

Recalling a file saved with the above command can reproduce the status when it was saved. To recall the settings from a file, use the following command:

- :MMEM:LOAD on page 345

Auto recall

The file saved with the name autorec.sta or A:autorec.sta will be automatically recalled the E5061A/E5062A is powered ON.

Saving state for each channel into a register

For the active channel, when you want to save the instrument state specific to that channel only into one of registers A to D, use the following command:

- :MMEM:STOR:CHAN on page 354

Recalling an instrument state saved in a register can reproduce it as the state of the active channel. To recall a register, use the following command:

- :MMEM:LOAD:CHAN on page 346

NOTE

It is possible to recall a file from a different channel where it was saved.

The contents in the registers are lost when you turn OFF the power. You can delete (clear) the contents of all the registers using the following command.

- :MMEM:STOR:CHAN:CLE on page 354

Saving measurement data

Measurement data (in a formatted data array) can be saved in the file with CSV (Comma Separated Value) format.

To save measurement data on a file, use the following command:

- :MMEM:STOR:FDAT on page 356

Executing the above command will save the measurement data of the active trace. Note that the data save using the above command cannot be recalled from the E5061A/E5062A.

Saving the images on the LCD screen

Images displayed on the LCD screen can be saved on a file in the bitmap (.bmp) or portable network graphics (.png) format.

To save screen image on a file, use the following command:

- :MMEM:STOR:IMAG on page 357

Executing the above command will save the screen image when the command is invoked.

NOTE

Note that this gives different result than operation from the front panel where screen image is saved at the time **[Capture]** key is pressed.

Saving and recalling the segment sweep table

Segment sweep table can be saved in the file with CSV (Comma Separated Value) format.

To save segment sweep table on a file, use the following command:

- :MMEM:STOR:SEGM on page 362

Executing the above command will save the segment sweep table for the active channel.

Recalling the file saved using the above command can reproduce the segment sweep table on the active channel.

To recall the settings from a file, use the following command:

- :MMEM:LOAD:SEGM on page 351

NOTE

It is possible to recall a file from a different channel where it was saved. Note that recalling operation is not guaranteed for the file that might have been modified with editor.

Saving and recalling the limit table

Limit table can be saved in the file with CSV (Comma Separated Value) format. To save limit table on a file, use the following command:

- :MMEM:STOR:LIM on page 358

Executing the above command will save the limit table for the active trace of the active channel.

Recalling the file saved using the above command can reproduce the limit table on the active trace of the active channel. To recall the settings from a file, use the following command:

- :MMEM:LOAD:LIM on page 348

NOTE

It is possible to recall a file from a different channel or trace where it was saved. Note that recalling operation is not guaranteed for the file that might have been modified with editor.

Saving/loading (importing) the VBA program

Saving

Only the VBA project file can be saved using command.

To save the VBA project that is opened on the VBA editor on the file, use the following command.

- :MMEM:STOR:PROG on page 359

Loading (importing)

To load the VBA project to the VBA editor, or to import the module/form file, use the following command.

- :MMEM:LOAD:PROG on page 349

Executing above command will load/import the file according to its extension as follows:

Extension	File type
vba	VBA Project
bas	Standard module
frm	User Forms
cls	Class Modules

Sample program

Example 9-1 shows a sample program that demonstrates how to save a file. You can find the source file of this program, named `file_sav.bas`, on the sample program disk.

This program saves selected content on a file with a specified name.

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Line 60	Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while entering the number that identifies the content to be saved.
Lines 80 to 180	These lines display the list of options for content to be saved, and prompt the user to choose one of the items by typing in the appropriate number.
Line 190	Converts the entered value into an integer and stores it into the Content variable.
Line 200	Returns to the entry start line if an invalid value is contained in Content.
Line 230	Passes control to a subprogram named <code>Inp_file_name</code> , which lets the user input a file name for saving, and then stores the returned file name into the <code>File\$</code> variable.
Lines 270 to 280	If Content is equal to 1, these lines set the content to be saved as the instrument status to “instrument status only”, and store the state with the file name which is combined the <code>File\$</code> variable with the extension “.sta”.
Lines 300 to 310	If Content is equal to 2, these lines set the content to be saved as the instrument status to “instrument status and calibration coefficient”, and store the state with the file name which is combined the <code>File\$</code> variable with the extension “.sta”.
Lines 330 to 340	If Content is equal to 3, these lines set the content to be saved as the instrument status to “instrument status and measurement data”, and store the state with the file name which is combined the <code>File\$</code> variable with the extension “.sta”.
Lines 360 to 370	If Content is equal to 4, these lines set the content to be saved as the instrument status to “instrument status, calibration coefficient, and measurement data”, and store the state with the file name which is combined the <code>File\$</code> variable with the extension “.sta”.
Line 390	If Content is equal to 5, and store the state with the file name which is combined the <code>File\$</code> variable with the extension “.csv”.
Line 410	If Content is equal to 6, and store the image data of the LCD screen with the file name which is combined the <code>File\$</code> variable with the extension “.bmp”.

The Inp_file_name subprogram in lines 480 to 590, which is used to enter a save filename, is described below.

- Line 500 Allows the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while entering the target file name.
- Lines 520 to 540 These lines prompt the user to enter the target file name. The program does not continue till the user actually enters the file name.
- Lines 550 to 560 These lines display the entered file name and waits for a confirmation entry (y/n key).
- Line 570 Returns to the entry start line if the key the user pressed in line 560 is not the y key.

Example 9-1

Saving file (file_sav.htb)

```

10    DIM File$(300),Inp_char$(30)
20    INTEGER Content
30    CLEAR SCREEN
40    ASSIGN @Agte507x TO 717
50    !
60    ON ERROR GOTO Content_select
70 Content_select: !
80    PRINT "## Save Content Selection ##"
90    PRINT "Select Content"
100   PRINT " 1: State (State only)"
110   PRINT " 2: State (State & Cal)"
120   PRINT " 3: State (State & Trace)"
130   PRINT " 4: State (State & Cal & Trace)"
140   PRINT " 5: Trace Data (CSV)"
150   PRINT " 6: Screen"
160   PRINT ""
170   PRINT "Input 1 to 6"
180   INPUT "Number?",Inp_char$
190   Content=IVAL(Inp_char$,10)
200   IF Content<1 OR Content>6 THEN Content_select
210   OFF ERROR
220   !
230   CALL Inp_file_name(File$)
240   !
250   SELECT Content
260     CASE 1
270       OUTPUT @Agte507x;":MMEM:STOR:STYP STAT"
280       OUTPUT @Agte507x;":MMEM:STOR """"&File$&".sta""""
290     CASE 2
300       OUTPUT @Agte507x;":MMEM:STOR:STYP CST"
310       OUTPUT @Agte507x;":MMEM:STOR """"&File$&".sta""""
320     CASE 3
330       OUTPUT @Agte507x;":MMEM:STOR:STYP DST"
340       OUTPUT @Agte507x;":MMEM:STOR """"&File$&".sta""""
350     CASE 4
360       OUTPUT @Agte507x;":MMEM:STOR:STYP CDST"
370       OUTPUT @Agte507x;":MMEM:STOR """"&File$&".sta""""
380     CASE 5
390       OUTPUT @Agte507x;":MMEM:STOR:FDAT """"&File$&".csv""""
400     CASE 6

```

Saving and Recalling File

```
410      OUTPUT @Agte507x;":MMEM:STOR:IMAG ""&File$&".bmp""
420  END SELECT
430  !
440  END
450  !=====
460  ! File Name Input Function
470  !=====
480  SUB Inp_file_name(Inp_name$)
490    DIM Inp_char$(9)
500    ON ERROR GOTO Inp_start
510  Inp_start: !
520    PRINT "## File Name Input ##"
530    PRINT "Input Save File Name (without Extension)"
540    INPUT "Name?",Inp_name$
550    PRINT "Input Name: "&Inp_name$
560    INPUT "OK? [Y/N]",Inp_char$
570    IF UPC$(Inp_char$)<>"Y" THEN Inp_start
580    OFF ERROR
590  SUBEND
```

Managing Files

Creating directory (folder)

To create a directory (folder), use the following command:

- :MMEM:MDIR on page 352

Deleting file (directory)

To delete a file or a directory, use the following command:

- :MMEM:DEL on page 344

Copying file

To copy a file, use the following command:

- :MMEM:COPY on page 343

Transferring files

File transfer from the external controller to the E5061A/E5062A can be possible by reading data from a file on the controller and then writing them to the file on the E5061A/E5062A.

- :MMEM:TRAN on page 364

Also, file transfer from the E5061A/E5062A to the external controller can be possible by reading data from a file on the E5061A/E5062A using the commands as query and then writing them to the file on the controller.

Retrieving data from storage

To retrieve information for the storage that is built in the E5061A/E5062A (usage, property of file located in a specified directory), use the following command;

- :MMEM:CAT? on page 342

Sample program

Example 9-1 shows a sample program for transferring files between the external controller and the E5061A/E5062A. You can find the source file of this program, named file_xfr.bas, on the sample program disk.

This program reads out data from a specified file on the external controller (or the E5061A/E5062A), then write them to a specified file on the E5061A/E5062A(or the external controller).

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Lines 60 to 130	These line allow the user to return to the entry start line and re-enter the data if an error (such as an invalid entry) occurs while entering the number that indicates the transfer direction. Then, these line display the list of transfer directions and prompt the user to input a selected number.
Lines 80 to 130	These lines display the list of transfer directions, and prompt the user to choose one of the items by typing in the appropriate number.
Lines 140 to 150	Converts the entered value into an integer and stores it into the Direction variable. Returns to the entry start line if an invalid value is contained in Direction.
Lines 180 to 210	These lines obtain the name of the source file for copying from the user input, store it into the Src_file\$ variable, and display the value of Src_file\$.
Lines 180 to 210	These lines obtain the name of the source file for copying from the user input, store it into the Src_file\$ variable, and display the value of Src_file\$.
Lines 230 to 270	If Direction is equal to 2 (from the external controller to the E5061A/E5062A), these lines obtain the size of the source file for copying, store it into the Src_size_char\$, and display the value of Src_size_char\$.
Lines 290 to 320	These lines obtain the name of the destination file for copying from the user input, store it into the Dst_file\$ variable, and display the value of Dst_file\$.
Line 350	If Direction is equal to 1 (from the E5061A/E5062A to the external controller), these lines use the subprogram Copy_to_contr to transfer (copy) a file with the name Src_file\$ on the E5061A/E5062A to a file with the name Dst_file\$ on the external controller.
Line 370	If Direction is equal to 2, these lines use the subprogram Copy_to_e507x to transfer (copy) a file with the name Src_file\$ on the external controller to a file with the name Dst_file\$ on the E5061A/E5062A.

Copy_to_contr, a subprogram for transferring files from the E5061A/E5062A to the external controller that appears in lines 440 to 1000, is described below.

Lines 490 to 520	If any file with the name File\$ already exists, these lines delete the file and newly create a file with the name File\$.
Line 530	Assigns a destination file for copying to the I/O pass.

Line 540	This line stores a maximum number of transferred data (in bytes) per one transfer, that is 24 KByte to meet the size limitation of string arrays in the HTBasic, into Max_bsize variable.
Lines 560 to 600	These lines configure the system to generate an SRQ when it cannot find a source file for copying due to an error.
Lines 620 to 630	These lines set the branch target for an SRQ interrupt to enable SRQ interrupts.
Lines 640 to 650	These lines display a message showing that the transfer has started, and execute commands for reading data from a file on the E5061A/E5062A.
Lines 670 to 680	These lines read the header symbol (#) in a block data, read number of digits (characters) indicating the size of data in bytes, then store it into Digit\$ variable.
Line 690	This line creates a format for reading characters in Digit\$.
Line 700	This line reads the data size in byte and stores it into Src_size_char\$ variable.
Line 720	This line converts Src_size_char\$ to a real number and stores it into Src_size variable.
Lines 730 to 870	These lines repeat the procedures below until Src_size reaches 0. Lines 740 to 780: If Src_size is greater than Max_bsize, these lines assign the value of the Max_bsize to Block_size variable (transferred data in bytes). If Src_size is equal or less than Max_bsize, assign the value of Src_size to Block_size. Line 800 This line defines Dat\$ string variable with the size as large as Block_size and reserves memory area. Line 810 This line creates a format for reading characters as many as Block_size characters. Line 820 This line reads data from the file on the E5061A/E5062A, then stores them into Dat\$. Line 830 This line writes the contents of Dat\$ to the file on the external controller. Lines 840 to 860 These lines free the memory area for Dat\$ and subtract Block_size from Src_size.
Lines 890 to 900	These lines display a message showing the completion of transfer, then read a message terminator at the end of the data.
Lines 940 to 980	These lines define an error handler that retrieves and displays the number and message of an error that has occurred.
Copy_to_e507x, a subprogram for transferring files from the external controller to the E5061A/E5062A that appears in lines 1040 to 1540, is described below.	
Lines 1090 to 1110	Assigns a destination file for copying to the I/O pass.
Line 1120	This line stores a maximum number of transferred data (in bytes) per one transfer, that is 24 KByte, into Max_bsize variable.
Lines 1140 to 1160	Clears the error queue.

Saving and Recalling (File Management)

Managing Files

- Line 1180 Displays a measurement start message.
- Lines 1190 to 1200 These lines create the header part indicating that data will be sent as many as Src_size_char\$ bytes, then send the header part of the command and its parameters for writing the data to the file on the E5061A/E5062A.
- Line 1220 This line converts Src_size_char\$ to a real number and stores it into Src_size variable.
- Lines 1230 to 1370 These lines repeat the procedures below until Src_size reaches 0.
- Lines 1240 to 1280: If Src_size is greater than Max_bsize, these lines assign the value of the Max_bsize to Block_size variable (transferred data in bytes). If Src_size is equal or less than Max_bsize, assign the value of Src_size to Block_size.
- Line 1300 This line defines Dat\$ string variable with the size as large as Block_size and reserves memory area.
- Line 1310 This line creates a format for reading characters as many as Block_size characters.
- Line 1320 This line reads data from the file on the external controller, then stores them into Dat\$.
- Line 1330 This line writes the contents of Dat\$ to the file on the E5061A/E5062A.
- Lines 1340 to 1360 These lines free the memory area for Dat\$ and subtract Block_size from Src_size.
- Line 1390 This line sends a message terminator at the end of data.
- Lines 1420 to 1430 These lines retrieve the error number and error message from the error queue, and then store them into the variables Err_no and Err_msg\$, respectively.
- Lines 1440 to 1490 If Err_no is equal to 0 (no error occurred), these lines display the message indicating completion of transfer, and if Err_no is not equal to 0 (an error occurred), display Err_no along with Err_msg\$.
- Lines 1510 to 1520 These lines handle the case with no source file for copying is found.

Example 9-2

File transfer (file_xfr.htb)

```

10    DIM Src_file$[50],Dst_file$[50],Src_size_char$[50],Inp_char$[30]
20    INTEGER Direction
30    ASSIGN @Agte507x TO 717
40    !
50    CLEAR SCREEN
60    ON ERROR GOTO Direct_select
70 Direct_select: !
80    PRINT "#### File Transfer ####"
90    PRINT " 1: E507x -> Controller"
100   PRINT " 2: Controller -> E507x"
110   PRINT ""
120   PRINT "Input 1 or 2"
130   INPUT "Number?",Inp_char$
140   Direction=IVAL(Inp_char$,10)
150   IF Direction<1 OR Direction>2 THEN Direct_select
160   OFF ERROR
170   !
180   PRINT ""
190   PRINT " Input source file name.          ";
200   INPUT "Name?",Src_file$
210   PRINT ": "&Src_file$
220   !
230   IF Direction=2 THEN
240     PRINT " Input source file size.          ";
250     INPUT "Size[Byte]?",Src_size_char$
260     PRINT ": "&Src_size_char&"[Byte]"
270   END IF
280   !
290   PRINT " Input destination file name.    ";
300   INPUT "Name?",Dst_file$
310   PRINT ": "&Dst_file$
320   PRINT ""
330   !
340   IF Direction=1 THEN
350     Copy_to_contr(@Agte507x,Src_file$,Dst_file$)
360   ELSE
370     Copy_to_e507x(@Agte507x,Src_file$,Src_size_char$,Dst_file$)
380   END IF
390   !
400   END
410   !=====
420   ! File Transfer Function (E507x -> Controller)
430   !=====
440   SUB Copy_to_contr(@Agte507x,Src_file$,Dst_file$)
450     DIM Img$[32],Src_size_char$[10],Buff$[9],Err_msg$[100]
460     INTEGER Max_bsize,Block_size,Err_no
470     REAL Src_size
480     !
490     ON ERROR GOTO Skip_purge
500     PURGE Dst_file$
510 Skip_purge: OFF ERROR
520     CREATE Dst_file$,1
530     ASSIGN @Dst_file TO Dst_file$
540     Max_bsize=24576 ! 24KByte
550     !
560     OUTPUT @Agte507x;"*ESE 60"
570     OUTPUT @Agte507x;"*SRE 32"
580     OUTPUT @Agte507x;"*CLS"
590     OUTPUT @Agte507x;"*OPC?"
600     ENTER @Agte507x;Buff$
610     !

```

Saving and Recalling (File Management)

Managing Files

```

620   ON INTR 7 GOTO Err
630   ENABLE INTR 7;2
640   PRINT "Now Copying: "&Src_file$&"(E507x) -> "&Dst_file$&"(Controller)"
650   OUTPUT @Agte507x;":MMEM:TRAN? ""&Src_file$&""
660   WAIT .1
670   ENTER @Agte507x USING "#,A";Buff$
680   ENTER @Agte507x USING "#,A";Digit$
690   Img$="#,"&Digit$&"A"
700   ENTER @Agte507x USING Img$;Src_size_char$
710   !
720   Src_size=VAL(Src_size_char$)
730   WHILE Src_size>0
740     IF Src_size>Max_bsize THEN
750       Block_size=Max_bsize
760     ELSE
770       Block_size=Src_size
780     END IF
790     !
800     ALLOCATE Dat$(Block_size)
810     Img$="#,"&VAL$(Block_size)&"A"
820     ENTER @Agte507x USING Img$;Dat$
830     OUTPUT @Dst_file USING Img$;Dat$
840     DEALLOCATE Dat$
850     !
860     Src_size=Src_size-Block_size
870   END WHILE
880   !
890   PRINT "Done"
900   ENTER @Agte507x USING "#,A";Buff$
910   ASSIGN @Dst_file TO *
920   !
930   GOTO Skip_error
940 Err: OFF INTR 7
950   OUTPUT @Agte507x;":SYST:ERR?"
960   ENTER @Agte507x;Err_no,Err_msg$
970   PRINT "Error occurred!!"
980   PRINT "  No:"&Err_no,"Description: "&Err_msg$
990 Skip_error: OFF INTR 7
1000 SUBEND
1010  !=====
1020  ! File Transfer Function (Controller -> E507x)
1030  !=====
1040 SUB Copy_to_e507x(@Agte507x,Src_file$,Src_size_char$,Dst_file$)
1050 DIM Img$(32),Header$(10),Buff$(9),Err_msg$(100)
1060 INTEGER Max_bsize,Block_size,Err_no
1070 REAL Src_size
1080 !
1090 ON ERROR GOTO File_error
1100 ASSIGN @Src_file TO Src_file$
1110 OFF ERROR
1120 Max_bsize=24576 ! 24KByte
1130 !
1140 OUTPUT @Agte507x;"*CLS"
1150 OUTPUT @Agte507x;"*OPC?"
1160 ENTER @Agte507x;Buff$
1170 !
1180 PRINT "Now Copying: "&Src_file$&"(Controller) -> "&Dst_file$&"(E507x)"
1190 Header$="#"&VAL$(LEN(Src_size_char$))&Src_size_char$
1200 OUTPUT @Agte507x;":MMEM:TRAN ""&Dst_file$&""",&Header$;
1210 !
1220 Src_size=VAL(Src_size_char$)
1230 WHILE Src_size>0

```

```
1240     IF Src_size>Max_bsize THEN
1250         Block_size=Max_bsize
1260     ELSE
1270         Block_size=Src_size
1280     END IF
1290     !
1300     ALLOCATE Dat$[Block_size]
1310     Img$="#,&VAL$(Block_size)&"A"
1320     ENTER @Src_file USING Img$;Dat$
1330     OUTPUT @Agte507x USING Img$;Dat$
1340     DEALLOCATE Dat$
1350     !
1360     Src_size=Src_size-Block_size
1370 END WHILE
1380 !
1390 OUTPUT @Agte507x;"",END
1400 ASSIGN @Src_file TO *
1410 !
1420 OUTPUT @Agte507x;"::SYST:ERR?"
1430 ENTER @Agte507x;Err_no,Err_msg$
1440 IF Err_no=0 THEN
1450     PRINT "Done"
1460 ELSE
1470     PRINT "Error occurred!!"
1480     PRINT "  No:";Err_no,"Description: "&Err_msg$
1490 END IF
1500 GOTO Skip_error
1510 File_error:OFF ERROR
1520 PRINT "File name NOT found!"
1530 Skip_error:!
1540 SUBEND
```


Communication with External Instruments Using Handler I/O Port

This chapter provides necessary information for communicating with external instruments (for example, a handler in a production line) using the handler I/O port equipped with the Agilent E5061A/E5062A.

Handler I/O Port Overview


The E5061A/E5062A handler I/O port provides four independent parallel ports for data I/O associated with several control signal lines and the power line. All signals operate in TTL logic.

The data I/O ports are configured with 2 pairs of 8 bit output port and 2 pairs of 4 bit bi-directional port. Also those ports can cooperate to provide a maximum 16-bit-width output port or a maximum 8-bit-width input port.

The I/O signals operate on the negative logic basis. The control signal lines consist of various control output data, including completion of measurement or control signal for handshaking. Figure 10-1 outlines the I/O ports and control signal lines.

Figure 10-1

Handler I/O port overview

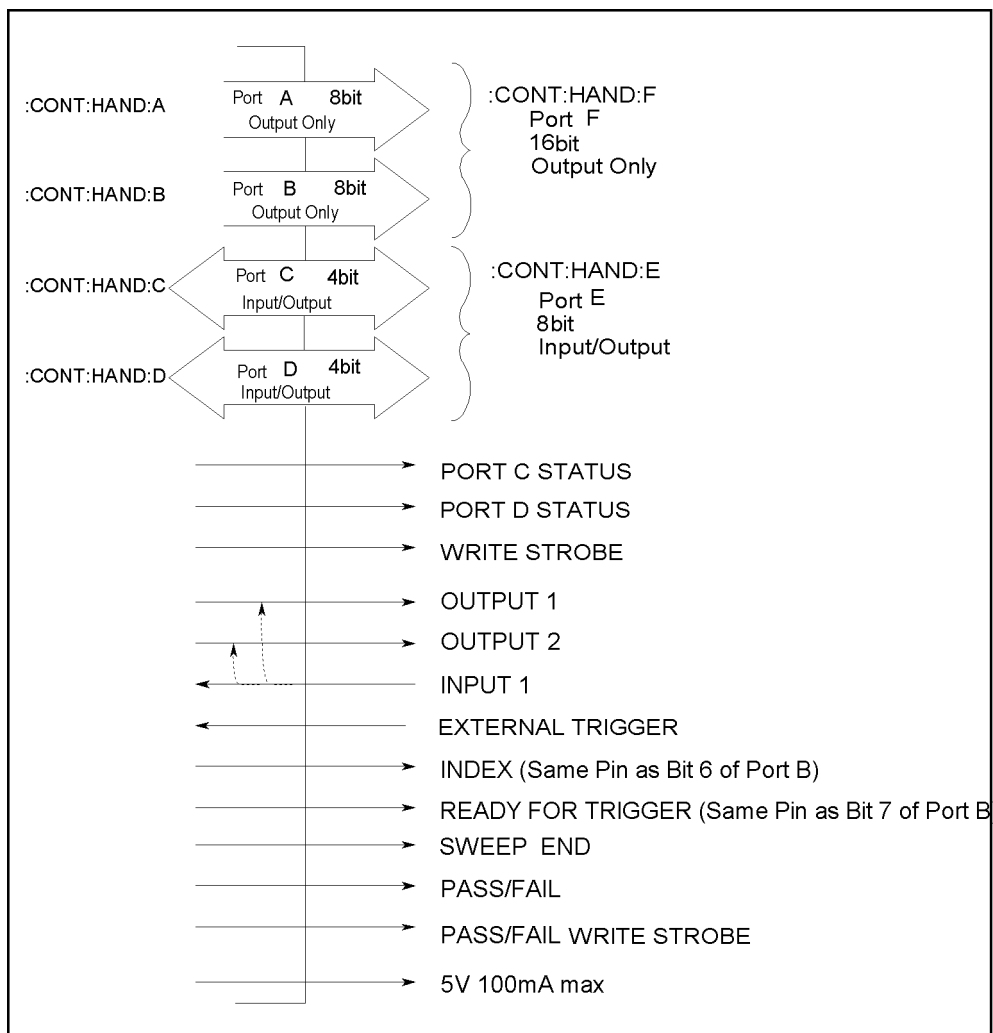


e5070ape001

I/O Signal Pin Layout and Description

Figure 10-2 illustrates the layout of the I/O signal pins on the handler interface connector while Table 10-1 on page 150 briefly describes those signals.

Figure 10-2

Handler interface connector pin layout

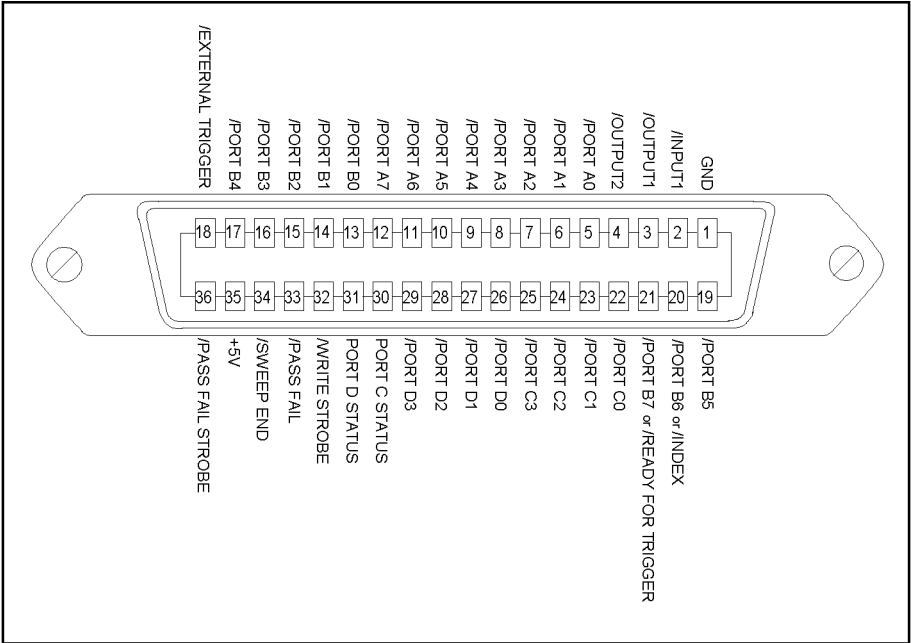

e5070ape002

NOTE

A slash (/) symbol preceding signal names means that they are negative logic (active low).

Table 10-1

Description of the handler interface I/O signals

Pin number	Signal name	Input/Output	Description
1	GND	—	Ground.
2	/INPUT1	Input	When this port receives a negative pulse, /OUTPUT1 and /OUTPUT2 are changed to the Low level.
3	/OUTPUT1	Output	Changes to the Low level when /INPUT1 receives a negative pulse. A command can be available for altering the Low/High level logic.
4	/OUTPUT2	Output	Changes to the Low level when /INPUT1 receives a negative pulse. A command can be available for altering the Low/High level logic.
5	/PORT A0	Output	Bit 0 of the port A (8 bit parallel output port)
6	/PORT A1	Output	Bit 1 of the port A.
7	/PORT A2	Output	Bit 2 of the port A.
8	/PORT A3	Output	Bit 3 of the port A.
9	/PORT A4	Output	Bit 4 of the port A.
10	/PORT A5	Output	Bit 5 of the port A.
11	/PORT A6	Output	Bit 6 of the port A.
12	/PORT A7	Output	Bit 7 of the port A.
13	/PORT B0	Output	Bit 0 of the port B (8 bit parallel output port)
14	/PORT B1	Output	Bit 1 of the port B.
15	/PORT B2	Output	Bit 2 of the port B.
16	/PORT B3	Output	Bit 3 of the port B.
17	/PORT B4	Output	Bit 4 of the port B.
18	/EXTERNAL TRIGGER	Input	An external trigger signal. When the trigger source is set to the “External,” this port generates a trigger in respond to the trailing edge of a negative pulse.
19	/PORT B5	Output	Bit 5 of the port B.
20* ¹	/PORT B6	Output	Bit 6 of the port B.
	/INDEX		Indicates that analog measurement is complete. The /INDEX signal changes to the Low level when analog measurement (all sweeps of all channels) is complete. When the handler receives the signal, it assumes that it is ready to connect the next DUT. However, no measurement data is available until data calculation completes.
21* ²	/PORT B7	Output	Bit 7 of the port B.
	/READY FOR TRIGGER		Indicates that the instrument is ready for triggering. This signal is changed to the Low level when the instrument is ready for receiving a trigger signal.

Table 10-1

Description of the handler interface I/O signals

Pin number	Signal name	Input/Output	Description
22	/PORT C0	Input/Output	Bit 0 of the port C (4 bit parallel I/O port)
23	/PORT C1	Input/Output	Bit 1 of the port C.
24	/PORT C2	Input/Output	Bit 2 of the port C.
25	/PORT C3	Input/Output	Bit 3 of the port C.
26	/PORT D0	Input/Output	Bit 0 of the port D (4 bit parallel I/O port)
27	/PORT D1	Input/Output	Bit 1 of the port D.
28	/PORT D2	Input/Output	Bit 2 of the port D.
29	/PORT D3	Input/Output	Bit 3 of the port D.
30	PORT C STATUS	Output	Port C status signal. This signal is changed to the High level when the port C is configured to output port. It is changed to the Low level when the port is configured to input port.
31	PORT D STATUS	Output	Port D status signal. This signal is changed to the High level when the port D is configured to output port. It is changed to the Low level when the port is configured to input port.
32	/WRITE STROBE	Output	A output port write strobe signal. When data is present (that is, output level changes) on any of the output ports, this signal provides a negative pulse.
33	/PASS FAIL	Output	A limit test result*3 signal. This signal changes to the High level when limit test, bandwidth test, or ripple test results return FAIL. It changes to the Low level when all limit test results return PASS.
34	/SWEEP END	Output	A sweep completion signal. When measurement (all sweeps of all channels) and data calculation are completed, this signal provides this signal provides a negative pulse.
35	+5V	Output	Provides +5V DC power supply for external instruments.
36	/PASS FAIL STROBE	Output	Limit test result write strobe signal. When limit test result is present on /PASS FAIL, this signal provides a negative pulse.

*1. This signal provides various functions depending upon the setting of
:CONT:HAND:IND:STAT command on page 302.

*2. This signal provides various functions depending upon the setting of
:CONT:HAND:RTR:STAT command on page 303.

*3. The overall test result that combine the test results for all traces in all channels.

Inputting/Outputting Data

The E5061A/E5062A handler I/O port provides the ports for data I/O shown in Table 10-2.

Table 10-2

I/O port

Port Name	Usage	Data Structure																
Port A	Output	<table><tr><td>A7</td><td>A6</td><td>A5</td><td>A4</td><td>A3</td><td>A2</td><td>A1</td><td>A0</td></tr></table> 8 bits	A7	A6	A5	A4	A3	A2	A1	A0								
A7	A6	A5	A4	A3	A2	A1	A0											
Port B	Output	<table><tr><td>B7</td><td>B6</td><td>B5</td><td>B4</td><td>B3</td><td>B2</td><td>B1</td><td>B0</td></tr></table> 8 bits	B7	B6	B5	B4	B3	B2	B1	B0								
B7	B6	B5	B4	B3	B2	B1	B0											
Port C	Input/Output	<table><tr><td>C3</td><td>C2</td><td>C1</td><td>C0</td></tr></table> 4 bits	C3	C2	C1	C0												
C3	C2	C1	C0															
Port D	Input/Output	<table><tr><td>D3</td><td>D2</td><td>D1</td><td>D0</td></tr></table> 4 bits	D3	D2	D1	D0												
D3	D2	D1	D0															
Port E	Input/Output	<table><tr><td>D3</td><td>D2</td><td>D1</td><td>D0</td><td>C3</td><td>C2</td><td>C1</td><td>C0</td></tr></table> 8 bits	D3	D2	D1	D0	C3	C2	C1	C0								
D3	D2	D1	D0	C3	C2	C1	C0											
Port F	Output	<table><tr><td>B7</td><td>B6</td><td>B5</td><td>B4</td><td>B3</td><td>B2</td><td>B1</td><td>B0</td><td>A7</td><td>A6</td><td>A5</td><td>A4</td><td>A3</td><td>A2</td><td>A1</td><td>A0</td></tr></table> 16 bits	B7	B6	B5	B4	B3	B2	B1	B0	A7	A6	A5	A4	A3	A2	A1	A0
B7	B6	B5	B4	B3	B2	B1	B0	A7	A6	A5	A4	A3	A2	A1	A0			

Specifying signal direction of port

Signal direction (input/output) can be changed for the ports C, D, and D as shown in Table 10-2. Thus, before the ports are used, the directions should be determined according to their usage.

To specify the signal direction for the ports C and D, use the following command.Direction for the port E depends on the setting for the ports C and D.

Port Name	Command
Port C	:CONT:HAND:C:MODE on page 297
Port D	:CONT:HAND:D:MODE on page 299

Reading data input to port

When the ports C, D, or E is configured to input ports, binary data represented with High(0)/Low(1) of each bit of the port will be read as decimal data.

To retrieve the data, use the following command as query:

Port Name	Command
Port C	:CONT:HAND:C on page 296
Port D	:CONT:HAND:D on page 298
Port E	:CONT:HAND:E on page 300

Data output to port

To the ports A through F (the ports C, D, and E should be configured to output ports), binary data (decimal data when output data is specified with a command) represented with High(0)/Low(1) of each bit of the port can be output.

To output data, use the following command.

Port Name	Command
Port A	:CONT:HAND:A on page 295
Port B	:CONT:HAND:B on page 295
Port C	:CONT:HAND:C on page 296
Port D	:CONT:HAND:D on page 298
Port E	:CONT:HAND:E on page 300
Port F	:CONT:HAND:F on page 301

NOTE

The bit 6 of the data outputted by :CONT:HAND:B command (the bit 14 of the data outputted by :CONT:HAND:F command) is ignored when outputting the /INDEX signal is turned on.

The bit 7 of the data outputted by :CONT:HAND:B command (the bit 15 of the data outputted by :CONT:HAND:F command) is ignored when outputting the /READY FOR TRIGGER signal is turned on.

Preset states at power-on

The handler I/O port is set at power-on as follows (not affected at reset).

Port A	High (All Bits)
Port B	High (All Bits)
Port C	Input
Port D	Input
PORT C STATUS	Low
PORT D STATUS	Low
/OUTPUT1	High
/OUTPUT2	High
/SWEEP END	High
/PASS FAIL	High

Timing Chart

Figure 10-3 shows a timing chart for each timing signal output covering from the start of measurement (pulse input to /EXTERNAL TRIGGER) until the end of measurement.

Table 10-3


Values of T1 through T2 in Figure 10-3 (typical)

		Minimum value	Typical Value	Maximum value
T1	Pulse width of /EXTERNAL TRIGGER	1 μ s*1	—	—
T2	Pulse width of /SWEEP END	10 μ s	12 μ s	—

*1. When a trigger signal is input from the handler I/O port.

Figure 10-3

Timing chart of /EXTERNAL TRIGGER, /INDEX, /SWEEP END and /READY FOR TRIGGER

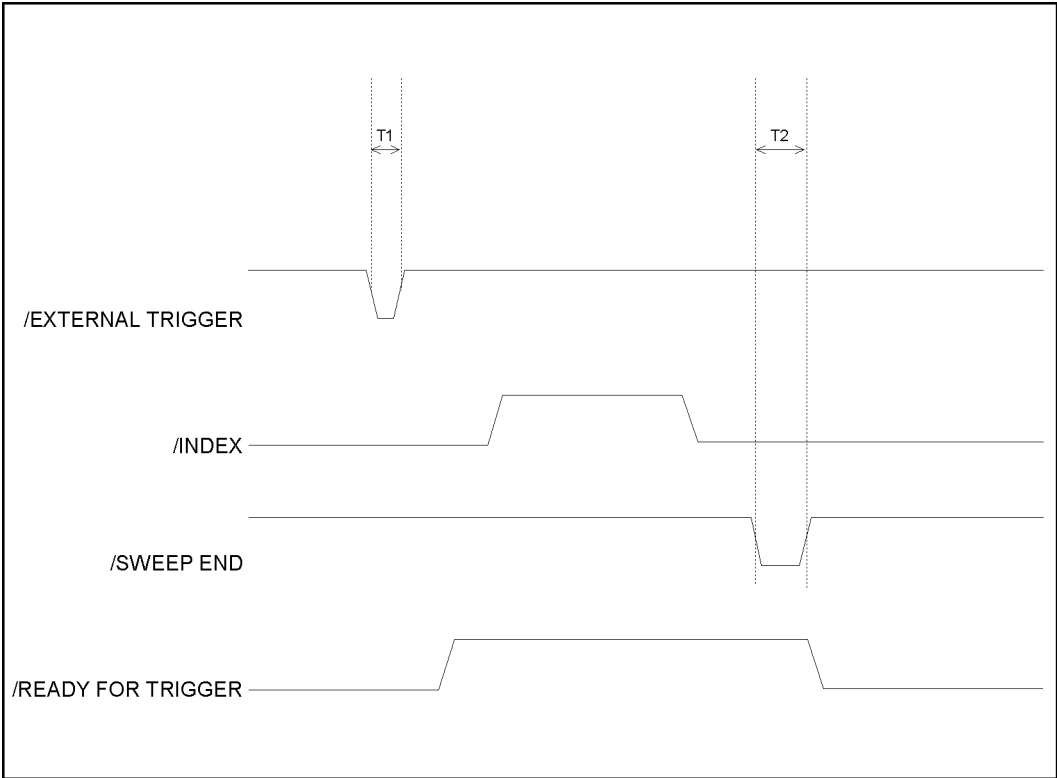

e5070apj009

/INDEX and /READY FOR TRIGGER signals are outputted when outputting of these signals are turned on using the following commands.

/INDEX	:CONT:HAND:IND:STAT on page 302
/READY FOR TRIGGER	:CONT:HAND:RTR:STAT on page 303

Figure 10-4 shows the timing chart for data output and write strobe signal output to the ports A through F.

Table 10-4 Values of T1 through T2 in Figure 10-4 (typical)

T1	Response time of write strobe signal	1 μ s
T2	Pulse width of write strobe signal	1 μ s

Figure 10-4 Timing chart of data output and write strobe signal

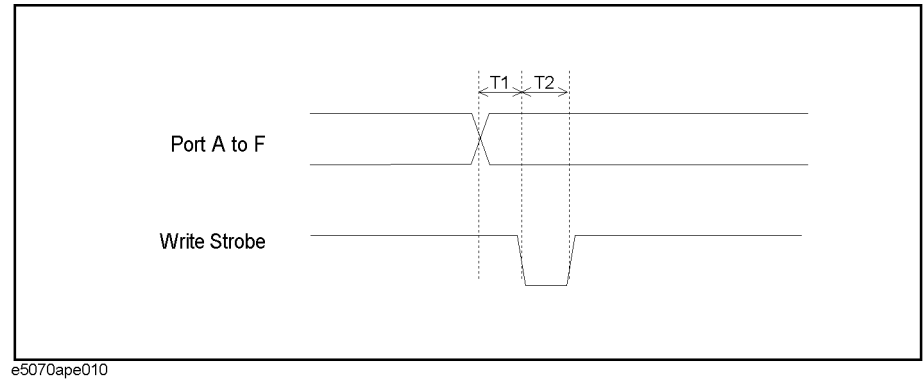


Figure 10-5 shows a timing chart of limit test result output (/PASS FAIL signal output) and /PASS FAIL write strobe signal output.

Timing chart of limit test result contains ripple test and bandwidth test.

Table 10-5 Values of T1 through T2 in Figure 10-5 (typical)

T1	Response time of /PASS FAIL write strobe	1 μ s
T2	Pulse width of /PASS FAIL write strobe	1 μ s

Figure 10-5 Timing chart of limit test result output and write strobe signal

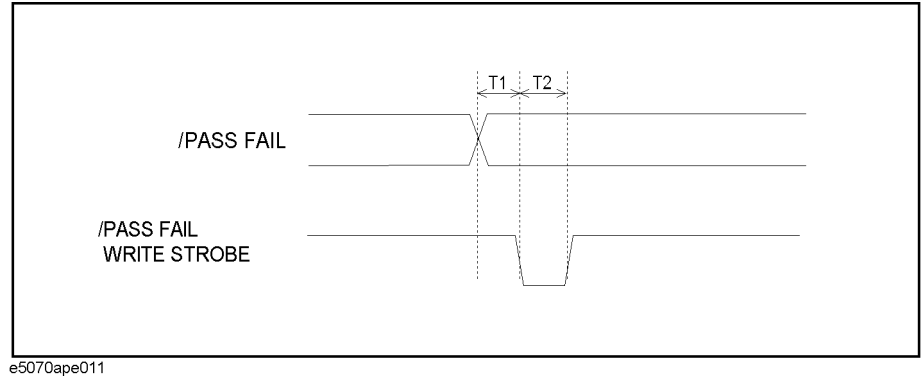


Figure 10-6 shows a timing chart of a pulse input to INPUT1, /OUTPUT1 signal output, and /OUTPUT2 signal output.


Table 10-6

Values of T1 through T2 in Figure 10-6 (typical)

		Minimum value	Maximum value
T1	Pulse width of /INPUT1	1 μ s	—
T2	Response time of /OUTPUT1, /OUTPUT2	0.4 μ s	0.6 μ s

Figure 10-6

Timing chart of /INPUT1 and /OUTPUT1, /OUTPUT2

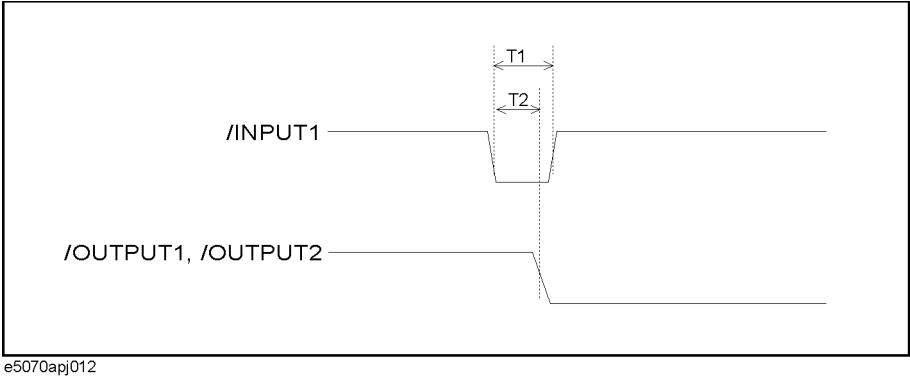

Electrical Characteristics

Input signal

All input signals are TTL compatible. Table 10-7 shows the electrical characteristics of input signals. Figure 10-7 shows the circuit diagram of input signals.


Table 10-7

Electrical characteristics of input signals (typical)

Maximum rate input voltage		-0.5 V to 5.5 V
Input voltage	High level	2.0 V to 5.0 V
	Low level	0 V to 0.5 V

Figure 10-7

Circuit diagram or input signals

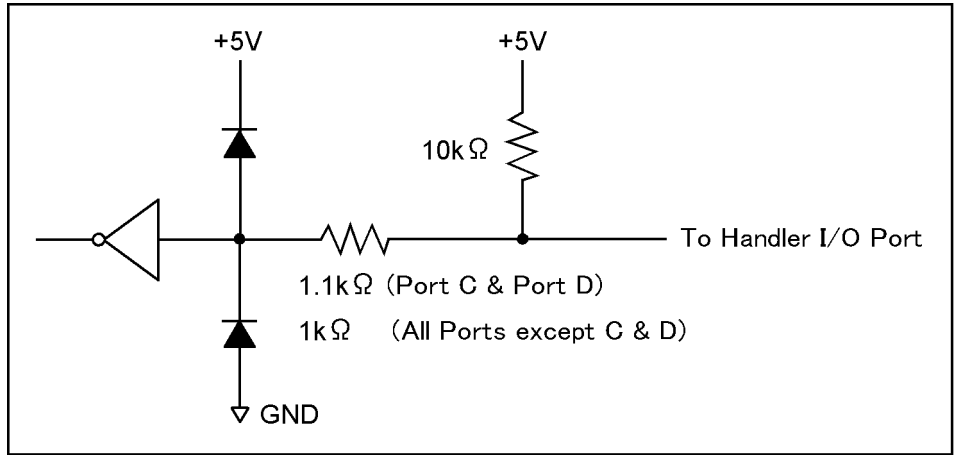

e5070ape027

Output signal

All output signals are TTL compatible. Table 10-8 shows the electrical characteristics of output signals. Figure 10-8 shows the circuit diagram of output signals.

Table 10-8


Electrical characteristics of output signals (typical)

Maximum rate output current		-10 mA to 10 mA
Output current	High level	-5 mA
	Low level	3 mA
Output voltage	High level	2.0 V to 3.3 V (when output current is from -5 mA to 0 mA) 3.20 V (when output current is -1 mA) 2.75 V (when output current is -5 mA)
	Low level	0 V to 0.8 V (when output current is from 0 mA to 3 mA) 0.25 V*1 (when output current is 1 mA) 0.55 V (when output current is 3 mA)

*1. Notice that, in case of C0 to C3 (port C) and D0 to D3 (port D), output voltage is 0.30 V.

Figure 10-8

Circuit diagram of output signals

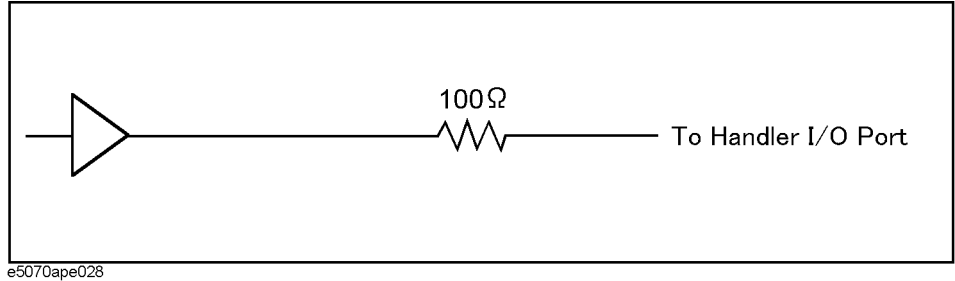

Power supply (+5 V)

Table 10-9 shows electrical characteristics of +5 V power supply for external instruments.

Table 10-9

Electrical characteristics of +5 V power supply (typical)

Output voltage	4.5 V to 5.5 V
Maximum output current	100 mA

Sample Program

Example 10-1 provides a sample program that communicates with an external instrument through the handler I/O port. You can find the source file of this program, named `handler.htb`, on the sample program disk.

This program outputs 5 (sets bit 2 and bit 0 to Low, and the other bits to High) to the port A of the handler I/O port, then waits until the bit 3 of the port C is set to Low.

The program is described in detail below:

Line 40	Assigns a GPIB address to the I/O pass.
Lines 60 to 70	These lines store the output data on the port A (binary) and bit location (bit 3) into <code>Out_data_bin\$</code> and <code>Flag_bit</code> variables, respectively.
Line 90	This line configures the port C to input port.
Lines 100 to 110	These lines enable <code>/INDEX</code> and <code>/READY FOR TRIGGER</code> signals.
Lines 130 to 140	These lines convert <code>Out_data_bin\$</code> to a decimal value and set it to the port A.
Lines 160 to 200	These lines repeat reading data from the port C until <code>Flag_bit</code> becomes TRUE.

Example 10-1

Communicating with external instruments (`handler.htb`)

```
10  INTEGER Out_data, In_data, Bit_stat
20  DIM Out_data_bin$(9)
30  !
40  ASSIGN @Agte507x TO 717
50  !
60  Out_data_bin$="00000101"
70  Flag_bit=3
80  !
90  OUTPUT @Agte507x;":CONT:HAND:C:MODE INP"
100 OUTPUT @Agte507x;":CONT:HAND:IND:STAT ON"
110 OUTPUT @Agte507x;":CONT:HAND:RTR:STAT ON"
120 !
130 Out_data=IVAL(Out_data_bin$,2)
140 OUTPUT @Agte507x;":CONT:HAND:A ";Out_data
150 !
160 REPEAT
170     OUTPUT @Agte507x;":CONT:HAND:C?"
180     ENTER @Agte507x;In_data
190     Bit_stat=BIT(In_data,Flag_bit)
200 UNTIL Bit_stat=1
210 END
```

11 Working with Automatic Test Systems

This chapter describes useful features when the Agilent E5061A/E5062A is integrated with the automatic test system.

Preventing Erroneous Key Operation on the Front Panel (Key Lock Feature)

When no operation is required from the front panel controls, the mouse, or the keyboard, disabling those input devices can prevent from any erroneous operation, which might be caused by accidentally touching such devices.

To turn on or off Key Locking, use the following command:

Locking the front panel controls and the keyboard.	:SYST:KLOC:KBD on page 477
Locking the mouse and the touch screen.	:SYST:KLOC:MOUS on page 478

Improving Command Processing Speed

SCPI commands should be processed in shorter time to improve throughput, when those commands are frequently executed (for example, reading out trace for each measurement).

With E5061A/E5062A, processing time for SCPI commands can be improved by decreasing refresh rate of the LCD display.

Measurement results (trace) need not to be updated

When the measurement trace needs not to be updated, turn off the update of the LCD display. This improves processing speed of SCPI commands and eliminates updating time of the screen.

To turn off the update of the LCD display, use the following command:

- :DISP:ENAB command on page 312

Measurement results (trace) need to be updated

When the measurement trace needs to be updated, processing speed of SCPI commands can be improved by controlling the update timing of the LCD display:

- Step 1.** Execute all SCPI commands that are required before measurement, including commands setting conditions.
- Step 2.** Turning Off the update of the LCD display.
- Step 3.** Perform the measurement.
- Step 4.** Execute the commands for reading out measurement result or analyzing the result. Note that reading out the result in binary format will accelerate data transfer.
- Step 5.** Execute the following command to update the LCD display once.
 - :DISP:UPD command on page 318
- Step 6.** Return to the step 3.

Sample program

Example 11-2 shows a sample program where the command processing time are improved by controlling the update timing of the LCD display. You can find the source file of this program, named `cont_upd.hrb`, on the sample program disk.

NOTE

This sample program correctly runs when the maximum number of channels/traces is set 9 channels/9 traces.

This program sets necessary measurement conditions then turn off the update of the LCD display. Next, it performs measurement, reads out the result, and update the screen once. This program repeats this measurement procedure ten times.

The program is described in detail below:

Lines 50 to 60	Assigns a GPIB address to the I/O pass.
Lines 80 to 110	These lines set the sweep type to linear sweep, the sweep center value to 950 MHz, the sweep span value to 100 MHz, and the number of measurement points to 201, respectively.
Lines 120 to 160	These lines set the trigger source to bus trigger, turn on Continuous Activation mode for channel 1, turn the mode off for channels 2 through 4.
Lines 180 to 190	These lines display the window for channel 1 only, and arrange two graphs tiled horizontally.
Lines 210 to 270	These lines set the number of traces for channel 1 to 2, the measurement parameter and its data format for trace 1 to S21 and Log Mag, and those for trace 2 to S11 and Log Mag, respectively.
Line 290	This line turns Off the update of the LCD screen.
Line 300	This line sets the data transfer format to binary.
Lines 320 to 540	These lines repeat the following procedure ten times. 1. Lines 330 to 350 These lines trigger the instrument, and waits until the measurement cycle finishes. 2. Lines 390 to 430: Reads out the formatted data array of trace 1 in channel 1. 3. Lines 450 to 490: Reads out the formatted data array of trace 2 channel 1. 4. Line 530 This line updates the LCD screen once.

Example 11-1

Controlling the update timing of LCD display(cont_upd.htb)

```

10     REAL Trace1(1:201,1:2),Trace2(1:201,1:2)
20     DIM Buff$[9],Img$[30]
30     INTEGER Nop,I
40     !
50     ASSIGN @Agte507x TO 717
60     ASSIGN @Binary TO 717;FORMAT OFF
70     !
80     OUTPUT @Agte507x;":SENS1:SWE:TYPE LIN"
90     OUTPUT @Agte507x;":SENS1:FREQ:CENT 950E6"
100    OUTPUT @Agte507x;":SENS1:FREQ:SPAN 100E6"
110    OUTPUT @Agte507x;":SENS1:SWE:POIN 201"
120    OUTPUT @Agte507x;":TRIG:SOUR BUS"
130    OUTPUT @Agte507x;":INIT1:CONT ON"
140    FOR I=2 TO 4
150        OUTPUT @Agte507x;":INIT"&VAL$(I)&":CONT OFF"
160    NEXT I
170    !
180    OUTPUT @Agte507x;":DISP:SPL D1"
190    OUTPUT @Agte507x;":DISP:WIND1:SPL D1_2"
200    !
210    OUTPUT @Agte507x;":CALC1:PAR:COUN 2"
220    OUTPUT @Agte507x;":CALC1:PAR1:DEF S21"
230    OUTPUT @Agte507x;":CALC1:PAR1:SEL "
240    OUTPUT @Agte507x;":CALC1:FORM MLOG"
250    OUTPUT @Agte507x;":CALC1:PAR2:DEF S11"
260    OUTPUT @Agte507x;":CALC1:PAR2:SEL "
270    OUTPUT @Agte507x;":CALC1:FORM MLOG"
280    !
290    OUTPUT @Agte507x;":DISP:ENAB OFF"
300    OUTPUT @Agte507x;":FORM:DATA REAL"
310    !
320    FOR I=1 TO 10
330        OUTPUT @Agte507x;":TRIG:SING"
340        OUTPUT @Agte507x;":*OPC?"
350        ENTER @Agte507x;Buff$
360        !
370        ! Read Trace Data
380        !
390        OUTPUT @Agte507x;":CALC1:PAR1:SEL "
400        OUTPUT @Agte507x;":CALC1:DATA:FDAT?"
410        ENTER @Agte507x USING "#,8A";Buff$
420        ENTER @Binary;Trace1(*)
430        ENTER @Agte507x USING "#,1A";Buff$
440        !
450        OUTPUT @Agte507x;":CALC1:PAR2:SEL "
460        OUTPUT @Agte507x;":CALC1:DATA:FDAT?"
470        ENTER @Agte507x USING "#,8A";Buff$
480        ENTER @Binary;Trace2(*)
490        ENTER @Agte507x USING "#,1A";Buff$
500        !
510        ! Update Display
520        !
530        OUTPUT @Agte507x;":DISP:UPD"
540    NEXT I
550    END

```

Detecting Occurrence of an Error

Using the status reporting system

The status of the E5061A/E5062A can be detected through the status registers. This section describes how to detect the end of measurement using the status registers. For the complete description of the status report mechanism, including the specifications of each bit, see Appendix B, “Status Reporting System.”

Occurrence of an error will be present in the standard event status register. An SRQ (service request) is useful when you create a program that uses the information reported by this register to detect occurrence of an error.

To detect the end of sweep via an SRQ, use one of the following commands:


- *SRE on page 200
- *ESE on page 197

Follow these steps:

- Step 1.** Set the E5061A/E5062A so that it generates an SRQ when any of the error occurrence bit is set to 1 in the standard event status register.
- Step 2.** When an SRQ is generated, the program interrupts the measurement cycle.

Figure 11-1

SRQ generation sequence (when an error occurs)

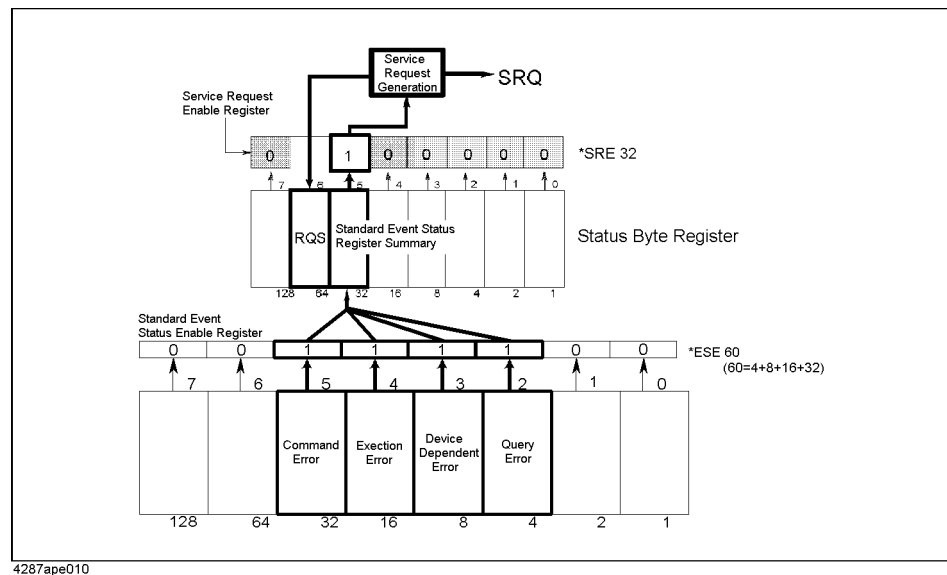

Using the error queue

An error queue holds the number for the error and the error message. Reading the error queue allows the user to verify the error that has been occurred. To retrieve the content of error queue, use the following command:

- :SYST:ERR? on page 476

The error queue can be used in the following ways:

1. It is used as a branch for error handling. When an error queue is retrieved, it returns 0 as the error number and “No error” as the error message if no errors detected. This can be used for detecting of an error and for branching flow of a program. Also this is useful when you wish to handle a specific error(s). Note that this method will not allow the user to perform any processing in synchronization with an occurrence of an error.
2. When an error is detected using SRQ, the error queue is used to examine the error. Refer to the example in Example 11-2.

Sample program

Example 11-2 is a sample program that demonstrates how to use an SRQ to detect occurrence of an error. You can find the source file of this program, named `srq_err.hb`, on the sample program disk.

This program sets SRQs then incidentally send an invalid parameter to generate an error, which is handled by this program. In the error handling part, this program examines the error, displays the error number and error message, and display the message indicating the suspend of the program.

Line 40	Assigns a GPIB address to the I/O pass.
Lines 60 to 70	These lines enables the bit 2, 3 4 and 5 in the standard event status register, and set the bit 5 to 1 in the service request enable register.
Lines 80 to 100	These lines clear the status byte register, the standard event status register, and the error queue.
Lines 120 to 130	These lines set the branch target for an SRQ interrupt to enable SRQ interrupts.
Lines 140 to 260	These lines set the measurement parameters and their data formats for trace 1 and 2. An invalid parameter is given to the data format setting for trace 2, causing an error.
Lines 280 to 330	These lines define an error handler that Lines 290 to 300: These lines retrieve the error number and error messages for the error from the error queue. Lines 310 to 330 These lines displays the message indicating occurrence of the error, the error number, the error message, and the message showing that the program is suspend.
Line 350	Displays a closing message. Note that this message will not display unless this program is re-executed after setting a corrected parameter to the data format setting for trace 2.

Example 11-2

Error detection using an SRQ (srq_err.bas)

```
10    DIM Buff$(9),Err_mes$(50)
20    INTEGER Err_no
30    !
40    ASSIGN @Agte507x TO 717
50    !
60    OUTPUT @Agte507x;"*ESE 60"
70    OUTPUT @Agte507x;"*SRE 32"
80    OUTPUT @Agte507x;"*CLS"
90    OUTPUT @Agte507x;"*OPC?"
100   ENTER @Agte507x;Buff$
110   !
120   ON INTR 7 GOTO Err_proc
130   ENABLE INTR 7;2
140   OUTPUT @Agte507x;":CALC1:PAR:COUN 2"
150   PRINT "Trace 1 Meas.Para: S21"
160   PRINT "Trace 1 Format   : Log Mag"
170   OUTPUT @Agte507x;":CALC1:PAR1:DEF S21"
180   OUTPUT @Agte507x;":CALC1:PAR1:SEL"
190   OUTPUT @Agte507x;":CALC1:FORM MLOG"
200   PRINT "Trace 2 Meas.Para: S11"
210   PRINT "Trace 2 Format   : Log Mag"
220   OUTPUT @Agte507x;":CALC1:PAR2:DEF S11"
230   OUTPUT @Agte507x;":CALC1:PAR2:SEL"
240   OUTPUT @Agte507x;":CALC1:FORM LOG"
250   OUTPUT @Agte507x;"*OPC?"
260   ENTER @Agte507x;Buff$
270   GOTO Skip_err_proc
280 Err_proc: OFF INTR 7
290   OUTPUT @Agte507x;";:SYST:ERR?"
300   ENTER @Agte507x;Err_no,Err_mes$
310   PRINT "Error occurred!!"
320   PRINT "  No: ";Err_no,"Description: "&Err_mes$
330   PRINT "PROGRAM INTERRUPT!!"
340   GOTO Prog_end
350 Skip_err_proc: PRINT "PROGRAM DONE."
360 Prog_end: END
```

12

Sample Application Programs

This chapter introduces several sample programs for basic measurement, measurement with a system using the handler I/O, and controlling the instrument over LAN.

Basic measurement (measuring a band pass filter)

Example 12-1 provides a sample program that measures a band pass filter. You can find the source file of this program, named `meas_bpf.htb`, on the sample program disk.

The sample program performs full 2-port calibration using the 85032F calibration kit, measure a band-pass filter (center frequency: 947.5 MHz), and calculates and displays its bandwidth, insertion loss, and so on. This measurement is the same as “Measuring a band pass filter” in *Installation and Quick Start Guide* of the E5061A/E5062A.

Therefore, for information on the flow of the measurement, the connection of the standard, and so on, refer to the description of *Installation and Quick Start Guide*.

When started, the program displays the message “Set OPEN to Port 1. Then push [Enter] key.” Connect the OPEN standard to the port 1 and press **[Enter]** to measure the OPEN calibration data. Likewise, connect the SHORT and the LOAD standards and measure each calibration data.

Next, the program displays the message “Set OPEN to Port 2. Then push [Enter] key.” Connect the OPEN standard to the port 2 and press **[Enter]** to measure the OPEN calibration data. Likewise, connect the SHORT and the LOAD standards and measure each calibration data.

Further, the program displays the message “Set THRU between Port 1 and Port 2. Then push [Enter] key.” Connect the THRU standard between the ports 1 and 2 and press **[Enter]** to measure the THRU calibration data.

When the calibration is finished, the program displays the message “Set DUT. Then Push [Enter] key.” Connect the DUT and press **[Enter]**. This initiates the measurement and display the result as shown in Figure 12-1.

Figure 12-2 shows a sample display of the LCD screen after the program exits execution.

Figure 12-1

Sample execution result of the program of Example 12-1

```
## Measurement Result ##
  BW:      3.63757249908E+7
 cent:     9.4836227902E+8
  low:     9.30174417035E+8
 high:     9.66550142015E+8
   Q:      26.0712980976
 loss:     -2.2447956671
```

Figure 12-2

Sample display of the screen after the program Example 12-1 exits execution



The program is described in detail below:

- Line 50 Assigns a GPIB address to the I/O pass.
- Lines 70 to 110 Store the sweep center value (947.5 MHz), the sweep span value (200 MHz), the number of measurement points (401), the IF bandwidth (10 kHz), the power level (-10 dBm) into the variables Center, Span, Nop, If_Bw, and Pow, respectively.
- Lines 120 to 160 Stores the number of traces (1), the measurement parameter (S21), the data format (log Mag), the calibration kit number (4: 85032F), and the save file name (State08.sta) into the variables, Num_of_tr, Para\$, Fmt\$, CalKit, and File\$, respectively.
- Line 200 Puts the instrument into preset state.
- Lines 220 to 260 These lines assign the sweep center value for channel 1 to Center, sweep span value to Span, number of measurement points to Nop, IF bandwidth to If_bw, and power level to Pow, respectively.
- Lines 280 to 310 These lines assign the number of trace for channel 1 to Num_of_tr, measurement parameters to Para\$, and data format to Fmt\$, respectively.
- Line 350 Stores the calibration kit number for channel 1 to the CalKit variable.
- Lines 360 to 380 These lines specifies ports 1 and 2 to be used and calls the sub program Cal_solt to perform full 2-port calibration for channel 1. For more information on the Cal_solt subprogram, refer to the description in Example 4-1 on page 71.
- Lines 420 to 430 Saves the settings of the E5061A/E5062A and the calibration coefficients under the file name File\$.
- Lines 480 to 490 These lines set the trigger source to the bus trigger and turns on the continuous initiation mode for channel 1.

Lines 510 to 520	These lines prompt the user to connect the DUT and wait for [Enter] to be pressed after the DUT is connected.
Lines 540 to 560	These lines trigger the instrument, and waits until the measurement cycle finishes.
Line 580	This line executes auto scale for the trace 1 of channel 1.
Lines 620 to 650	These lines turn on the display of marker 1, move the marker to the position where the stimulus value is equal to Center, read out the response value at the marker and assign the value to the Resp variable.
Lines 670 to 710	These lines configure the system to generate an SRQ when it cannot perform Bandwidth Search due to an error.
Lines 730 to 740	These lines set the branch target for an SRQ interrupt to enable SRQ interrupts.
Lines 750 to 790	Sets the bandwidth definition value to -3 dB and the bandwidth search result display to on, reads out the bandwidth search results (bandwidth, center frequency, Q value, and insertion loss), and stores them into the variables Bwid, Cent, Q, and Loss, respectively.
Lines 830 to 900	These lines define an error handler that retrieves the error number and error messages for the error, then assign 0 to Bwid, Cent and Q, Resp (response value at marker 1) to Loss.
Lines 930 to 940	These lines calculate the 2 (higher and lower) cutoff frequencies from the values in the Bw and Cent variables and stores them into the Cut_l and Cut_h variables.
Lines 980 to 1040	These lines display the measurement results (values of Bwid, Cent, Q, Loss, Cut_l, and Cut_h).
Lines 1060 to 1070	These lines prompt the user to decide to perform another measurement. When [y] is pressed followed by [Enter] key, the program will return to the part where the DUT is connected and continue measurement.

Example 12-1

Measurement of band pass filter (meas_bpf.htb)

```

10    DIM Para$[9],Fmt$[9],File$[20],Buff$[9],Inp_char$[9],Err_msg$[20]
20    REAL  Center,Span,If_bw,Pow,Resp,Bwid,Cent,Q,Loss,Cut_l,Cut_h
30    INTEGER Nop,Num_of_tr,Cal_kit,Port(1:4),Err_no
40    !
50    ASSIGN @Agte507x TO 717
60    !
70    Center=9.475E+8      ! Center Freq.      : 947.5 MHz
80    Span=2.00E+8        ! Span            : 200 MHz
90    Nop=401             ! Number of Points : 401
100   If_bw=1.0E+4        ! IF Bandwidth   : 10 kHz
110   Pow=-10             ! Power Level    : -10 dBm
120   Num_of_tr=1         ! Number of Traces : 1
130   Para$="S21"         ! Meas. Parameter : S21
140   Fmt$="MLOG"         ! Data Format     : Log Mag
150   Cal_kit=4           ! Calibration Kit  : 85032F
160   File$="State08.sta" ! Save File Name  : State08.sta
170   !
180   ! Measurement Condition
190   !
200   OUTPUT @Agte507x;":SYST:PRES"
210   !
220   OUTPUT @Agte507x;":SENS1:FREQ:CENT ";Center
230   OUTPUT @Agte507x;":SENS1:FREQ:SPAN ";Span
240   OUTPUT @Agte507x;":SENS1:SWE:POIN ";Nop
250   OUTPUT @Agte507x;":SENS1:BAND ";If_bw
260   OUTPUT @Agte507x;":SOUR1:POW ";Pow
270   !
280   OUTPUT @Agte507x;":CALC1:PAR:COUN ";Num_of_tr
290   OUTPUT @Agte507x;":CALC1:PAR1:DEF "&Para$
300   OUTPUT @Agte507x;":CALC1:PAR1:SEL"
310   OUTPUT @Agte507x;":CALC1:FORM "&Fmt$
320   !
330   ! Full 2 Port Calibration (@ Port 1 & Port 2)
340   !
350   OUTPUT @Agte507x;":SENS1:CORR:COLL:CKIT ";Cal_kit
360   Port(1)=1
370   Port(2)=2
380   Cal_solt(@Agte507x,"1",2,Port(*))
390   !
400   ! Save State & Cal
410   !
420   OUTPUT @Agte507x;":MMEM:STOR:STYP CST"
430   OUTPUT @Agte507x;":MMEM:STOR """"&File$&""""
440   !
450   ! Measurement
460   !
470   CLEAR SCREEN
480   OUTPUT @Agte507x;":TRIG:SOUR BUS"
490   OUTPUT @Agte507x;":INIT1:CONT ON"
500   Meas_start:!
510   PRINT "Set DUT, then Push [Enter] key"
520   INPUT "",Inp_char$
530   !
540   OUTPUT @Agte507x;":TRIG:SING"
550   OUTPUT @Agte507x;":*OPC?"
560   ENTER @Agte507x;Buff$
570   !
580   OUTPUT @Agte507x;":DISP:WIND1:TRAC1:Y:AUTO"
590   !
600   ! Analysis
610   !

```

```

620  OUTPUT @Agte507x;":CALC1:MARK1 ON"
630  OUTPUT @Agte507x;":CALC1:MARK1:X ";Center
640  OUTPUT @Agte507x;":CALC1:MARK1:Y?"
650  ENTER @Agte507x;Resp
660  !
670  OUTPUT @Agte507x;"*ESE 60"
680  OUTPUT @Agte507x;"*SRE 32"
690  OUTPUT @Agte507x;"*CLS"
700  OUTPUT @Agte507x;"*OPC?"
710  ENTER @Agte507x;Buff$
720  !
730  ON INTR 7 GOTO Bw_err
740  ENABLE INTR 7;2
750  OUTPUT @Agte507x;":CALC1:MARK1:BWID:THR -3"
760  OUTPUT @Agte507x;":CALC1:MARK1:BWID ON"
770  OUTPUT @Agte507x;":CALC1:MARK1:BWID:DATA?"
780  WAIT .5
790  ENTER @Agte507x;Bwid,Cent,Q, Loss
800  GOTO Skip_bw_err
810  !
820 Bw_err: OFF INTR 7
830  OUTPUT @Agte507x;":SYST:ERR?"
840  ENTER @Agte507x;Err_no,Err_msg$
850  PRINT "Error occurred!!"
860  PRINT " No: ";Err_no,"Description: "&Err_msg$
870  Bwid=0
880  Cent=0
890  Q=0
900  Loss=Resp
910  !
920 Skip_bw_err: OFF INTR 7
930  Cut_l=Cent-(Bwid/2)
940  Cut_h=Cent+(Bwid/2)
950  !
960  ! Display
970  !
980  PRINT "## Measurement Result ##"
990  PRINT " BW:",Bwid
1000 PRINT " cent:",Cent
1010 PRINT " low:",Cut_l
1020 PRINT " high:",Cut_h
1030 PRINT " Q:",Q
1040 PRINT " loss:",Loss
1050 !
1060 INPUT "Once more? [Y]es/[N]o",Inp_char$
1070 IF UPC$(Inp_char$)="Y" OR UPC$(Inp_char$)="YES" THEN Meas_start
1080 !
1090 END
1100 !=====
1110 ! Full n Port Calibration Function
1120 !=====
1130 SUB Cal_solt(@Agte507x,Ch$,INTEGER Num_of_ports,INTEGER Port(*))
1140 DIM Buff$[9]
1150 INTEGER I,J
1160 !
1170 PRINT "## Full "&VAL$(Num_of_ports)&" Port Calibration ##"
1180 !
1190 ! Calibration Type Selection
1200 !
1210 OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:METH:SOLT"&VAL$(Num_of_
ports)&" ";
1220 FOR I=1 TO Num_of_ports-1
1230 OUTPUT @Agte507x;Port(I);", ";
1240 NEXT I

```

```

1250  OUTPUT @Agte507x;Port(Num_of_ports)
1260  !
1270  ! Reflection Measurement
1280  !
1290  FOR I=1 TO Num_of_ports
1300    PRINT "Set OPEN to Port "&VAL$(Port(I))&". Then push [Enter]
key."
1310      INPUT "",Buff$
1320      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:OPEN ";Port(I)
1330      OUTPUT @Agte507x;"*OPC?"
1340      ENTER @Agte507x;Buff$
1350      PRINT "Set SHORT to Port "&VAL$(Port(I))&". Then push [Enter]
key."
1360      INPUT "",Buff$
1370      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:SHOR ";Port(I)
1380      OUTPUT @Agte507x;"*OPC?"
1390      ENTER @Agte507x;Buff$
1400      PRINT "Set LOAD to Port "&VAL$(Port(I))&". Then push [Enter]
key."
1410      INPUT "",Buff$
1420      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:LOAD ";Port(I)
1430      OUTPUT @Agte507x;"*OPC?"
1440      ENTER @Agte507x;Buff$
1450  NEXT I
1460  !
1470  ! Transmission Measurement
1480  !
1490  FOR I=1 TO Num_of_ports-1
1500    FOR J=I+1 TO Num_of_ports
1510      PRINT "Set THRU between Port "&VAL$(Port(I))&" and Port "&
VAL$(Port(J))&". Then push [Enter] key."
1520      INPUT "",Buff$
1530      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:THRU ";Port(I);", "
;Port(J)
1540      OUTPUT @Agte507x;"*OPC?"
1550      ENTER @Agte507x;Buff$
1560      OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:THRU ";Port(J);", "
;Port(I)
1570      OUTPUT @Agte507x;"*OPC?"
1580      ENTER @Agte507x;Buff$
1590    NEXT J
1600  NEXT I
1610  !
1620  ! Done
1630  !
1640  OUTPUT @Agte507x;":SENS"&Ch$&":CORR:COLL:SAVE"
1650  PRINT "Done"
1660  SUBEND

```

Controlling Using SICL-LAN Server


This section describes how to control the E5061A/E5062A using SICL in the Windows environment, with a sample program (a VBA macro for Microsoft Excel) written in Visual Basic. The source file of this program, ctrl_lansicl.xls, is available in the sample program disk.

NOTE To control the E5061A/E5062A using the SICL-LAN server, you need to make preparations described in “Control over SICL-LAN server” on page 28.

Using VBA macro

Opening ctrl_lansicl.xls in Microsoft Excel display a screen as shown in Figure 12-3.

Figure 12-3 ctrl_lansicl.xls

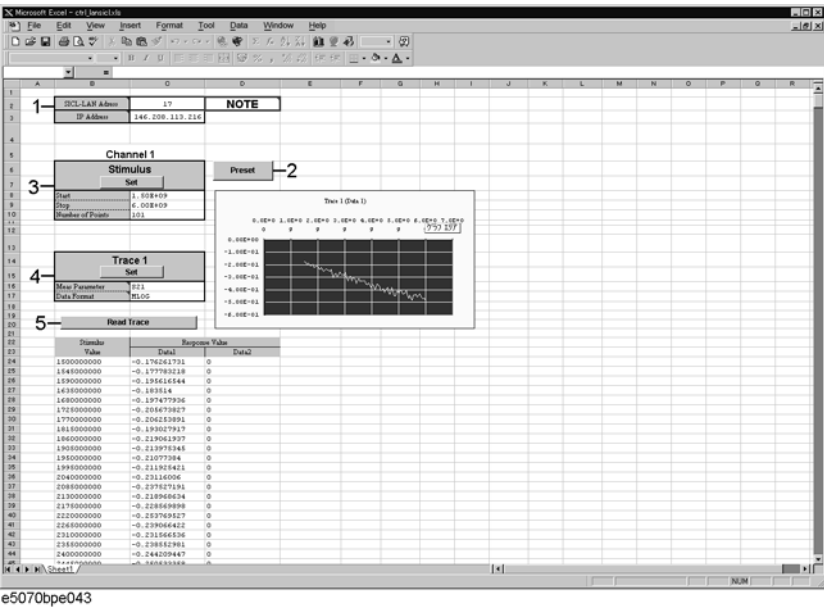

For how to use each element in Figure 12-3, refer to the following description.

We begin describing the part 1. In the cell to the right of SICL-LAN Address, enter the address of the E5061A/E5062A for control with the SICL-LAN server. This address is xx, which has been set with the command [System] - Misc Setup - Network Setup - SICL-LAN Address [xx]. Enter the IP address of the E5061A/E5062A in the cell right side of IP Address. This VBA macro will not work properly without appropriate values in the two cells.

Clicking the button labeled as Preset in the part 2 executes the presetting operation.

In the part 3, sweep range (start and stop points) and number of measurement points for channel 1 are set. Clicking the button labeled as Set executes the setting as shown in the setting table.

The part 4 set the measurement parameters and data format for trace 1 in channel 1.

Clicking the button labeled as Set executes the setting as shown in the setting table.

Clicking the button labeled as Read Trace in the part 5 retrieves the formatted data array of trace 1 in channel 1 and displays it in tabular and graphical formats.

Description of operation in VBA macro

Here described is operation of the VBA macro, focusing on the part related to controlling with SICL.

In order to use SICL in your VBA macro, you must declare functions and define variables with a definition file of SICL (for VB). In the VBA macro, ctrl_sicllan.xls, the standard module whose object name is “SICL” is the definition file.


Basic control flow with SICL is shown in Figure 12-4.

NOTE

In this sample program, the **ivprintf** function, the **ivscanf** function, and the **iread** function are used in its communication part; you can use other SICL functions as well. For detail, refer to [sicl.hlp](#) (the online help of SICL).

Figure 12-4

Flow of control using SICL

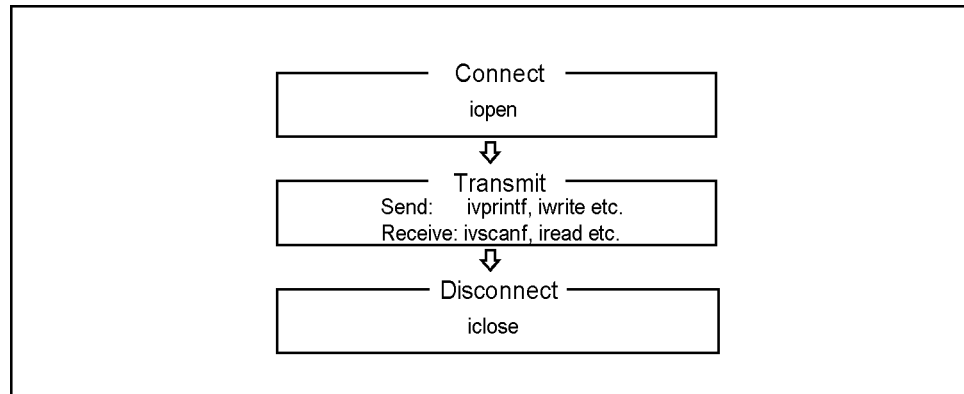

e5070bpe041

NOTE

For more information on how to use each function of SICL, refer to the manual of SICL.

Procedures in each step in Figure 12-4 are described below.

Connection

The procedure corresponding to connection is OpenSession (Example 12-2). OpenSession establishes connection to the **E5061A/E5062A** with the **iopen** function of SICL, using SICL-LAN Address and IP Address entered in the part 1 in Figure 12-3. The **iopen** function takes the address information of the **E5061A/E5062A** you specify as its parameters.

Syntax

addr = iopen(*dev*)

Variable

	<i>addr</i>
Description	Session information (output)
Data type	Integer type

	<i>dev</i>
Description	Address information of the instrument you specify (input)
Data type	Character string type
Grammar	<i>sicl-name</i> *1[<i>ip-address</i> *2]: <i>interface</i> *3, <i>sicl-lan-address</i> *4

*1. The SICL interface name you have set with the Agilent I/O Libraries in external control.

*2. The IP address of the E5061A/E5062A.

*3. For the E5061A/E5062A, specify hpib9.

*4. The address of the E5061A/E5062A for control with the SICL-LAN server.

For example, if the parameter (*dev*) is "lan[128.10.0.3]:hpib9,17," connection is made to the address of **17** of the interface of **hpib9** with the **E5061A/E5062A** whose IP address is **128.10.0.3** using the external controller whose SICL interface name is **lan**.

Example 12-2

OpenSession

Function OpenSession() As Integer

Dim ServAddr As String

Dim IpAddr As String

On Error GoTo ErrHandler

```
'''Get Sicl-Lan Address
Sheets("Sheet1").Select
Range("C2").Select
ServAddr = ActiveCell.FormulaR1C1
```

```
'''Get Ip Address
Sheets("Sheet1").Select
Range("C3").Select
IpAddr = ActiveCell.FormulaR1C1
```

OpenSession = iopen("lan[" & IpAddr & "]:hpib9," & ServAddr)

```

Call itimeout(OpenSession, 10000)
Exit Function

ErrorHandler:
  MsgBox "**** Error : " & Error$
  Call siclcleanup
End

End Function

```

Sending

The procedure corresponding to sending in communication is OutputSicLan (Example 12-3). OutputSicLan uses the **ivprintf** function of SICL to send messages (SCPI commands). The **ivprintf** function takes the session information outputted from the **iopen** function and a program message as its parameters.

Syntax

Status = ivprintf(*addr*,*mes*)

Variable

Table 12-1

Variable (*Status*)

	<i>Status</i>
Description	Return value of the function (output)
Data type	Integer type

Table 12-2

Variable (*addr*)

	<i>addr</i>
Description	Session information (input)
Data type	Integer type

	<i>mes</i>
Description	Program message (input) ^{*1}
Data type	Character string type

*1. When sending a program message of a SCPI command, add the message terminator at the end of the message (in Example 12-3, Chr\$(10)).

Example 12-3

OutputSicLan

```

Sub OutputSicLan(addr As Integer, message As String)

  Dim Status As Integer
  Dim actualcnt As Long
  Dim length As Long

  On Error GoTo ErrorHandler

  length = Len(message)

```

```
Status = ivprintf(addr, message & Chr$(10))
Exit Sub

ErrorHandler:
MsgBox "**** Error : " & Error$
Call siclcleanup
End

End Sub
```

Receiving

The procedure corresponding to receiving ASCII format messages in communication is EnterSicLan (Example 12-4). EnterSicLan uses the **ivscanf** function of SICL to receive a message in ASCII format and store it into the output variable. The **ivscanf** function takes the session information outputted from the **iopen** function, the format for output, and data to be outputted as its parameters.

Syntax

```
Status = ivscanf(addr,fmt,ap)
```

Variable

	<i>fmt</i>
Description	Format for output (input)
Data type	Character string type

	<i>ap</i>
Description	Data to be outputted (output)
Data type	Character string type

For information on the variable (*Status*) and the variable (*addr*), refer to Table 12-1, “Variable (*Status*),” on page 179 and Table 12-2, “Variable (*addr*),” on page 179, respectively.

NOTE

In Visual Basic, variables must be declared as a fixed length string when receiving string data using the **ivscanf** function.

Example 12-4

EnterSicLan

```
Sub EnterSicLan(addr As Integer, Query As String)

Dim Status As Integer
Dim actualcnt As Long
Dim res As String * 256

On Error GoTo ErrorHandler

Status = ivscanf(addr, "%t", res)
Query = Trim(res)
Exit Sub
```

```

ErrorHandler:
  MsgBox "**** Error : " & Error$
  Call siclcleanup
End
End Sub

```

The procedure corresponding to receiving array data in communication is EnterSicLanArrayReal64 (Example 12-5). EnterSicLanArrayReal64 uses the **iread** function of SICL to receive array data in the IEEE 64 bit floating point binary transfer format and store it into the output variable. The **iread** function takes the session information outputted from the **iopen** function, data to be outputted, the number of data bytes, the condition to finish reading data, and the number of data bytes actually read out as its parameters.

Syntax

Status = iread(*addr,buf,bufsize,reason,actual*)

Variable

	<i>buf</i>
Description	Data to be outputted (output)
Data type	Character string type

	<i>bufsize</i>
Description	The number of data bytes (input)
Data type	Long integer type

	<i>reason</i>
Description	The condition to finish reading out data (input)
Data type	Integer type

	<i>actual</i>
Description	The number of data bytes actually read out (output)
Data type	Long integer type

For information on the variable (*Status*) and the variable (*addr*), refer to Table 12-1, “Variable (Status),” on page 179 and Table 12-2, “Variable (addr),” on page 179, respectively.

Each functional part of EnterSicLanArrayReal64 is described below.

- (1) retrieves the data header.
- (2) stores the number of data bytes into the size variable in the header part.
- (3) retrieves the formatted data array for trace 1 in channel 1, and stores it into the databuf variable.

(4) retrieves the message terminator at the end of the data.

Example 12-5

EnterSicLanArrayReal64

```
Function EnterSicLanArrayReal64(addr As Integer, databuf() As Double)
As Long

    Dim Status As Integer
    Dim actualcnt As Long
    Dim buf As String * 8
    Dim size As Long

    On Error GoTo ErrHandler

    '''Read header info of "#6NNNNNN"
    Status = iread(addr, buf, 8, I_TERM_MAXCNT, actualcnt)
'.....(1)

    size = Val(Mid$(buf, 3, 6))
'.....(2)

    '''Read data
    Status = iread(addr, databuf, size, I_TERM_MAXCNT, actualcnt)
'.....(3)

    '''Read ending LF
    Status = iread(addr, buf, 1, I_TERM_MAXCNT, actualcnt)
'.....(4)

    EnterSicLanArrayReal64 = size / 8
    Exit Function

ErrHandler:
    MsgBox "*** Error : " & Error$
    Call siclcleanup
    End

End Function
```

Disconnection

The **iclose** function of SICL is used to disconnect communication. The **iclose** function takes the session information outputted from the **iopen** function as its parameter.

Syntax

Status = iclose(*addr*)

For information on the variable (*Status*) and the variable (*addr*), refer to Table 12-1, “Variable (*Status*),” on page 179 and Table 12-2, “Variable (*addr*),” on page 179, respectively.

Sample control

The E5061A/E5062A can be controlled by executing the above procedures in order, following the control flow in Figure 12-4. This is demonstrated by the procedure Preset (a procedure which is executed when the Preset button is clicked) as described in Example 12-6.

Example 12-6

Preset

```
Sub Preset()  
    ''' Open Session  
    E507x = OpenSession  
  
    '''Presetting the analyzer  
    Call OutputSiclLan(E507x, ":SYST:PRES")  
  
    '''Close Session  
    Call iclose(E507x)  
  
End Sub
```

Controlling Using Telnet Server


This section describes how to control the E5061A/E5062A using WinSock API in the Windows environment, with a sample program written in Visual Basic (VBA macro). You can find the source file of this program, named ctrl_lan.xls (Microsoft Excel file), on the sample program disk.

Using VBA macro

Opening ctrl_lan.xls in Microsoft Excel display a screen as shown in Figure 12-5.

Figure 12-5

ctrl_lan.xls

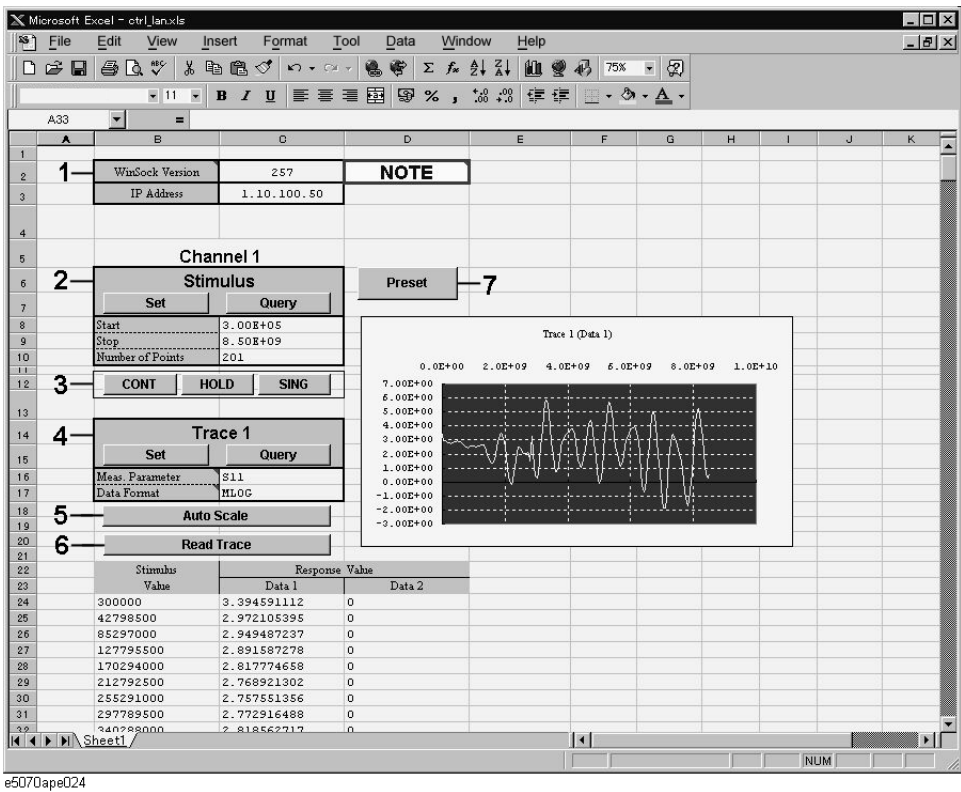

For how to use each element in Figure 12-5, refer to the following description.

We begin describing the part 1. Enter the version number of WinSock API in the cell right side of "Winsock Version." The version number is obtained by multiplying 256 by the major version then adding the minor version. For example, when the version of your Winsock API is 1.1, the version number is obtained as follows: $256 \times 1 + 1 = 257$. Enter the IP address of the E5061A/E5062A in the cell right side of "IP Address." This VBA macro will not work properly without appropriate values in the two cells.

In the part 2, sweep range (start and stop points) and number of measurement points are set. Clicking the button labeled as "Set" executes setting operation as specified with the setting table, while clicking the button labeled as "Query" retrieves the current settings of the E5061A/E5062A.

The part 3 is dedicated to setting the trigger mode.

The part 4 set the measurement parameters and data format for trace 1 in channel 1. Clicking the button labeled as 'Set' executes setting operation as specified with the setting table, while clicking the button labeled as "Query" retrieves the current settings of the E5061A/E5062A.

In the part 5, clicking the button labeled as "Auto Scale" executes auto scaling for trace 1 in channel 1.

Clicking the button labeled as "Read Trace" in the part 6 retrieves the formatted data of trace 1 in channel 1 and displays it in tabular and graphical formats.

Clicking the button labeled as "Preset" executes the presetting operation.

Description of operation in VBA macro

Here described is operation of the VBA macro, focusing on the part related to controlling with WinSock API.

In order to use WinSock API, you must declare functions and define variables with a definition file of WinSock API, as shown in Example 12-7.

Example 12-7

Definition file of WinSock API

```
'This is the Winsock API definition file for Visual Basic

'Setup the variable type 'hostent' for the WSStartup command
Type Hostent
    h_name As Long
    h_aliases As Long
    h_addrtype As String * 2
    h_length As String * 2
    h_addr_list As Long
End Type
Public Const SZHOSTENT = 16

'Set the Internet address type to a long integer (32-bit)
Type in_addr
    s_addr As Long
End Type

'A note to those familiar with the C header file for Winsock
'Visual Basic does not permit a user-defined variable type
'to be used as a return structure. In the case of the
'variable definition below, sin_addr must
'be declared as a long integer rather than the user-defined
'variable type of in_addr.
Type sockaddr_in
    sin_family As Integer
    sin_port As Integer
    sin_addr As Long
    sin_zero As String * 8
End Type

Public Const WSADESCRIPTION_LEN = 256
Public Const WSASYS_STATUS_LEN = 128
Public Const WSA_DescriptionSize = WSADESCRIPTION_LEN + 1
Public Const WSA_SysStatusSize = WSASYS_STATUS_LEN + 1
```

Sample Application Programs

Controlling Using Telnet Server

```
'Setup the structure for the information returned from
'the WSStartup() function.
Type WSADATA
    wVersion As Integer
    wHighVersion As Integer
    szDescription As String * WSA_DescriptionSize
    szSystemStatus As String * WSA_SysStatusSize
    iMaxSockets As Integer
    iMaxUdpDg As Integer
    lpVendorInfo As String * 200
End Type

'Define socket return codes
Public Const INVALID_SOCKET = &HFFFF
Public Const SOCKET_ERROR = -1

'Define socket types
Public Const SOCK_STREAM = 1           'Stream socket
Public Const SOCK_DGRAM = 2           'Datagram socket
Public Const SOCK_RAW = 3             'Raw data socket
Public Const SOCK_RDM = 4             'Reliable Delivery socket
Public Const SOCK_SEQPACKET = 5       'Sequenced Packet socket

'Define address families
Public Const AF_UNSPEC = 0             'unspecified
Public Const AF_UNIX = 1              'local to host (pipes, portals)
Public Const AF_INET = 2              'internetwork: UDP, TCP, etc.
Public Const AF_IMPLINK = 3           'arpanet imp addresses
Public Const AF_PUP = 4               'pup protocols: e.g. BSP
Public Const AF_CHAOS = 5             'mit CHAOS protocols
Public Const AF_NS = 6               'XEROX NS protocols
Public Const AF_ISO = 7              'ISO protocols
Public Const AF_OSI = AF_ISO          'OSI is ISO
Public Const AF_ECMA = 8              'european computer manufacturers
Public Const AF_DATAKIT = 9           'datakit protocols
Public Const AF_CCITT = 10            'CCITT protocols, X.25 etc
Public Const AF_SNA = 11              'IBM SNA
Public Const AF_DECnet = 12           'DECnet
Public Const AF_DLI = 13              'Direct data link interface
Public Const AF_LAT = 14              'LAT
Public Const AF_HYLINK = 15          'NSC Hyperchannel
Public Const AF_APPLETALK = 16        'AppleTalk
Public Const AF_NETBIOS = 17          'NetBios-style addresses
Public Const AF_MAX = 18              'Maximum # of address families

'Setup sockaddr data type to store Internet addresses
Type sockaddr
    sa_family As Integer
    sa_data As String * 14
End Type
Public Const SADDRLEN = 16

'Declare Socket functions

Public Declare Function closesocket Lib "wsock32.dll" (ByVal s As Long)
As Long

Public Declare Function connect Lib "wsock32.dll" (ByVal s As Long, addr
As sockaddr_in, ByVal namelen As Long) As Long

Public Declare Function htons Lib "wsock32.dll" (ByVal hostshort As Long)
```

As Integer

```
Public Declare Function inet_addr Lib "wsck32.dll" (ByVal cp As String)
As Long
```

```
Public Declare Function recv Lib "wsck32.dll" (ByVal s As Long, ByVal
buf As Any, ByVal buflen As Long, ByVal flags As Long) As Long
```

```
Public Declare Function recvB Lib "wsck32.dll" Alias "recv" (ByVal s As
Long, buf As Any, ByVal buflen As Long, ByVal flags As Long) As Long
```

```
Public Declare Function send Lib "wsck32.dll" (ByVal s As Long, buf As
Any, ByVal buflen As Long, ByVal flags As Long) As Long
```

```
Public Declare Function socket Lib "wsck32.dll" (ByVal af As Long, ByVal
socktype As Long, ByVal protocol As Long) As Long
```

```
Public Declare Function WSASStartup Lib "wsck32.dll" (ByVal
wVersionRequired As Long, lpWSAData As WSAData) As Long
```

```
Public Declare Function WSACleanup Lib "wsck32.dll" () As Long
```


```
Public Declare Function WSAUnhookBlockingHook Lib "wsck32.dll" () As
Long
```

```
Public Declare Sub CopyMemory Lib "kernel32" Alias "RtlMoveMemory"
(hpvDest As Any, hpvSource As Any, ByVal cbCopy As Long)
```

Basic control flow with WinSock API is shown in Figure 12-6.

Figure 12-6

Control flow with WinSock API

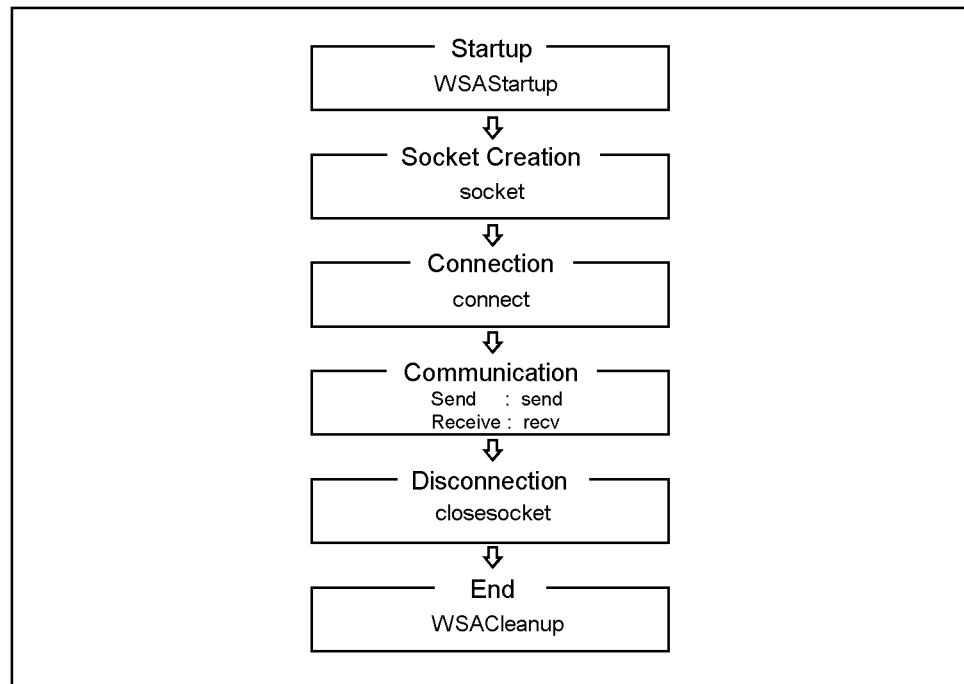

e5070ape029

Procedures in each step in Figure 12-6 are described below.

Startup

The procedure corresponding to Startup is StartIt (Example 12-8). StartIt launches and initialize WinSock API with **WSAStartup** in WinSock API, whose version is in the part 1 of Figure 12-5. The function WSAStartup should be always used when initiating WinSock. This function takes version number (input) and launching information (output) as its parameters.

Example 12-8

StartIt

```
Sub StartIt()  
  
    Dim StartUpInfo As WSADATA  
  
    'Version 1.1 (1*256 + 1) = 257  
    'version 2.0 (2*256 + 0) = 512  
  
    'Get WinSock version  
    Sheets("Sheet1").Select  
    Range("C2").Select  
    version = ActiveCell.FormulaR1C1  
  
    'Initialize Winsock DLL  
    x = WSAStartup(version, StartUpInfo)  
  
End Sub
```

Socket Creation and Connection

The procedure for Socket Creation and Connection is OpenSocket (Example 12-9). OpenSocket makes a connection to an instrument associated with the IP address specified with the input parameter Hostname. It uses a socket of the port specified with the input parameter PortNumber. Each functional part of OpenSocket is described below.

In (1), the inet_addr function of WinSock API is used to convert an IP address delimited by “.” to an Internet address.

In (2), a new socket is created with **socket** function of WinSock API and its socket descriptor is obtained. If an error occurs, the control returns to the main program with a message. socket function takes parameters for an address family (input), a socket type (input), and a protocol number (input).

In (3), the socket address is specified. Note that htons, which is used for specifying the port number, is a function of WinSock API. The function converts a 2-byte integer from the Windows byte order (little endian) to the network byte order (big endian).

In (4), a connection to the E5061A/E5062A is made using **connect** function of WinSock API. If an error occurs, the control returns to the main program with a message. connect function takes parameters for a socket descriptor (input), a socket address (input), and size of the socket address (input).

Example 12-9

OpenSocket

```
Function OpenSocket(ByVal Hostname As String, ByVal PortNumber As Integer) As Integer

    Dim I_SocketAddress As sockaddr_in
    Dim ipAddress As Long

    ipAddress = inet_addr(Hostname) ' .....(1)

    'Create a new socket
    socketId = socket(AF_INET, SOCK_STREAM, 0) '
    If socketId = SOCKET_ERROR Then '
        MsgBox ("ERROR: socket = " + Str$(socketId)) ' .....(2)
        OpenSocket = COMMAND_ERROR '
        Exit Function '
    End If '

    'Open a connection to a server

    I_SocketAddress.sin_family = AF_INET '
    I_SocketAddress.sin_port = htons(PortNumber) ' .....(3)
    I_SocketAddress.sin_addr = ipAddress '
    I_SocketAddress.sin_zero = String$(8, 0) '

    x = connect(socketId, I_SocketAddress, Len(I_SocketAddress)) '
    If socketId = SOCKET_ERROR Then '
        MsgBox ("ERROR: connect = " + Str$(x)) ' ..(4)
        OpenSocket = COMMAND_ERROR '
        Exit Function '
    End If '

    OpenSocket = socketId

End Function
```

Communication

The procedure corresponding to Communication is SendCommand (Example 12-10). SendCommand transmits a message (SCPI command) specified with the input parameter “command” to the E5061A/E5062A using **send** function of WinSock API. send function takes parameters for a socket descriptor (input), a message to be transmitted (input), message length (input) and a flag (input).

Example 12-10

SendCommand

```
Function SendCommand(ByVal command As String) As Integer

    Dim strSend As String

    strSend = command + vbCrLf

    count = send(socketId, ByVal strSend, Len(strSend), 0)

    If count = SOCKET_ERROR Then
        MsgBox ("ERROR: send = " + Str$(count))
        SendCommand = COMMAND_ERROR
        Exit Function
    End If

    SendCommand = NO_ERROR

End Function
```

The procedure corresponding to a receiving part of communication is RecvAscii (Example 12-11) and other functions. RecvAscii receives a message as ASCII format and stores it in the dataBuf output parameter. Maximum length of the message is specified with the maxLength input parameter. Each functional part of RecvAscii is described below.

In (1), a message (a response to a query for SCPI command) is received from the **E5061A/E5062A** as a series of characters using **recv** function of **WinSock API**. If an error occurs, the control returns to the main program with a message. recv function takes parameters for a socket descriptor (input), a message to be received (input), message length (input) and a flag (input).

In (2), it is determined whether each received character is LF (ASCII code: 10). When it is LF, receiving is terminated adding NULL (ASCII code: 0) to the end of dataBuf string and the control returns to the main program.

In (3), number of the last characters that was read out is added to the count value for checking a number of received characters, and append the characters to the end of dataBuf string.

Example 12-11

RecvAscii

Function RecvAscii(dataBuf As String, ByVal maxLength As Integer) As Integer

```
    Dim c As String * 1
    Dim length As Integer

    dataBuf = ""
    While length < maxLength
        DoEvents
        count = recv(socketId, c, 1, 0)
        If count < 1 Then
            RecvAscii = RECV_ERROR
            dataBuf = Chr$(0)
            Exit Function
        End If

        If c = Chr$(10) Then
            dataBuf = dataBuf + Chr$(0)
            RecvAscii = NO_ERROR
            Exit Function
        End If

        length = length + count
        dataBuf = dataBuf + c
    Wend

    RecvAscii = RECV_ERROR

End Function
```

Disconnection

The procedure corresponding to Disconnection is CloseConnection (Example 12-12). CloseConnection disconnects communication and removes a socket using **closesocket** function of **WinSock API**. closesocket function takes a parameter for a socket descriptor (input).

Example 12-12

CloseConnection

```
Sub CloseConnection()  
    x = closesocket(socketId)  
  
    If x = SOCKET_ERROR Then  
        MsgBox ("ERROR: closesocket = " + Str$(x))  
        Exit Sub  
    End If  
  
End Sub
```

End

The procedure corresponding to End is EndIt (Example 12-13). EndIt disconnects **WinSock API** using **WSACleanup** function of **WinSock API**. The function WSACleanup should be always used when terminating WinSock.

Example 12-13

EndIt

```
Sub EndIt()  
  
    'Shutdown Winsock DLL  
    x = WSACleanup()  
  
End Sub
```

Example of control

The E5061A/E5062A can be controlled by executing the above procedures in order, following the control flow in Figure 12-6. This is demonstrated by the procedure autoscale (a procedure which is executed when the Auto Scale button is clicked) as described in Example 12-14.

Example 12-14

autoscale

```
Sub autoscale()  
,  
, auto scaling  
,  
    Call StartIt  
    Call get_hostname  
    x = OpenSocket(Hostname$, ScpiPort)  
  
    x = SendCommand(":DISP:WIND1:TRAC1:Y:AUTO")  
  
    Call CloseConnection  
    Call EndIt  
  
End Sub
```

NOTE

When you execute more than one command by connecting and disconnecting a socket for every command, the sequence of execution may change.

❑ Connection → Command 1 → Command 2 → Disconnection

Commands 1 and 2 are always executed in this sequence.

❑ Connection → Command 1 → Disconnection → Connection → Command 2 → Disconnection

These commands may be in the sequence of Command 2 → command 1.

13

SCPI Command Reference

This chapter describes the SCPI command reference for the Agilent E5061A/E5062A. It describes the commands using their abbreviated format in alphabetical order. If you want to look up commands by softkeys, refer to the User's Guide.

Notational conventions in this command reference

This section describes the rules to read the description of the commands in this chapter.

Syntax

Part with heading “Syntax” describes the syntax to send a command from the external controller to the E5061A/E5062A. A syntax consists of a command part and a parameter part. The separator between the command part and the parameter part is a space.

If there are several parameters, the separator between adjacent parameters is a comma (,). 3 points (...) between commas indicate that parameters in that part are omitted. For example, <numeric 1>,...,<numeric 4> indicates that 4 parameters, <numeric 1>,<numeric 2>,<numeric 3>,<numeric 4>, are required.

String-type parameters, <string>, <string 1>, and so on, must be enclosed in double quotation marks ("). <block> shows block format data.

You can omit the lowercase letters in syntax. For example, ":CALibration:CABLe" can be shortened as ":CAL:CABL."

The definition of symbols used in the syntax is as follows:

<>	Characters enclosed in this pair of symbols are necessary parameters when sending the command.
[]	Part enclosed in this parenthesis pair can be omitted.
{}	Part enclosed in this parenthesis pair indicates that you must select one of the items in this part. Individual items are separated by a vertical bar ().

For example, ":CALC:CORR:EDEL:TIME 0.1,"
":CALCULATE1:SELECTED:CORR:EDEL:TIME 25E-3," and so on are valid for the syntax given below.

Syntax :CALCulate{[1]|2|3|4|5|6|7|8|9}[[:SElected]:CORRection:EDELay:TIME <numeric>

Description

Part with heading “Description” describes how to use the command or the operation when executed.

Parameters

Part with heading “Parameters” describes necessary parameters when sending the command. When a parameter is a value type or a string type enclosed with <>, its description, allowable setup range, preset (factory-set) value, and so on are given; when a parameter is a selection type enclosed with {}, the description of each selection item is given.

Query response

Part with heading “Query response” describes the data format read out when query (reading out data) is available with the command.

Each readout parameter is enclosed with {}. If there are several items within {} separated by the pipe (|), only one of them is read out.

When several parameters are read out, they are separated with a comma (.). Note that, 3 points (...) between commas indicate that the data of that part is omitted. For example, {numeric 1},...,{numeric 4} indicates that 4 data items, {numeric 1}, {numeric 2}, {numeric 3}, and {numeric 4}, are read out.

<newline><^END> after the parameters is the program message terminator.

Related commands

Part with heading “Related commands” describes the commands related to this command.

Equivalent key

Part with heading “Equivalent key” shows the operational procedure of the front panel keys that has the same effect as this command.

- | | |
|---------------------|--|
| [Key] | Indicates that you press the key named Key. |
| [Key] - Item | Indicates a series of key operation in which you press the [Key] key, select (highlight) the item called Item on the displayed menu using the [↓] key and so on, and then press the [Enter] key. |

IEEE Common Commands

This section describes the IEEE common commands.

***CLS**

Syntax	*CLS
Description	Clears the followings. (No query) • Error Queue • Status Byte Register • Standard Event Status Register • Operation Status Event Register • Questionable Status Event Register • Questionable Limit Status Event Register • Questionable Limit Channel{1-4} Status Event Register
Example of use	10 OUTPUT 717; "*CLS"
Equivalent key	No equivalent key is available on the front panel.

*ESE

Syntax	*ESE <numeric> *ESE?
Description	Sets the value of the Standard Event Status Enable Register.
Parameters	

	<numeric>
Description	Setup value of the register
Range	0 to 255
Preset value	0
Resolution	1

If the specified parameter is out of the allowable setup range, the result of bitwise AND with 255 (0xff) is set.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;"*ESE 16" 20 OUTPUT 717;"*ESE?" 30 ENTER 717;A
Related commands	*SRE on page 200
Equivalent key	No equivalent key is available on the front panel.

*ESR?

Syntax	*ESR?
Description	Reads out the value of the Standard Event Status Register. Executing this command clears the register value. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;"*ESR?" 20 ENTER 717;A
Equivalent key	No equivalent key is available on the front panel.

***IDN?**

Syntax	*IDN?
Description	Reads out the product information (manufacturer, model number, serial number, and firmware version number) of the E5061A/E5062A. (Query only)
Query response	{string 1},{string 2},{string 3},{string 4}<newline><^END> Readout data is as follows: {string 1} Manufacturer. Agilent Technologies is always read out. {string 2} Model number (example: E5061A). {string 3} Serial number (example: JP1KI00101). {string 4} Firmware version number (example: 03.00).
Example of use	10 OUTPUT 717;"*IDN?" 20 ENTER 717;A\$
Equivalent key	[System] - Firmware Revision [System] - Service Menu - Enable Options - Serial Number

***OPC**

Syntax	*OPC
Description	Sets the OPC bit (bit 0) of the Standard Event Status Register at the completion of all pending operations. (No query)
Example of use	10 OUTPUT 717;"*OPC"
Equivalent key	No equivalent key is available on the front panel.

***OPC?**

Syntax	*OPC?
Description	1 is read out at the completion of all pending operations. (Query only)
Query response	{1}<newline><^END>
Example of use	10 OUTPUT 717;"*OPC?" 20 ENTER 717;A
Equivalent key	No equivalent key is available on the front panel.

***OPT?**

Syntax	*OPT?
Description	Reads out the identification number of an option installed in the E5061A/E5062A. (Query only)
Query response	{numeric}<newline><^END> If there is no installed option, 0 is read out.
Example of use	10 OUTPUT 717;"*OPT?" 20 ENTER 717;A\$
Equivalent key	No equivalent key is available on the front panel.

***RST**

Syntax	*RST
Description	Performs preset. There is the following difference from the setting state preset with the :SYST:PRES command. (No query) The continuous initiation mode of channel 1 is set to OFF.
Example of use	10 OUTPUT 717;"*RST"
Related commands	:SYST:PRES on page 479 :INIT{1-4}:CONT on page 341
Equivalent key	No equivalent key is available on the front panel.

***SRE**

Syntax *SRE <numeric>
 *SRE?

Description Sets the value of the Service Request Enable Register.

Parameters

	<numeric>
Description	Setup value of the register
Range	0 to 255
Preset value	0
Resolution	1

If the specified parameter is out of the allowable setup range, the result of bitwise AND with 255 (0xff) is set. Note that bit 6 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;"*SRE 128"
 20 OUTPUT 717;"*SRE?"
 30 ENTER 717;A

Related commands *ESE on page 197
 :STAT:OPER:ENAB on page 442
 :STAT:QUES:ENAB on page 454

Equivalent key No equivalent key is available on the front panel.

***STB?**

Syntax	*STB?
Description	Reads out the value of the Status Byte Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;"*STB?" 20 ENTER 717;A
Equivalent key	No equivalent key is available on the front panel.

***TRG**

Syntax	*TRG
Description	If the trigger source is set to GPIB/LAN (set to BUS with the :TRIG:SOUR command), triggers the E5061A/E5062A waiting for a trigger. (No query)
Example of use	10 OUTPUT 717;"*TRG"
Related commands	:TRIG:SOUR on page 485
Equivalent key	No equivalent key is available on the front panel.

***WAI**

Syntax	*WAI
Description	Waits for the execution of all commands sent before this command to be completed. (No query)
Example of use	10 OUTPUT 717;"*WAI"
Equivalent key	No equivalent key is available on the front panel.

E5061A/E5062A commands

This section describes the commands specific to the E5061A/E5062A.

:ABOR

Syntax	:ABORt
Description	Aborts the measurement and changes the trigger sequence for all channels to idle state. (No query) After the change to the idle state, the channels for which the continuous initiation mode is set to ON (set to ON with the :INIT{1-4}:CONT command) change into the initiate state. For details about the trigger system, refer to “Trigger system” on page 80. (No query)
Example of use	10 OUTPUT 717; ":ABOR"
Related commands	:INIT{1-4} on page 340 :INIT{1-4}:CONT on page 341
Equivalent key	[Trigger] - Restart

:CALC{1-4}:BLIM

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:BLIMit[:STATe] {ON|OFF|1|0}
:CALCulate{[1]|2|3|4}[:SELEcted]:BLIMit[:STATe]?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the bandwidth test function.

Parameters

	Description
ON or 1	Turns ON the bandwidth test function.
OFF or 0 (preset value)	Turns OFF the bandwidth test function.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;" :CALC1:BLIM ON"
20 OUTPUT 717;" :CALC1:BLIM?"
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:BLIM:DB on page 204
:CALC{1-4}:BLIM:DISP:MARK on page 205
:CALC{1-4}:BLIM:DISP:VAL on page 206
:CALC{1-4}:BLIM:FAIL? on page 207
:CALC{1-4}:BLIM:MAX on page 208
:CALC{1-4}:BLIM:MIN on page 209
:CALC{1-4}:BLIM:REP? on page 210

Equivalent key **[Analysis] - Bandwidth Limit - BW Test**

:CALC{1-4}:BLIM:DB

Syntax	:CALCulate{[1] 2 3 4}{:SElected}:BLIMit:DB <numeric> :CALCulate{[1] 2 3 4}{:SElected}:BLIMit:DB?										
Description	For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the bandwidth threshold value (attenuation from the peak) of the bandwidth test.										
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Bandwidth N dB points</td></tr><tr><td>Range</td><td>0 to 5E8</td></tr><tr><td>Preset value</td><td>3</td></tr><tr><td>Unit</td><td>dB</td></tr></table>		<numeric>	Description	Bandwidth N dB points	Range	0 to 5E8	Preset value	3	Unit	dB
	<numeric>										
Description	Bandwidth N dB points										
Range	0 to 5E8										
Preset value	3										
Unit	dB										
Query response	{numeric}<newline><^END>										
Example of use	10 OUTPUT 717;":CALC1:BLIM:DB 3" 20 OUTPUT 717;":CALC1:BLIM:DB?" 30 ENTER 717;A										
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286 :CALC{1-4}:BLIM on page 203										
Equivalent key	[Analysis] - Bandwidth Limit - N dB Points										

:CALC{1-4}:BLIM:DISP:MARK

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:BLIMit:DISPlay:MARKer {ON|OFF|1|0}
:CALCulate{[1]|2|3|4}[:SELEcted]:BLIMit:DISPlay:MARKer?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the marker display of the bandwidth test.

Parameters

	Description
ON or 1	Turns ON the bandwidth marker.
OFF or 0 (preset value)	Turns OFF the bandwidth marker.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:BLIM:DISP:MARK ON"
20 OUTPUT 717;":CALC1:BLIM:DISP:MARK?"
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:BLIM on page 203
:CALC{1-4}:BLIM:DISP:VAL on page 206

Equivalent key [Analysis] - Bandwidth Limit - BW Marker

:CALC{1-4}:BLIM:DISP:VAL

Syntax :CALCulate{[1]|2|3|4}{:SElected]:BLIMit:DISPlay:VALue {ON|OFF|1|0}
:CALCulate{[1]|2|3|4}{:SElected]:BLIMit:DISPlay:VALue?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the bandwidth value display of the bandwidth test.

Parameters

	Description
ON or 1	Turns ON the bandwidth display.
OFF or 0 (preset value)	Turns OFF the bandwidth display.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717; ":CALC1:BLIM:DISP:VAL ON"
20 OUTPUT 717; ":CALC1:BLIM:DISP:VAL?"
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:BLIM on page 203
:CALC{1-4}:BLIM:DISP:MARK on page 205

Equivalent key **[Analysis] - Bandwidth Limit - BW Display**

:CALC{1-4}:BLIM:FAIL?

Syntax	:CALCulate{[1] 2 3 4}[:SELeCted]:BLIMit:FAIL?
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the bandwidth test result. (Query only)
Query response	{1 0}<newline><^END>

	Description
1	The bandwidth test result is FAIL.
0	The bandwidth test result is PASS.

When the bandwidth limit test is set to OFF, 0 is always read out.

Example of use	10 OUTPUT 717;":CALC1:BLIM:FAIL?" 20 ENTER 717;A
----------------	---

Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286 :CALC{1-4}:BLIM on page 203
------------------	--

Equivalent key	No equivalent key is available on the front panel.
----------------	--

:CALC{1-4}:BLIM:MAX

Syntax	:CALCulate{[1][2][3][4][:SElected]:BLIMit:MAXimum <numeric> :CALCulate{[1][2][3][4][:SElected]:BLIMit:MAXimum?										
Description	For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the upper limit value of the bandwidth test.										
Parameters	<table><tr><th></th><th><numeric></th></tr><tr><td>Description</td><td>Maximum bandwidth.</td></tr><tr><td>Range</td><td>0 to 1E12</td></tr><tr><td>Preset value</td><td>10 k</td></tr><tr><td>Unit</td><td>Hz (hertz), dB or second</td></tr></table>		<numeric>	Description	Maximum bandwidth.	Range	0 to 1E12	Preset value	10 k	Unit	Hz (hertz), dB or second
	<numeric>										
Description	Maximum bandwidth.										
Range	0 to 1E12										
Preset value	10 k										
Unit	Hz (hertz), dB or second										
Query response	{numeric}<newline><^END>										
Example of use	10 OUTPUT 717;":CALC1:BLIM:MAX 3E5" 20 OUTPUT 717;":CALC1:BLIM:MAX?" 30 ENTER 717;A										
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286 :CALC{1-4}:BLIM on page 203 :CALC{1-4}:BLIM:MIN on page 209										
Equivalent key	[Analysis] - Bandwidth Limit - Max Bandwidth										

:CALC{1-4}:BLIM:MIN

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:BLIMit:MINimum <numeric>
:CALCulate{[1]|2|3|4}[:SELEcted]:BLIMit:MINimum?

Description For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the lower limit value of the bandwidth test.

Parameters

	<numeric>
Description	Minimum bandwidth.
Range	0 to 1E12
Preset value	300 k
Unit	Hz (hertz), dB or second

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:BLIM:MIN 1E4"
20 OUTPUT 717;":CALC1:BLIM:MIN?"
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:BLIM on page 203
:CALC{1-4}:BLIM:MAX on page 208

Equivalent key **[Analysis] - Bandwidth Limit - Min Bandwidth**

:CALC{1-4}:BLIM:REP?

Syntax	:CALCulate{[1] 2 3 4}{[:SElected]:BLIMit:REPort[:DATA]?
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the bandwidth value of the bandwidth test. The data transfer format when this command is executed depends on the setting with the :FORM:DATA command. (Query only)
Query response	{numeric}<newline><^END>
Example of use	<pre>10 OUTPUT 717; ":CALC1:BLIM:REP?" 20 ENTER 717;A</pre>
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286 :FORM:DATA on page 338 :CALC{1-4}:BLIM on page 203
Equivalent key	No equivalent key is available on the front panel.

:CALC{1-4}:CONV

Syntax	:CALCulate{[1] 2 3 4}[:SELeCted]:CONVersion[:STATe] {ON OFF 1 0} :CALCulate{[1] 2 3 4}[:SELeCted]:CONVersion[:STATe]?						
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the parameter conversion function.						
Parameters	<table><tr><th></th><th>Description</th></tr><tr><td>ON or 1</td><td>Turns ON the parameter conversion function.</td></tr><tr><td>OFF or 0 (preset value)</td><td>Turns OFF the parameter conversion function.</td></tr></table>		Description	ON or 1	Turns ON the parameter conversion function.	OFF or 0 (preset value)	Turns OFF the parameter conversion function.
	Description						
ON or 1	Turns ON the parameter conversion function.						
OFF or 0 (preset value)	Turns OFF the parameter conversion function.						
Query response	{1 0}<newline><^END>						
Example of use	10 OUTPUT 717; ":CALC1:CONV ON" 20 OUTPUT 717; ":CALC1:CONV?" 30 ENTER 717;A						
Related commands	:CALC{1-4}:CONV:FUNC on page 212 :CALC{1-4}:PAR{1-4}:SEL on page 286						
Equivalent key	[Analysis] - Conversion - Conversion						

:CALC{1-4}:CONV:FUNC

Syntax	<code>:CALCulate{[1] 2 3 4}[:SELEcted]:CONVersion:FUNcTion {ZREFlection ZTRansmit YREFlection YTRansmit INVersion}</code> <code>:CALCulate{[1] 2 3 4}[:SELEcted]:CONVersion:FUNcTion?</code>												
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), select the parameter after conversion using the parameter conversion function.												
Parameters	<table><tr><th></th><th>Description</th></tr><tr><td>ZREFlection (preset value)</td><td>Specifies the equivalent impedance in reflection measurement.</td></tr><tr><td>ZTRansmit</td><td>Specifies the equivalent impedance in transmission measurement.</td></tr><tr><td>YREFlection</td><td>Specifies the equivalent admittance in reflection measurement.</td></tr><tr><td>YTRansmit</td><td>Specifies the equivalent admittance in transmission measurement.</td></tr><tr><td>INVersion</td><td>Specifies the inverse S-parameter.</td></tr></table>		Description	ZREFlection (preset value)	Specifies the equivalent impedance in reflection measurement.	ZTRansmit	Specifies the equivalent impedance in transmission measurement.	YREFlection	Specifies the equivalent admittance in reflection measurement.	YTRansmit	Specifies the equivalent admittance in transmission measurement.	INVersion	Specifies the inverse S-parameter.
	Description												
ZREFlection (preset value)	Specifies the equivalent impedance in reflection measurement.												
ZTRansmit	Specifies the equivalent impedance in transmission measurement.												
YREFlection	Specifies the equivalent admittance in reflection measurement.												
YTRansmit	Specifies the equivalent admittance in transmission measurement.												
INVersion	Specifies the inverse S-parameter.												
Query response	<code>{ZREF ZTR YREF YTR INV}<newline><^END></code>												
Example of use	<pre>10 OUTPUT 717;":CALC1:CONV:FUNC ZTR" 20 OUTPUT 717;":CALC1:CONV:FUNC?" 30 ENTER 717;A\$</pre>												
Related commands	:CALC{1-4}:CONV on page 211 :CALC{1-4}:PAR{1-4}:SEL on page 286												
Equivalent key	[Analysis] - Conversion - Z:Reflection Z:Transmission Y:Reflection Y:Transmission 1/S												

:CALC{1-4}:CORR:EDEL:TIME

Syntax :CALCulate{[1]|2|3|4}[[:SELEcted]:CORRection:EDELay:TIME <numeric>
:CALCulate{[1]|2|3|4}[[:SELEcted]:CORRection:EDELay:TIME?

Description Sets the electrical delay time of the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command).

Parameters

	<numeric>
Description	Electrical delay time
Range	-10 to 10
Preset value	0
Unit	s (second)

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:CORR:EDEL:TIME 0.2"
20 OUTPUT 717;":CALC1:CORR:EDEL:TIME?"
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key [Scale] - Electrical Delay

:CALC{1-4}:CORR:OFFS:PHAS

Syntax	:CALCulate{[1] 2 3 4}[:SELEcted]:CORRection:OFFSet:PHASe <numeric> :CALCulate{[1] 2 3 4}[:SELEcted]:CORRection:OFFSet:PHASe?										
Description	Sets the phase offset of the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command).										
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Phase offset</td></tr><tr><td>Range</td><td>-360 to 360</td></tr><tr><td>Preset value</td><td>0</td></tr><tr><td>Unit</td><td>° (degree)</td></tr></table> If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.		<numeric>	Description	Phase offset	Range	-360 to 360	Preset value	0	Unit	° (degree)
	<numeric>										
Description	Phase offset										
Range	-360 to 360										
Preset value	0										
Unit	° (degree)										
Query response	{numeric}<newline><^END>										
Example of use	10 OUTPUT 717;":CALC1:CORR:OFFS:PHAS 2.5" 20 OUTPUT 717;":CALC1:CORR:OFFS:PHAS?" 30 ENTER 717;A										
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286										
Equivalent key	[Scale] - Phase Offset										

:CALC{1-4}:DATA:FDAT

Syntax	<pre>:CALCulate{[1] 2 3 4}[:SElected]:DATA:FDATa <numeric1>,...,<numeric NOP×2></pre> <pre>:CALCulate{[1] 2 3 4}[:SElected]:DATA:FDATa?</pre>						
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets/reads out the formatted data array. (It is the data array for which processing such as format has been performed for corrected data array. For details, refer to “Formatted data array” on page 109.) The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.						
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td><numeric n×2-1></td><td>Data (primary value) at the n-th measurement point.</td></tr> <tr> <td><numeric n×2></td><td>Data (secondary value) at the n-th measurement point. Always 0 when the data format is not the Smith chart format or the polar format.</td></tr> </tbody> </table> Where NOP is the number of measurement points and n is an integer between 1 and NOP.		Description	<numeric n×2-1>	Data (primary value) at the n-th measurement point.	<numeric n×2>	Data (secondary value) at the n-th measurement point. Always 0 when the data format is not the Smith chart format or the polar format.
	Description						
<numeric n×2-1>	Data (primary value) at the n-th measurement point.						
<numeric n×2>	Data (secondary value) at the n-th measurement point. Always 0 when the data format is not the Smith chart format or the polar format.						
Query response	{numeric 1},...,{numeric NOP×2}<newline><^END>						
Example of use	<pre>10 DIM A(1:201,1:2)</pre> <pre>20 OUTPUT 717;" :CALC1:DATA:FDAT?"</pre> <pre>30 ENTER 717;A(*)</pre>						
Related commands	<pre>:CALC{1-4}:PAR{1-4}:SEL</pre> on page 286 <pre>:CALC{1-4}:DATA:FMEM</pre> on page 216 <pre>:CALC{1-4}:DATA:SDAT</pre> on page 217 <pre>:FORM:DATA</pre> on page 338						
Equivalent key	No equivalent key is available on the front panel.						

:CALC{1-4}:DATA:FMEM

Syntax :CALCulate{[1]|2|3|4}[:SElected]:DATA:FMEMemory <numeric 1>,...,<numeric NOP×2>
:CALCulate{[1]|2|3|4}[:SElected]:DATA:FMEMemory?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets/reads out the formatted memory array. (It is the data array for which processing such as format has been performed for corrected memory array. For details, refer to “Formatted memory arrays” on page 110.)

The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.

Parameters

	Description
<numeric n×2-1>	Data (primary value) at the n-th measurement point.
<numeric n×2>	Data (secondary value) at the n-th measurement point. Always 0 when the data format is not the Smith chart format or the polar format.

Where NOP is the number of measurement points and n is an integer between 1 and NOP.

Query response {numeric 1},...,{numeric NOP×2}<newline><^END>

Example of use

```
10 DIM A(1:201,1:2)
20 OUTPUT 717;" :CALC1:DATA:FMEM?"
30 ENTER 717;A(*)
```

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:DATA:FDAT on page 215
:CALC{1-4}:DATA:SMEM on page 218
:FORM:DATA on page 338

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:DATA:SDAT

Syntax	:CALCulate{[1] 2 3 4}[:SElected]:DATA:SDATa <numeric 1>,...,<numeric NOP×2> :CALCulate{[1] 2 3 4}[:SElected]:DATA:SDATa?						
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets/reads out the corrected data array. (It is the data array for which processing such as error correction to measured raw data has been performed. For details, refer to “Corrected data arrays” on page 108.) The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.						
Query response	{numeric 1},...,{numeric NOP×2}<newline><^END> <table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>{numeric n×2-1}</td><td>Real part of the data (complex number) at the n-th measurement point.</td></tr> <tr> <td>{numeric n×2}</td><td>Imaginary part of the data (complex number) at the n-th measurement point.</td></tr> </tbody> </table> Where NOP is the number of measurement points and n is an integer between 1 and NOP.		Description	{numeric n×2-1}	Real part of the data (complex number) at the n-th measurement point.	{numeric n×2}	Imaginary part of the data (complex number) at the n-th measurement point.
	Description						
{numeric n×2-1}	Real part of the data (complex number) at the n-th measurement point.						
{numeric n×2}	Imaginary part of the data (complex number) at the n-th measurement point.						
Example of use	<pre>10 DIM A(1:201,1:2) 20 OUTPUT 717;" :CALC1:DATA:SDAT?" 30 ENTER 717;A(*)</pre>						
Related commands	:CALC{1-4}:DATA:SMEM on page 218 :CALC{1-4}:DATA:FDAT on page 215 :FORM:DATA on page 338						
Equivalent key	No equivalent key is available on the front panel.						

:CALC{1-4}:DATA:SMEM

Syntax :CALCulate{[1]|2|3|4}[:SElected]:DATA:SMEMory <numeric 1>,...,<numeric NOP×2>
:CALCulate{[1]|2|3|4}[:SElected]:DATA:SMEMory?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets/reads out the corrected memory array. (It is the copy of the corrected data array when the :CALC{1-4}:MATH:MEM command is executed. For details, refer to “Corrected memory arrays” on page 108.)

The data transfer format when this command is executed depends on the setting with the :FORM:DATA command. (Query only)

Query response {numeric 1},...,{numeric NOP×2}<newline><^END>

	Description
{numeric n×2-1}	Real part of the data (complex number) at the n-th measurement point.
{numeric n×2}	Imaginary part of the data (complex number) at the n-th measurement point.

Where NOP is the number of measurement points and n is an integer between 1 and NOP.

Example of use

```
10  DIM A(1:201,1:2)
20  OUTPUT 717;" :CALC1:DATA:SMEM?"
30  ENTER 717;A( *)
```

Related commands :CALC{1-4}:MATH:MEM on page 281
:CALC{1-4}:DATA:SDAT on page 217
:CALC{1-4}:DATA:FMEM on page 216
:FORM:DATA on page 338

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:FORM

Syntax :CALCulate{[1]|2|3|4}{:SELEcted}:FORMat {MLOGarithmic|PHASe|GDELaY|SLINear|SLOGarithmic|SCOMplex|SMITH|SADMittance|PLINear|PLOGarithmic|POLar|MLINear|SWR|REAL|IMAGinary|UPHase|PPHase}
:CALCulate{[1]|2|3|4}{:SELEcted}:FORMat?

Description Selects the data format of the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command).

Parameters

	Description
MLOGarithmic (preset value)	Specifies the logarithmic magnitude format.
PHASe	Specifies the phase format.
GDELaY	Specifies the group delay format.
SLINear	Specifies the Smith chart format (Lin/Phase).
SLOGarithmic	Specifies the Smith chart format (Log/Phase).
SCOMplex	Specifies the Smith chart format (Real/Imag).
SMITH	Specifies the Smith chart format (R+jX).
SADMittance	Specifies the Smith chart format (G+jB).
PLINear	Specifies the polar format (Lin).
PLOGarithmic	Specifies the polar format (Log).
POLar	Specifies the polar format (Re/Im).
MLINear	Specifies the linear magnitude format.
SWR	Specifies the SWR format.
REAL	Specifies the real format.
IMAGinary	Specifies the imaginary format.
UPHase	Specifies the expanded phase format.
PPHase	Specifies the positive phase format.

Query response {MLOG|PHAS|GDEL|SLIN|SLOG|SCOM|SMIT|SADM|PLIN|PLOG|POL|MLIN|SWR|REAL|IMAG|UPH|PPH}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:FORM SLIN"
20 OUTPUT 717;":CALC1:FORM?"
30 ENTER 717;A\$

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key [Format] - Log Mag|Phase|Group Delay|Lin Mag|SWR|Real|Imaginary|Expand Phase|Positive Phase

[Format] - Smith - Lin/Phase|Log/Phase|Real/Imag|R+jX|G+jB

[Format] - Polar - Lin/Phase|Log/Phase|Real/Imag

:CALC{1-4}:FUNC:DATA?

Syntax :CALCulate{[1][2][3][4][:SELected]:FUNCtion:DATA?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the analysis result of the :CALC{1-4}:FUNC:EXEC command.

The data transfer format when this command is executed depends on the setting with the :FORM:DATA command. (Query only)

Query response {numeric 1},...,{numeric N×2}<newline><^END>

	Description
{numeric n×2-1}	Response value or analysis result of the searched n-th measurement point.
{numeric n×2}	Stimulus value of the searched n-th measurement point. Always set to 0 for the analysis of maximum and minimum values/standard deviation/mean value.

Where N is the number of data pairs (can be read out with :CALC{1-4}:FUNC:POIN? command) and n is an integer between 1 and N.

Example of use

```

10  OUTPUT 717;" :CALC1:FUNC:POIN?"
20  ENTER 717;A
30  REDIM B(1:2*A)
40  OUTPUT 717;" :CALC1:FUNC:DATA?"
50  ENTER 717;B(*)

```

Related commands :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:POIN? on page 227
:CALC{1-4}:PAR{1-4}:SEL on page 286
:FORM:DATA on page 338

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:DOM

Syntax	<code>:CALCulate{[1] 2 3 4}[:SElected]:FUNCtion:DOMain[:STATe] {ON OFF 1 0}</code> <code>:CALCulate{[1] 2 3 4}[:SElected]:FUNCtion:DOMain[:STATe]?</code>						
Description	For channel 1 (:CALC1) to channel 4 (:CALC4), sets whether to use an arbitrary range when executing the analysis with the :CALC{1-4}:FUNC:EXEC command. When the trace coupling is off, the active trace is the target to be set.						
Parameters	<table><tr><th></th><th>Description</th></tr><tr><td>ON or 1</td><td>Specifies an arbitrary range ^{*1}.</td></tr><tr><td>OFF or 0 (preset value)</td><td>Specifies the entire sweep range.</td></tr></table> ^{*1}. Use the :CALC{1-4}:FUNC:DOM:STAR command and the :CALC{1-4}:FUNC:DOM:STOP command to specify a range.		Description	ON or 1	Specifies an arbitrary range ^{*1} .	OFF or 0 (preset value)	Specifies the entire sweep range.
	Description						
ON or 1	Specifies an arbitrary range ^{*1} .						
OFF or 0 (preset value)	Specifies the entire sweep range.						
Query response	{1 0}<newline><^END>						
Example of use	10 OUTPUT 717; ":CALC1:FUNC:DOM ON" 20 OUTPUT 717; ":CALC1:FUNC:DOM?" 30 ENTER 717;A						
Related commands	:CALC{1-4}:FUNC:EXEC on page 225 :CALC{1-4}:FUNC:DOM:COUP on page 223 :CALC{1-4}:FUNC:DOM:STAR on page 224 :CALC{1-4}:FUNC:DOM:STOP on page 225						
Equivalent key	No equivalent key is available on the front panel.						

:CALC{1-4}:FUNC:DOM:COUP

Syntax	:CALCulate{[1] 2 3 4}[:SElected]:FUNCtion:DOMain:COUPle {ON OFF 1 0} :CALCulate{[1] 2 3 4}[:SElected]:FUNCtion:DOMain:COUPle?						
Description	For channel 1 (:CALC1) to channel 4 (:CALC4), specifies whether to set the coupling of the analysis range of the :CALC{1-4}:FUNC:EXEC command for all traces.						
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>ON or 1 (preset value)</td><td>Specifies the analysis range with the trace coupling.</td></tr> <tr> <td>OFF or 0</td><td>Specifies the analysis range for each trace.</td></tr> </tbody> </table>		Description	ON or 1 (preset value)	Specifies the analysis range with the trace coupling.	OFF or 0	Specifies the analysis range for each trace.
	Description						
ON or 1 (preset value)	Specifies the analysis range with the trace coupling.						
OFF or 0	Specifies the analysis range for each trace.						
Query response	{1 0}<newline><^END>						
Example of use	<pre>10 OUTPUT 717; ":CALC1:FUNC:DOM:COUP OFF" 20 OUTPUT 717; ":CALC1:FUNC:DOM:COUP?" 30 ENTER 717;A</pre>						
Related commands	:CALC{1-4}:FUNC:EXEC on page 225						
Equivalent key	No equivalent key is available on the front panel.						

:CALC{1-4}:FUNC:DOM:STAR

Syntax	<code>:CALCulate{[1] 2 3 4}[:SElected]:FUNCtion:DOMain:STARt <numeric></code> <code>:CALCulate{[1] 2 3 4}[:SElected]:FUNCtion:DOMain:STARt?</code>								
Description	For channel 1 (:CALC1) to channel 4 (:CALC4), sets the start value of the analysis range of the :CALC{1-4}:FUNC:EXEC command. When the trace coupling is off, the active trace is the target to be set.								
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Start value of the analysis range</td></tr><tr><td>Preset value</td><td>0</td></tr><tr><td>Unit</td><td>Hz (hertz), dBm or second</td></tr></table>		<numeric>	Description	Start value of the analysis range	Preset value	0	Unit	Hz (hertz), dBm or second
	<numeric>								
Description	Start value of the analysis range								
Preset value	0								
Unit	Hz (hertz), dBm or second								
Query response	{numeric}<newline><^END>								
Example of use	<pre>10 OUTPUT 717; ":CALC1:FUNC:DOM:STAR 1.7E9" 20 OUTPUT 717; ":CALC1:FUNC:DOM:STAR?" 30 ENTER 717;A</pre>								
Related commands	:CALC{1-4}:FUNC:EXEC on page 225 :CALC{1-4}:FUNC:DOM on page 222 :CALC{1-4}:FUNC:DOM:COUP on page 223 :CALC{1-4}:FUNC:DOM:STOP on page 225								
Equivalent key	No equivalent key is available on the front panel.								

:CALC{1-4}:FUNC:DOM:STOP

- Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:FUNCtion:DOMain:STOP <numeric>
:CALCulate{[1]|2|3|4}[:SELEcted]:FUNCtion:DOMain:STOP?
- Description** For channel 1 (:CALC1) to channel 4 (:CALC4), sets the stop value of the analysis range of the :CALC{1-4}:FUNC:EXEC command.
When the trace coupling is off, the active trace is the target to be set.

Parameters

	<numeric>
Description	Stop value of the analysis range
Preset value	0
Unit	Hz (hertz), dBm or second

- Query response** {numeric}<newline><^END>
- Example of use**
10 OUTPUT 717;":CALC1:FUNC:DOM:STOP 1.8E9"
20 OUTPUT 717;":CALC1:FUNC:DOM:STOP?"
30 ENTER 717;A
- Related commands** :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:DOM on page 222
:CALC{1-4}:FUNC:DOM:COUP on page 223
:CALC{1-4}:FUNC:DOM:STAR on page 224
- Equivalent key** No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:EXEC

- Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:FUNCtion:EXECute
- Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), executes the analysis specified with the :CALC{1-4}:FUNC:TYPE command. (No query)
- Example of use** 10 OUTPUT 717;":CALC1:FUNC:EXEC"
- Related commands** :CALC{1-4}:FUNC:TYPE on page 231
:CALC{1-4}:FUNC:DOM on page 222
:CALC{1-4}:PAR{1-4}:SEL on page 286
- Equivalent key** No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:PEXC

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:FUNCtion:PEXCursion <numeric>
:CALCulate{[1]|2|3|4}[:SELEcted]:FUNCtion:PEXCursion?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the lower limit for the peak excursion value when executing the peak search with the :CALC{1-4}:FUNC:EXEC command.

Parameters

	<numeric>
Description	Lower limit for the peak excursion value
Range	0 to 5e8
Preset value	3
Unit	Varies depending on the data format as follows: Logarithmic Magnitude: dB (decibel) Phase, Expand Phase, Positive Phase: ° (degree) Group Delay: s (second) Others: No unit

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:FUNC:PEXC 0.2"
20 OUTPUT 717;":CALC1:FUNC:PEXC?"
30 ENTER 717;A

Related commands :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:PPOL on page 228
:CALC{1-4}:FUNC:TYPE on page 231
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:POIN?

Syntax	:CALCulate{[1] 2 3 4}[:SELected]:FUNCtion:POINts?
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the number of data pairs of the analysis result of the :CALC{1-4}:FUNC:EXEC command. For the analysis of the mean value or the search of the maximum value, 1 is always read out; for the search of all peaks or the search of all targets, the total number of searched measurement points is read out. (Query only)
Query response	{numeric}<newline><^END>
Example of use	<pre>10 OUTPUT 717; ":CALC1:FUNC:POIN?" 20 ENTER 717;A</pre>
Related commands	:CALC{1-4}:FUNC:EXEC on page 225 :CALC{1-4}:FUNC:DATA? on page 221 :CALC{1-4}:PAR{1-4}:SEL on page 286
Equivalent key	No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:PPOL

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:FUNCTion:PPOLarity {POSitive|
NEGative|BOTH}
:CALCulate{[1]|2|3|4}[:SELEcted]:FUNCTion:PPOLarity?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the polarity when performing the peak search with the :CALC{1-4}:FUNC:EXEC command.

Parameters

	Description
POSitive (preset value)	Specifies the positive peak.
NEGative	Specifies the negative peak.
BOTH	Specifies both the positive peak and the negative peak.

Query response {POS|NEG|BOTH}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:FUNC:PPOL BOTH"
20 OUTPUT 717;":CALC1:FUNC:PPOL?"
30 ENTER 717;A\$

Related commands :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:PEXC on page 226
:CALC{1-4}:FUNC:TYPE on page 231
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:TARG

Syntax :CALCulate{[1]|2|3|4}[[:SELEcted]:FUNCtion:TARGet <numeric>
:CALCulate{[1]|2|3|4}[[:SELEcted]:FUNCtion:TARGet?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the target value when performing the target search with the :CALC{1-4}:FUNC:EXEC command.

Parameters

	<numeric>
Description	Target value
Range	-5E8 to 5E8
Preset value	0
Unit	Varies depending on the data format as follows: Logarithmic Magnitude: dB (decibel) Phase, Expand Phase, Positive Phase: ° (degree) Group Delay: s (second) Others: No unit

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:FUNC:TARG -12.5"
20 OUTPUT 717;":CALC1:FUNC:TARG?"
30 ENTER 717;A

Related commands :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:TTR on page 230
:CALC{1-4}:FUNC:TYPE on page 231
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:TTR

Syntax :CALCulate{[1]|2|3|4}[[:SElected]:FUNCtion:TTRansition {POSitive|NEGative|BOTH}]
:CALCulate{[1]|2|3|4}[[:SElected]:FUNCtion:TTRansition?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the transition type when performing the target search with the :CALC{1-4}:FUNC:EXEC command.

Parameters

	Description
POSitive	Specifies positive.
NEGative	Specifies negative.
BOTH (preset value)	Specifies both positive and negative.

Query response {POS|NEG|BOTH}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:FUNC:TTR NEG"
20 OUTPUT 717;":CALC1:FUNC:TTR?"
30 ENTER 717;A\$

Related commands :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:TARG on page 229
:CALC{1-4}:FUNC:TYPE on page 231
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:FUNC:TYPE

Syntax :CALCulate{[1]|2|3|4}{:SElected}:FUNCtion:TYPE {PTPeak| STDEV|MEAN| MAXimum|MINimum|PEAK|APEak|ATARget}
:CALCulate{[1]|2|3|4}{:SElected}:FUNCtion:TYPE?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the type of analysis.

Parameters

	Description
PTPeak (preset value)	Specifies the analysis of the difference between the maximum value and the minimum value (Peak to Peak).
STDEV	Specifies the analysis of the standard deviation.
MEAN	Specifies the analysis of the mean value.
MAXimum	Specifies the search for the maximum value.
MINimum	Specifies the search for the minimum value.
PEAK	Specifies the search for the maximum positive (minimum negative) peak ^{*1} .
APEak	Specifies the search for all peaks ^{*1} .
ATARget	Specifies the search for all targets ^{*2} .

*1. To specify the conditions of the peak, use the :CALC{1-4}:FUNC:PEXC command and the :CALC{1-4}:FUNC:PPOL command.

*2. To specify the conditions of the target, use the :CALC{1-4}:FUNC:TARG command and the :CALC{1-4}:FUNC:TTR command.

Query response {PTP|STDEV|MEAN|MAX|MIN|PEAK|APE|ATAR}<newline><^END>

Example of use
10 OUTPUT 717;" :CALC1:FUNC:TYPE PEAK"
20 OUTPUT 717;" :CALC1:FUNC:TYPE?"
30 ENTER 717;A\$

Related commands :CALC{1-4}:FUNC:EXEC on page 225
:CALC{1-4}:FUNC:PEXC on page 226
:CALC{1-4}:FUNC:PPOL on page 228
:CALC{1-4}:FUNC:TARG on page 229
:CALC{1-4}:FUNC:TTR on page 230
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:LIM

Syntax	:CALCulate{[1] 2 3 4}[:SElected]:LIMit[:STATe] {ON OFF 1 0} :CALCulate{[1] 2 3 4}[:SElected]:LIMit[:STATe]?						
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the limit test function.						
Parameters	<table><tr><th></th><th>Description</th></tr><tr><td>ON or 1</td><td>Turns ON the limit test.</td></tr><tr><td>OFF or 0 (preset value)</td><td>Turns OFF the limit test.</td></tr></table>		Description	ON or 1	Turns ON the limit test.	OFF or 0 (preset value)	Turns OFF the limit test.
	Description						
ON or 1	Turns ON the limit test.						
OFF or 0 (preset value)	Turns OFF the limit test.						
Query response	{1 0}<newline><^END>						
Example of use	10 OUTPUT 717;" :CALC1:LIM ON" 20 OUTPUT 717;" :CALC1:LIM?" 30 ENTER 717;A						
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286 :CALC{1-4}:LIM:DISP on page 235 :DISP:FSIG on page 313						
Equivalent key	[Analysis] - Limit Test - Limit Test						

:CALC{1-4}:LIM:DATA

- Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:LIMit:DATA <numeric 1>,...,<numeric 1+(N×5)>
:CALCulate{[1]|2|3|4}[[:SELEcted]:LIMit:DATA?
- Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the limit table.
- The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.

Parameters

	Description
<numeric 1>	The number of lines. (0 to 100)
<numeric 1+(n×5)-4>	The type of the n-th line. Specify an integer 0 to 2: 0: Off 1: Upper limit line 2: Lower limit line
<numeric 1+(n×5)-3>	The value on the horizontal axis (frequency/power/time) of the start point of the n-th line.
<numeric 1+(n×5)-2>	The value on the horizontal axis (frequency/power/time) of the end point of the n-th line.
<numeric 1+(n×5)-1>	The value on the vertical axis of the start point of the n-th line.
<numeric 1+(n×5)>	The value on the vertical axis of the end point of the n-th line.

Where N is the number of lines (specified with <numeric 1>) and n is an integer between 1 and N.

If you set the number of lines to 0 (clear the limit table), this command needs only <numeric 1> as the parameter.

- Query response** {numeric 1},...,{numeric 1+(N×5)}<newline><^END>
- Example of use**
- ```

10 DIM B(1:2,1:5)
20 OUTPUT 717;":CALC1:LIM:DATA 2,1,1E9,3E9,0,0,2,1E9,3E9,-3,-3"
30 OUTPUT 717;":CALC1:LIM:DATA?"
40 ENTER 717;A,B(*)

10 OUTPUT 717;":CALC1:LIM:DATA 0" ! Clear Limit Table

```
- Related commands** :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:LIM on page 232  
:CALC{1-4}:LIM:DISP on page 235  
:FORM:DATA on page 338

Equivalent key      **[Analysis] - Limit Test - Edit Limit Line**

## :CALC{1-4}:LIM:DISP

|             |                                                                                                                                                             |
|-------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :CALCulate{[1] 2 3 4}[:SELEcted]:LIMit:DISPlay[:STATe] {ON OFF 1 0}<br>:CALCulate{[1] 2 3 4}[:SELEcted]:LIMit:DISPlay[:STATe]?                              |
| Description | For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the limit line display. |
| Parameters  |                                                                                                                                                             |

|                         | Description                       |
|-------------------------|-----------------------------------|
| ON or 1                 | Turns ON the limit line display.  |
| OFF or 0 (preset value) | Turns OFF the limit line display. |

|                  |                                                                                            |
|------------------|--------------------------------------------------------------------------------------------|
| Query response   | {1 0}<newline><^END>                                                                       |
| Example of use   | 10 OUTPUT 717; ":CALC1:LIM:DISP ON"<br>20 OUTPUT 717; ":CALC1:LIM:DISP?"<br>30 ENTER 717;A |
| Related commands | :CALC{1-4}:LIM on page 232<br>:CALC{1-4}:PAR{1-4}:SEL on page 286                          |
| Equivalent key   | <b>[Analysis] - Limit Test - Limit Line</b>                                                |

**:CALC{1-4}:LIM:DISP:CLIP**

Syntax :CALCulate{[1]|2|3|4}[:SElected]:LIMit:DISPlay:CLIP {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[:SElected]:LIMit:DISPlay:CLIP?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), specifies whether to display the part of the limit line(s) that is not used for evaluation.

Parameters

|                        | Description                         |
|------------------------|-------------------------------------|
| ON or 1 (preset value) | Displays the clipped limit line(s). |
| OFF or 0               | Displays the entire limit line(s).  |

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:LIM:DISP:CLIP OFF"  
20 OUTPUT 717;":CALC1:LIM:DISP:CLIP?"  
30 ENTER 717;A

Related commands :CALC{1-4}:LIM on page 232  
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Analysis] - Limit Test - Clip Lines**

## :CALC{1-4}:LIM:FAIL?

**Syntax** :CALCulate{[1][2][3][4][:SELEcted]:LIMit:FAIL?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the limit test result. (Query only)

**Query response** {1|0}<newline><^END>

|   | Description                    |
|---|--------------------------------|
| 1 | The limit test result is FAIL. |
| 0 | The limit test result is PASS. |

When the limit test is set to OFF, 0 is always read out.

**Example of use** 10 OUTPUT 717;" :CALC1:LIM:FAIL?"  
20 ENTER 717;A

**Related commands** :CALC{1-4}:LIM on page 232  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** No equivalent key is available on the front panel.

## :CALC{1-4}:LIM:OFFS:AMPL

### Syntax

```
:CALCulate{[1]|2|3|4}[:SELeCted]:LIMit:OFFSet:AMPLitude <numeric>
:CALCulate{[1]|2|3|4}[:SELeCted]:LIMit:OFFSet:AMPLitude?
```

### Description

For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the limit line amplitude offset.

The setting of the limit line doesn't change even if the offset value is changed.

### Parameters

|              | <numeric>                                                 |
|--------------|-----------------------------------------------------------|
| Description  | The limit line amplitude offset value for the limit test. |
| Range        | -5E8 to 5E8                                               |
| Preset value | 0                                                         |
| Unit         | dB                                                        |

### Query response

```
{numeric}<newline><^END>
```

### Example of use

```
10 OUTPUT 717; ":CALC1:LIM:OFFS:AMPL -10"
20 OUTPUT 717; ":CALC1:LIM:OFFS:AMPL?"
30 ENTER 717;A
```

### Related commands

```
:CALC{1-4}:LIM on page 232
:CALC{1-4}:LIM:OFFS:MARK on page 239
:CALC{1-4}:LIM:OFFS:STIM on page 240
```

### Equivalent key

**[Analysis] - Limit Test - Limit Line Offsets - Amplitude Offset**

## :CALC{1-4}:LIM:OFFS:MARK

|                  |                                                                                                                                                                                                                                                                                                                                                      |
|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[:SELEcted]:LIMit:OFFSet:MARKer                                                                                                                                                                                                                                                                                                 |
| Description      | <p>For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the active marker value to amplitude offset using the limit line.</p> <p>The setting of the limit line does not change even if the offset value is changed.</p> <p>When the markers are not displayed, this command does not operate.</p> |
| Example of use   | 10 OUTPUT 717; ":CALC1:LIM:OFFS:MARK"                                                                                                                                                                                                                                                                                                                |
| Related commands | <p>:CALC{1-4}:LIM on page 232</p> <p>:CALC{1-4}:LIM:OFFS:AMPL on page 238</p> <p>:CALC{1-4}:LIM:OFFS:STIM on page 240</p>                                                                                                                                                                                                                            |
| Equivalent key   | <b>[Analysis] - Limit Test - Limit Line Offsets - Marker -&gt; Amplitude Offset</b>                                                                                                                                                                                                                                                                  |

**:CALC{1-4}:LIM:OFFS:STIM**

| Syntax           | <code>:CALCulate{[1] 2 3 4}[:SELEcted]:LIMit:OFFSet:STIMulus &lt;numeric&gt;</code><br><code>:CALCulate{[1] 2 3 4}[:SELEcted]:LIMit:OFFSet:STIMulus?</code>                                                                                                                              |  |           |             |                                              |       |               |              |   |      |                           |
|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-----------|-------------|----------------------------------------------|-------|---------------|--------------|---|------|---------------------------|
| Description      | <p>For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the stimulus offset of the limit line.</p> <p>The setting of the limit line doesn't change even if the offset value is changed.</p>                                           |  |           |             |                                              |       |               |              |   |      |                           |
| Parameters       | <table><tr><th></th><th>&lt;numeric&gt;</th></tr><tr><td>Description</td><td>The stimulus offset value of the limit line.</td></tr><tr><td>Range</td><td>-1E12 to 1E12</td></tr><tr><td>Preset value</td><td>0</td></tr><tr><td>Unit</td><td>Hz (hertz), dBm or second</td></tr></table> |  | <numeric> | Description | The stimulus offset value of the limit line. | Range | -1E12 to 1E12 | Preset value | 0 | Unit | Hz (hertz), dBm or second |
|                  | <numeric>                                                                                                                                                                                                                                                                                |  |           |             |                                              |       |               |              |   |      |                           |
| Description      | The stimulus offset value of the limit line.                                                                                                                                                                                                                                             |  |           |             |                                              |       |               |              |   |      |                           |
| Range            | -1E12 to 1E12                                                                                                                                                                                                                                                                            |  |           |             |                                              |       |               |              |   |      |                           |
| Preset value     | 0                                                                                                                                                                                                                                                                                        |  |           |             |                                              |       |               |              |   |      |                           |
| Unit             | Hz (hertz), dBm or second                                                                                                                                                                                                                                                                |  |           |             |                                              |       |               |              |   |      |                           |
| Query response   | {numeric}<newline><^END>                                                                                                                                                                                                                                                                 |  |           |             |                                              |       |               |              |   |      |                           |
| Example of use   | <pre>10  OUTPUT 717; ":CALC1:LIM:OFFS:STIM 5E3" 20  OUTPUT 717; ":CALC1:LIM:OFFS:STIM?" 30  ENTER 717;A</pre>                                                                                                                                                                            |  |           |             |                                              |       |               |              |   |      |                           |
| Related commands | <p>:CALC{1-4}:LIM on page 232</p> <p>:CALC{1-4}:LIM:OFFS:AMPL on page 238</p> <p>:CALC{1-4}:LIM:OFFS:MARK on page 239</p>                                                                                                                                                                |  |           |             |                                              |       |               |              |   |      |                           |
| Equivalent key   | <b>[Analysis] - Limit Test - Limit Line Offsets - Stimulus Offset</b>                                                                                                                                                                                                                    |  |           |             |                                              |       |               |              |   |      |                           |

## :CALC{1-4}:LIM:REP:ALL?

**Syntax** :CALCulate{[1]|2|3|4}[:SElected]:LIMit:REPort:ALL?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the bandwidth test results (stimulus value, limit test result, upper limit value, lower limit value of all measurement points).  
  
The data transfer format when this command is executed depends on the setting with the :FORM:DATA command. (Query only)

**Query Response** {numeric 1},...,{numeric N×4}<newline><^END>

|                 | Description                                                                                        |
|-----------------|----------------------------------------------------------------------------------------------------|
| <numeric n×4-3> | The stimulus value for the measurement point.                                                      |
| <numeric n×4-2> | The limit test result.<br>Specify an integer -1 to 1:<br>0: Fail<br>1: Pass<br>-1: No limit        |
| <numeric n×4-1> | The upper limit value at the measurement point. (If there is no limit at this point, reads out 0.) |
| <numeric n×4>   | The lower limit value at the measurement point. (If there is no limit at this point, reads out 0.) |

Where N is the number of measurement points (specified with the :SENS{1-4}:SWE:POIN command) and n is an integer between 1 and N.

**Example of use**

```

10 OUTPUT 717;" :SENS1:SWE:POIN?"
20 ENTER 717;A
30 REDIM B(1:4*A)
40 OUTPUT 717;" :CALC1:LIM:REP:ALL?"
50 ENTER 717;B(*)

```

**Related commands** :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:LIM on page 232  
:CALC{1-4}:LIM:REP? on page 242  
:CALC{1-4}:LIM:REP:POIN? on page 242

**Equivalent key** No equivalent key is available on the front panel.

## **:CALC{1-4}:LIM:REP?**

|                  |                                                                                                                                                                                                                                                                                                                                                                                     |
|------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[:SELected]:LIMit:REPort[:DATA]?                                                                                                                                                                                                                                                                                                                               |
| Description      | <p>For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the stimulus values (frequency, power level or time) at all the measurement point that failed the limit test.</p> <p>The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.(Query only)</p> |
| Query response   | <p>{numeric 1},...,{numeric N}&lt;newline&gt;&lt;^END&gt;</p> <p>Where N is the number of the measurement points that failed (can be read out with the :CALC{1-4}:LIM:REP:POIN? command).</p>                                                                                                                                                                                       |
| Example of use   | <pre>10  OUTPUT 717; ":CALC1:LIM:REP:POIN?" 20  ENTER 717;A 30  REDIM B(1:A) 40  OUTPUT 717; ":CALC1:LIM:REP?" 50  ENTER 717;B( *)</pre>                                                                                                                                                                                                                                            |
| Related commands | <p>:CALC{1-4}:PAR{1-4}:SEL on page 286</p> <p>:FORM:DATA on page 338</p> <p>:CALC{1-4}:LIM:REP:POIN? on page 242</p> <p>:CALC{1-4}:LIM on page 232</p>                                                                                                                                                                                                                              |
| Equivalent key   | No equivalent key is available on the front panel.                                                                                                                                                                                                                                                                                                                                  |

## **:CALC{1-4}:LIM:REP:POIN?**

|                  |                                                                                                                                                                                                                       |
|------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[:SELected]:LIMit:REPort:POINts?                                                                                                                                                                 |
| Description      | <p>For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the number of the measurement points that failed the limit test. (Query only)</p> |
| Query response   | {numeric}<newline><^END>                                                                                                                                                                                              |
| Example of use   | <pre>10  OUTPUT 717; ":CALC1:LIM:REP:POIN?" 20  ENTER 717;A</pre>                                                                                                                                                     |
| Related commands | <p>:CALC{1-4}:PAR{1-4}:SEL on page 286</p> <p>:CALC{1-4}:LIM on page 232</p>                                                                                                                                          |
| Equivalent key   | No equivalent key is available on the front panel.                                                                                                                                                                    |

## :CALC{1-4}:MARK:BWID

|             |                                                                                                                                                                          |
|-------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :CALCulate{[1] 2 3 4}[:SELEcted]:MARKer:BWIDth[:STATe] {ON OFF 1 0}<br>:CALCulate{[1] 2 3 4}[:SELEcted]:MARKer:BWIDth[:STATe]?                                           |
| Description | For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the bandwidth search result display. |
| Parameters  |                                                                                                                                                                          |

|                         | Description                                    |
|-------------------------|------------------------------------------------|
| ON or 1                 | Turns ON the bandwidth search result display.  |
| OFF or 0 (preset value) | Turns OFF the bandwidth search result display. |

|                  |                                                                                                                                   |
|------------------|-----------------------------------------------------------------------------------------------------------------------------------|
| Query response   | {1 0}<newline><^END>                                                                                                              |
| Example of use   | 10 OUTPUT 717; ":CALC1:MARK:BWID ON"<br>20 OUTPUT 717; ":CALC1:MARK:BWID?"<br>30 ENTER 717;A                                      |
| Related commands | :CALC{1-4}:MARK{1-10}:BWID:DATA? on page 265<br>:CALC{1-4}:MARK{1-10}:BWID:THR on page 266<br>:CALC{1-4}:PAR{1-4}:SEL on page 286 |
| Equivalent key   | <b>[Marker Search] - Bandwidth</b>                                                                                                |

**:CALC{1-4}:MARK:COUP**

| Syntax                 | <code>:CALCulate{[1] 2 3 4}[:SElected]:MARKer:COUPle {ON OFF 1 0}</code><br><code>:CALCulate{[1] 2 3 4}[:SElected]:MARKer:COUPle?</code>                                                             |  |             |                        |                               |          |                                |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-------------|------------------------|-------------------------------|----------|--------------------------------|
| Description            | For channel 1 (:CALC1) to channel 4 (:CALC4), turns ON/OFF the marker coupling between traces.                                                                                                       |  |             |                        |                               |          |                                |
| Parameters             | <table><tr><th></th><th>Description</th></tr><tr><td>ON or 1 (preset value)</td><td>Turns ON the marker coupling.</td></tr><tr><td>OFF or 0</td><td>Turns OFF the marker coupling.</td></tr></table> |  | Description | ON or 1 (preset value) | Turns ON the marker coupling. | OFF or 0 | Turns OFF the marker coupling. |
|                        | Description                                                                                                                                                                                          |  |             |                        |                               |          |                                |
| ON or 1 (preset value) | Turns ON the marker coupling.                                                                                                                                                                        |  |             |                        |                               |          |                                |
| OFF or 0               | Turns OFF the marker coupling.                                                                                                                                                                       |  |             |                        |                               |          |                                |
| Query response         | {1 0}<newline><^END>                                                                                                                                                                                 |  |             |                        |                               |          |                                |
| Example of use         | 10    OUTPUT 717;" :CALC1:MARK:COUP OFF"<br>20    OUTPUT 717;" :CALC1:MARK:COUP?"<br>30    ENTER 717;A                                                                                               |  |             |                        |                               |          |                                |
| Equivalent key         | <b>[Marker Fctn] - Couple</b>                                                                                                                                                                        |  |             |                        |                               |          |                                |

## :CALC{1-4}:MARK:FUNC:DOM

**Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:FUNCTion:DOMain[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:FUNCTion:DOMain[:STATe]?

**Description** For channel 1 (:CALC1) to channel 4 (:CALC4), sets whether to use an arbitrary range when executing the marker search.

When the trace coupling is off, the active trace is the target to be set.

### Parameters

|                         | Description                                  |
|-------------------------|----------------------------------------------|
| ON or 1                 | Specifies an arbitrary range <sup>*1</sup> . |
| OFF or 0 (preset value) | Specifies the entire sweep range.            |

<sup>\*1</sup>. Use the :CALC{1-4}:MARK:FUNC:DOM:STAR command and the :CALC{1-4}:MARK:FUNC:DOM:STOP command to specify a range.

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:MARK:FUNC:DOM ON"  
20 OUTPUT 717; ":CALC1:MARK:FUNC:DOM?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:MARK{1-10}:FUNC:EXEC on page 268  
:CALC{1-4}:MARK:FUNC:DOM:COUP on page 246  
:CALC{1-4}:MARK:FUNC:DOM:STAR on page 247  
:CALC{1-4}:MARK:FUNC:DOM:STOP on page 248

**Equivalent key** [Marker Search] - Search Range - Search Range [ON/OFF]

## :CALC{1-4}:MARK:FUNC:DOM:COUP

**Syntax** :CALCulate{[1]|2|3|4}[:SElected]:MARKer:FUNCtion:DOMain:COUPle {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[:SElected]:MARKer:FUNCtion:DOMain:COUPle?

**Description** For channel 1 (:CALC1) to channel 4 (:CALC4), specifies whether to set the coupling of the marker search range for all traces.

**Parameters**

|                        | Description                                         |
|------------------------|-----------------------------------------------------|
| ON or 1 (preset value) | Specifies the search range with the trace coupling. |
| OFF or 0               | Specifies the search range for each trace.          |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:MARK:FUNC:DOM:COUP OFF"  
20 OUTPUT 717; ":CALC1:MARK:FUNC:DOM:COUP?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:MARK:FUNC:DOM on page 245  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Search Range - Couple**

## :CALC{1-4}:MARK:FUNC:DOM:STAR

|                  |                                                                                                                                                                                                                                                        |  |           |             |                                     |              |   |      |                           |
|------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-----------|-------------|-------------------------------------|--------------|---|------|---------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[[:SELEcted]:MARKer:FUNCTion:DOMain:STARt <numeric><br>:CALCulate{[1] 2 3 4}[[:SELEcted]:MARKer:FUNCTion:DOMain:STARt?                                                                                                            |  |           |             |                                     |              |   |      |                           |
| Description      | For channel 1 (:CALC1) to channel 4 (:CALC4), sets the start value of the marker search range.<br><br>When the trace coupling is off, the active trace is the target to be set.                                                                        |  |           |             |                                     |              |   |      |                           |
| Parameters       | <table border="1"> <tr> <td></td><td>&lt;numeric&gt;</td></tr> <tr> <td>Description</td><td>The start value of the search range</td></tr> <tr> <td>Preset value</td><td>0</td></tr> <tr> <td>Unit</td><td>Hz (hertz), dBm or second</td></tr> </table> |  | <numeric> | Description | The start value of the search range | Preset value | 0 | Unit | Hz (hertz), dBm or second |
|                  | <numeric>                                                                                                                                                                                                                                              |  |           |             |                                     |              |   |      |                           |
| Description      | The start value of the search range                                                                                                                                                                                                                    |  |           |             |                                     |              |   |      |                           |
| Preset value     | 0                                                                                                                                                                                                                                                      |  |           |             |                                     |              |   |      |                           |
| Unit             | Hz (hertz), dBm or second                                                                                                                                                                                                                              |  |           |             |                                     |              |   |      |                           |
| Query response   | {numeric}<newline><^END>                                                                                                                                                                                                                               |  |           |             |                                     |              |   |      |                           |
| Example of use   | <pre> 10  OUTPUT 717; ":CALC1:MARK:FUNC:DOM:STAR 1.7E9" 20  OUTPUT 717; ":CALC1:MARK:FUNC:DOM:STAR?" 30  ENTER 717;A </pre>                                                                                                                            |  |           |             |                                     |              |   |      |                           |
| Related commands | :CALC{1-4}:MARK{1-10}:FUNC:EXEC on page 268<br>:CALC{1-4}:MARK:FUNC:DOM on page 245<br>:CALC{1-4}:MARK:FUNC:DOM:STOP on page 248                                                                                                                       |  |           |             |                                     |              |   |      |                           |
| Equivalent key   | <b>[Marker Search] - Search Range - Start</b>                                                                                                                                                                                                          |  |           |             |                                     |              |   |      |                           |

**:CALC{1-4}:MARK:FUNC:DOM:STOP**

|                  |                                                                                                                                                                                                                                   |  |           |             |                                    |              |   |      |                           |
|------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-----------|-------------|------------------------------------|--------------|---|------|---------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[:SElected]:MARKer:FUNCtion:DOMain:STOP <numeric><br>:CALCulate{[1] 2 3 4}[:SElected]:MARKer:FUNCtion:DOMain:STOP?                                                                                           |  |           |             |                                    |              |   |      |                           |
| Description      | For channel 1 (:CALC1) to channel 4 (:CALC4), sets the stop value of the marker search range.<br><br>When the trace coupling is off, the active trace is the target to be set.                                                    |  |           |             |                                    |              |   |      |                           |
| Parameters       | <table><tr><td></td><td>&lt;numeric&gt;</td></tr><tr><td>Description</td><td>The stop value of the search range</td></tr><tr><td>Preset value</td><td>0</td></tr><tr><td>Unit</td><td>Hz (hertz), dBm or second</td></tr></table> |  | <numeric> | Description | The stop value of the search range | Preset value | 0 | Unit | Hz (hertz), dBm or second |
|                  | <numeric>                                                                                                                                                                                                                         |  |           |             |                                    |              |   |      |                           |
| Description      | The stop value of the search range                                                                                                                                                                                                |  |           |             |                                    |              |   |      |                           |
| Preset value     | 0                                                                                                                                                                                                                                 |  |           |             |                                    |              |   |      |                           |
| Unit             | Hz (hertz), dBm or second                                                                                                                                                                                                         |  |           |             |                                    |              |   |      |                           |
| Query response   | {numeric}<newline><^END>                                                                                                                                                                                                          |  |           |             |                                    |              |   |      |                           |
| Example of use   | 10 OUTPUT 717; ":CALC1:MARK:FUNC:DOM:STOP 1.8E9"<br>20 OUTPUT 717; ":CALC1:MARK:FUNC:DOM:STOP?"<br>30 ENTER 717;A                                                                                                                 |  |           |             |                                    |              |   |      |                           |
| Related commands | :CALC{1-4}:MARK{1-10}:FUNC:EXEC on page 268<br>:CALC{1-4}:MARK:FUNC:DOM on page 245<br>:CALC{1-4}:MARK:FUNC:DOM:STAR on page 247                                                                                                  |  |           |             |                                    |              |   |      |                           |
| Equivalent key   | <b>[Marker Search] - Search Range - Stop</b>                                                                                                                                                                                      |  |           |             |                                    |              |   |      |                           |

## :CALC{1-4}:MARK:FUNC:MULT:PEXC

**Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:FUNCtion: MULTi:PEXCursion <numeric>  
:CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:FUNCtion: MULTi:PEXCursion?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the lower limit for the peak excursion value of the multi peak search.

### Parameters

|              | <numeric>                                                                                                                                                                               |
|--------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Description  | Lower limit for the peak excursion value                                                                                                                                                |
| Range        | 0 to 5E8                                                                                                                                                                                |
| Preset value | 3                                                                                                                                                                                       |
| Unit         | Varies depending on the data format as follows:<br>Logarithmic Magnitude: dB (decibel)<br>Phase, Expand Phase, Positive Phase: ° (degree)<br>Group Delay: s (second)<br>Others: No unit |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":CALC1:MARK:FUNC:MULT:PEXC 0.2"  
20 OUTPUT 717;":CALC1:MARK:FUNC:MULT:PEXC?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:MARK:FUNC:MULT:PPOL on page 250  
:CALC{1-4}:MARK:FUNC:MULT:TYPE on page 254  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** [Marker Search] - Multi Peak - Peak Excursion

## :CALC{1-4}:MARK:FUNC:MULT:PPOL

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCtion: MULTi: PPOLarity  
{POSitive|NEGative|BOTH}

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCtion: MULTi: PPOLarity?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the polarity of the peak to be searched with the multi peak search.

### Parameters

|                         | Description                                             |
|-------------------------|---------------------------------------------------------|
| POSitive (preset value) | Specifies the positive peak.                            |
| NEGative                | Specifies the negative peak.                            |
| BOTH                    | Specifies both the positive peak and the negative peak. |

**Query response** {POS|NEG|BOTH}<newline><^END>

**Example of use**

```

10 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:PPOL NEG"
20 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:PPOL?"
30 ENTER 717;A$

```

**Related commands** :CALC{1-4}:MARK:FUNC:MULT:PEXC on page 249

:CALC{1-4}:MARK:FUNC:MULT:TYPE on page 254

:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Multi Peak - Peak Polarity**

## :CALC{1-4}:MARK:FUNC:MULT:TARG

**Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:FUNCtion: MULTi: TARGet <numeric>  
:CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:FUNCtion: MULTi: TARGet?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the target value to be searched with the multi target search.

### Parameters

|              |                                                                                                                                                                                         |
|--------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|              | <numeric>                                                                                                                                                                               |
| Description  | Target value for target search                                                                                                                                                          |
| Range        | -5E8 to 5E8                                                                                                                                                                             |
| Preset value | 0                                                                                                                                                                                       |
| Unit         | Varies depending on the data format as follows:<br>Logarithmic Magnitude: dB (decibel)<br>Phase, Expand Phase, Positive Phase: ° (degree)<br>Group Delay: s (second)<br>Others: No unit |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**

```
10 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:TARG -12.5"
20 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:TARG?"
30 ENTER 717;A
```

**Related commands** :CALC{1-4}:MARK:FUNC:MULT:TTR on page 253  
:CALC{1-4}:MARK:FUNC:MULT:TYPE on page 254  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Multi Target - Target Value**

## :CALC{1-4}:MARK:FUNC:MULT:TRAC

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCCtion: MULTi: TRACking  
{ON|OFF|1|0}

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCCtion: MULTi: TRACking?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the search tracking (function to repeat the search for each sweep) of the multi target or peak search.

**Parameters**

|                         | Description                    |
|-------------------------|--------------------------------|
| ON or 1                 | Turns ON the search tracking.  |
| OFF or 0 (preset value) | Turns OFF the search tracking. |

**Query response** {1|0}<newline><^END>

**Example of use**

```

10 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:TRAC ON"
20 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:TRAC?"
30 ENTER 717;A

```

**Related commands** :CALC{1-4}:MARK:FUNC:MULT:TYPE on page 254  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Tracking**

## :CALC{1-4}:MARK:FUNC:MULT:TTR

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCtion: MULTi: TTRansition {POSitive|NEGative|BOTH}

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCtion: MULTi: TTRansition?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the transition type when performing the multi target search.

### Parameters

|                     | Description                           |
|---------------------|---------------------------------------|
| POSitive            | Specifies positive.                   |
| NEGative            | Specifies negative.                   |
| BOTH (preset value) | Specifies both positive and negative. |

**Query response** {POS|NEG|BOTH}<newline><^END>

**Example of use**

```

10 OUTPUT 717;" :CALC1:MARK1:FUNC:MULT:TTR NEG"
20 OUTPUT 717;" :CALC1:MARK1:FUNC:MULT:TTR?"
30 ENTER 717;A$

```

**Related commands** :CALC{1-4}:MARK:FUNC:MULT:TARG on page 251

:CALC{1-4}:MARK:FUNC:MULT:TYPE on page 254

:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Multi Target - Target Transition**

## :CALC{1-4}:MARK:FUNC:MULT:TYPE

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCtion:MULTi:  
:TYPE {MAXimum|MINimum|PEAK|LPEak|RPEak|TARGet|LTARget|RTARget}  
:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:FUNCtion: MULTi  
:TYPE?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects and turns on the multi search type.

### Parameters

|        | Description                     |
|--------|---------------------------------|
| OFF    | Turn off the multi search mode  |
| PEAK   | Turn on the multi peak search   |
| TARGet | Turn on the multi target search |

**Query response** {OFF|PEAK|TARG}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:TYPE PEAK"  
20 OUTPUT 717; ":CALC1:MARK1:FUNC:MULT:TYPE?"  
30 ENTER 717;A\$

**Related commands** :CALC{1-4}:MARK:FUNC:MULT:PEXC on page 249  
:CALC{1-4}:MARK:FUNC:MULT:PPOL on page 250  
:CALC{1-4}:MARK:FUNC:MULT:TARG on page 251  
:CALC{1-4}:MARK:FUNC:MULT:TRAC on page 252  
:CALC{1-4}:MARK:FUNC:MULT:TTR on page 253  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Multi Peak - Search Multi Peak**  
**[Marker Search] - Multi Target - Search Multi Target**

## :CALC{1-4}:MARK:MATH:FLAT

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:MATH:FLATness[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:MATH:FLATness[:STATe]?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turn on and off the marker flatness function.

**Parameters**

|                            | Description                    |
|----------------------------|--------------------------------|
| ON or 1                    | Turns ON the marker flatness.  |
| OFF or 0<br>(preset value) | Turns OFF the marker flatness. |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717;":CALC1:MARK:MATH:FLAT ON"  
20 OUTPUT 717;":CALC1:MARK:MATH:FLAT?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:MARK:MATH:FLAT:DATA? on page 256

**Equivalent key** [Marker Fctn] - Flatness

**:CALC{1-4}:MARK:MATH:FLAT:DATA?**

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:MATH:FLATness:DATA?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), returns marker flatness data.

Query response

|           | Description |
|-----------|-------------|
| Numeric 1 | Span        |
| Numeric 2 | Gain        |
| Numeric 3 | Slope       |
| Numeric 4 | Flatness    |

{numeric1}{numeric2}{numeric3}{numeric4}<newline><^END>

Example of use 10 OUTPUT 717;" :CALC1:MARK:MATH:FLAT:DATA?"  
20 ENTER 717;A,B,C,D

Related commands :CALC{1-4}:MARK:MATH:FLAT on page 255

Equivalent key No equivalent key is available on the front panel.

## :CALC{1-4}:MARK:MATH:FST

**Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:MATH:FSTatistics[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:MATH:FSTatistics[:STATe]?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turn on and off the filter statistics.

**Parameters**

|                            | Description                      |
|----------------------------|----------------------------------|
| ON or 1                    | Turns ON the filter statistics.  |
| OFF or 0<br>(preset value) | Turns OFF the filter statistics. |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717;":CALC1:MARK:MATH:FST ON"  
20 OUTPUT 717;":CALC1:MARK:MATH:FST?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:MARK:MATH:FST:DATA? on page 258

**Equivalent key** [Marker Fctn] - RF Filter Stats

**:CALC{1-4}:MARK:MATH:FST:DATA?**

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:MATH:FSTatistics:DATA?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), returns filter statistics data.

Query response

|           | Description |
|-----------|-------------|
| Numeric 1 | Loss        |
| Numeric 2 | Ripple      |
| Numeric 3 | Attenuation |

{numeric1}{numeric2}{numeric3}<newline><^END>

Example of use 10 OUTPUT 717;" :CALC1:MARK:MATH:FST:DATA?"  
20 ENTER 717;A, B, C

Related commands :CALC{1-4}:MARK:MATH:FST on page 257

Equivalent key No equivalent key is available on the front panel.

## :CALC{1-4}:MARK:MATH:STAT

**Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:MATH:STATistics[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:MATH:STATistics[:STATe]?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turn on and off the marker statistics function.

**Parameters**

|                            | Description                      |
|----------------------------|----------------------------------|
| ON or 1                    | Turns ON the marker statistics.  |
| OFF or 0<br>(preset value) | Turns OFF the marker statistics. |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:MARK:MATH:STAT ON"  
20 OUTPUT 717; ":CALC1:MARK:MATH:STAT?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:MARK:MATH:STAT:DATA? on page 260

**Equivalent key** [Marker Fctn] - Statistics

**:CALC{1-4}:MARK:MATH:STAT:DATA?**

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:MATH:STATistics:DATA?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), returns marker statistics data.

Query response

|           | Description        |
|-----------|--------------------|
| Numeric 1 | Span               |
| Numeric 2 | Average            |
| Numeric 3 | Standard Deviation |
| Numeric 4 | Peak to Peak       |

{numeric1}{numeric2}{numeric3}{numeric4}<newline><^END>

Example of use 10 OUTPUT 717;" :CALC1:MARK:MATH:STAT:DATA?"  
20 ENTER 717;A,B,C,D

Related commands :CALC{1-4}:MARK:MATH:STAT on page 259

Equivalent key No equivalent key is available on the front panel.

## :CALC{1-4}:MARK:NOTC

**Syntax** :CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:NOTCh[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[[:SELEcted]:MARKer:NOTCh[:STATe]?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the notch search result display.

**Parameters**

|                         | Description                                |
|-------------------------|--------------------------------------------|
| ON or 1                 | Turns ON the notch search result display.  |
| OFF or 0 (preset value) | Turns OFF the notch search result display. |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:MARK:NOTC ON"  
20 OUTPUT 717; ":CALC1:MARK:NOTC?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:MARK{1-10}:NOTC:DATA? on page 276  
:CALC{1-4}:MARK{1-10}:NOTC:THR on page 277

**Equivalent key** **[Marker Search] - Notch**

**:CALC{1-4}:MARK:REF**

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:REFerence[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer:REFerence[:STATe]?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the reference marker mode.  
The reference marker mode is turned on or off when you turn on or off the display of the reference marker.

Parameters

|                         | Description                          |
|-------------------------|--------------------------------------|
| ON or 1                 | Turns ON the reference marker mode.  |
| OFF or 0 (preset value) | Turns OFF the reference marker mode. |

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:MARK:REF ON"  
20 OUTPUT 717;":CALC1:MARK:REF?"  
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:MARK{1-10} on page 263

Equivalent key **[Marker] - Ref Maker Mode**

## :CALC{1-4}:MARK{1-10}

|             |                                                                                                                                                                                                                                                                                                                                             |
|-------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :CALCulate{[1] 2 3 4}{:SELected}:MARKer{[1] 2 3 4 5 6 7 8 9 10}{[:STATe]<br>{ON OFF 1 0}}<br><br>:CALCulate{[1] 2 3 4}{:SELected}:MARKer{[1] 2 3 4 5 6 7 8 9 10}{[:STATe]}?                                                                                                                                                                 |
| Description | For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the display of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).<br><br>The display of the reference marker is turned on or off when you turn on or off the reference marker mode. |

### Parameters

|                         | Description                          |
|-------------------------|--------------------------------------|
| ON or 1                 | Turns ON the display of the marker.  |
| OFF or 0 (preset value) | Turns OFF the display of the marker. |

|                  |                                                                                                                                                                                                |
|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Query response   | {1 0}<newline><^END>                                                                                                                                                                           |
| Example of use   | 10 OUTPUT 717;":CALC1:MARK1 ON"<br>20 OUTPUT 717;":CALC1:MARK1?"<br>30 ENTER 717;A                                                                                                             |
| Related commands | :CALC{1-4}:PAR{1-4}:SEL on page 286<br>:CALC{1-4}:MARK:REF on page 262                                                                                                                         |
| Equivalent key   | When turning ON the display of the marker<br><b>[Marker] - Marker 1 Marker 2 Marker 3 Marker 4 Ref Marker</b><br><b>[Marker] - More Markers - Marker 5 Marker 6 Marker 7 Marker 8 Marker 9</b> |

|             |                                                                                                                                                                                                                                                                                                          |
|-------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>NOTE</b> | When performing the operation from the front panel, a marker set to ON is automatically set to the active marker.<br><br>When turning OFF the display of the marker<br><b>[Marker] - Clear Marker Menu - Marker 1 Marker 2 Marker 3 Marker 4 Marker 5 Marker 6 Marker 7 Marker 8 Marker 9 Ref Marker</b> |
|-------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

**:CALC{1-4}:MARK{1-10}:ACT**

|                  |                                                                                                                                                                                                                                    |
|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[:SELEcted]:MARKer{[1] 2 3 4 5 6 7 8 9 10}:ACTivate                                                                                                                                                           |
| Description      | For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10) to the active marker. (No query) |
| <b>NOTE</b>      | If you set a marker set to OFF to the active marker, it is automatically set to ON.                                                                                                                                                |
| Example of use   | 10    OUTPUT 717; ":CALC1:MARK1:ACT"                                                                                                                                                                                               |
| Related commands | :DISP:WIND{1-4}:ACT on page 318<br>:CALC{1-4}:PAR{1-4}:SEL on page 286                                                                                                                                                             |
| Equivalent key   | <b>[Marker]</b> - Marker 1 Marker 2 Marker 3 Marker 4 Ref Marker<br><b>[Marker]</b> - More Markers - Marker 5 Marker 6 Marker 7 Marker 8 Marker 9                                                                                  |

## :CALC{1-4}:MARK{1-10}:BWID:DATA?

- Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:BWIDth:DATA?
- Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the bandwidth search result of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).  
  
If the bandwidth search is impossible, an error occurs and the command is ignored. In this case, no query response is obtained. (Query only)
- Query response** {numeric 1},{numeric 2},{numeric 3},{numeric 4}<newline><^END>

|             | Description           |
|-------------|-----------------------|
| {numeric 1} | The bandwidth.        |
| {numeric 2} | The center frequency. |
| {numeric 3} | The Q value.          |
| {numeric 4} | The loss.             |

- Example of use** 10 OUTPUT 717;" :CALC1:MARK1:BWID:DATA?"  
20 ENTER 717;A,B,C,D
- Related commands** :CALC{1-4}:MARK:BWID on page 243  
:CALC{1-4}:MARK{1-10}:BWID:THR on page 266  
:CALC{1-4}:PAR{1-4}:SEL on page 286
- Equivalent key** No equivalent key is available on the front panel.

## :CALC{1-4}:MARK{1-10}:BWID:THR

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:BWIDth: THReshold <numeric>

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:BWIDth: THReshold?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the bandwidth definition value of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

### Parameters

|              |                                                                                                                                                                                         |
|--------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|              | <numeric>                                                                                                                                                                               |
| Description  | Bandwidth definition value                                                                                                                                                              |
| Range        | -5E8 to 5E8                                                                                                                                                                             |
| Preset value | -3                                                                                                                                                                                      |
| Unit         | Varies depending on the data format as follows:<br>Logarithmic Magnitude: dB (decibel)<br>Phase, Expand Phase, Positive Phase: ° (degree)<br>Group Delay: s (second)<br>Others: No unit |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**

```

10 OUTPUT 717;":CALC1:MARK1:BWID:THR 6"
20 OUTPUT 717;":CALC1:MARK1:BWID:THR?"
30 ENTER 717;A

```

**Related commands** :CALC{1-4}:MARK:BWID on page 243  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Bandwidth Value**

## :CALC{1-4}:MARK{1-10}:DISC

**Syntax** :CALCulate{[1]|2|3|4}[[:SELected]:MARKer{[1]|2|3|4|5|6|7|8|9|10}]:DIScrete  
{ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[[:SELected]:MARKer{[1]|2|3|4|5|6|7|8|9|10}]:DIScrete?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the discrete mode (mode in which the marker moves only at the measurement points) with marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

**Parameters**

|                         | Description                  |
|-------------------------|------------------------------|
| ON or 1                 | Turn OFF the discrete mode.  |
| OFF or 0 (preset value) | Turns OFF the discrete mode. |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:MARK1:DISC OFF"  
20 OUTPUT 717; ":CALC1:MARK1:DISC?"  
30 ENTER 717;A

**Equivalent key** [Marker Fctn] - Discrete

## :CALC{1-4}:MARK{1-10}:FUNC:EXEC

|                  |                                                                                                                                                                                                                                                                                                                                     |
|------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :CALCulate{[1] 2 3 4}[:SELEcted]:MARKer{[1] 2 3 4 5 6 7 8 9 10}:FUNCtion:EXECute                                                                                                                                                                                                                                                    |
| Description      | <p>For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), executes the search with marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).</p> <p>To specify the type of the search, use the :CALC{1-4}:MARK{1-10}:FUNC:TYPE command. (No query)</p> |
| Example of use   | 10 OUTPUT 717; ":CALC1:MARK1:FUNC:EXEC"                                                                                                                                                                                                                                                                                             |
| Related commands | <p>:CALC{1-4}:MARK{1-10}:FUNC:TYPE on page 274</p> <p>:CALC{1-4}:PAR{1-4}:SEL on page 286</p> <p>:CALC{1-4}:MARK:FUNC:DOM on page 245</p>                                                                                                                                                                                           |
| Equivalent key   | <p><b>[Marker Search] - Max Min</b></p> <p><b>[Marker Search] - Peak - Search Peak Search Left Search Right</b></p> <p><b>[Marker Search] - Target - Search Target Search Left Search Right</b></p>                                                                                                                                 |

---

**NOTE** When performing the operation from the front panel, you select the search type and execute the search at the same time.

---

## :CALC{1-4}:MARK{1-10}:FUNC:PEXC

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion:  
PEXCursion <numeric>

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion:  
PEXCursion?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the lower limit for the peak excursion value of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

**Parameters**

|              |                                                                                                                                                                                         |
|--------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|              | <numeric>                                                                                                                                                                               |
| Description  | Lower limit for the peak excursion value                                                                                                                                                |
| Range        | 0 to 5E8                                                                                                                                                                                |
| Preset value | 3                                                                                                                                                                                       |
| Unit         | Varies depending on the data format as follows:<br>Logarithmic Magnitude: dB (decibel)<br>Phase, Expand Phase, Positive Phase: ° (degree)<br>Group Delay: s (second)<br>Others: No unit |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**

```

10 OUTPUT 717;":CALC1:MARK1:FUNC:PEXC 0.2"
20 OUTPUT 717;":CALC1:MARK1:FUNC:PEXC?"
30 ENTER 717;A

```

**Related commands** :CALC{1-4}:MARK{1-10}:FUNC:PPOL on page 270  
:CALC{1-4}:MARK{1-10}:FUNC:TYPE on page 274  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Peak - Peak Excursion**

## :CALC{1-4}:MARK{1-10}:FUNC:PPOL

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion: PPOLarity {POSitive|NEGative|BOTH}

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion: PPOLarity?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the polarity of the peak to be searched with marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

### Parameters

|                         | Description                                             |
|-------------------------|---------------------------------------------------------|
| POSitive (preset value) | Specifies the positive peak.                            |
| NEGative                | Specifies the negative peak.                            |
| BOTH                    | Specifies both the positive peak and the negative peak. |

**Query response** {POS|NEG|BOTH}<newline><^END>

**Example of use**

```
10 OUTPUT 717; ":CALC1:MARK1:FUNC:PPOL NEG"
20 OUTPUT 717; ":CALC1:MARK1:FUNC:PPOL?"
30 ENTER 717;A$
```

**Related commands** :CALC{1-4}:MARK{1-10}:FUNC:PEXC on page 269  
:CALC{1-4}:MARK{1-10}:FUNC:TYPE on page 274  
:CALC{1-4}:PAR{1-4}:SEL on page 286

**Equivalent key** **[Marker Search] - Peak - Peak Polarity**

## :CALC{1-4}:MARK{1-10}:FUNC:TARG

- Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion: TARGet <numeric>  
:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion: TARGet?
- Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the target value to be searched with marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

**Parameters**

|              |                                                                                                                                                                                         |
|--------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|              | <numeric>                                                                                                                                                                               |
| Description  | Target value for target search                                                                                                                                                          |
| Range        | -5E8 to 5E8                                                                                                                                                                             |
| Preset value | 0                                                                                                                                                                                       |
| Unit         | Varies depending on the data format as follows:<br>Logarithmic Magnitude: dB (decibel)<br>Phase, Expand Phase, Positive Phase: ° (degree)<br>Group Delay: s (second)<br>Others: No unit |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

- Query response** {numeric}<newline><^END>
- Example of use**
- ```
10  OUTPUT 717;" :CALC1:MARK1:FUNC:TARG -12.5"
20  OUTPUT 717;" :CALC1:MARK1:FUNC:TARG?"
30  ENTER 717;A
```
- Related commands** :CALC{1-4}:MARK{1-10}:FUNC:TTR on page 273
:CALC{1-4}:MARK{1-10}:FUNC:TYPE on page 274
:CALC{1-4}:PAR{1-4}:SEL on page 286
- Equivalent key** **[Marker Search] - Target - Target Value**

:CALC{1-4}:MARK{1-10}:FUNC:TRAC

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion:TRACking {ON|OFF|1|0}

:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion:TRACking?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the search tracking (function to repeat the search for each sweep) of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

Parameters

	Description
ON or 1	Turns ON the search tracking.
OFF or 0 (preset value)	Turns OFF the search tracking.

Query response {1|0}<newline><^END>

Example of use

```
10 OUTPUT 717; ":CALC1:MARK1:FUNC:TRAC ON"
20 OUTPUT 717; ":CALC1:MARK1:FUNC:TRAC?"
30 ENTER 717;A
```

Related commands :CALC{1-4}:MARK{1-10}:FUNC:EXEC on page 268
:CALC{1-4}:MARK{1-10}:FUNC:TYPE on page 274
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Marker Search] - Tracking**

:CALC{1-4}:MARK{1-10}:FUNC:TTR

Syntax	<pre>:CALCulate{[1] 2 3 4}{:SELEcted}:MARKer{[1] 2 3 4 5 6 7 8 9 10}:FUNCtion: TTRansition {POSitive NEGative BOTH} :CALCulate{[1] 2 3 4}{:SELEcted}:MARKer{[1] 2 3 4 5 6 7 8 9 10}:FUNCtion: TTRansition?</pre>								
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the transition type when performing the target search with marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).								
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>POSitive</td><td>Specifies positive.</td></tr> <tr> <td>NEGative</td><td>Specifies negative.</td></tr> <tr> <td>BOTH (preset value)</td><td>Specifies both positive and negative.</td></tr> </tbody> </table>		Description	POSitive	Specifies positive.	NEGative	Specifies negative.	BOTH (preset value)	Specifies both positive and negative.
	Description								
POSitive	Specifies positive.								
NEGative	Specifies negative.								
BOTH (preset value)	Specifies both positive and negative.								
Query response	{POS NEG BOTH}<newline><^END>								
Example of use	<pre>10 OUTPUT 717;" :CALC1:MARK1:FUNC:TTR NEG" 20 OUTPUT 717;" :CALC1:MARK1:FUNC:TTR?" 30 ENTER 717;A\$</pre>								
Related commands	:CALC{1-4}:MARK{1-10}:FUNC:TARG on page 271 :CALC{1-4}:MARK{1-10}:FUNC:TYPE on page 274 :CALC{1-4}:PAR{1-4}:SEL on page 286								
Equivalent key	[Marker Search] - Target - Target Transition								

:CALC{1-4}:MARK{1-10}:FUNC:TYPE

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion
:TYPE {MAXimum|MINimum|PEAK|LPEak|RPEak|TARGet|LTARget|RTARget}
:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:FUNCtion
:TYPE?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the search type of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

Parameters

	Description
MAXimum (preset value)	Specifies the maximum value search.
MINimum	Specifies the minimum value search.
PEAK	Specifies the maximum positive (minimum negative) peak ^{*1} search.
LPEak	Specifies the peak ^{*1} search to the left from the marker position.
RPEak	Specifies the peak ^{*1} search to the right from the marker position.
TARGet	Specifies the search for the target ^{*2} closest to the current marker position.
LTARget	Specifies the target ^{*2} search to the left from the marker position.
RTARget	Specifies the target ^{*2} search to the right from the marker position.

*1. To specify the conditions of the peak, use the :CALC{1-4}:MARK{1-10}:FUNC:PEXC command and the :CALC{1-4}:MARK{1-10}:FUNC:PPOL command.

*2. To specify the conditions of the target, use the :CALC{1-4}:MARK{1-10}:FUNC:TARG command and the :CALC{1-4}:MARK{1-10}:FUNC:TTR command.

Query response {MAX|MIN|PEAK|LPE|RPE|TARG|LTAR|RTAR}<newline><^END>

Example of use

```
10  OUTPUT 717; ":CALC1:MARK1:FUNC:TYPE PEAK"
20  OUTPUT 717; ":CALC1:MARK1:FUNC:TYPE?"
30  ENTER 717;A$
```

Related commands :CALC{1-4}:MARK{1-10}:FUNC:EXEC on page 268
:CALC{1-4}:MARK{1-10}:FUNC:PEXC on page 269
:CALC{1-4}:MARK{1-10}:FUNC:PPOL on page 270
:CALC{1-4}:MARK{1-10}:FUNC:TARG on page 271
:CALC{1-4}:MARK{1-10}:FUNC:TTR on page 273
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Marker Search] - Max|Min**
[Marker Search] - Peak - Search Peak|Search Left|Search Right

[Marker Search] - Target - Search Target|Search Left|Search Right

NOTE

When performing the operation from the front panel, you select the search type and execute the search at the same time.

:CALC{1-4}:MARK{1-10}:NOTC:DATA?

Syntax :CALCulate{[1]|2|3|4}[:SElected]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:NOTCh:DATA?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the notch search result of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

If the notch search is impossible, an error occurs and the command is ignored.

In this case, no query response is obtained. (Query only)

Query response {value 1},{value 2},{value 3},{value 4}<newline><^END>

	Description
{value 1}	Bandwidth.
{value 2}	Center frequency.
{value 3}	Q value.
{value 4}	Loss.

Example of use 10 OUTPUT 717;" :CALC1:MARK1:NOTC:DATA?"
20 ENTER 717;A,B,C,D

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:MARK:NOTC on page 261
:CALC{1-4}:MARK{1-10}:NOTC:THR on page 277

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:MARK{1-10}:NOTC:THR

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:NOTCh:THReshold
<value>
:CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:NOTCh:THReshold?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the notch definition value of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

Parameters

	<value>
Description	Notch definition value
Range	-5E8 to 5E8
Preset value	-3
Unit	Varies depending on the data format as follows:Amplitude (MLOG): dB (decibel) Phase (PHAS), expanded phase (UPH), positive phase (PPH): ° (degree) Group delay (GDEL): s (second) Others: No unit

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {value}<newline><^END>

Example of use
10 OUTPUT 717;" :CALC1:MARK1:NOTC:THR 5"
20 OUTPUT 717;" :CALC1:MARK1:NOTC:THR?"
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:MARK:NOTC on page 261
:CALC{1-4}:MARK{1-10}:NOTC:DATA? on page 276

Equivalent key [Marker Search] - Notch Value

:CALC{1-4}:MARK{1-10}:SET

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:SET {START|STOP|CENTer|RLEVel|DELay}

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the value of the specified item to the value of the position of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

Regardless of the ON/OFF of the reference marker mode (specified with the :CALC{1-4}:MARK:REF command), the value when the reference marker mode is OFF is always set. (No query)

Parameters

	Description
START	Sets the sweep start value to the stimulus value at the marker position.
STOP	Sets the sweep stop value to the stimulus value at the marker position.
CENTer	Sets the sweep center value to the stimulus value at the marker position.
RLEVel	Sets the reference line value to the response value at the marker position.
DELay	Sets the electrical delay time value to the group delay value at the marker position.

Example of use 10 OUTPUT 717; ":CALC1:MARK1:SET CENT"

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:MARK:REF on page 262

Equivalent key [Marker Fctn] - Marker -> Start|Marker -> Stop|Marker -> Center|Marker -> Reference|Marker -> Delay

:CALC{1-4}:MARK{1-10}:X

Syntax	:CALCulate{[1] 2 3 4}[[:SELEcted]:MARKer{[1] 2 3 4 5 6 7 8 9 10}:X <numeric> :CALCulate{[1] 2 3 4}[[:SELEcted]:MARKer{[1] 2 3 4 5 6 7 8 9 10}:X?
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the stimulus value of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

Parameters

	<numeric>
Description	Stimulus value ^{*1}
Range	Sweep start value to sweep stop value ^{*2}
Preset value	Sweep start value ^{*3}
Unit	Hz (hertz), dBm or second

- *1. When the reference marker mode is ON (ON is specified with the :CALC{1-4}:MARK:REF command), it is the value relative to the reference marker.
- *2. When the span value of the sweep range is 0, the range is from 0 to sweep time value.
- *3. When the span value of the sweep range is 0, the unit is 0.

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":CALC1:MARK1:X 1E9" 20 OUTPUT 717; ":CALC1:MARK1:X?" 30 ENTER 717;A

Related commands	:CALC{1-4}:MARK{1-10}:Y? on page 280 :CALC{1-4}:PAR{1-4}:SEL on page 286 :CALC{1-4}:MARK:REF on page 262
------------------	--

Equivalent key	[Marker] - Marker 1 Marker 2 Marker 3 Marker 4 Ref Marker [Marker] - More Markers - Marker 5 Marker 6 Marker 7 Marker 8 Marker 9
----------------	---

NOTE	When performing the operation from the front panel, you turn ON the marker and set the stimulus value at the same time.
-------------	---

:CALC{1-4}:MARK{1-10}:Y?

Syntax :CALCulate{[1]|2|3|4}[:SElected]:MARKer{[1]|2|3|4|5|6|7|8|9|10}:Y?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the response value of marker 1 (:MARK1) to marker 9 (:MARK9) and reference marker (:MARK10).

When the reference marker mode is ON (ON is specified with the :CALC{1-4}:MARK:REF command), the readout value is the value relative to the reference marker. (Query only)

Query response {numeric 1},{numeric 2}<newline><^END>

	Description
{numeric 1}	Response value (primary value) at the marker position.
{numeric 2}	Response value (secondary value) at the marker position. Always 0 when the data format is not the Smith chart format or the polar format.

Example of use 10 OUTPUT 717;" :CALC1:MARK1:Y?"
30 ENTER 717;A,B

Related commands :CALC{1-4}:MARK{1-10}:X on page 279
:CALC{1-4}:PAR{1-4}:SEL on page 286
:CALC{1-4}:MARK:REF on page 262

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:MATH:FUNC

Syntax :CALCulate{[1]|2|3|4}{:SELected]:MATH:FUNCtion {NORMal|SUBTract|DIVide|ADD|MULTiply}
:CALCulate{[1]|2|3|4}{:SELected]:MATH:FUNCtion?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the data trace display method (math method between measurement data and memory trace data).
The math result according to this setting is displayed on the data trace.

Parameters

	Description
NORMal (preset value)	Specifies <i>Data</i> (no math).
DIVide	Specifies <i>Data</i> / <i>Mem</i> .
MULTiply	Specifies <i>Data</i> × <i>Mem</i> .
SUBTract	Specifies <i>Data</i> - <i>Mem</i> .
ADD	Specifies <i>Data</i> + <i>Mem</i> .

Where *Data* is the measurement data and *Mem* is the data stored in the memory trace.

Query response {NORM|DIV|MUL|SUBT|ADD}<newline><^END>

Example of use
10 OUTPUT 717;":CALC1:MATH:FUNC DIV"
20 OUTPUT 717;":CALC1:MATH:FUNC?"
30 ENTER 717;A\$

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key [Display] - Data Math - OFF|Data / Mem|Data * Mem|Data – Mem|Data + Mem

:CALC{1-4}:MATH:MEM

Syntax :CALCulate{[1]|2|3|4}{:SELected]:MATH:MEMorize

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), copies the measurement data at the execution of the command to the memory trace. (No query)

Example of use 10 OUTPUT 717;":CALC1:MATH:MEM"

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key [Display] - Data → Mem

:CALC{1-4}:MST

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:MSTatistics[:STATe] {ON|OFF|1|0}
:CALCulate{[1]|2|3|4}[:SELEcted]:MSTatistics[:STATe]?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the statistics value display (the mean vale, the standard deviation, and the difference between the maximum value and the minimum value).

Parameters

	Description
ON or 1	Turns ON the statistics value display.
OFF or 0 (preset value)	Turns OFF the statistics value display.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:MST ON"
20 OUTPUT 717;":CALC1:MST?"
30 ENTER 717;A

Related commands :CALC{1-4}:MST:DATA? on page 283
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Marker Fctn] - Statistics**

:CALC{1-4}:MST:DATA?

Syntax :CALCulate{[1]|2|3|4}[[:SELected]:MSTatistics:DATA?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the statistics values (the mean value, the standard deviation, and the difference between the maximum value and the minimum value) display. (Query only)

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

	Description
{numeric 1}	Mean value
{numeric 2}	Standard deviation
{numeric 3}	Difference between the maximum value and the minimum value (Peak to Peak)

Example of use
10 OUTPUT 717;":CALC1:MST:DATA?"
20 ENTER 717;A,B,C

Related commands :CALC{1-4}:MST on page 282
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key No equivalent key is available on the front panel.

:CALC{1-4}:PAR:COUN

Syntax :CALCulate{[1]|2|3|4}:PARAmeter:COUNt <numeric>
 :CALCulate{[1]|2|3|4}:PARAmeter:COUNt?

Description Sets the number of traces of channel 1 (:CALC1) to channel 4 (:CALC4).

Parameters

	<numeric>
Description	Number of traces
Range	1 to 4
Preset value	1
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:PAR:COUN 4"
 20 OUTPUT 717;":CALC1:PAR:COUN?"
 30 ENTER 717;A

Equivalent key **[Display] - Num of Traces**

:CALC{1-4}:PAR{1-4}:DEF

Syntax	:CALCulate{[1] 2 3 4}:PARAmeter{[1] 2 3 4}:DEFine {S11 S21 S12 S22} :CALCulate{[1] 2 3 4}:PARAmeter{[1] 2 3 4}:DEFine?
Description	Sets the measurement parameter of trace 1 (:PAR1) to trace 4 (:PAR4) of channel 1 (:CALC1) to channel 4 (:CALC4).

Parameters

	Description
S11 (preset value)	Specifies S11.
S21	Specifies S21.
S12	Specifies S12.
S22	Specifies S22.

Query response	{S11 S21 S12 S22}<newline><^END>
Example of use	10 OUTPUT 717;":CALC1:PAR1:DEF S21" 20 OUTPUT 717;":CALC1:PAR1:DEF?" 30 ENTER 717;A\$
Equivalent key	[Meas] - S11 S21 S12 S22

:CALC{1-4}:PAR{1-4}:SEL

Syntax	:CALCulate{[1] 2 3 4}:PARameter{[1] 2 3 4}:SELect
Description	Sets trace 1 (:PAR1) to trace 4 (:PAR4) of channel 1 (:CALC1) to channel 4 (:CALC4) to the active trace. You can set only the displayed trace to the active trace. If you execute this command trying to set a not displayed trace to the active trace, an error occurs and the command is ignored. (No query)
Example of use	10 OUTPUT 717; ":CALC1:PAR1:SEL "
Related commands	:DISP:WIND{1-4}:ACT on page 318
Equivalent key	[Trace Prev] / [Trace Next]

:CALC{1-4}:RLIM

Syntax	:CALCulate{[1] 2 3 4}:SELected]:RLIMit[:STATe] {ON OFF 1 0} :CALCulate{[1] 2 3 4}:SELected]:RLIMit[:STATe]?						
Description	For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the ripple test function.						
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>ON or 1</td><td>Turns ON the ripple test function.</td></tr> <tr> <td>OFF or 0 (preset value)</td><td>Turns OFF the ripple test function.</td></tr> </tbody> </table>		Description	ON or 1	Turns ON the ripple test function.	OFF or 0 (preset value)	Turns OFF the ripple test function.
	Description						
ON or 1	Turns ON the ripple test function.						
OFF or 0 (preset value)	Turns OFF the ripple test function.						
Query response	{1 0}<newline><^END>						
Example of use	10 OUTPUT 717; ":CALC1:RLIM ON" 20 OUTPUT 717; ":CALC1:RLIM?" 30 ENTER 717;A						
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286 :CALC{1-4}:RLIM:DATA on page 287 :CALC{1-4}:RLIM:DISP:LINE on page 288 :CALC{1-4}:RLIM:DISP:SEL on page 289 :CALC{1-4}:RLIM:DISP:VAL on page 290 :CALC{1-4}:RLIM:FAIL? on page 291 :CALC{1-4}:RLIM:REP? on page 292						
Equivalent key	[Analysis] - Ripple Limit - Ripple Limit Test						

:CALC{1-4}:RLIM:DATA

- Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:RLIMit:DATA <numeric 1>,...,<numeric 1+(N×4)>
:CALCulate{[1]|2|3|4}[:SELEcted]:RLIMit:DATA?
- Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the ripple limit table.
- The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.

Parameters

	Description
<numeric 1>	The number of ripple limit bands. (0 to 12)
<numeric 1+(n×4)-3>	The type of the n-th ripple limit band. Specify an integer 0 to 1: 0: Off 1: On
<numeric 1+(n×4)-2>	The value on the horizontal axis (frequency/power/time) of the start point of the n-th line.
<numeric 1+(n×4)-1>	The value on the horizontal axis (frequency/power/time) of the end point of the n-th line.
<numeric 1+(n×4)>	The value of maximum ripple (dB) range.

Where N is the number of lines (specified with <numeric 1>) and n is an integer between 1 and N.

If you set the number of lines to 0 (clear the limit table), this command needs only <numeric 1> as the parameter.

- Query response** {numeric 1},...,{numeric 1+(N×4)}<newline><^END>
- Example of use**
- ```

10 DIM B(1:2,1:4)
20 OUTPUT 717;" :CALC1:RLIM:DATA 2,1,1E9,3E9,3,1,5E9,7E9,3"
30 OUTPUT 717;" :CALC1:RLIM:DATA?"
40 ENTER 717;A,B(*)

10 OUTPUT 717;" :CALC1:RLIM:DATA 0" ! Clear Ripple Limit Table

```
- Related commands** :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:RLIM on page 286
- Equivalent key** [Analysis] - Ripple Limit - Edit Ripple Limit - Add

**:CALC{1-4}:RLIM:DISP:LINE**

Syntax :CALCulate{[1]|2|3|4}{:SElected]:RLIMit:DISPlay:LINE {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}{:SElected]:RLIMit:DISPlay:LINE?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the ripple limit line display.

Parameters

|                         | Description                              |
|-------------------------|------------------------------------------|
| ON or 1                 | Turns ON the ripple limit line display.  |
| OFF or 0 (preset value) | Turns OFF the ripple limit line display. |

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:RLIM:DISP:LINE ON"  
20 OUTPUT 717;":CALC1:RLIM:DISP:LINE?"  
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:RLIM on page 286  
:CALC{1-4}:RLIM:DISP:SEL on page 289  
:CALC{1-4}:RLIM:DISP:VAL on page 290

Equivalent key **[Analysis] - Ripple Limit - Ripple Limit**

## :CALC{1-4}:RLIM:DISP:SEL

| Syntax           | :CALCulate{[1] 2 3 4}[:SElected]:RLIMit:DISPlay:SElect <numeric><br>:CALCulate{[1] 2 3 4}[:SElected]:RLIMit:DISPlay:SElect?                                                                                              |  |           |             |                        |       |         |              |   |
|------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-----------|-------------|------------------------|-------|---------|--------------|---|
| Description      | For channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), sets the ripple limit band for ripple value display.                                                                  |  |           |             |                        |       |         |              |   |
| Parameters       | <table border="1"> <tr> <th></th><th>&lt;numeric&gt;</th></tr> <tr> <td>Description</td><td>The ripple limit band.</td></tr> <tr> <td>Range</td><td>1 to 12</td></tr> <tr> <td>Preset value</td><td>1</td></tr> </table> |  | <numeric> | Description | The ripple limit band. | Range | 1 to 12 | Preset value | 1 |
|                  | <numeric>                                                                                                                                                                                                                |  |           |             |                        |       |         |              |   |
| Description      | The ripple limit band.                                                                                                                                                                                                   |  |           |             |                        |       |         |              |   |
| Range            | 1 to 12                                                                                                                                                                                                                  |  |           |             |                        |       |         |              |   |
| Preset value     | 1                                                                                                                                                                                                                        |  |           |             |                        |       |         |              |   |
| Query response   | {numeric}<newline><^END>                                                                                                                                                                                                 |  |           |             |                        |       |         |              |   |
| Example of use   | <pre> 10  OUTPUT 717;" :CALC1:RLIM:DISP:SEL 5" 20  OUTPUT 717;" :CALC1:RLIM:DISP:SEL?" 30  ENTER 717;A </pre>                                                                                                            |  |           |             |                        |       |         |              |   |
| Related commands | :CALC{1-4}:PAR{1-4}:SEL on page 286<br>:CALC{1-4}:RLIM on page 286<br>:CALC{1-4}:RLIM:DISP:LINE on page 288<br>:CALC{1-4}:RLIM:DISP:VAL on page 290                                                                      |  |           |             |                        |       |         |              |   |
| Equivalent key   | <b>[Analysis] - Ripple Limit - Ripple Band</b>                                                                                                                                                                           |  |           |             |                        |       |         |              |   |

## :CALC{1-4}:RLIM:DISP:VAL

**Syntax** :CALCulate{[1]|2|3|4}{:SElected]:RLIMit:DISPlay:VALue {OFF|ABS|MAR}  
:CALCulate{[1]|2|3|4}{:SElected]:RLIMit:DISPlay:VALue?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), selects the display type for the ripple value.

**Parameters**

|                    | Description                                    |
|--------------------|------------------------------------------------|
| OFF (preset value) | Specifies the display off.                     |
| ABS                | Specifies the absolute value for display type. |
| MAR                | Specifies the margin for display type.         |

**Query response** {OFF|ABS|MAR}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":CALC1:RLIM:DISP:VAL ABS"  
20 OUTPUT 717; ":CALC1:RLIM:DISP:VAL?"  
30 ENTER 717;A\$

**Related commands** :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:RLIM on page 286  
:CALC{1-4}:RLIM:DISP:LINE on page 288  
:CALC{1-4}:RLIM:DISP:SEL on page 289

**Equivalent key** [Analysis] - Ripple Limit - Ripple Value - OFF | Absolute | Margin

## :CALC{1-4}:RLIM:FAIL?

|                |                                                                                                                                                                       |
|----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax         | :CALCulate{[1][2][3][4][:SELEcted]:RLIMit:FAIL?                                                                                                                       |
| Description    | For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the ripple test result. (Query only) |
| Query response | {1 0}<newline><^END>                                                                                                                                                  |

|   | Description                     |
|---|---------------------------------|
| 1 | The ripple test result is FAIL. |
| 0 | The ripple test result is PASS. |

When the ripple test is set to OFF, 0 is always read out.

|                  |                                                                    |
|------------------|--------------------------------------------------------------------|
| Example of use   | 10 OUTPUT 717;" :CALC1:RLIM:FAIL?"<br>20 ENTER 717;A               |
| Related commands | :CALC{1-4}:PAR{1-4}:SEL on page 286<br>:CALC{1-4}:RLIM on page 286 |
| Equivalent key   | No equivalent key is available on the front panel.                 |

**:CALC{1-4}:RLIM:REP?**

Syntax :CALCulate{[1][2][3][4]}[:SElected]:RLIMit:REPort[:DATA]?

Description For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), reads out the ripple value of the ripple test.

The data transfer format when this command is executed depends on the setting with the :FORM:DATA command. (Query only)

Query response {numeric 1},...,{numeric 1+N×3}<newline><^END>

|                     | Description                                  |
|---------------------|----------------------------------------------|
| <numeric 1>         | Number of ripple limit line (1 to 12)        |
| <numeric 1+(n×3)-2> | Number of ripple limit bands                 |
| <numeric 1+(n×3)-1> | Ripple value                                 |
| <numeric 1+(n×3)>   | Results of ripple test<br>0: Pass<br>1: Fail |

Where N is the number of lines (specified with <numeric 1>) and n is an integer between 1 and 12.

Example of use

```
10 DIM B(1:2,1:3)
20 OUTPUT 717;" :CALC1:RLIM:REP?"
30 ENTER 717;A,B(*)
```

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:RLIM on page 286

Equivalent key No equivalent key is available on the front panel.

## :CALC{1-4}:SMO

**Syntax** :CALCulate{[1]|2|3|4}[:SELEcted]:SMOothing[:STATe] {ON|OFF|1|0}  
:CALCulate{[1]|2|3|4}[:SELEcted]:SMOothing[:STATe]?

**Description** For the active trace of channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command), turns ON/OFF the smoothing.

**Parameters**

|                         | Description              |
|-------------------------|--------------------------|
| ON or 1                 | Turns ON the smoothing.  |
| OFF or 0 (preset value) | Turns OFF the smoothing. |

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717;":CALC1:SMO:STAT ON"  
20 OUTPUT 717;":CALC1:SMO:STAT?"  
30 ENTER 717;A

**Related commands** :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:SMO:APER on page 294

**Equivalent key** [Avg] - Smoothing

**:CALC{1-4}:SMO:APER**

Syntax :CALCulate{[1]|2|3|4}[:SELEcted]:SMOothing:APERture <numeric>  
:CALCulate{[1]|2|3|4}[:SELEcted]:SMOothing:APERture?

Description Sets the smoothing aperture for channel 1 (:CALC1) to channel 4 (:CALC4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command).

Parameters

|              |                                             |
|--------------|---------------------------------------------|
|              | <numeric>                                   |
| Description  | Percentage relative to the sweep span value |
| Range        | 0.05 to 25                                  |
| Preset value | 1.5                                         |
| Unit         | % (percent)                                 |
| Resolution   | 1E-14                                       |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":CALC1:SMO:APER 2.5"  
20 OUTPUT 717;":CALC1:SMO:APER?"  
30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286  
:CALC{1-4}:SMO on page 293

Equivalent key **[Avg] - Smo Aperture**

## :CONT:HAND:A

**Syntax** :CONTrol:HANDler:A[:DATA] <numeric>

**Description** Outputs data to output port A (A0 to A7) of the handler I/O. Data is outputted as 8-bit binary using A0 as LSB and A7 as MSB. (No query)

For details about the handler I/O, see Chapter 10.

**Parameters**

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Output data |
| Range       | 0 to 255    |
| Resolution  | 1           |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Example of use** 10 OUTPUT 717;":CONT:HAND:A 15"

**Equivalent key** No equivalent key is available on the front panel.

## :CONT:HAND:B

**Syntax** :CONTrol:HANDler:B[:DATA] <numeric>

**Description** Outputs data to output port B (B0 to B7) of the handler I/O. Data is outputted as 8-bit binary using B0 as LSB and B7 as MSB. (No query)

For details about the handler I/O, see Chapter 10.

**Parameters**

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Output data |
| Range       | 0 to 255    |
| Resolution  | 1           |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Example of use** 10 OUTPUT 717;":CONT:HAND:B 15"

**Equivalent key** No equivalent key is available on the front panel.

**:CONT:HAND:C**

|                  |                                                                                                                                                                                                                                                                                                                                                                                                                                |  |                        |             |                        |       |         |            |   |
|------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|------------------------|-------------|------------------------|-------|---------|------------|---|
| Syntax           | <code>:CONTrol:HANDler:C[:DATA] &lt;numeric&gt;</code><br><code>:CONTrol:HANDler:C[:DATA]?</code>                                                                                                                                                                                                                                                                                                                              |  |                        |             |                        |       |         |            |   |
| Description      | <p>When input/output port C of the handler I/O is set to the output port, outputs data to output port C (C0 to C3).</p> <p>When input/output port C is set to the input port, reads out data inputted to port C (C0 to C3).</p> <p>Data is outputted as 4-bit binary using C0 as LSB and C3 as MSB.</p> <p>For details about the handler I/O, see Chapter 10.</p>                                                              |  |                        |             |                        |       |         |            |   |
| Parameters       | <table><tr><td></td><td><b>&lt;numeric&gt;</b></td></tr><tr><td>Description</td><td>Output data/input data</td></tr><tr><td>Range</td><td>0 to 15</td></tr><tr><td>Resolution</td><td>1</td></tr></table> <p>If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.</p> |  | <b>&lt;numeric&gt;</b> | Description | Output data/input data | Range | 0 to 15 | Resolution | 1 |
|                  | <b>&lt;numeric&gt;</b>                                                                                                                                                                                                                                                                                                                                                                                                         |  |                        |             |                        |       |         |            |   |
| Description      | Output data/input data                                                                                                                                                                                                                                                                                                                                                                                                         |  |                        |             |                        |       |         |            |   |
| Range            | 0 to 15                                                                                                                                                                                                                                                                                                                                                                                                                        |  |                        |             |                        |       |         |            |   |
| Resolution       | 1                                                                                                                                                                                                                                                                                                                                                                                                                              |  |                        |             |                        |       |         |            |   |
| Query response   | <code>{numeric}&lt;newline&gt;&lt;^END&gt;</code>                                                                                                                                                                                                                                                                                                                                                                              |  |                        |             |                        |       |         |            |   |
| Example of use   | <pre>10  OUTPUT 717;":CONT:HAND:C:MODE OUTP" 20  OUTPUT 717;":CONT:HAND:C 15"  10  OUTPUT 717;":CONT:HAND:C:MODE INP" 20  OUTPUT 717;":CONT:HAND:C?" 30  ENTER 717;A</pre>                                                                                                                                                                                                                                                     |  |                        |             |                        |       |         |            |   |
| Related commands | <code>:CONT:HAND:C:MODE</code> on page 297                                                                                                                                                                                                                                                                                                                                                                                     |  |                        |             |                        |       |         |            |   |
| Equivalent key   | No equivalent key is available on the front panel.                                                                                                                                                                                                                                                                                                                                                                             |  |                        |             |                        |       |         |            |   |

## :CONT:HAND:C:MODE

- Syntax** :CONTrol:HANDler:C:MODE {INPut|OUTPut}  
:CONTrol:HANDler:C:MODE?
- Description** Sets the input/output direction of port C of the handler I/O.  
For details about the handler I/O, see Chapter 10.

**Parameters**

|                      | Description       |
|----------------------|-------------------|
| INPut (preset value) | Specifies input.  |
| OUTPut               | Specifies output. |

- Query response** {INP|OUTP}<newline><^END>
- Example of use**
- ```
10 OUTPUT 717;":CONT:HAND:C:MODE OUTP"
20 OUTPUT 717;":CONT:HAND:C:MODE?"
30 ENTER 717;A$
```
- Related commands** :CONT:HAND:C on page 296
- Equivalent key** No equivalent key is available on the front panel.

:CONT:HAND:D

Syntax	<code>:CONTrol:HANDler:D[:DATA] <numeric></code> <code>:CONTrol:HANDler:D[:DATA]?</code>								
Description	When input/output port D of the handler I/O is set to the output port, outputs data to output port D (D0 to D3). When input/output port D is set to the input port, reads out data inputted to port D (D0 to D3). Data is outputted as 4-bit binary using D0 as LSB and D3 as MSB. For details about the handler I/O, see Chapter 10.								
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Output data/input data</td></tr><tr><td>Range</td><td>0 to 15</td></tr><tr><td>Resolution</td><td>1</td></tr></table> If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.		<numeric>	Description	Output data/input data	Range	0 to 15	Resolution	1
	<numeric>								
Description	Output data/input data								
Range	0 to 15								
Resolution	1								
Query response	<code>{numeric}<newline><^END></code>								
Example of use	<pre>10 OUTPUT 717; ":CONT:HAND:D:MODE OUTP" 20 OUTPUT 717; ":CONT:HAND:D 15" 10 OUTPUT 717; ":CONT:HAND:D:MODE INP" 20 OUTPUT 717; ":CONT:HAND:D?" 30 ENTER 717;A</pre>								
Related commands	<code>:CONT:HAND:D:MODE</code> on page 299								
Equivalent key	No equivalent key is available on the front panel.								

:CONT:HAND:D:MODE

Syntax :CONTrol:HANDler:C:MODE {INPut|OUTPut}
:CONTrol:HANDler:C:MODE?

Description Sets the input/output direction of port D of the handler I/O.
For details about the handler I/O, see Chapter 10.

Parameters

	Description
INPut (preset value)	Specifies input.
OUTPut	Specifies output.

Query response {INP|OUTP}<newline><^END>

Example of use
10 OUTPUT 717;":CONT:HAND:D:MODE OUTP"
20 OUTPUT 717;":CONT:HAND:D:MODE?"
30 ENTER 717;A\$

Related commands :CONT:HAND:D on page 298

Equivalent key No equivalent key is available on the front panel.

:CONT:HAND:E

Syntax :CONTrol:HANDler:E[:DATA] <numeric>
 :CONTrol:HANDler:E[:DATA]?

Description When input/output port E (port C + port D) of the handler I/O is set to the output port, outputs data to output port E.

 When input/output port E is set to the input port, reads out data inputted to port E.

 Data is outputted as 8-bit binary using C0 as LSB and D3 as MSB.

 For details about the handler I/O, see Chapter 10.

Parameters

	<numeric>
Description	Output data/input data
Range	0 to 255
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":CONT:HAND:C:MODE OUTP"
 20 OUTPUT 717;":CONT:HAND:D:MODE OUTP"
 30 OUTPUT 717;":CONT:HAND:E 128"

 10 OUTPUT 717;":CONT:HAND:C:MODE INP"
 20 OUTPUT 717;":CONT:HAND:D:MODE INP"
 30 OUTPUT 717;":CONT:HAND:E?"
 40 ENTER 717;A

Related commands :CONT:HAND:C:MODE on page 297
 :CONT:HAND:D:MODE on page 299
 :CONT:HAND:C on page 296
 :CONT:HAND:D on page 298

Equivalent key No equivalent key is available on the front panel.

:CONT:HAND:F

Syntax :CONTrol:HANDler:F[:DATA] <numeric>

Description Outputs data to output port F (port A + port B) of the handler I/O. Data is outputted as 16-bit binary using A0 as LSB and B7 as MSB. (No query)
For details about the handler I/O, see Chapter 10.

Parameters

	<numeric>
Description	Output data
Range	0 to 65535
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Example of use 10 OUTPUT 717; ":CONT:HAND:F 511"

Related commands :CONT:HAND:A on page 295
:CONT:HAND:B on page 295

Equivalent key No equivalent key is available on the front panel.

:CONT:HAND:IND:STAT

Syntax :CONTrol:HANDler[:EXTension]:INDex:STATe {ON|OFF|1|0}
:CONTrol:HANDler[:EXTension]:INDex:STATe?

Description Turns ON/OFF outputting the INDEX signal to B6 of the handler I/O.
For details about the handler I/O, see Chapter 10.

Parameters

	Description
ON or 1	Turns ON the INDEX signal output.
OFF or 0 (preset value)	Turns OFF the INDEX signal output.

Query response {1|0}<newline><^END>

Example of use

```
10 OUTPUT 717; ":CONT:HAND:IND:STAT ON"
20 OUTPUT 717; ":CONT:HAND:IND:STAT?"
30 ENTER 717;A
```

Related commands :CONT:HAND:RTR:STAT on page 303

Equivalent key No equivalent key is available on the front panel.

:CONT:HAND:OUTP{1-2}

Syntax :CONTrol:HANDler:OUTPut{[1]|2}[:DATA] {1|0}
:CONTrol:HANDler:OUTPut{[1]|2}[:DATA]?

Description Sets HIGH/LOW of OUTPUT1 (:OUTP1) or OUTPUT2 (:OUTP2) of the handler I/O.
For details about the handler I/O, see Chapter 10.

Parameters

	Description
1	Specifies LOW.
0	Specifies HIGH.

Query response {1|0}<newline><^END>

Example of use

```
10 OUTPUT 717; ":CONT:HAND:OUTP1 1"
20 OUTPUT 717; ":CONT:HAND:OUTP1?"
30 ENTER 717;A
```

Equivalent key No equivalent key is available on the front panel.

:CONT:HAND:RTR:STAT

Syntax :CONTrol:HANDler[:EXTension]:RTRigger:STATe {ON|OFF|1|0}
:CONTrol:HANDler[:EXTension]:RTRigger:STATe?

Description Turns ON/OFF outputting the READY FOR TRIGGER signal to B7 of the handler I/O.
For details about the handler I/O, see Chapter 10.

Parameters

	Description
ON or 1	Turns ON the READY FOR TRIGGER signal output.
OFF or 0 (preset value)	Turns OFF the READY FOR TRIGGER signal output.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":CONT:HAND:RTR:STAT ON"
20 OUTPUT 717;":CONT:HAND:RTR:STAT?"
30 ENTER 717;A

Related commands :CONT:HAND:IND:STAT on page 302

Equivalent key No equivalent key is available on the front panel.

:DISP:ANN:FREQ

Syntax :DISPlay:ANNotation:FREQuency[:STATe] {ON|OFF|1|0}
:DISPlay:ANNotation:FREQuency[:STATe]?

Description Turns ON/OFF the frequency display on the LCD display.

Parameters

	Description
ON or 1 (preset value)	Turns ON the frequency display.
OFF or 0	Turns OFF the frequency display.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":DISP:ANN:FREQ OFF"
20 OUTPUT 717;":DISP:ANN:FREQ?"
30 ENTER 717;A

Equivalent key **[Display] - Frequency**

:DISP:CCL

Syntax :DISPlay:CCLear

Description Clears the error message display on the instrument status bar (at the bottom of the LCD display). (No query)

Example of use 10 OUTPUT 717;":DISP:CCL"

Equivalent key All front panel keys.

:DISP:CLOC

Syntax :DISPlay:CLOCk {ON|OFF|1|0}
 :DISPlay:CLOCk?

Description Turns ON/OFF the clock display at the right edge of the instrument status bar (at the bottom of the LCD display).

Parameters

	Description
ON or 1 (preset value)	Turns ON the clock display.
OFF or 0	Turns OFF the clock display.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:CLOC OFF"
 20 OUTPUT 717;":DISP:CLOC?"
 30 ENTER 717;A

Equivalent key [System] - Misc Setup - Clock Setup - Show Clock

:DISP:COL{1-2}:BACK

Syntax :DISPlay:COLor{[1]|2}:BACK <numeric 1>,<numeric 2>,<numeric 3>
:DISPlay:COLor{[1]|2}:BACK?

Description Sets the background color for normal display (:COL1) and inverted display (:COL2).

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Amount of red	Amount of green	Amount of blue
Range	0 to 5	0 to 5	0 to 5
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:COL:BACK 1,2,3"
20 OUTPUT 717;":DISP:COL:BACK?"
30 ENTER 717;A,B,C

Related commands :DISP:COL{1-2}:RES on page 308

Equivalent key **[System] - Misc Setup - Color Setup - Normal|Invert - Background**

:DISP:COL{1-2}:GRAT{1-2}

Syntax :DISPlay:COLor{[1]|2}:GRATicule{[1]|2} <numeric 1>,<numeric 2>,<numeric 3>
:DISPlay:COLor{[1]|2}:GRATicule{[1]|2}?

Description Sets the color of the graticule label and the outer frame line of the graph (:GRAT1) and the color of the grid line of the graph (:GRAT2) for normal display (:COL1) and inverted display (:COL2).

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Amount of red	Amount of green	Amount of blue
Range	0 to 5	0 to 5	0 to 5
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use

```
10 OUTPUT 717;" :DISP:COL1:GRAT1 1,2,3"
20 OUTPUT 717;" :DISP:COL1:GRAT1?"
30 ENTER 717;A,B,C
```

Related commands :DISP:COL{1-2}:RES on page 308

Equivalent key [System] - Misc Setup - Color Setup - Normal|Invert - Graticule Main|Graticule Sub

:DISP:COL{1-2}:LIM{1-2}

Syntax :DISPlay:COLor{[1]|2}:LIMit{[1]|2} <numeric 1>,<numeric 2>,<numeric 3>
:DISPlay:COLor{[1]|2}:LIMit{[1]|2}?

Description Sets the fail display color used for the limit test result (:LIM1) and the color of the limit line (:LIM2) for normal display (:COL1) and inverted display (:COL2).

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Amount of red	Amount of green	Amount of blue
Range	0 to 5	0 to 5	0 to 5
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use
10 OUTPUT 717;":DISP:COL1:LIM1 1,2,3"
20 OUTPUT 717;":DISP:COL1:LIM1?"
30 ENTER 717;A,B,C

Related commands :DISP:COL{1-2}:RES on page 308

Equivalent key [System] - Misc Setup - Color Setup - Normal|Invert - Limit Fail|Limit Line

:DISP:COL{1-2}:RES

Syntax :DISPlay:COLor{[1]|2}:RESet

Description Resets the display color settings for all the items to the factory preset state for normal display (:COL1) and inverted display (:COL2). (No query)

Example of use 10 OUTPUT 717;":DISP:COL1:RES"

Related commands :DISP:COL{1-2}:BACK on page 306
:DISP:COL{1-2}:GRAT{1-2} on page 307
:DISP:COL{1-2}:LIM{1-2} on page 308
:DISP:COL{1-2}:BACK on page 306
:DISP:COL{1-2}:BACK on page 306

Equivalent key [System] - Misc Setup - Color Setup - Normal|Invert - Reset Color - OK

:DISP:COL{1-2}:TRAC{1-4}:DATA

Syntax :DISPlay:COLor{[1]|2}:TRAC{[1]|2|3|4}:DATA <numeric 1>,<numeric 2>,<numeric 3>
:DISPlay:COLor{[1]|2}:TRAC{[1]|2|3|4}:DATA?

Description Sets the color of the data trace of trace 1 (:TRAC1) to trace 4 (:TRAC4) for normal display (:COL1) and inverted display (:COL2).

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Amount of red	Amount of green	Amount of blue
Range	0 to 5	0 to 5	0 to 5
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use
10 OUTPUT 717;" :DISP:COL1:TRAC1:DATA 1,2,3"
20 OUTPUT 717;" :DISP:COL1:TRAC1:DATA?"
30 ENTER 717;A,B,C

Related commands :DISP:COL{1-2}:RES on page 308

Equivalent key [System] - Misc Setup - Color Setup - Normal|Invert - Data Trace 1|Data Trace 2|Data Trace 3|Data Trace 4

:DISP:COL{1-2}:TRAC{1-4}:MEM

Syntax :DISPlay:COLor{[1]|2}:TRAC{[1]|2|3|4}:MEMory <numeric 1>,<numeric 2>,<numeric 3>

:DISPlay:COLor{[1]|2}:TRAC{[1]|2|3|4}:MEMory?

Description Sets the color of the memory trace of trace 1 (:TRAC1) to trace 4 (:TRAC4) for normal display (:COL1) and inverted display (:COL2).

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Amount of red	Amount of green	Amount of blue
Range	0 to 5	0 to 5	0 to 5
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use

```

10 OUTPUT 717;":DISP:COL1:TRAC1:MEM 1,2,3"
20 OUTPUT 717;":DISP:COL1:TRAC1:MEM?"
30 ENTER 717;A,B,C

```

Related commands :DISP:COL{1-2}:RES on page 308

Equivalent key [System] - Misc Setup - Color Setup - Normal|Invert - Mem Trace 1|Mem Trace 2|Mem Trace 3|Mem Trace 4

:DISP:ECHO

Syntax	:DISPlay:ECHO[:DATA] <string>
Description	Displays a character string in the echo window. (No query)
Parameters	

	<string>
Description	Character string you want to display
Range	254 characters or less

Example of use	10 OUTPUT 717; ":DISP:ECHO ""TEST RESULT"""
Related commands	:DISP:ECHO:CLE on page 311 :DISP:TABL on page 316 :DISP:TABL:TYPE on page 317
Equivalent key	No equivalent key is available on the front panel.

:DISP:ECHO:CLE

Syntax	:DISPlay:ECHO:CLEar
Description	Clears all character strings displayed in the echo window. (No query)
Example of use	10 OUTPUT 717; ":DISP:ECHO:CLE"
Related commands	:DISP:ECHO on page 311
Equivalent key	[Macro Setup] - Clear Echo

:DISP:ENAB

Syntax :DISPlay:ENABle {ON|OFF|1|0}
 :DISPlay:ENABle?

Description Turns ON/OFF the update of the LCD display.

When the update of the LCD display is OFF, You can update the LCD display once using :DISP:UPD command.

Parameters

	Description
ON or 1 (preset value)	Turns ON the update.
OFF or 0	Turns OFF the update.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:ENAB OFF"
 20 OUTPUT 717;":DISP:ENAB?"
 30 ENTER 717;A

Related commands :DISP:UPD on page 318

Equivalent key **[Display] - Update**

:DISP:FSIG

Syntax :DISPlay:FSIGn {ON|OFF|1|0}
:DISPlay:FSIGn?

Description Turns on or off the Fail display when the limit test fails.

Parameters

	Description
ON or 1 (preset value)	Turns on the Fail display.
OFF or 0	Turns off the Fail display.

Query response {1|0}<newline><^END>

Example of use

```
10 OUTPUT 717;":DISP:FSIG OFF"
20 OUTPUT 717;":DISP:FSIG?"
30 ENTER 717;A
```

Related commands :CALC{1-4};LIM on page 232

Equivalent key **[Analysis] - Limit Test - Fail Sign**

:DISP:IMAG

Syntax :DISPlay:IMAGe {NORMal|INVert}
:DISPlay:IMAGe?

Description Selects the display type of the LCD display.

Parameters

	Description
NORMal (preset value)	Specifies the normal display (background color: black).
INVert	Specifies the display in which the color of the normal display is inverted (background color: white).

Query response {NORM|INV}<newline><^END>

Example of use

```
10 OUTPUT 717;":DISP:IMAG INV"
20 OUTPUT 717;":DISP:IMAG?"
30 ENTER 717;A$
```

Equivalent key **[Display] - Invert Color**

:DISP:MAX

Syntax :DISPlay:MAXimize {ON|OFF|1|0}
:DISPlay:MAXimize?

Description Turns ON/OFF the window maximization of the active channel (specified with the :DISP:WIND{1-4}:ACT command).
If you turned ON the maximization, only the window of the active channel is maximized on the LCD display and the windows of the other channels are not displayed.

Parameters

	Description
ON or 1	Turns ON the maximization.
OFF or 0 (preset value)	Turns OFF the maximization.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":DISP:MAX ON"
20 OUTPUT 717;":DISP:MAX?"
30 ENTER 717;A

Related commands :DISP:WIND{1-4}:ACT on page 318

Equivalent key **[Channel Max]**

:DISP:SKEY

Syntax :DISPlay:SKEY[:STATe] {ON|OFF|1|0}
:DISPlay:SKEY[:STATe]?

Description Turns ON/OFF the display of the softkey labels.

Parameters

	Description
ON or 1 (preset value)	Specifies ON.
OFF or 0	Specifies OFF.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":DISP:MAX ON"
20 OUTPUT 717;":DISP:MAX?"
30 ENTER 717;A

Equivalent key **[Entry Off] ([Softkey On/Off])**

:DISP:SPL

Syntax	<pre>:DISPlay:SPLit {D1 D12 D1_2 D112 D1_1_2 D123 D1_2_3 D12_33 D11_23 D13_23 D12_13 D1234 D1_2_3_4 D12_34} :DISPlay:SPLit?</pre>																														
Description	Sets the layout of the windows on the LCD display. For details about the window layout, refer to Figure 3-1 on page 45.																														
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>D1 (preset value)</td><td>Specifies the layout in which the window for channel 1 only is displayed on the entire display.</td></tr> <tr> <td>D12</td><td>Specifies the layout in which the window for channel 1 is displayed on the left side of the display area and the window for channel 2 on the right side.</td></tr> <tr> <td>D1_2</td><td>Specifies the layout in which the window for channel 1 is displayed in the upper part and the window for channel 2 in the lower part.</td></tr> <tr> <td>D112</td><td>Specifies the layout in which the window for channel 1 is displayed on the left side of 2/3 and the window for channel 2 on the right side of 1/3.</td></tr> <tr> <td>D1_1_2</td><td>Specifies the layout in which the window for channel 1 is displayed in the upper part of 2/3 and the window for channel 2 in the lower part of 1/3.</td></tr> <tr> <td>D123</td><td>Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the left side, middle part, and right side, respectively.</td></tr> <tr> <td>D1_2_3</td><td>Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper part, middle part, and the lower part, respectively.</td></tr> <tr> <td>D12_33</td><td>Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper left, upper right, and lower part, respectively.</td></tr> <tr> <td>D11_23</td><td>Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper part, lower left, and lower right, respectively.</td></tr> <tr> <td>D13_23</td><td>Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper left, lower left, and right side, respectively.</td></tr> <tr> <td>D12_13</td><td>Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the left side, upper right, and lower right, respectively.</td></tr> <tr> <td>D1234</td><td>Specifies the layout in which the windows for channel 1, 2, 3 and 4 are displayed by splitting the screen horizontally into four equal parts.</td></tr> <tr> <td>D1_2_3_4</td><td>Specifies the layout in which the windows for channel 1, 2, 3 and 4 are displayed by splitting the screen vertically into four equal parts.</td></tr> <tr> <td>D12_34</td><td>Specifies the layout in which the windows for channel 1, 2, 3, and 4 are displayed in the upper left, upper right, lower left, and lower right, respectively.</td></tr> </tbody> </table>		Description	D1 (preset value)	Specifies the layout in which the window for channel 1 only is displayed on the entire display.	D12	Specifies the layout in which the window for channel 1 is displayed on the left side of the display area and the window for channel 2 on the right side.	D1_2	Specifies the layout in which the window for channel 1 is displayed in the upper part and the window for channel 2 in the lower part.	D112	Specifies the layout in which the window for channel 1 is displayed on the left side of 2/3 and the window for channel 2 on the right side of 1/3.	D1_1_2	Specifies the layout in which the window for channel 1 is displayed in the upper part of 2/3 and the window for channel 2 in the lower part of 1/3.	D123	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the left side, middle part, and right side, respectively.	D1_2_3	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper part, middle part, and the lower part, respectively.	D12_33	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper left, upper right, and lower part, respectively.	D11_23	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper part, lower left, and lower right, respectively.	D13_23	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper left, lower left, and right side, respectively.	D12_13	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the left side, upper right, and lower right, respectively.	D1234	Specifies the layout in which the windows for channel 1, 2, 3 and 4 are displayed by splitting the screen horizontally into four equal parts.	D1_2_3_4	Specifies the layout in which the windows for channel 1, 2, 3 and 4 are displayed by splitting the screen vertically into four equal parts.	D12_34	Specifies the layout in which the windows for channel 1, 2, 3, and 4 are displayed in the upper left, upper right, lower left, and lower right, respectively.
	Description																														
D1 (preset value)	Specifies the layout in which the window for channel 1 only is displayed on the entire display.																														
D12	Specifies the layout in which the window for channel 1 is displayed on the left side of the display area and the window for channel 2 on the right side.																														
D1_2	Specifies the layout in which the window for channel 1 is displayed in the upper part and the window for channel 2 in the lower part.																														
D112	Specifies the layout in which the window for channel 1 is displayed on the left side of 2/3 and the window for channel 2 on the right side of 1/3.																														
D1_1_2	Specifies the layout in which the window for channel 1 is displayed in the upper part of 2/3 and the window for channel 2 in the lower part of 1/3.																														
D123	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the left side, middle part, and right side, respectively.																														
D1_2_3	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper part, middle part, and the lower part, respectively.																														
D12_33	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper left, upper right, and lower part, respectively.																														
D11_23	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper part, lower left, and lower right, respectively.																														
D13_23	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the upper left, lower left, and right side, respectively.																														
D12_13	Specifies the layout in which the windows for channel 1, 2, and 3 are displayed in the left side, upper right, and lower right, respectively.																														
D1234	Specifies the layout in which the windows for channel 1, 2, 3 and 4 are displayed by splitting the screen horizontally into four equal parts.																														
D1_2_3_4	Specifies the layout in which the windows for channel 1, 2, 3 and 4 are displayed by splitting the screen vertically into four equal parts.																														
D12_34	Specifies the layout in which the windows for channel 1, 2, 3, and 4 are displayed in the upper left, upper right, lower left, and lower right, respectively.																														
Query response	{D1 D12 D1_2 D112 D1_1_2 D123 D1_2_3 D12_33 D11_23 D13_23 D12_13 D1234 D1_2_3_4 D12_34}<newline><^END>																														
Example of use	<pre>10 OUTPUT 717;" :DISP:SPL D1_2" 20 OUTPUT 717;" :DISP:SPL?" 30 ENTER 717;A\$</pre>																														
Related commands	:DISP:WIND{1-4}:SPL on page 323																														
Equivalent key	[Display] - Allocate Channels																														

:DISP:TABL

Syntax :DISPlay:TABLE[:STATe] {ON|OFF|1|0}
:DISPlay:TABLE[:STATe]?

Description Turns ON/OFF the display of the window selected with the :DISP:TABL:TYPE command.

Parameters

	Description
ON or 1	Turns ON the display.
OFF or 0 (preset value)	Turns OFF the display.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:TABL ON"
20 OUTPUT 717;":DISP:TABL?"
30 ENTER 717;A

Related commands :DISP:TABL:TYPE on page 317

Equivalent key **[Sweep Setup] - Edit Segment Table**
[Marker] - Marker Table
[Analysis] - Limit Test - Edit Limit Line
[Macro Setup] - Echo Window

NOTE When performing the operation from the front panel, you select the window and turn ON/OFF the display at the same time.

:DISP:TABL:TYPE

Syntax :DISPlay:TABLE:TYPE {MARKer|LIMit|SEGment|ECHO}
:DISPlay:TABLE:TYPE?

Description Selects the window whose display is turned ON/OFF with the :DISP:TABL command.

Parameters

	Description
MARKer (preset value)	Specifies the marker table window.
LIMit	Specifies the limit test table window.
SEGment	Specifies the segment table window.
ECHO	Specifies the echo window.

Query response {MARK|LIM|SEGM|ECHO}<newline><^END>

Example of use
10 OUTPUT 717;":DISP:TABL:TYPE SEGM"
20 OUTPUT 717;":DISP:TABL:TYPE?"
30 ENTER 717;A\$

Related commands :DISP:TABL on page 316

Equivalent key
[Sweep Setup] - Edit Segment Table
[Marker] - Marker Table
[Analysis] - Limit Test - Edit Limit Line
[Macro Setup] - Echo Window

NOTE When performing the operation from the front panel, you select the window and turn ON/OFF the display at the same time.

:DISP:UPD

Syntax	:DISPlay:UPDate[:IMMediate]
Description	Updates the LCD display once when the update of the LCD display is OFF (OFF is specified with the :DISP:ENAB command). (No query)
Example of use	10 OUTPUT 717; ":DISP:UPD"
Related commands	:DISP:ENAB on page 312
Equivalent key	No equivalent key is available on the front panel.

:DISP:WIND{1-4}:ACT

Syntax	:DISPlay:WINDow{[1] 2 3 4}:ACTivate
Description	Sets one of channel 1 (:WIND1) to channel 4 (:WIND4) to the active channel. You can set only the displayed channel to the active channel. If you execute this command trying to set a not displayed channel to the active channel, an error occurs and the command is ignored. (No query)
Example of use	10 OUTPUT 717; ":DISP:WIND1:ACT"
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286
Equivalent key	[Channel Prev] / [Channel Next]

:DISP:WIND{1-4}:ANN:MARK:ALIG

Syntax	:DISPlay:WINDow{[1] 2 3 4}:ANNotation:MARKer:ALIGn[:STATe] {ON OFF 1 0} :DISPlay:WINDow{[1] 2 3 4}:ANNotation:MARKer:ALIGn[:STATe]?						
Description	For channel 1 (:WIND1) to channel 4 (:WIND4), turns ON/OFF the alignment mode in which the display positions of the marker values for each trace are aligned relative to trace 1.						
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>ON or 1 (preset value)</td><td>Turns ON the alignment mode using trace 1 as the reference.</td></tr> <tr> <td>OFF or 0</td><td>Turn OFF the alignment mode.</td></tr> </tbody> </table>		Description	ON or 1 (preset value)	Turns ON the alignment mode using trace 1 as the reference.	OFF or 0	Turn OFF the alignment mode.
	Description						
ON or 1 (preset value)	Turns ON the alignment mode using trace 1 as the reference.						
OFF or 0	Turn OFF the alignment mode.						
Query response	{1 0}<newline><^END>						
Example of use	<pre> 10 OUTPUT 717;":DISP:WIND1:ANN:MARK:ALIG OFF" 20 OUTPUT 717;":DISP:WIND1:ANN:MARK:ALIG?" 30 ENTER 717;A </pre>						
Equivalent key	[Marker Fctn] - Annotation Options - Align						

:DISP:WIND{1-4}:ANN:MARK:SING

Syntax :DISPlay:WINDow{[1]|2|3|4}:ANNotation:MARKer:SINGle[:STATe] {ON|OFF|1|0}
 :DISPlay:WINDow{[1]|2|3|4}:ANNotation:MARKer:SINGle[:STATe]?

Description For channel 1 (:WIND1) to channel 4 (:WIND4), turns ON/OFF the active trace marker value display.

 When set to OFF, the marker values of all displayed traces (markers) are displayed.

Parameters

	Description
ON or 1 (preset value)	Displays the marker value of the active trace only (ON).
OFF or 0	Displays the marker values of all traces (OFF).

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:WIND1:ANN:MARK:SING OFF"
 20 OUTPUT 717;":DISP:WIND1:ANN:MARK:SING?"
 30 ENTER 717;A

Equivalent key **[Marker Fctn] - Annotation Options - Active Only**

:DISP:WIND{1-4}:LAB

Syntax :DISPlay:WINDow{[1]|2|3|4}:LABel {ON|OFF|1|0}
:DISPlay:WINDow{[1]|2|3|4}:LABel?

Description Turns ON/OFF the display of the graticule label of channel 1 (:WIND1) to channel 4 (:WIND4).

Parameters

	Description
ON or 1 (preset value)	Turns ON the graticule label display.
OFF or 0	Turns OFF the graticule label display.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:WIND1:LAB ON"
20 OUTPUT 717;":DISP:WIND1:LAB?"
30 ENTER 717;A

Equivalent key **[Display] - Graticule Label**

:DISP:WIND{1-4}:MAX

Syntax :DISPlay:WINDow{[1]|2|3|4}:MAXimize {ON|OFF|1|0}
 :DISPlay:WINDow{[1]|2|3|4}:MAXimize?

Description Turns ON/OFF the maximization of the active trace of channel 1 (:WIND1) to channel 4 (:WIND4) (specified with the :CALC{1-4}:PAR{1-4}:SEL command).

If you turned ON the maximization, only the maximized active trace is displayed in the window and the other traces are not displayed.

Parameters

	Description
ON or 1	Turns ON the maximization.
OFF or 0 (preset value)	Turns OFF the maximization.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:WIND1:MAX ON"
 20 OUTPUT 717;":DISP:WIND1:MAX?"
 30 ENTER 717;A

Related commands :CALC{1-4}:PAR{1-4}:SEL on page 286
 :DISP:MAX on page 314

Equivalent key **[Trace Max]**

:DISP:WIND{1-4}:SPL

Syntax :DISPlay:WINDow{[1]|2|3|4}:SPLit {D1|D12|D1_2|D112|D1_1_2|D123|D1_2_3|D12_33|D11_23|D13_23|D12_13|D1234|D1_2_3_4|D12_34}

Description Sets the graph layout of channel 1 (:WIND1) to channel 4 (:WIND4). For details about the graph layout, refer to Figure 3-1 on page 45.

Parameters

	Description
D1 (preset value)	Specifies the layout in which one graph is displayed in the entire window.
D12	Specifies the layout in which 2 graphs in total are displayed on the left side and right side of the window.
D1_2	Specifies the layout in which 2 graphs in total are displayed in the upper part and lower part of the window.
D112	Specifies the layout in which 2 graphs in total are displayed on the left side of 2/3 and right side of 1/3 of the window.
D1_1_2	Specifies the layout in which 2 graphs in total are displayed in the upper part of 2/3 and lower part of 1/3 of the window.
D123	Specifies the layout in which 3 graphs in total are displayed on the left side, middle part, and right side of the window.
D1_2_3	Specifies the layout in which 3 graphs in total are displayed in the upper part, middle part, and lower part of the window.
D12_33	Specifies the layout in which 3 graphs in total are displayed in the upper left, upper right, and lower part of the window.
D11_23	Specifies the layout in which 3 graphs in total are displayed in the upper part, lower left, and lower right of the window.
D13_23	Specifies the layout in which 3 graphs in total are displayed in the upper left, lower left, and right side of the window.
D12_13	Specifies the layout in which 3 graphs in total are displayed in the left side, upper right, and lower right of the window.
D1234	Specifies the layout in which 4 graphs in total are displayed by splitting the window horizontally into four equal parts.
D1_2_3_4	Specifies the layout in which 4 graphs in total are displayed by splitting the window vertically into four equal parts.
D12_34	Specifies the layout in which 4 graphs in total are displayed in the upper left, upper right, lower left, and lower right of the window.

Query response {D1|D12|D1_2|D112|D1_1_2|D123|D1_2_3|D12_33|D11_23|D13_23|D12_13|D1234|D1_2_3_4|D12_34}<newline><^END>

Example of use

```

10  OUTPUT 717;":DISP:WIND:SPL D1_2"
20  OUTPUT 717;":DISP:WIND:SPL?"
30  ENTER 717;A$

```

Related commands :DISP:SPL on page 315

Equivalent key [Display] - Allocate Traces

:DISP:WIND{1-4}:TITL

Syntax :DISPlay:WINDow{[1]|2|3|4}:TITLe[:STATe] {ON|OFF|1|0}
:DISPlay:WINDow{[1]|2|3|4}:TITLe[:STATe]?

Description Turns ON/OFF the display of the title label of channel 1 (:WIND1) to channel 4 (:WIND4) in the title area.

Parameters

	Description
ON or 1	Turns ON the title label display.
OFF or 0 (preset value)	Turns OFF the title label display.

Query response 10 OUTPUT 717;":DISP:WIND1:TITL ON"
20 OUTPUT 717;":DISP:WIND1:TITL?"
30 ENTER 717;A

Related commands :DISP:WIND{1-4}:TITL:DATA on page 324

Equivalent key **[Display] - Title Label**

:DISP:WIND{1-4}:TITL:DATA

Syntax :DISPlay:WINDow{[1]|2|3|4}:TITLe:DATA <string>
:DISPlay:WINDow{[1]|2|3|4}:TITLe:DATA?

Description Sets the title label displayed in the title area of channel 1 (:WIND1) to channel 4 (:WIND4).

Parameters

	<string>
Description	Title label
Range	254 characters or less
Preset value	""

Query response {string}<newline><^END>

Example of use 10 OUTPUT 717;":DISP:WIND1:TITL:DATA ""Title"""
20 OUTPUT 717;":DISP:WIND1:TITL?"
30 ENTER 717;A\$

Related commands :DISP:WIND{1-4}:TITL on page 324

Equivalent key **[Display] - Edit Title Label**

:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:X

Syntax	:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:ANNotation:MARKer:POSition:X <value> :DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:ANNotationMARKer:POSition:X?												
Description	For trace 1 (:TRAC1) through trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), sets the X-axis position where the marker value is displayed as the percentage of the display area width.												
Parameters	<table border="1"> <tr> <td></td><td><value></td></tr> <tr> <td>Description</td><td>The X-axis position where the marker value is displayed.</td></tr> <tr> <td>Range</td><td>-15 to 100</td></tr> <tr> <td>Preset value</td><td>1</td></tr> <tr> <td>Unit</td><td>% (percent)</td></tr> <tr> <td>Resolution</td><td>1</td></tr> </table>		<value>	Description	The X-axis position where the marker value is displayed.	Range	-15 to 100	Preset value	1	Unit	% (percent)	Resolution	1
	<value>												
Description	The X-axis position where the marker value is displayed.												
Range	-15 to 100												
Preset value	1												
Unit	% (percent)												
Resolution	1												
Query response	{value}<newline><^END>												
Example of use	10 OUTPUT 717;" :DISP:WIND1:TRAC1:ANN:MARK:POS:X 20" 20 OUTPUT 717;" :DISP:WIND1:TRAC1:ANN:MARK:POS:X?" 30 ENTER 717;A												
Related commands	:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:Y on page 326												
Equivalent key	[Marker Fctn] - Annotation Options - Marker Info X Pos												

:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:Y

Syntax	:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:ANNotation:MARKer:POSition:Y <value> :DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:ANNotationMARKer:POSition:Y?												
Description	For trace 1 (:TRAC1) through trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), sets the Y-axis position where the marker value is displayed as the percentage of the display area height.												
Parameters	<table><tr><td></td><td><value></td></tr><tr><td>Description</td><td>Y-axis position where the marker value is displayed.</td></tr><tr><td>Range</td><td>-15 to 100</td></tr><tr><td>Preset value</td><td>1</td></tr><tr><td>Unit</td><td>% (percent)</td></tr><tr><td>Resolution</td><td>1</td></tr></table>		<value>	Description	Y-axis position where the marker value is displayed.	Range	-15 to 100	Preset value	1	Unit	% (percent)	Resolution	1
	<value>												
Description	Y-axis position where the marker value is displayed.												
Range	-15 to 100												
Preset value	1												
Unit	% (percent)												
Resolution	1												
Query response	{value}<newline><^END>												
Example of use	10 OUTPUT 717;" :DISP:WIND1:TRAC1:ANN:MARK:POS:Y 40" 20 OUTPUT 717;" :DISP:WIND1:TRAC1:ANN:MARK:POS:Y?" 30 ENTER 717;A												
Related commands	:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:X on page 325												
Equivalent key	[Marker Fctn] - Annotation Options - Marker Info Y Pos												

:DISP:WIND{1-4}:TRAC{1-4}:ANN:YAX:MODE

Syntax	:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:ANNotation:YAXis:MODE {AUTO RELative} :DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:ANNotation:YAXis:MODE?						
Description	For trace 1 (:TRAC1) through trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), sets the graticule label display format on the left side of the Y-axis in the rectangular display format.						
Parameters	<table border="1"> <thead> <tr> <th></th><th>Description</th></tr> </thead> <tbody> <tr> <td>AUTO (preset value)</td><td>Specifies the normal display format.</td></tr> <tr> <td>RELative</td><td>Specifies the relative display, based on the reference value.</td></tr> </tbody> </table>		Description	AUTO (preset value)	Specifies the normal display format.	RELative	Specifies the relative display, based on the reference value.
	Description						
AUTO (preset value)	Specifies the normal display format.						
RELative	Specifies the relative display, based on the reference value.						
Query response	{value}<newline><^END>						
Example of use	<pre> 10 OUTPUT 717;" :DISP:WIND1:TRAC1:ANN:YAX:MODE REL " 20 OUTPUT 717;" :DISP:WIND1:TRAC1:ANN:YAX:MODE?" 30 ENTER 717;A </pre>						
Related commands	:DISP:WIND{1-4}:Y:DIV on page 336 :DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV on page 331 :DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS on page 332						
Equivalent key	[Display] - Graticule Label						

:DISP:WIND{1-4}:TRAC{1-4}:MEM

Syntax	:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4} :MEMory[:STATe] {ON OFF 1 0} :DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4} :MEMory[:STATe]?						
Description	For trace 1 (:TRAC1) to trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), turns ON/OFF the display of the memory trace.						
Parameters	<table><tr><th></th><th>Description</th></tr><tr><td>ON or 1</td><td>Turns ON the memory trace display.</td></tr><tr><td>OFF or 0 (preset value)</td><td>Turns OFF the memory trace display.</td></tr></table>		Description	ON or 1	Turns ON the memory trace display.	OFF or 0 (preset value)	Turns OFF the memory trace display.
	Description						
ON or 1	Turns ON the memory trace display.						
OFF or 0 (preset value)	Turns OFF the memory trace display.						
Query response	{1 0}<newline><^END>						
Example of use	10 OUTPUT 717; ":DISP:WIND1:TRAC1:MEM ON" 20 OUTPUT 717; ":DISP:WIND1:TRAC1:MEM?" 30 ENTER 717;A						
Related commands	:DISP:WIND{1-4}:TRAC{1-4}:STAT on page 329 :CALC{1-4}:MATH:MEM on page 281						
Equivalent key	[Display] - Display - Mem (when the data trace display is OFF) [Display] - Display - Data & Mem (when the data trace display is ON)						

:DISP:WIND{1-4}:TRAC{1-4}:STAT

Syntax	:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4} :STATe {ON OFF 1 0} :DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4} :STATe?
Description	For trace 1 (:TRAC1) to trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), turns ON/OFF the display of the data trace.
Parameters	

	Description
ON or 1 (preset value)	Turns ON the data trace display.
OFF or 0	Turns OFF the data trace display.

Query response	{1 0}<newline><^END>
Example of use	10 OUTPUT 717;":DISP:WIND1:TRAC1:STAT ON" 20 OUTPUT 717;":DISP:WIND1:TRAC1:STAT?" 30 ENTER 717;A
Related commands	:DISP:WIND{1-4}:TRAC{1-4}:MEM on page 328
Equivalent key	[Display] - Display - Data (when the memory trace display is OFF) [Display] - Display - Data & Mem (when the memory trace display is ON)

:DISP:WIND{1-4}:TRAC{1-4}:Y:AUTO

Syntax	:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4} :Y[:SCALE]:AUTO
Description	For trace 1 (:TRAC1) to trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), executes the auto scale (function to automatically adjust the value of the reference graticule line and the scale per division to display the trace appropriately). (No query)
Example of use	10 OUTPUT 717;":DISP:WIND1:TRAC1:Y:AUTO"
Related commands	:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV on page 330 :DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV on page 331
Equivalent key	[Scale] - Auto Scale

:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV

Syntax :DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4} :Y[:SCALe]:PDIVision <numeric>
:DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4} :Y[:SCALe]:PDIVision?

Description For trace 1 (:TRAC1) to trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4): when the data format is not the Smith chart format or the polar format, sets the scale per division; when the data format is the Smith chart format or the polar format, sets the full scale value (the value of the outermost circle).

Parameters

	<numeric>
Description	Scale value
Range	1E-18 to 1E8
Preset value	Varies depending on the data format as follows: Logarithmic Magnitude: 10 Phase, Expand Phase, Positive Phase: 90 Group Delay: 1E-8 Smith, Polar, SWR: 1 Linear Magnitude: 0.1 Real, Imaginary: 0.2
Unit	Varies depending on the data format as follows: Logarithmic Magnitude: dB (decibel) Phase, Expand Phase, Positive Phase: ° (degree) Group Delay: s (second) Others: No unit

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":DISP:WIND1:TRAC1:Y:PDIV 2.5"
20 OUTPUT 717;":DISP:WIND1:TRAC1:Y:PDIV?"
30 ENTER 717;A

Related commands :DISP:WIND{1-4}:Y:DIV on page 336
:DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV on page 331
:DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS on page 332

Equivalent key [Scale] - Scale/Div

:DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV

- Syntax** :DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4} :Y[:SCALe]:RLEVel <numeric>
:DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4} :Y[:SCALe]:RLEVel?
- Description** For trace 1 (:TRAC1) to trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), sets the value of the reference graticule line.

Parameters

	<numeric>
Description	Value of reference graticule line
Range	-5E8 to 5E8
Preset value	0*1
Unit	Varies depending on the data format as follows: Logarithmic Magnitude: dB (decibel) Phase, Expand Phase, Positive Phase: ° (degree) Group Delay: s (second) Others: No unit

*1. When the data format is "SWR," the preset value is 1.

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

- Query response** {numeric}<newline><^END>
- Example of use**
- ```
10 OUTPUT 717;" :DISP:WIND1:TRAC1:Y:RLEV 1E2"
20 OUTPUT 717;" :DISP:WIND1:TRAC1:Y:RLEV?"
30 ENTER 717;A
```
- Related commands** :DISP:WIND{1-4}:Y:DIV on page 336  
:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV on page 330  
:DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS on page 332
- Equivalent key** **[Scale] - Reference Value**

## :DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS

**Syntax** :DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4} :Y[:SCALe]:RPOSition <numeric>  
:DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4} :Y[:SCALe]:RPOSition?

**Description** For trace 1 (:TRAC1) to trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), specifies a reference graticule line with its number (an integer assigned starting from 0 from the lowest division).

### Parameters

|              |                                            |
|--------------|--------------------------------------------|
|              | <numeric>                                  |
| Description  | Number of graticule line                   |
| Range        | 0 to the number of divisions <sup>*1</sup> |
| Preset value | 5 <sup>*2</sup>                            |
| Resolution   | 1                                          |

\*1. Set with the :DISP:WIND{1-4}:Y:DIV commands.

\*2. When the data format is "Linear Magnitude" or "SWR," the preset value is 1.

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;" :DISP:WIND1:TRAC1:Y:RPOS 6"  
20 OUTPUT 717;" :DISP:WIND1:TRAC1:Y:RPOS?"  
30 ENTER 717;A

**Related commands** :DISP:WIND{1-4}:Y:DIV on page 336  
:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV on page 330  
:DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV on page 331

**Equivalent key** [Scale] - Reference Position

## :DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:FREQ

|                  |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |  |         |             |                        |       |               |              |   |      |                                 |
|------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|---------|-------------|------------------------|-------|---------------|--------------|---|------|---------------------------------|
| Syntax           | :DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:Y:TRACk:FREQuency <value><br>:DISPlay:WINDow{[1] 2 3 4}:TRACe{[1] 2 3 4}:Y:TRACk:FREQuency?                                                                                                                                                                                                                                                                                                                                                                     |  |         |             |                        |       |               |              |   |      |                                 |
| Description      | For trace 1 (:TRAC1) through trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), sets a frequency when you want to specify a frequency on trace data as the reference value. Tracking is not performed when the specified frequency lies outside the preset range. When a frequency that does not match any measurement point is specified, interpolation is performed using the preceding and following measurement points, and the resulting value is used as the reference value for tracking. |  |         |             |                        |       |               |              |   |      |                                 |
| Parameters       | <table border="1"> <tr> <td></td><td>&lt;value&gt;</td></tr> <tr> <td>Description</td><td>Frequency for tracking</td></tr> <tr> <td>Range</td><td>-1E12 to 1E12</td></tr> <tr> <td>Preset value</td><td>0</td></tr> <tr> <td>Unit</td><td>Hz (hertz), dBm, or s (seconds)</td></tr> </table>                                                                                                                                                                                                                |  | <value> | Description | Frequency for tracking | Range | -1E12 to 1E12 | Preset value | 0 | Unit | Hz (hertz), dBm, or s (seconds) |
|                  | <value>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |  |         |             |                        |       |               |              |   |      |                                 |
| Description      | Frequency for tracking                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |  |         |             |                        |       |               |              |   |      |                                 |
| Range            | -1E12 to 1E12                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |  |         |             |                        |       |               |              |   |      |                                 |
| Preset value     | 0                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |  |         |             |                        |       |               |              |   |      |                                 |
| Unit             | Hz (hertz), dBm, or s (seconds)                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |  |         |             |                        |       |               |              |   |      |                                 |
| Query response   | {value}<newline><^END>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |  |         |             |                        |       |               |              |   |      |                                 |
| Example of use   | <pre>10  OUTPUT 717;" :DISP:WIND1:TRAC1:Y:TRAC:FREQ 1E9" 20  OUTPUT 717;" :DISP:WIND1:TRAC1:Y:TRAC:FREQ?" 30  ENTER 717;A</pre>                                                                                                                                                                                                                                                                                                                                                                             |  |         |             |                        |       |               |              |   |      |                                 |
| Related commands | :DISP:WIND{1-4}:Y:DIV on page 336<br>:DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:MODE on page 334                                                                                                                                                                                                                                                                                                                                                                                                                      |  |         |             |                        |       |               |              |   |      |                                 |
| Equivalent key   | <b>[Scale] - Reference Tracking - Track Frequency</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                       |  |         |             |                        |       |               |              |   |      |                                 |

## :DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:MODE

Syntax :DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4}:Y:TRACk:MODE  
{OFF|PEAK|FREQuency}  
:DISPlay:WINDow{[1]|2|3|4}:TRACe{[1]|2|3|4}:Y:TRACk:MODE?

Description For trace 1 (:TRAC1) and trace 4 (:TRAC4) of channel 1 (:WIND1) to channel 4 (:WIND4), sets the tracking method to offset the trace data after sweep.

Parameters

|                    | Description                                               |
|--------------------|-----------------------------------------------------------|
| OFF (preset value) | Does not perform tracking for trace data.                 |
| PEAK               | Specifies the peak value as the reference value.          |
| FREQuency          | Specifies the specified frequency as the reference value. |

Query response {OFF|PEAK|FREQ}<newline><^END>

Example of use  
10 OUTPUT 717;":DISP:WIND1:TRAC1:Y:TRAC:MODE PEAK"  
20 OUTPUT 717;":DISP:WIND1:TRAC1:Y:TRAC:MODE?"  
30 ENTER 717;A

Related commands :DISP:WIND{1-4}:Y:DIV on page 336  
:DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:FREQ on page 333

Equivalent key **[Scale] - Reference Tracking - Tracking**

## :DISP:WIND{1-4}:X:SPAC

**Syntax** :DISPlay:WINDow{[1]|2|3|4}:X:SPACing {LINear|OBASe}  
:DISPlay:WINDow{[1]|2|3|4}:X:SPACing?

**Description** Selects the display method of the graph horizontal axis of channel 1 (:WIND1) to channel 4 (:WIND4) for segment sweep.

**Parameters**

|                         | Description                                                                                                                                   |
|-------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------|
| LINear                  | Specifies the frequency base (linear frequency axis with the minimum frequency at the left edge and the maximum frequency at the right edge). |
| OBASe<br>(preset value) | Specifies the order base (axis in which the measurement point numbers are positioned evenly in the order of measurement).                     |

**Query response** {LIN|OBAS}<newline><^END>

**Example of use**  
10 OUTPUT 717;":DISP:WIND1:X:SPAC OBAS"  
20 OUTPUT 717;":DISP:WIND1:X:SPAC?"  
30 ENTER 717;A\$

**Related commands** :SENS{1-4}:SWE:TYPE on page 428

**Equivalent key** [Sweep Setup] - Segment Display

**:DISP:WIND{1-4}:Y:DIV**

|                  |                                                                                                                                                                                                                                                                                                                                                                                                                                                     |  |           |             |           |       |         |              |    |            |   |
|------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-----------|-------------|-----------|-------|---------|--------------|----|------------|---|
| Syntax           | <code>:DISPlay:WINDow{[1] 2 3 4}:Y[:SCALe]:DIVisions &lt;numeric&gt;</code><br><code>:DISPlay:WINDow{[1] 2 3 4}:Y[:SCALe]:DIVisions?</code>                                                                                                                                                                                                                                                                                                         |  |           |             |           |       |         |              |    |            |   |
| Description      | <p>Sets the number of divisions of all the graphs of channel 1 (:WIND1) to channel 4 (:WIND4).</p> <p>The number of graticule line (specified with the :DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS command) depends on this setting.</p>                                                                                                                                                                                                                       |  |           |             |           |       |         |              |    |            |   |
| Parameters       | <table><tr><td></td><td>&lt;numeric&gt;</td></tr><tr><td>Description</td><td>Divisions</td></tr><tr><td>Range</td><td>4 to 30</td></tr><tr><td>Preset value</td><td>10</td></tr><tr><td>Resolution</td><td>2</td></tr></table> <p>If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.</p> |  | <numeric> | Description | Divisions | Range | 4 to 30 | Preset value | 10 | Resolution | 2 |
|                  | <numeric>                                                                                                                                                                                                                                                                                                                                                                                                                                           |  |           |             |           |       |         |              |    |            |   |
| Description      | Divisions                                                                                                                                                                                                                                                                                                                                                                                                                                           |  |           |             |           |       |         |              |    |            |   |
| Range            | 4 to 30                                                                                                                                                                                                                                                                                                                                                                                                                                             |  |           |             |           |       |         |              |    |            |   |
| Preset value     | 10                                                                                                                                                                                                                                                                                                                                                                                                                                                  |  |           |             |           |       |         |              |    |            |   |
| Resolution       | 2                                                                                                                                                                                                                                                                                                                                                                                                                                                   |  |           |             |           |       |         |              |    |            |   |
| Query response   | {numeric}<newline><^END>                                                                                                                                                                                                                                                                                                                                                                                                                            |  |           |             |           |       |         |              |    |            |   |
| Example of use   | <pre>10  OUTPUT 717;":DISP:WIND1:Y:DIV 12" 20  OUTPUT 717;":DISP:WIND1:Y:DIV?" 30  ENTER 717;A</pre>                                                                                                                                                                                                                                                                                                                                                |  |           |             |           |       |         |              |    |            |   |
| Related commands | <code>:DISP:WIND{1-4}:TRAC{1-4}:Y:PDIV</code> on page 330<br><code>:DISP:WIND{1-4}:TRAC{1-4}:Y:RLEV</code> on page 331<br><code>:DISP:WIND{1-4}:TRAC{1-4}:Y:RPOS</code> on page 332                                                                                                                                                                                                                                                                 |  |           |             |           |       |         |              |    |            |   |
| Equivalent key   | <b>[Scale] - Divisions</b>                                                                                                                                                                                                                                                                                                                                                                                                                          |  |           |             |           |       |         |              |    |            |   |

## :FORM:BORD

**Syntax** :FORMat:BORDer {NORMal|SWAPped}  
:FORMat:BORDer?

**Description** When the data transfer format is set to the binary transfer format, sets the transfer order of each byte in data (byte order).  
For details about the data transfer format, refer to “Data Transfer Format” on page 104.

### Parameters

|                          | Description                                                                                            |
|--------------------------|--------------------------------------------------------------------------------------------------------|
| NORMal<br>(preset value) | Specifies the byte order in which transfer starts from the byte including MSB (Most Significant Bit).  |
| SWAPped                  | Specifies the byte order in which transfer starts from the byte including LSB (Least Significant Bit). |

**Query response** {NORM|SWAP}<newline><^END>

**Example of use**  
10 OUTPUT 717;":FORM:BORD SWAP"  
20 OUTPUT 717;":FORM:BORD?"  
30 ENTER 717;A\$

**Related commands** :FORM:DATA on page 338

**Equivalent key** No equivalent key is available on the front panel.

## :FORM:DATA

Syntax :FORMat:DATA {ASCii|REAL|REAL32}

:FORMat:DATA?

Description Use the following commands to set the format to transfer data.

- :CALC{1-4}:DATA:FDAT on page 215
- :CALC{1-4}:DATA:FMEM on page 216
- :CALC{1-4}:DATA:SDAT on page 217
- :CALC{1-4}:DATA:SMEM on page 218
- :CALC{1-4}:FUNC:DATA? on page 221
- :CALC{1-4}:LIM:DATA on page 233
- :CALC{1-4}:LIM:REP? on page 242
- :SENS{1-4}:FREQ:DATA? on page 416
- :SENS{1-4}:SEGM:DATA on page 421

For details about the data transfer format, refer to “Data Transfer Format” on page 104.

Parameters

|                         | Description                                                      |
|-------------------------|------------------------------------------------------------------|
| ASCii<br>(preset value) | Specifies the ASCII transfer format.                             |
| REAL                    | Specifies the IEEE 64-bit floating point binary transfer format. |
| REAL32                  | Specifies the IEEE 32-bit floating point binary transfer format. |

Query response {ASC|REAL|REAL32}<newline><^END>

Example of use  
10 OUTPUT 717; ":FORM:DATA REAL"  
20 OUTPUT 717; ":FORM:DATA?"  
30 ENTER 717;A\$

Related commands :FORM:BORD on page 337

Equivalent key No equivalent key is available on the front panel.

## :HCOP

|                  |                                                                                                        |
|------------------|--------------------------------------------------------------------------------------------------------|
| Syntax           | :HCOP[:IMMediate]                                                                                      |
| Description      | Outputs the display image on the LCD display to the printer connected to the E5061A/E5062A. (No query) |
| Example of use   | 10 OUTPUT 717;":HCOP"                                                                                  |
| Related commands | :HCOP:ABOR on page 339<br>:HCOP:IMAG on page 339                                                       |
| Equivalent key   | <b>[System] - Print</b>                                                                                |

## :HCOP:ABOR

|                  |                                     |
|------------------|-------------------------------------|
| Syntax           | :HCOPy:ABORt                        |
| Description      | Aborts the print output. (No query) |
| Example of use   | 10 OUTPUT 717;":HCOP:ABOR"          |
| Related commands | :HCOP on page 339                   |
| Equivalent key   | <b>[System] - Abort Printing</b>    |

## :HCOP:IMAG

|             |                                                    |
|-------------|----------------------------------------------------|
| Syntax      | :HCOPy:IMAGe {NORMal INVert}<br>:HCOPy:IMAGe?      |
| Description | Selects the print color for output to the printer. |
| Parameters  |                                                    |

|                       | Description                                                    |
|-----------------------|----------------------------------------------------------------|
| NORMal                | Specifies printing in close color to the display color.        |
| INVert (preset value) | Specifies printing in the inverted color of the display color. |

|                  |                                                                                    |
|------------------|------------------------------------------------------------------------------------|
| Query response   | {NORM INV}<newline><^END>                                                          |
| Example of use   | 10 OUTPUT 717;":HCOP:IMAG NORM"<br>20 OUTPUT 717;":HCOP:IMAG?"<br>30 ENTER 717;A\$ |
| Related commands | :HCOP on page 339                                                                  |
| Equivalent key   | <b>[System] - Invert Image</b>                                                     |

## **:INIT{1-4}**

|                  |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | <code>:INITiate{[1] 2 3 4}[:IMMediate]</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| Description      | <p>Changes the state of each channel of channel 1 (:INIT1) to channel 4 (:INIT4) to the startup state in the trigger system.</p> <p>When this command is executed for a channel in the idle state, it goes into the initiate state immediately. Then, after measurement is executed once, it goes back to the idle state.</p> <p>If this command is executed for a channel that is not in the idle state or for which the continuous initiation mode is set to ON (ON is specified with the :INIT{1-4}:CONT command), an error occurs and the command is ignored.</p> <p>For details about the trigger system, refer to “Trigger system” on page 80. (No query)</p> |
| Example of use   | <code>10 OUTPUT 717; ":INIT1"</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| Related commands | :INIT{1-4}:CONT on page 341                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| Equivalent key   | <b>[Trigger] - Single</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |

## :INIT{1-4}:CONT

**Syntax** :INITiate{[1]|2|3|4}:CONTinuous {ON|OFF|1|0}  
:INITiate{[1]|2|3|4}:CONTinuous?

**Description** Turns ON/OFF of the continuous initiation mode of channel 1 (:INIT1) to channel 4 (:INIT4) in the trigger system.  
For details about the trigger system, refer to “Trigger system” on page 80.

**Parameters**

|          | Description                               |
|----------|-------------------------------------------|
| ON or 1  | Turns ON the continuous initiation mode.  |
| OFF or 0 | Turns OFF the continuous initiation mode. |

Regarding to this setting, only channel 1 is initialized to ON with the :SYST:PRES command; all the channels are initialized to OFF with the \*RST command.

**Query response** {1|0}<newline><^END>

**Example of use**  
10 OUTPUT 717;":INIT1:CONT OFF"  
20 OUTPUT 717;":INIT1:CONT?"  
30 ENTER 717;A

**Related commands** :INIT{1-4} on page 340

**Equivalent key** **[Trigger] - Continuous** (continuous initiation mode ON)  
**[Trigger] - Hold** (continuous initiation mode OFF)

## :MMEM:CAT?

|                |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |  |            |             |                                                       |       |                        |
|----------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|------------|-------------|-------------------------------------------------------|-------|------------------------|
| Syntax         | :MMEMory:CATalog? <string 1>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |  |            |             |                                                       |       |                        |
| Description    | <p>Reads out the following information on the built-in storage device of the E5061A/E5062A.</p> <p>To read out the information in the root directory (folder), specify “\” (backslash). If you want to specify a directory on the floppy disk drive, you need to add “A:” at the beginning of the file name. Separate directory names with “/” (slash) or “\” (backslash). (Query only)</p> <ul style="list-style-type: none"><li>• Space in use</li><li>• Available space</li><li>• Name and size of all files (including directories) in the specified directory.</li></ul>                                                                                      |  |            |             |                                                       |       |                        |
| Parameters     | <table><tr><td></td><td>&lt;string 1&gt;</td></tr><tr><td>Description</td><td>Directory name whose information you want to read out</td></tr><tr><td>Range</td><td>254 characters or less</td></tr></table>                                                                                                                                                                                                                                                                                                                                                                                                                                                        |  | <string 1> | Description | Directory name whose information you want to read out | Range | 254 characters or less |
|                | <string 1>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |  |            |             |                                                       |       |                        |
| Description    | Directory name whose information you want to read out                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |  |            |             |                                                       |       |                        |
| Range          | 254 characters or less                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |  |            |             |                                                       |       |                        |
| Query response | <p>{string 2}&lt;newline&gt;&lt;^END&gt;</p> <p>The format of the readout character string is as follows:</p> <p>"{used_size},{free_size},{name 1},{size 1},...,{name N},{size N}"</p> <p>Where N is the number of all files in the specified directory and n is an integer between 1 and N.</p> <p>{used_size}:           Space in use of the built-in storage device (byte)<sup>*1</sup>.</p> <p>{free_size}:           Available space of the built-in storage device (byte)<sup>*1</sup>.</p> <p>{name n}:             Name of the n-th file (directory).</p> <p>{size n}:             Size (byte) of the n-th file (directory). Always 0 for directories.</p> |  |            |             |                                                       |       |                        |
| Example of use | <pre>10  DIM A\$[1000] 20  OUTPUT 717;":MMEM:CAT? ""\""" 30  ENTER 717;A\$</pre>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |  |            |             |                                                       |       |                        |
| Equivalent key | No equivalent key is available on the front panel.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |  |            |             |                                                       |       |                        |

<sup>\*1</sup>.If you specify a directory on the floppy disk drive, it is the capacity of the floppy disk in the drive.

## :MMEM:COPY

**Syntax** :MMEMory:COPY <string 1>,<string 2>

**Description** Copies a file.

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory (folder) names and file name, separate them with "/" (slash) or "\" (backslash).

If the specified copy source file does not exist, an error occurs and the command is ignored. Notice that, if a file with the same name as the specified copy destination file name exists, its contents are overwritten. (No query)

**Parameters**

|             | <string 1>             | <string 2>                 |
|-------------|------------------------|----------------------------|
| Description | Copy source file name  | Copy destination file name |
| Range       | 254 characters or less | 254 characters or less     |

**Example of use** 10 OUTPUT 717;":MMEM:COPY "Test1/State01.sta","A:Test1\_01.sta""

**Equivalent key** Practical front key operation is not available.

**:MMEM:DEL**

|                |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |  |          |             |                                                |       |                        |
|----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|----------|-------------|------------------------------------------------|-------|------------------------|
| Syntax         | :MMEMory:DELeTe <string>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |  |          |             |                                                |       |                        |
| Description    | <p>Deletes an existing file or directory (folder).</p> <p>When you delete a directory, all the files and directories in it are deleted.</p> <p>Specify the file name with the extension. If you want to specify a file or directory on the floppy disk drive, you need to add “A:” at the beginning of its name. When you specify a file (directory) under an existing directory, separate them with “/” (slash) or “\” (backslash).</p> <p>If the specified file or directory does not exist, an error occurs and the command is ignored. (No query)</p> |  |          |             |                                                |       |                        |
| Parameters     | <table><tr><td></td><td>&lt;string&gt;</td></tr><tr><td>Description</td><td>File name or directory name you want to delete</td></tr><tr><td>Range</td><td>254 characters or less</td></tr></table>                                                                                                                                                                                                                                                                                                                                                        |  | <string> | Description | File name or directory name you want to delete | Range | 254 characters or less |
|                | <string>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |  |          |             |                                                |       |                        |
| Description    | File name or directory name you want to delete                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |  |          |             |                                                |       |                        |
| Range          | 254 characters or less                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |  |          |             |                                                |       |                        |
| Example of use | <pre>10 OUTPUT 717; ":MMEM:DEL ""Test1/State01.sta"" 10 OUTPUT 717; ":MMEM:DEL ""A:State01.sta""</pre>                                                                                                                                                                                                                                                                                                                                                                                                                                                    |  |          |             |                                                |       |                        |
| Equivalent key | Practical front key operation is not available.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |  |          |             |                                                |       |                        |

## :MMEM:LOAD

Syntax :MMEMory:LOAD[:STATe] <string>

Description Recalls the specified instrument state file (file with the .sta extension saved with the :MMEM:STOR command).

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

If the specified file does not exist, an error occurs and the command is ignored. (No query)

### Parameters

|             |                            |
|-------------|----------------------------|
|             | <string>                   |
| Description | Instrument state file name |
| Range       | 254 characters or less     |

Example of use 10 OUTPUT 717;":MMEM:LOAD ""Test1/State01.sta""

10 OUTPUT 717;":MMEM:LOAD ""A:State01.sta""

Related commands :MMEM:STOR on page 353

Equivalent key **[Save/Recall] - Recall State**

## :MMEM:LOAD:CHAN

**Syntax** :MMEMory:LOAD:CHANnel[:STATe] {A|B|C|D}

**Description** Recalls the instrument state for an individual channel (saved with the :MMEM:STOR:CHAN command) from the specified register as the setting of the active channel (specified with the :DISP:WIND{1-4}:ACT command).

It is possible to recall the register from a different channel where it was saved.

If no instrument state has been saved in the specified register, an error occurs and the command is ignored. (No query)

### Parameters

|   | Description           |
|---|-----------------------|
| A | Specifies register A. |
| B | Specifies register B. |
| C | Specifies register C. |
| D | Specifies register D. |

**Example of use** 10 OUTPUT 717; ":MMEM:LOAD:CHAN A"

**Related commands** :MMEM:STOR:CHAN on page 354  
:DISP:WIND{1-4}:ACT on page 318

**Equivalent key** **[Save/Recall] - Recall Channel - A|B|C|D**

## :MMEM:LOAD:CHAN:COEF

**Syntax** :MMEMory:LOAD:CHANnel:COEFficient {A|B|C|D}

**Description** Recalls the calibration coefficient for an individual channel (saved with the :MMEM:STOR:CHAN:COEF command) from the specified register as the setting of the active channel (specified with the :DISP:WIND{1-4}:ACT command).

It is possible to recall the register from a different channel where it was saved.

If no instrument state has been saved in the specified register, an error occurs and the command is ignored. (No query)

### Parameters

|   | Description           |
|---|-----------------------|
| A | Specifies register A. |
| B | Specifies register B. |
| C | Specifies register C. |
| D | Specifies register D. |

**Example of use** 10 OUTPUT 717;":MMEM:LOAD:CHAN:COEF A"

**Related commands**

**Equivalent key** [Save/Recall] - Recall Channel - Cal Only A|B|C|D

### NOTE

The calibration coefficient registers A to D are different from the channel state registers A to D. :MMEM:STOR:CHAN command does not affect the calibration coefficient registers.

## :MMEM:LOAD:LIM

Syntax :MMEMory:LOAD:LIMit <string>

Description As the limit table for the active trace (specified with the :CALC{1-4}:PAR{1-4}:SEL command) of the active channel (specified with the :DISP:WIND{1-4}:ACT command), recalls the specified limit table file (file with the .csv extension saved with the :MMEM:STOR:LIM command).

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

If the specified file does not exist, an error occurs and the command is ignored. (No query)

### Parameters

|             |                          |
|-------------|--------------------------|
|             | <string>                 |
| Description | File name of limit table |
| Range       | 254 characters or less   |

Example of use 10 OUTPUT 717;":MMEM:LOAD:LIM ""Test1/Limit01.csv""  
10 OUTPUT 717;":MMEM:LOAD:LIM ""A:Limit01.csv""

Related commands :MMEM:STOR:LIM on page 358  
:DISP:WIND{1-4}:ACT on page 318

Equivalent key **[Analysis] - Limit Test - Edit Limit Line - Import from CSV File**

## :MMEM:LOAD:PROG

**Syntax** :MMEMory:LOAD:PROGram <string>

**Description** Loads (or imports) a VBA project (a file with the .vba extension), a module (a file with the .bas extension), a user form (a file with the .frm extension) or a class module (a file with the .cls extension).

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

If the specified file does not exist, an error occurs and the command is ignored. (No query)

### Parameters

|             |                        |
|-------------|------------------------|
|             | <string>               |
| Description | File name              |
| Range       | 254 characters or less |

**Example of use**

```
10 OUTPUT 717;":MMEM:LOAD:PROG ""Test1/Test1_01.vba""
10 OUTPUT 717;":MMEM:LOAD:PROG ""A:Test1_01.vba""
```

**Related commands** :MMEM:STOR:PROG on page 359

**Equivalent key** [Macro Setup] - Load VBA Project

## :MMEM:LOAD:RLIM

Syntax :MMEMory:LOAD:RLIMit <string>

Description As the ripple limit table for the active trace (specified with the :CALC{1-4}:PAR{1-4}:SEL command) of the active channel (specified with the :DISP:WIND{1-4}:ACT command), recalls the specified ripple limit table file (file with the .csv extension saved with the :MMEM:STOR:RLIM command).

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you write directory names and the file name, separate them with a "/" (slash) or "\" (backslash).

If the specified file does not exist, an error occurs and the command is ignored. (No query)

### Parameters

|             | <string>                             |
|-------------|--------------------------------------|
| Description | File name of the ripple limit table. |
| Range       | 254 characters or less               |

Example of use 10 OUTPUT 717;":MMEM:LOAD:RLIM ""RTest1/Rlim01.csv""  
10 OUTPUT 717;":MMEM:LOAD:RLIM ""A:Rlim01.csv""

Related commands :MMEM:STOR:RLIM on page 360  
:DISP:WIND{1-4}:ACT on page 318  
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Analysis] - Ripple Limit - Edit Ripple Limit - Import from CSV File**

## :MMEM:LOAD:SEGM

**Syntax** :MMEMory:LOAD:SEGMent <string>

**Description** As the segment sweep table for the active channel (specified with the :DISP:WIND{1-4}:ACT command), recalls the specified segment sweep table file (a file with the .csv extension saved with the :MMEM:STOR:SEGM command).

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

If the specified file does not exist, an error occurs and the command is ignored. (No query)

### Parameters

|             |                                  |
|-------------|----------------------------------|
|             | <string>                         |
| Description | File name of segment sweep table |
| Range       | 254 characters or less           |

**Example of use**

```
10 OUTPUT 717;":MMEM:LOAD:SEGM ""Test1/Segm01.csv""
10 OUTPUT 717;":MMEM:LOAD:SEGM ""A:Segm01.csv""
```

**Related commands** :MMEM:STOR:SEGM on page 362  
:DISP:WIND{1-4}:ACT on page 318

**Equivalent key** [Sweep Setup] - Edit Segment Table - Import from CSV File

**:MMEM:MDIR**

Syntax :MMEMory:MDIRectory <string>

Description Creates a new directory (folder).

If you want to create a directory on the floppy disk drive, you need to add “A:” at the beginning of the directory name. When you create a directory under an existing directory, separate between the directory names with “/” (slash) or “\” (backslash).

If a directory with the same name as the specified directory name exists, an error occurs and the command is ignored. (No query)

Parameters

|             |                                   |
|-------------|-----------------------------------|
|             | <string>                          |
| Description | Directory name you want to create |
| Range       | 254 characters or less            |

Example of use 10 OUTPUT 717;":MMEM:MDIR ""Test1""

10 OUTPUT 717;":MMEM:MDIR ""A:Test1""

Equivalent key Practical front key operation is not available.

## :MMEM:STOR

Syntax :MMEMory:STORe[:STATe] <string>

Description Saves the instrument state (data to be saved specified with the :MMEM:STOR:STYP command) into a file.

Specify the file name with the .sta extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

Notice that, if a file with the specified file name exists, its contents are overwritten. (No query)

**NOTE** The instrument setting file saved with the autorec.sta (or A:autorec.sta) file name is automatically recalled when turning on the E5061A/E5062A.

### Parameters

|             |                                                          |
|-------------|----------------------------------------------------------|
|             | <string>                                                 |
| Description | File name in which you want to save the instrument state |
| Range       | 254 characters or less                                   |

Example of use 10 OUTPUT 717;":MMEM:STOR ""Test1/State01.sta""

10 OUTPUT 717;":MMEM:STOR ""A:State01.sta""

Related commands :MMEM:LOAD on page 345

:MMEM:STOR:STYP on page 363

Equivalent key **[Save/Recall] - Save State|Re-Save State**

## :MMEM:STOR:CHAN

|             |                                                                                                                                                                                                                                                                                                                                        |
|-------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :MMEMory:STORe:CHANnel[:STATe] {A B C D}                                                                                                                                                                                                                                                                                               |
| Description | Saves the instrument state of the items set for the active channel (specified with the :DISP:WIND{1-4}:ACT command) specific to that channel only into the specified register (volatile memory).<br><br>Notice that, if an instrument state has been saved already in the specified register, its contents are overwritten. (No query) |

### Parameters

|   | Description           |
|---|-----------------------|
| A | Specifies register A. |
| B | Specifies register B. |
| C | Specifies register C. |
| D | Specifies register D. |

Example of use     10     OUTPUT 717; ":MMEM:STOR:CHAN A"

Related commands   :MMEM:LOAD:CHAN on page 346  
                      :DISP:WIND{1-4}:ACT on page 318

Equivalent key     **[Save/Recall] - Save Channel - A|B|C|D**

## :MMEM:STOR:CHAN:CLE

|                  |                                                                                                                         |
|------------------|-------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :MMEMory:STORe:CHANnel:CLEar                                                                                            |
| Description      | Deletes the instrument state for each channel (saved with the :MMEM:STOR:CHAN command) in all the registers. (No query) |
| Example of use   | 10     OUTPUT 717; ":MMEM:STOR:CHAN:CLE"                                                                                |
| Related commands | :MMEM:STOR:CHAN on page 354                                                                                             |
| Equivalent key   | <b>[Save/Recall] - Save Channel - Clear States - OK</b>                                                                 |

## :MMEM:STOR:CHAN:COEF

**Syntax** :MMEMory:STORe:CHANnel:COEFficient {A|B|C|D}

**Description** Saves the calibration coefficient of the active channel (specified with the :DISP:WIND{1-4}:ACT command) into the specified register (volatile memory).  
Notice that, if an instrument state has been saved already in the specified register, its contents are overwritten. (No query)

**Parameters**

|   | Description           |
|---|-----------------------|
| A | Specifies register A. |
| B | Specifies register B. |
| C | Specifies register C. |
| D | Specifies register D. |

**Example of use** 10 OUTPUT 717; ":MMEM:STOR:CHAN:COEF A"

**Related commands** :MMEM:LOAD:CHAN:COEF on page 347

**Equivalent key** **[Save/Recall] - Save Channel - Cal Only A|B|C|D**

**NOTE** The calibration coefficient registers A to D are different from the channel state registers A to D. :MMEM:STOR:CHAN command does not affect the calibration coefficient registers.

## :MMEM:STOR:FDAT

Syntax :MMEMory:STORe:FDATa <string>

Description Saves the formatted data array of the active trace (specified with the :CALC{1-4}:PAR{1-4}:SEL command) of the active channel (specified with the :DISP:WIND{1-4}:ACT command) into a file in the CSV format.

Specify the file name with the .csv extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

Notice that, if a file with the specified file name exists, its contents are overwritten. (No query)

Parameters

|             |                                                              |
|-------------|--------------------------------------------------------------|
|             | <string>                                                     |
| Description | File name in which you want to save the formatted data array |
| Range       | 254 characters or less                                       |

Example of use 10 OUTPUT 717;":MMEM:STOR:FDAT ""Result/Trace01.csv""  
10 OUTPUT 717;":MMEM:STOR:FDAT ""A:Trace01.csv""

Related commands :DISP:WIND{1-4}:ACT on page 318  
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Save/Recall] - Save Trace Data**

## :MMEM:STOR:IMAG

**Syntax** :MMEMory:STORe:IMAGe <string>

**Description** Saves the display image on the LCD display at the execution of the command into a file in the bitmap (.bmp) or portable network graphics (.png) format.

Specify the file name with the .bmp or .png extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

Notice that, if a file with the specified file name exists, its contents are overwritten. (No query)

**Parameters**

|             |                                                                          |
|-------------|--------------------------------------------------------------------------|
|             | <string>                                                                 |
| Description | File name in which you want to save the display image on the LCD display |
| Range       | 254 characters or less                                                   |

**Example of use**

```
10 OUTPUT 717;":MMEM:STOR:IMAG ""Result/Image01.bmp""
10 OUTPUT 717;":MMEM:STOR:IMAG ""A:Image01.png""
```

**Equivalent key** **[System] - Dump Screen Image**

When performing the operation from the front panel, the image on the LCD display memorized in the volatile memory (clipboard) (the image on the LCD display when the **[Capture]** key is pressed) is saved. Notice that, if no image is memorized in the clipboard, in the same way as the command, the image on the LCD display at the execution is memorized in the clipboard and then it is saved.

## :MMEM:STOR:LIM

Syntax :MMEMory:STORe:LIMit <string>

Description Saves the limit table for the active trace (specified with the :CALC{1-4}:PAR{1-4}:SEL command) of the active channel (specified with the :DISP:WIND{1-4}:ACT command) into a file in the CSV format.

Specify the file name with the .csv extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

Notice that, if a file with the specified file name exists, its contents are overwritten. (No query)

### Parameters

|             |                                                     |
|-------------|-----------------------------------------------------|
|             | <string>                                            |
| Description | File name in which you want to save the limit table |
| Range       | 254 characters or less                              |

Example of use 10 OUTPUT 717;":MMEM:STOR:LIM ""Test1/Limit01.csv""  
10 OUTPUT 717;":MMEM:STOR:LIM ""A:Limit01.csv""

Related commands :DISP:WIND{1-4}:ACT on page 318  
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Analysis] - Limit Test - Edit Limit Line - Export to CSV File**

## :MMEM:STOR:PROG

**Syntax** :MMEMory:STORe:PROGrama <string>

**Description** Saves a VBA project opened on the VBA editor into a file.

Specify the file name with the .vba extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

Notice that, if a file with the specified file name exists, its contents are overwritten. (No query)

### Parameters

|             |                                                     |
|-------------|-----------------------------------------------------|
|             | <string>                                            |
| Description | File name in which you want to save the VBA project |
| Range       | 254 characters or less                              |

**Example of use**

```
10 OUTPUT 717;":MMEM:STOR:PROG ""Test1/Test1_01.vba""
10 OUTPUT 717;":MMEM:STOR:PROG ""A:Test1_01.vba""
```

**Related commands** :MMEM:LOAD:PROG on page 349

**Equivalent key** **[Macro Setup] - Save VBA Project**

## :MMEM:STOR:RLIM

Syntax :MMEMory:STORe:RLIMit <string>

Description Saves the ripple limit table of the active trace (specified with the :CALC{1-4}:PAR{1-4}:SEL command) of the active channel (specified with the :DISP:WIND{1-4}:ACT command) into a file in the CSV format.

Specify the file name with the .sta extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you write directory names and the file name, separate them with a "/" (slash) or "\" (backslash).

Note that if a file with the specified file name already exists, its contents will be overwritten. (No query)

### Parameters

|             | <string>                                       |
|-------------|------------------------------------------------|
| Description | File name used to save the ripple limit table. |
| Range       | 254 characters or less                         |

Example of use 10 OUTPUT 717;":MMEM:STOR:RLIM ""RTest1/Rlim01.csv""  
10 OUTPUT 717;":MMEM:STOR:RLIM ""A:Rlim01.csv""

Related commands :MMEM:LOAD:RLIM on page 350  
:DISP:WIND{1-4}:ACT on page 318  
:CALC{1-4}:PAR{1-4}:SEL on page 286

Equivalent key **[Analysis] - Ripple Limit - Edit Ripple Limit - Export to CSV File**

## :MMEM:STOR:SALL

Syntax :MMEMory:STORe:SALL {ON|OFF|1|0}  
:MMEMory:STORe:SALL?

Description Selects whether to save the setting of all channels/traces or that of the displayed channels/traces only as the instrument state to be saved.

Parameters

|                            | Description                                                                        |
|----------------------------|------------------------------------------------------------------------------------|
| ON or 1                    | Specifies the setting of all channels/traces as the target to be saved.            |
| OFF or 0<br>(preset value) | Specifies the setting of displayed channels/traces only as the target to be saved. |

Query response {1|0}<newline><^END>

Example of use  
10 OUTPUT 717;":MMEM:STOR:SALL ON"  
20 OUTPUT 717;":MMEM:STOR:SALL?"  
30 ENTER 717;A

Related commands :MMEM:STOR on page 353

Equivalent key **[Save/Recall] - Channel/Trace**

## :MMEM:STOR:SEGM

Syntax :MMEMory:STORe:SEGMent <string>

Description Saves the segment sweep table for the active channel (specified with the :DISP:WIND{1-4}:ACT command) into a file in the CSV format.

Specify the file name with the .csv extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

Notice that, if a file with the specified file name exists, its contents are overwritten. (No query)

### Parameters

|             |                                                             |
|-------------|-------------------------------------------------------------|
|             | <string>                                                    |
| Description | File name in which you want to save the segment sweep table |
| Range       | 254 characters or less                                      |

Example of use 10 OUTPUT 717;":MMEM:STOR:SEGM "Test1/Segm01.csv""

10 OUTPUT 717;":MMEM:STOR:SEGM "A:Segm01.csv""

Related commands :MMEM:LOAD:SEGM on page 351

:DISP:WIND{1-4}:ACT on page 318

Equivalent key **[Sweep Setup] - Edit Segment Table - Export to CSV File**

## :MMEM:STOR:STYP

Syntax :MMEMory:STORe:STYPe {STATe|CSTate|DSTate|CDSTate}  
:MMEMory:STORe:STYPe?

Description Selects the contents saved when saving the instrument state into a file with the :MMEM:STOR command.

Parameters

|                          | Description                                                                                                           |
|--------------------------|-----------------------------------------------------------------------------------------------------------------------|
| STATe                    | Specifies the save of the measurement conditions <sup>*1</sup> only.                                                  |
| CSTate<br>(preset value) | Specifies the save of the measurement conditions <sup>*1</sup> and the calibration state.                             |
| DSTate                   | Specifies the save of the measurement conditions <sup>*1</sup> and the formatted data array.                          |
| CDSTate                  | Specifies the save of the measurement conditions <sup>*1</sup> , the calibration state, and the formatted data array. |

<sup>\*1</sup>.For details about the measurement conditions that can be saved, refer to the *User's Guide*.

Query response {STAT|CST|DST|CDST}<newline><^END>

Example of use  
10 OUTPUT 717;" :MMEM:STOR:STYP CDST"  
20 OUTPUT 717;" :MMEM:STOR:STYP?"  
30 ENTER 717;A\$

Related commands :MMEM:STOR on page 353

Equivalent key **[Save/Recall] - Save Type - State Only|State & Cal|State & Trace|All**

## :MMEM:TRAN

**Syntax** :MMEMory:TRANsfer <string>,<block>  
:MMEMory:TRANsfer? <string>

**Description** Writes/reads data to/from a file on the built-in storage device of the E5061A/E5062A.

By reading out data with this command and writing it to a file on the external controller, file transfer from the E5061A/E5062A to the external controller can be realized. On the other hand, by reading out data from the external controller and writing it to a file on the E5061A/E5062A with this command, file transfer from the external controller to the E5061A/E5062A can be realized.

Specify the file name with the extension. If you want to specify a file on the floppy disk drive, you need to add "A:" at the beginning of the file name. When you use directory names and file name, separate them with "/" (slash) or "\" (backslash).

If a file with the specified file name already exists for writing or if the specified file does not exist for reading out (Query), an error occurs and the command is ignored.

### Parameters

|             | <string>                       | <block>                                            |
|-------------|--------------------------------|----------------------------------------------------|
| Description | File name on the E5061A/E5062A | Data written on/read out from the file.            |
| Range       | 254 characters or less         | GPIB: 20 Mbytes or less<br>LAN: 100 Kbytes or less |

**Query response** {block}<newline><^END>

**Example of use**

```

10 OUTPUT 717;":MMEM:TRAN ""Trace01.csv","",#6012345";Dat$
10 OUTPUT 717;":MMEM:TRAN? ""Trace01.csv""
20 ENTER 717 USING "#,A";A$
30 ENTER 717 USING "#,A";Digit$
40 Img$="#",&Digit$&"A"
50 ENTER 717 USING Img$;Byte$
60 Img$=Byte$&"A"
70 ALLOCATE Dat$[VAL(Byte$)]
80 ENTER 717 USING Img$;Dat$

```

**Equivalent key** No equivalent key is available on the front panel.

## :OUTP

|             |                                                                                                                          |
|-------------|--------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :OUTPut[:STATe] {ON OFF 1 0}<br>:OUTPut[:STATe]?                                                                         |
| Description | Turns on/off of the stimulus signal output. You cannot perform measurement until you turn on the stimulus signal output. |
| Parameters  |                                                                                                                          |

|                        | Description                           |
|------------------------|---------------------------------------|
| ON or 1 (preset value) | Turns on the stimulus signal output.  |
| OFF or 0               | Turns off the stimulus signal output. |

|                |                                                                      |
|----------------|----------------------------------------------------------------------|
| Query response | {1 0}<newline><^END>                                                 |
| Example of use | 10 OUTPUT 717;":OUTP ON"<br>20 OUTPUT 717;":OUTP?"<br>30 ENTER 717;A |
| Equivalent key | [Sweep Setup] - Power - RF Out                                       |

## :PROG:CAT?

|                |                                                                                                                                                                                                                                                                                                                 |
|----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax         | :PROGram:CATalog?                                                                                                                                                                                                                                                                                               |
| Description    | Reads out the list of all executable VBA macros (procedures defined by Public including the VBA project loaded on the VBA editor). (Query only)                                                                                                                                                                 |
| Query response | {string}<newline><^END><br><br>The character string in the following format, in which each macro is separated by a comma (.), is read out.<br><br>"{macro 1},{macro 2},...,{macro N}"<br><br>Where N is the total number of VBA macros.<br><br>{macro n}:           VBA macro name (module name.procedure name) |
| Example of use | 10 DIM A\$[1000]<br>20 OUTPUT 717;":PROG:CAT?"<br>30 ENTER 717;A\$                                                                                                                                                                                                                                              |
| Equivalent key | [Macro Setup] - Select Macro                                                                                                                                                                                                                                                                                    |

**:PROG:NAME**

|                  |                                                                                                                                                                                                                                          |  |          |             |                                             |       |                        |              |    |
|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|----------|-------------|---------------------------------------------|-------|------------------------|--------------|----|
| Syntax           | :PROGram[:SElected]:NAME <string><br>:PROGram[:SElected]:NAME?                                                                                                                                                                           |  |          |             |                                             |       |                        |              |    |
| Description      | Selects the VBA macro controlled with the :PROG:STAT command.<br>Selectable VBA macro names can be read out with the :PROG:CAT? command.                                                                                                 |  |          |             |                                             |       |                        |              |    |
| Parameters       | <table><tr><td></td><td>&lt;string&gt;</td></tr><tr><td>Description</td><td>VBA macro name (module name.procedure name)</td></tr><tr><td>Range</td><td>254 characters or less</td></tr><tr><td>Preset value</td><td>""</td></tr></table> |  | <string> | Description | VBA macro name (module name.procedure name) | Range | 254 characters or less | Preset value | "" |
|                  | <string>                                                                                                                                                                                                                                 |  |          |             |                                             |       |                        |              |    |
| Description      | VBA macro name (module name.procedure name)                                                                                                                                                                                              |  |          |             |                                             |       |                        |              |    |
| Range            | 254 characters or less                                                                                                                                                                                                                   |  |          |             |                                             |       |                        |              |    |
| Preset value     | ""                                                                                                                                                                                                                                       |  |          |             |                                             |       |                        |              |    |
| Query response   | {string}<newline><^END>                                                                                                                                                                                                                  |  |          |             |                                             |       |                        |              |    |
| Example of use   | 10 OUTPUT 717;":PROG:NAME ""Module1.main"""<br>20 OUTPUT 717;":PROG:NAME?"<br>30 ENTER 717;A\$                                                                                                                                           |  |          |             |                                             |       |                        |              |    |
| Related commands | :PROG:CAT? on page 365<br>:PROG:STAT on page 367                                                                                                                                                                                         |  |          |             |                                             |       |                        |              |    |
| Equivalent key   | <b>[Macro Setup] - Select Macro</b>                                                                                                                                                                                                      |  |          |             |                                             |       |                        |              |    |

|             |                                                                                                               |
|-------------|---------------------------------------------------------------------------------------------------------------|
| <b>NOTE</b> | When performing the operation from the front panel, you select the VBA macro and execute it at the same time. |
|-------------|---------------------------------------------------------------------------------------------------------------|

## :PROG:STAT

**Syntax** :PROG:STAT {STOP|RUN}  
:PROG:STAT?

**Description** Reads out the control/state of the VBA macro selected with the :PROG:STAT command.

**Parameters**

|                     | Description     |
|---------------------|-----------------|
| STOP (preset value) | Specifies stop. |
| RUN                 | Specifies run.  |

**Query response** {STOP|RUN}<newline><^END>

**Example of use**  
10 OUTPUT 717; ":PROG:STAT RUN"  
20 OUTPUT 717; ":PROG:STAT?"  
30 ENTER 717;A\$

**Related commands** :PROG:NAME on page 366

**Equivalent key** **[Macro Break]** (to stop)  
**[Macro Setup] - Select Macro** (to run)

**NOTE** When performing the operation from the front panel, you select the VBA macro and execute it at the same time.

**:SENS:CORR:COLL:ECAL:PATH?**

Syntax :SENSe:CORRection:COLLect:ECAL:PATH? <numeric>

Description Reads out which port of the ECal module is connected with the specified port of the E5061A/E5062A. (Query only)

Parameters

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

Query response {0|1|2|3|4}<newline><^END>

|   |                       |
|---|-----------------------|
|   | <b>Description</b>    |
| 0 | Nothing is connected. |
| 1 | Port A is connected.  |
| 2 | Port B is connected.  |
| 3 | Port C is connected.  |
| 4 | Port D is connected.  |

Example of use 10 OUTPUT 717;" :SENS1:CORR:COLL:ECAL:PATH? 1"  
20 ENTER 717;A

Equivalent key No equivalent key is available on the front panel.

## :SENS:CORR:IMP

**Syntax** :SENSe:CORRection:IMPedance[:INPut][:MAGNitude] <numeric>  
:SENSe:CORRection:IMPedance[:INPut][:MAGNitude]?

**Description** Sets the system characteristic impedance (Z0) value.

**NOTE** This command is available with the firmware version 3.01 or greater.

### Parameters

|              | <numeric>       |
|--------------|-----------------|
| Description  | System Z0 value |
| Range        | 1E-3 to 1000    |
| Preset value | 50 or 75        |
| Unit         | $\Omega$ (ohm)  |
| Resolution   | 0.001           |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS:CORR:IMP 75"  
20 OUTPUT 717;":SENS:CORR:IMP?"  
30 ENTER 717;A

**Equivalent key** [Cal] - Set Z0

## :SENS{1-4}:AVER:CLE

|                  |                                                                                                                                                                                         |
|------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :SENSe{[1] 2 3 4}:AVERage:CLEar                                                                                                                                                         |
| Description      | Clears the measurement data used for averaging of channel 1 (:SENS1) to channel 4 (:SENS4). Measurement data before the execution of this command is not used for averaging. (No query) |
| Example of use   | 10 OUTPUT 717; ":SENS1:AVER:CLE"                                                                                                                                                        |
| Related commands | :SENS{1-4}:AVER on page 370<br>:SENS{1-4}:AVER:COUN on page 371                                                                                                                         |
| Equivalent key   | <b>[Avg] - Averaging Restart</b>                                                                                                                                                        |

## :SENS{1-4}:AVER

|             |                                                                                      |
|-------------|--------------------------------------------------------------------------------------|
| Syntax      | :SENSe{[1] 2 3 4}:AVERage[:STATe] {ON OFF 1 0}<br>:SENSe{[1] 2 3 4}:AVERage[:STATe]? |
| Description | Turns ON/OFF the averaging function of channel 1 (:SENS1) to channel 4 (:SENS4).     |
| Parameters  |                                                                                      |

|                         | Description                       |
|-------------------------|-----------------------------------|
| ON or 1                 | Turns ON the averaging function.  |
| OFF or 0 (preset value) | Turns OFF the averaging function. |

|                  |                                                                                    |
|------------------|------------------------------------------------------------------------------------|
| Query response   | {1 0}<newline><^END>                                                               |
| Example of use   | 10 OUTPUT 717; ":SENS1:AVER ON"<br>20 OUTPUT 717; ":SENS1:AVER?"<br>30 ENTER 717;A |
| Related commands | :SENS{1-4}:AVER:CLE on page 370<br>:SENS{1-4}:AVER:COUN on page 371                |
| Equivalent key   | <b>[Avg] - Averaging</b>                                                           |

## :SENS{1-4}:AVER:COUN

**Syntax** :SENSe{[1]|2|3|4}:AVERage:COUNt <numeric>  
:SENSe{[1]|2|3|4}:AVERage:COUNt?

**Description** Sets the averaging factor of channel 1 (:SENS1) to channel 4 (:SENS4).

**Parameters**

|              |                  |
|--------------|------------------|
|              | <numeric>        |
| Description  | Averaging factor |
| Range        | 1 to 999         |
| Preset value | 16               |
| Resolution   | 1                |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:AVER:COUN 4"  
20 OUTPUT 717;":SENS1:AVER:COUN?"  
30 ENTER 717;A

**Related commands** :SENS{1-4}:AVER on page 370  
:SENS{1-4}:AVER:CLE on page 370

**Equivalent key** [Avg] - Avg Factor

**:SENS{1-4}:BAND**

**Syntax** :SENSe{[1]|2|3|4}:BANDwidth[:RESolution] <numeric>  
:SENSe{[1]|2|3|4}:BANDwidth[:RESolution]?

**Description** Sets the IF bandwidth of channel 1 (:SENS1) to channel 4 (:SENS4).  
This command provides the same function as the :SENS{1-4}:BWID command.

**Parameters**

|              |                    |
|--------------|--------------------|
|              | <numeric>          |
| Description  | IF bandwidth       |
| Range        | 10 to 30000        |
| Preset value | 30000              |
| Unit         | Hz (hertz)         |
| Resolution   | In steps of 1 or 3 |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use** 10 OUTPUT 717; ":SENS1:BAND 1E3"  
20 OUTPUT 717; ":SENS1:BAND?"  
30 ENTER 717;A

**Related commands** :SENS{1-4}:BWID on page 373

**Equivalent key** [Avg] - IF Bandwidth

## :SENS{1-4}:BWID

**Syntax** :SENSe{[1]|2|3|4}:BWIDth[:RESolution] <numeric>  
:SENSe{[1]|2|3|4}:BWIDth[:RESolution]?

**Description** Sets the IF bandwidth of channel 1 (:SENS1) to channel 4 (:SENS4).  
This command provides the same function as the :SENS{1-4}:BAND command.

**Parameters**

|              |                    |
|--------------|--------------------|
|              | <numeric>          |
| Description  | IF bandwidth       |
| Range        | 10 to 30000        |
| Preset value | 30000              |
| Unit         | Hz (hertz)         |
| Resolution   | In steps of 1 or 3 |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:BWID 1E3"  
20 OUTPUT 717;":SENS1:BWID?"  
30 ENTER 717;A

**Related commands** :SENS{1-4}:BAND on page 372

**Equivalent key** [Avg] - IF Bandwidth

## :SENS{1-4}:CORR:CLE

**Syntax** :SENSe{[1]|2|3|4}:CORRection:CLear

**Description** Clears all calibration coefficient and measured standard data for calibration in the channel 1 (SENS 1) to channel 4 (SENS 4).

**Example of use** 10 OUTPUT 717;":SENS1:CORR:CLE"

**Related commands**

**Equivalent key** [Cal] - Clear All

**:SENS{1-4}:CORR:COEF?**

Syntax :SENSe{[1]|2|3|4}:CORRection:COEFFicient[:DATA]? {ES|ER|ED|EL|ET|EX},<numeric 1>, <numeric 2>

Description Returns the calibration coefficient for specified channel.

Parameters

|           |                       |
|-----------|-----------------------|
|           | <numeric>             |
| ES        | Source match          |
| ER        | Reflection tracking   |
| ED        | Directivity           |
| EL        | Load match            |
| ET        | Transmission tracking |
| EX        | Isolation             |
| numeric 1 | Response port         |
| numeric 2 | Stimulus port         |

If ES, ER, or ED is used, the response port and the stimulus port must be the same, while EL, ET, or EX is used, the response port and the stimulus port must be different.

Query response {numeric 1},...,{numeric NOP×2}<newline><^END>

|                 |                                                                            |
|-----------------|----------------------------------------------------------------------------|
|                 | <b>Description</b>                                                         |
| {numeric n×2-1} | Real part of the data (complex number) at the n-th measurement point.      |
| {numeric n×2}   | Imaginary part of the data (complex number) at the n-th measurement point. |

Where NOP is the number of measurement points and n is an integer between 1 and NOP.

Example of use  
10 DIM A(1:201)  
20 OUTPUT 717;":SENS1:CORR:COEF? EL,1,2"  
30 ENTER 717;A(\*)

Equivalent key No equivalent key is available on the front panel.

## :SENS{1-4}:CORR:COLL:CKIT

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT[:SElect] <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT[:SElect]?

**Description** Selects the calibration kit of channel 1 (:SENS1) to channel 4 (:SENS4).

**Parameters**

|              |                                         |
|--------------|-----------------------------------------|
|              | <numeric>                               |
| Description  | Number of calibration kit <sup>*1</sup> |
| Range        | 1 to 10                                 |
| Preset value | 50 ohm test set: 5, 75 ohm test set: 6  |
| Resolution   | 1                                       |

\*1. The numbers of 1 to 10 assigned from the top to the calibration kit names displayed on the softkey labels when performing **[Cal] - Cal Kit**.

If the specified parameter is out of the allowable setup range, an error occurs and the command is ignored.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT 3"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT?"  
30 ENTER 717;A

**Equivalent key** **[Cal] - Cal Kit**

**:SENS{1-4}:CORR:COLL:CKIT:LAB**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLection:CKIT:LABel <string>  
:SENSe{[1]|2|3|4}:CORRection:COLLection:CKIT:LABel?

Description Sets a calibration kit name for the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

|              |                                                                                                                                                                                                             |
|--------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|              | <string>                                                                                                                                                                                                    |
| Description  | Calibration kit name                                                                                                                                                                                        |
| Range        | 254 characters or less                                                                                                                                                                                      |
| Preset value | Varies depending on the calibration kit number as follows:<br>1: "85033E"<br>2: "85033D"<br>3: "85052D"<br>4: "85032F"<br>5: "85032B"<br>6: "85036B/E"<br>7: "85039B"<br>8: "85038A/F/M"<br>9 to 10: "User" |

Query response {string}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:LAB ""MY\_KIT"""  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:LAB?"  
30 ENTER 717;A\$

Related commands :SENS{1-4}:CORR:COLL:CKIT on page 375

Equivalent key **[Cal] - Modify Cal Kit - Label Kit**

## :SENS{1-4}:CORR:COLL:CKIT:ORD:LOAD

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:LOAD <numeric 1>,<numeric 2>

:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:LOAD? <numeric 1>

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), selects the standard used for the load measurement of the specified port.

**Parameters**

|             | <numeric 1> | <numeric 2>     |
|-------------|-------------|-----------------|
| Description | Port number | Standard number |
| Range       | 1 to 2      | 1 to 21         |
| Resolution  | 1           | 1               |

If the specified parameter is out of the allowable setup range, an error occurs and the command is ignored.

**Query response** {numeric 2}<newline><^END>

**Example of use**

```

10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:LOAD 1,9"
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:LOAD? 1"
30 ENTER 717;A

```

**Related commands** :SENS{1-4}:CORR:COLL:CKIT on page 375

**Equivalent key** **[Cal]** - **Modify Cal Kit - Specify CLSs - Load - Port 1|Port 2**

**:SENS{1-4}:CORR:COLL:CKIT:ORD:OPEN**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:OPEN <numeric 1>,<numeric 2>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:OPEN? <numeric 1>

Description For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), selects the standard used for the open measurement of the specified port.

Parameters

|             | <numeric 1> | <numeric 2>     |
|-------------|-------------|-----------------|
| Description | Port number | Standard number |
| Range       | 1 to 2      | 1 to 21         |
| Resolution  | 1           | 1               |

If the specified parameter is out of the allowable setup range, an error occurs and the command is ignored.

Query response {numeric 2}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:OPEN 1,2"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:OPEN? 1"  
30 ENTER 717;A

Related commands :SENS{1-4}:CORR:COLL:CKIT on page 375

Equivalent key **[Cal] - Modify Cal Kit - Specify CLSs - Open - Port 1|Port 2**

## :SENS{1-4}:CORR:COLL:CKIT:ORD:SHOR

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:SHORt <numeric 1>,<numeric 2>

:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:SHORt? <numeric 1>

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), selects the standard used for the short measurement of the specified port.

**Parameters**

|             | <numeric 1> | <numeric 2>     |
|-------------|-------------|-----------------|
| Description | Port number | Standard number |
| Range       | 1 to 2      | 1 to 21         |
| Resolution  | 1           | 1               |

If the specified parameter is out of the allowable setup range, an error occurs and the command is ignored.

**Query response** {numeric 2}<newline><^END>

**Example of use**

```

10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:SHOR 1,1"
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:SHOR? 1"
30 ENTER 717;A

```

**Related commands** :SENS{1-4}:CORR:COLL:CKIT on page 375

**Equivalent key** [Cal] - Modify Cal Kit - Specify CLSs - Short - Port 1|Port 2

## :SENS{1-4}:CORR:COLL:CKIT:ORD:THRU

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:THRU <numeric 1>,<numeric 2>,<numeric 3>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:ORDer:THRU? <numeric 1>,<numeric 2>

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), selects the standard used for the thru measurement between the specified 2 ports.

### Parameters

|             | <numeric 1>   | <numeric 2>   | <numeric 3>     |
|-------------|---------------|---------------|-----------------|
| Description | Port number 1 | Port number 2 | Standard number |
| Range       | 1 to 2        | 1 to 2        | 1 to 21         |
| Resolution  | 1             | 1             | 1               |

For <numeric 1> and <numeric 2>, you must specify a different port number. If you specify the same port number, an error occurs and the command is ignored.

If the specified parameter is out of the allowable setup range, an error occurs and the command is ignored.

**Query response** {numeric 3}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:THRU 1,2,11"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:ORD:THRU? 1,2"  
30 ENTER 717;A

**Related commands** :SENS{1-4}:CORR:COLL:CKIT on page 375

**Equivalent key** [Cal] - Modify Cal Kit - Specify CLSs - Thru

## :SENS{1-4}:CORR:COLL:CKIT:RES

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:RESet

**Description** Resets the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4) to the factory setting state. (No query)

**Example of use** 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:RES"

**Related commands** :SENS{1-4}:CORR:COLL:CKIT on page 375

**Equivalent key** [Cal] - Modify Cal Kit - Restore Cal Kit

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:ARB

**Syntax**

```
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:ARBitrary <numeric>
```

```
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:ARBitrary?
```

**Description**

For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the arbitrary impedance of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | Arbitrary impedance                                       |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | $\Omega$ (ohm)                                            |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response**

```
{numeric}<newline><^END>
```

**Example of use**

```
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:ARB 50.5"
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:ARB?"
30 ENTER 717;A
```

**Equivalent key**

**[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - Arb. Impedance**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

**:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C0**

**Syntax**                   :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C0 <numeric>  
  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C0?

**Description**           For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the C0 of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | C0                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | fF (femtofarad)                                           |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response**       {numeric}<newline><^END>

**Example of use**       10    OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:C0 12.3"  
                          20    OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:C0?"  
                          30    ENTER 717;A

**Equivalent key**       **[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - C0**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C1

**Syntax**

```
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C1 <numeric>
```

```
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C1?
```

**Description**

For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the C1 of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | C1                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | 1E-27 F/Hz (1E-27 farad/hertz)                            |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response**

```
{numeric}<newline><^END>
```

**Example of use**

```
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:C1 12.3"
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:C1?"
30 ENTER 717;A
```

**Equivalent key**

**[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - C1**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

**:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C2**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C2 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C2?

Description For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the C2 of the standard1 (:STAN1) to standard 21 (:STAN21).

Parameters

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | C2                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | 1E-36 F/Hz <sup>2</sup> (1E-36 farad/hertz <sup>2</sup> ) |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:C2 12.3"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:C2?"  
30 ENTER 717;A

Equivalent key [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - C2

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:C3

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C3 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:C3?

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the C3 of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | C3                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | 1E-45 F/Hz <sup>3</sup> (1E-45 farad/hertz <sup>3</sup> ) |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:C3 12.3"  
20 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:C3?"  
30 ENTER 717;A

**Equivalent key** [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - C3

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

**:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:DEL**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:DELaY <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:DELaY?

Description For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the offset delay of the standard1 (:STAN1) to standard 21 (:STAN21).

Parameters

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | Offset delay                                              |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | s (second)                                                |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:DEL 12.3"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:DEL?"  
30 ENTER 717;A

Equivalent key **[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - Offset Delay**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L0

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L0 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L0?

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the L0 of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | L0                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | pH (picohenry)                                            |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:L0 12.3"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:L0?"  
30 ENTER 717;A

**Equivalent key** [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - L0

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

**:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L1**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L1 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L1?

Description For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the L1 of the standard1 (:STAN1) to standard 21 (:STAN21).

Parameters

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | L1                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | 1E-24 H/Hz (1E-24 henry/hertz)                            |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:L1 12.3"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:L1?"  
30 ENTER 717;A

Equivalent key **[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - L1**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L2

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L2 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L2?

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the L2 of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | L2                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | 1E-33 H/Hz <sup>2</sup> (1E-33 henry/hertz <sup>2</sup> ) |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:L2 12.3"  
20 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:L2?"  
30 ENTER 717;A

**Equivalent key** [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - L2

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

**:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:L3**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L3 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:L3?

Description For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the L3 of the standard1 (:STAN1) to standard 21 (:STAN21).

Parameters

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | L3                                                        |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | 1E-42 H/Hz <sup>3</sup> (1E-42 henry/hertz <sup>3</sup> ) |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:L3 12.3"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:L3?"  
30 ENTER 717;A

Equivalent key **[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - L3**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:LAB

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:LABel <string>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:LABel?

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the name of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <string>                                                  |
| Description  | Standard name                                             |
| Range        | 254 characters or less                                    |
| Preset value | Varies depending on the calibration kit and the standard. |

**Query response** {string}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:LAB ""OPEN""  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:LAB?"  
30 ENTER 717;A\$

**Equivalent key** [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - Label

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

**:SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:LOSS**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:LOSS <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:LOSS?

Description For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the offset loss of the standard1 (:STAN1) to standard 21 (:STAN21).

Parameters

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | Offset Loss                                               |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | $\Omega$ /s (ohm/second)                                  |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:LOSS 12.3"  
20 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:LOSS?"  
30 ENTER 717;A

Equivalent key **[Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - Offset Loss**

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:TYPE

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:TYPE {OPEN|SHORT|LOAD|THRU|ARBI|NONE}  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:TYPE?

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the standard type of the standard1 (:STAN1) to standard 21 (:STAN21).

**Parameters**

|       | Description                                      |
|-------|--------------------------------------------------|
| OPEN  | Specifies open.                                  |
| SHORT | Specifies short.                                 |
| LOAD  | Specifies load.                                  |
| THRU  | Specifies thru.                                  |
| ARBI  | Specify arbitrary impedance.                     |
| NONE  | Specifies DUT of which theoretical values are 0. |

**Query response** {OPEN|SHORT|LOAD|THRU|ARBI|NONE}<newline><^END>

**Example of use**  
10 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:TYPE OPEN"  
20 OUTPUT 717;" :SENS1:CORR:COLL:CKIT:STAN1:TYPE?"  
30 ENTER 717;A\$

**Equivalent key** [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - STD Type

<sup>\*1</sup>no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:CKIT:STAN{1-21}:Z0

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:Z0 <numeric>  
:SENSe{[1]|2|3|4}:CORRection:COLLect:CKIT:STAN{[1]|2|3|4|5|6|7|8|9|10|11|12|13|14|15|16|17|18|19|20|21}:Z0?

**Description** For the calibration kit selected for channel 1 (:SENS1) to channel 4 (:SENS4), sets the value of the Offset Z0 of the standard1 (:STAN1) to standard 21 (:STAN21).

### Parameters

|              |                                                           |
|--------------|-----------------------------------------------------------|
|              | <numeric>                                                 |
| Description  | Offset Z0                                                 |
| Range        | -1E18 to 1E18                                             |
| Preset value | Varies depending on the calibration kit and the standard. |
| Unit         | $\Omega$ (ohm)                                            |

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

**Query response** {numeric}<newline><^END>

**Example of use**  
10 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:Z0 50"  
20 OUTPUT 717;":SENS1:CORR:COLL:CKIT:STAN1:Z0?"  
30 ENTER 717;A

**Equivalent key** [Cal] - Modify Cal Kit - Define STDs - no. name<sup>\*1</sup> - Offset Z0

<sup>\*1</sup>1.no: standard number (1 to 21), name: standard name (variable)

## :SENS{1-4}:CORR:COLL:ECAL:ERES

|             |                                                                                                                                                                                                                                                              |
|-------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :SENSe{[1] 2 3 4}:CORRection:COLLect:ECAL:ERES <numeric 1>,<numeric 2>                                                                                                                                                                                       |
| Description | Executes enhanced response calibration of channel 1 (:SENS1) to channel 4 (:SENS4) using the ECal (Electrical Calibration) module. If you execute this command when the ECal module is not connected, an error occurs and the command is ignored. (No query) |
| Parameters  |                                                                                                                                                                                                                                                              |

|             | <numeric 1>          | <numeric 2>          |
|-------------|----------------------|----------------------|
| Description | Response port number | Stimulus port number |
| Range       | 1 to 2               | 1 to 2               |
| Resolution  | 1                    | 1                    |

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

|                |                                                                                            |
|----------------|--------------------------------------------------------------------------------------------|
| Example of use | 10 OUTPUT 717;":SENS1:CORR:COLL:ECAL:ERES 1,2"<br>20 OUTPUT 717;":*OPC?"<br>30 ENTER 717;A |
|----------------|--------------------------------------------------------------------------------------------|

|                |                                                      |
|----------------|------------------------------------------------------|
| Equivalent key | [Cal] - ECal - Enhanced Response - 2-1(S21) 1-2(S12) |
|----------------|------------------------------------------------------|

## :SENS{1-4}:CORR:COLL:ECAL:ISOL

|             |                                                                                                                                          |
|-------------|------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :SENSe{[1] 2 3 4}:CORRection:COLLect:ECAL:ISOLation[:STATe] {ON OFF 1 0}<br>:SENSe{[1] 2 3 4}:CORRection:COLLect:ECAL:ISOLation[:STATe]? |
| Description | For channel 1 (:SENS1) to channel 4 (:SENS4), turns ON/OFF the isolation measurement when executing Ecal (Electrical Calibration).       |
| Parameters  |                                                                                                                                          |

|                         | Description                          |
|-------------------------|--------------------------------------|
| ON or 1                 | Turns ON the isolation measurement.  |
| OFF or 0 (preset value) | Turns OFF the isolation measurement. |

|                  |                                                                                                                |
|------------------|----------------------------------------------------------------------------------------------------------------|
| Query response   | {1 0}<newline><^END>                                                                                           |
| Example of use   | 10 OUTPUT 717;":SENS1:CORR:COLL:ECAL:ISOL ON"<br>20 OUTPUT 717;":SENS1:CORR:COLL:ECAL:ISOL?"<br>30 ENTER 717;A |
| Related commands | :SENS{1-4}:CORR:COLL:ECAL:SOLT1 on page 397<br>:SENS{1-4}:CORR:COLL:ECAL:SOLT2 on page 397                     |

Equivalent key      **[Cal] - ECal - Isolation**

## :SENS{1-4}:CORR:COLL:ECAL:SOLT1

- Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:ECAL:SOLT1 <numeric>
- Description** Executes full 1-port calibration of the specified port of channel 1 (:SENS1) to channel 4 (:SENS4) using the ECal (Electrical Calibration) module.
- If you execute this command when the ECal module is not connected, an error occurs and the command is ignored. (No query)

### Parameters

|             | <numeric>   |
|-------------|-------------|
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

- Example of use**
- ```
10 OUTPUT 717;":SENS1:CORR:COLL:ECAL:SOLT1 1"
20 OUTPUT 717;"*OPC?"
30 ENTER 717;A
```

- Equivalent key** [Cal] - ECal - 1-Port Cal - Port 1|Port 2

:SENS{1-4}:CORR:COLL:ECAL:SOLT2

- Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:ECAL:SOLT2 <numeric 1>,<numeric 2>
- Description** Executes full 2-port calibration between the 2 specified ports of channel 1 (:SENS1) to channel 4 (:SENS4) using the ECal (Electrical Calibration) module.
- If you execute this command when the ECal module is not connected, an error occurs and the command is ignored. (No query)

Parameters

	<numeric 1>	<numeric 2>
Description	Port number	Port number
Range	1 to 2	1 to 2
Resolution	1	1

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

- Example of use**
- ```
10 OUTPUT 717;":SENS1:CORR:COLL:ECAL:SOLT2 1,2"
20 OUTPUT 717;"*OPC?"
30 ENTER 717;A
```

- Equivalent key** [Cal] - ECal - 2-Port Cal

**:SENS{1-4}:CORR:COLL:ECAL:THRU**

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:ECAL:THRU <numeric 1>,<numeric 2>

**Description** Executes response calibration (thru) between the 2 specified ports of channel 1 (:SENS1) to channel 4 (:SENS4) using the ECal (Electrical Calibration) module.

If you execute this command when the ECal module is not connected, an error occurs and the command is ignored. (No query)

**Parameters**

|             | <numeric 1>          | <numeric 2>          |
|-------------|----------------------|----------------------|
| Description | Response port number | Stimulus port number |
| Range       | 1 to 2               | 1 to 2               |
| Resolution  | 1                    | 1                    |

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

**Example of use**

```
10 OUTPUT 717;":SENS1:CORR:COLL:ECAL:SOLT2 1,2"
20 OUTPUT 717;"*OPC?"
30 ENTER 717;A
```

**Equivalent key** [Cal] - ECal - Thru Cal - 2-1 (S21)/1-2 (S12)

## :SENS{1-4}:CORR:COLL:ISOL

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect[:ACQuire]:ISOLation <numeric 1>,<numeric 2>

**Description** For channel 1 (:SENS1) to channel 4 (:SENS4), measure the calibration data of the isolation from the stimulus port to the response port. (No query)

**Parameters**

|             | <numeric 1>          | <numeric 2>          |
|-------------|----------------------|----------------------|
| Description | Response port number | Stimulus port number |
| Range       | 1 to 2               | 1 to 2               |
| Resolution  | 1                    | 1                    |

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

**Example of use**

```

10 OUTPUT 717;":SENS1:CORR:COLL:ISOL 1,2"
20 OUTPUT 717;"*OPC?"
30 ENTER 717;A

```

**Equivalent key** [Cal] - Calibrate - Response (Thru) - Isolation (Optional)  
[Cal] - Calibrate - n-Port Cal - Isolation (Optional) - Port m-n Isol

## :SENS{1-4}:CORR:COLL:METH:ERES

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:METHod:ERES <numeric 1>,<numeric 2>

**Description** For channel 1 (:SENS1) to channel 4 (:SENS4), sets the calibration type to the enhanced response calibration. (No query)

**Parameters**

|             | <numeric 1>          | <numeric 2>          |
|-------------|----------------------|----------------------|
| Description | Response port number | Stimulus port number |
| Range       | 1 to 2               | 1 to 2               |
| Resolution  | 1                    | 1                    |

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

**Example of use**

```

10 OUTPUT 717;":SENS1:CORR:COLL:METH:ERES 1,2"

```

Related commands

Equivalent key      **[Cal] - Calibrate - Enhanced Response - Ports**

## :SENS{1-4}:CORR:COLL:LOAD

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect[:ACQuire]:LOAD <numeric>

**Description** For channel 1 (:SENS1) to channel 4 (:SENS4), measures the calibration data of the load standard of the specified port. (No query)

**Parameters**

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

**Example of use**

```

10 OUTPUT 717;":SENS1:CORR:COLL:LOAD 1"
20 OUTPUT 717;"*OPC?"
30 ENTER 717;A

```

**Equivalent key**

[Cal] - Calibrate - Response (Open)|Response (Short) - Load (Optional)

[Cal] - Calibrate - 1-Port Cal - Load

[Cal] - Calibrate - n-Port Cal - Reflection - Port m Load

## :SENS{1-4}:CORR:COLL:METH:OPEN

- Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:METHod[:RESPOnse]:OPEN <numeric>
- Description** For channel 1 (:SENS1) to channel 4 (:SENS4), sets the calibration type to the response calibration (open) of the specified port. (No query)
- Parameters**

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

**Example of use** 10 OUTPUT 717; ":SENS1:CORR:COLL:METH:OPEN 1"

**Related commands** :SENS{1-4}:CORR:COLL:METH:TYPE? on page 405

**Equivalent key** [Cal] - Calibrate - Response (Open) - Port

## :SENS{1-4}:CORR:COLL:METH:SHOR

- Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:METHod[:RESPOnse]:SHORt <numeric>
- Description** For channel 1 (:SENS1) to channel 4 (:SENS4), sets the calibration type to the response calibration (short) of the specified port. (No query)
- Parameters**

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

**Example of use** 10 OUTPUT 717; ":SENS1:CORR:COLL:METH:SHOR 1"

**Related commands** :SENS{1-4}:CORR:COLL:METH:TYPE? on page 405

**Equivalent key** [Cal] - Calibrate - Response (Short) - Port

## :SENS{1-4}:CORR:COLL:METH:SOLT1

|             |                                                                                                                                          |
|-------------|------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :SENSe{[1] 2 3 4}:CORRection:COLLect:METHod:SOLT1 <numeric>                                                                              |
| Description | For channel 1 (:SENS1) to channel 4 (:SENS4), sets the calibration type to the full 1-port calibration of the specified port. (No query) |
| Parameters  |                                                                                                                                          |

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

Example of use      10    OUTPUT 717; ":SENS1:CORR:COLL:METH:SOLT1 1"

Related commands   :SENS{1-4}:CORR:COLL:METH:TYPE? on page 405

Equivalent key      **[Cal] - Calibrate - 1-Port Cal - Port**

## :SENS{1-4}:CORR:COLL:METH:SOLT2

|             |                                                                                                                                                  |
|-------------|--------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :SENSe{[1] 2 3 4}:CORRection:COLLect:METHod:SOLT2 <numeric 1>,<numeric 2>                                                                        |
| Description | For channel 1 (:SENS1) to channel 4 (:SENS4), sets the calibration type to the full 2-port calibration between the 2 specified ports. (No query) |
| Parameters  |                                                                                                                                                  |

|             |             |             |
|-------------|-------------|-------------|
|             | <numeric 1> | <numeric 2> |
| Description | Port number | Port number |
| Range       | 1 to 2      | 1 to 2      |
| Resolution  | 1           | 1           |

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

Example of use      10    OUTPUT 717; ":SENS1:CORR:COLL:METH:SOLT2 1,2"

Related commands   :SENS{1-4}:CORR:COLL:METH:TYPE? on page 405

Equivalent key      **[Cal] - Calibrate - 2-Port Cal - Ports**

**:SENS{1-4}:CORR:COLL:METH:THRU**

| Syntax           | :SENSe{[1] 2 3 4}:CORRection:COLLect:METHod[:RESPonse]:THRU <numeric 1>,<numeric 2>                                                                                                                                                                                                                                                                                                                                                            |             |  |             |             |             |             |             |       |        |        |            |   |   |
|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------|--|-------------|-------------|-------------|-------------|-------------|-------|--------|--------|------------|---|---|
| Description      | For channel 1 (:SENS1) to channel 4 (:SENS4), sets the calibration type to the response calibration (thru) between the 2 specified ports. (No query)                                                                                                                                                                                                                                                                                           |             |  |             |             |             |             |             |       |        |        |            |   |   |
| Parameters       | <table><tr><th></th><th>&lt;numeric 1&gt;</th><th>&lt;numeric 2&gt;</th></tr><tr><td>Description</td><td>Port number</td><td>Port number</td></tr><tr><td>Range</td><td>1 to 2</td><td>1 to 2</td></tr><tr><td>Resolution</td><td>1</td><td>1</td></tr></table> <p>For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.</p> |             |  | <numeric 1> | <numeric 2> | Description | Port number | Port number | Range | 1 to 2 | 1 to 2 | Resolution | 1 | 1 |
|                  | <numeric 1>                                                                                                                                                                                                                                                                                                                                                                                                                                    | <numeric 2> |  |             |             |             |             |             |       |        |        |            |   |   |
| Description      | Port number                                                                                                                                                                                                                                                                                                                                                                                                                                    | Port number |  |             |             |             |             |             |       |        |        |            |   |   |
| Range            | 1 to 2                                                                                                                                                                                                                                                                                                                                                                                                                                         | 1 to 2      |  |             |             |             |             |             |       |        |        |            |   |   |
| Resolution       | 1                                                                                                                                                                                                                                                                                                                                                                                                                                              | 1           |  |             |             |             |             |             |       |        |        |            |   |   |
| Example of use   | 10    OUTPUT 717; ":SENS1:CORR:COLL:METH:THRU 1,2"                                                                                                                                                                                                                                                                                                                                                                                             |             |  |             |             |             |             |             |       |        |        |            |   |   |
| Related commands | :SENS{1-4}:CORR:COLL:METH:TYPE? on page 405                                                                                                                                                                                                                                                                                                                                                                                                    |             |  |             |             |             |             |             |       |        |        |            |   |   |
| Equivalent key   | <b>[Cal] - Calibrate - Response (Thru) - Ports</b>                                                                                                                                                                                                                                                                                                                                                                                             |             |  |             |             |             |             |             |       |        |        |            |   |   |

## :SENS{1-4}:CORR:COLL:METH:TYPE?

**Syntax** :SENSe{[1]|2|3|4}:CORRection:COLLect:METHod:TYPE?

**Description** For channel 1 (:SENS1) to channel 4 (:SENS4), reads out the calibration type selected for calculation of the calibration coefficients. (Query only)

**Query response** {ERES|NONE|RESPO|RESPS|RESPT|SOLT1|SOLT2}<newline><^END>

|       | Description                                                |
|-------|------------------------------------------------------------|
| ERES  | The calibration type is the enhanced response calibration. |
| NONE  | The calibration type is set to nothing.                    |
| RESPO | The calibration type is the response calibration (open).   |
| RESPS | The calibration type is the response calibration (short).  |
| RESPT | The calibration type is the response calibration (thru).   |
| SOLT1 | The calibration type is the full 1-port calibration.       |
| SOLT2 | The calibration type is the full 2-port calibration.       |

**Example of use**

```
10 OUTPUT 717;":SENS1:CORR:COLL:METH:TYPE?"
20 ENTER 717;A$
```

**Equivalent key** No equivalent key is available on the front panel.

**:SENS{1-4}:CORR:COLL:OPEN**

|                |                                                                                                                                                                                        |  |           |             |             |       |        |            |   |
|----------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|-----------|-------------|-------------|-------|--------|------------|---|
| Syntax         | :SENSe{[1] 2 3 4}:CORRection:COLLect[:ACQuire]:OPEN <numeric>                                                                                                                          |  |           |             |             |       |        |            |   |
| Description    | For channel 1 (:SENS1) to channel 4 (:SENS4), measures the calibration data of the open standard of the specified port. (No query)                                                     |  |           |             |             |       |        |            |   |
| Parameters     | <table><tr><td></td><td>&lt;numeric&gt;</td></tr><tr><td>Description</td><td>Port number</td></tr><tr><td>Range</td><td>1 to 2</td></tr><tr><td>Resolution</td><td>1</td></tr></table> |  | <numeric> | Description | Port number | Range | 1 to 2 | Resolution | 1 |
|                | <numeric>                                                                                                                                                                              |  |           |             |             |       |        |            |   |
| Description    | Port number                                                                                                                                                                            |  |           |             |             |       |        |            |   |
| Range          | 1 to 2                                                                                                                                                                                 |  |           |             |             |       |        |            |   |
| Resolution     | 1                                                                                                                                                                                      |  |           |             |             |       |        |            |   |
| Example of use | 10    OUTPUT 717;":SENS1:CORR:COLL:OPEN 1"<br>20    OUTPUT 717;"*OPC?"<br>30    ENTER 717;A                                                                                            |  |           |             |             |       |        |            |   |
| Equivalent key | <b>[Cal] - Calibrate - Response (Open) 1-Port Cal - Open</b><br><b>[Cal] - Calibrate - n-Port Cal - Reflection - Port m Open</b>                                                       |  |           |             |             |       |        |            |   |

## :SENS{1-4}:CORR:COLL:SAVE

|                  |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
|------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Syntax           | :SENSe{[1] 2 3 4}:CORRection:COLLect:SAVE                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| Description      | <p>From the measured calibration data, calculates the calibration coefficients depending on the selected calibration type.</p> <p>Calculating the calibration coefficients clears all calibration data whether or not used for the calculation and also clears the calibration type selections.</p> <p>If you execute this command before all necessary calibration data for calculating the calibration coefficients is measured, an error occurs and the command is ignored. (No query)</p> |
| Example of use   | 10 OUTPUT 717;" :SENS1:CORR:COLL:SAVE"                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| Related commands | <p>:SENS{1-4}:CORR:COLL:METH:OPEN on page 402</p> <p>:SENS{1-4}:CORR:COLL:METH:SHOR on page 402</p> <p>:SENS{1-4}:CORR:COLL:METH:THRU on page 404</p> <p>:SENS{1-4}:CORR:COLL:METH:SOLT1 on page 403</p> <p>:SENS{1-4}:CORR:COLL:METH:SOLT2 on page 403</p>                                                                                                                                                                                                                                   |

Equivalent key **[Cal] - Calibrate - Response|n-Port Cal - Done**

## :SENS{1-4}:CORR:COLL:SHOR

|             |                                                                                                                                     |
|-------------|-------------------------------------------------------------------------------------------------------------------------------------|
| Syntax      | :SENSe{[1] 2 3 4}:CORRection:COLLect[:ACQuire]:SHORt <numeric>                                                                      |
| Description | For channel 1 (:SENS1) to channel 4 (:SENS4), measures the calibration data of the short standard of the specified port. (No query) |

Parameters

|             |             |
|-------------|-------------|
|             | <numeric>   |
| Description | Port number |
| Range       | 1 to 2      |
| Resolution  | 1           |

|                |                                                                                                                                     |
|----------------|-------------------------------------------------------------------------------------------------------------------------------------|
| Example of use | 10 OUTPUT 717;" :SENS1:CORR:COLL:SHOR 1"<br>20 OUTPUT 717;"*OPC?"<br>30 ENTER 717;A                                                 |
| Equivalent key | <b>[Cal] - Calibrate - Response (Short) 1-Port Cal - Short</b><br><b>[Cal] - Calibrate - n-Port Cal - Reflection - Port m Short</b> |

**:SENS{1-4}:CORR:COLL:THRU**

Syntax :SENSe{[1]|2|3|4}:CORRection:COLLect[:ACQuire]:THRU <numeric 1>,<numeric 2>

Description For channel 1 (:SENS1) to channel 4 (:SENS4), measure the calibration data of the thru standard from the stimulus port to the response port. (No query)

Parameters

|             | <numeric 1>          | <numeric 2>          |
|-------------|----------------------|----------------------|
| Description | Response port number | Stimulus port number |
| Range       | 1 to 2               | 1 to 2               |
| Resolution  | 1                    | 1                    |

For each parameter, you must specify a different port number. If you specify the same port number for 2 or more parameters, an error occurs and the command is ignored.

Example of use 10 OUTPUT 717;":SENS1:CORR:COLL:THRU 1,2"  
20 OUTPUT 717;"\*OPC?"  
30 ENTER 717;A

Equivalent key **[Cal] - Calibrate - Response (Thru) - Thru**  
**[Cal] - Calibrate - n-Port Cal - Transmission - Port m-n Thru**

## :SENS{1-4}:CORR:EXT

- Syntax** :SENSe{[1]|2|3|4}:CORRection:EXTension[:STATe] {ON|OFF|1|0}  
:SENSe{[1]|2|3|4}:CORRection:EXTension[:STATe]?
- Description** For channel 1 (:SENS1) to channel 4 (:SENS4), turns ON/OFF the port extension.
- Parameters**

|                         | Description                   |
|-------------------------|-------------------------------|
| ON or 1                 | Turns ON the port extension.  |
| OFF or 0 (preset value) | Turns OFF the port extension. |

- Query response** {1|0}<newline><^END>
- Example of use**
- ```
10  OUTPUT 717; ":SENS1:CORR:EXT ON"
20  OUTPUT 717; ":SENS1:CORR:EXT?"
30  ENTER 717;A
```
- Related commands** :SENS{1-4}:CORR:EXT:PORT{1-2} on page 410
- Equivalent key** **[Cal] - Port Extensions - Extensions**

:SENS{1-4}:CORR:EXT:PORT{1-2}

Syntax :SENSe{[1]|2|3|4}:CORRection:EXTension:PORT{[1]|2} <numeric>
:SENSe{[1]|2|3|4}:CORRection:EXTension:PORT{[1]|2}?

Description For channel 1 (:SENS1) to channel 4 (:SENS4), sets the correction amount for the port extension of port 1 (:PORT1) to port 2 (:PORT2) as the delay time.

Parameters

	<numeric>
Description	Delay time
Range	-10 to 10
Preset value	0
Unit	s (second)

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:EXT:PORT1 1E-3"
20 OUTPUT 717;":SENS1:CORR:EXT?"
30 ENTER 717;A

Related commands :SENS{1-4}:CORR:EXT on page 409

Equivalent key **[Cal] - Port Extensions - Extension Port 1|Extension Port 2**

:SENS{1-4}:CORR:PROP

Syntax	:SENSe{[1] 2 3 4}:CORRection:PROPeRty {ON OFF 1 0} :SENSe{[1] 2 3 4}:CORRection:PROPeRty?
Description	Turns ON/OFF the display of the calibration property of channel 1 (:SENS1) to channel 4 (:SENS4).
Parameters	

	Description
ON or 1	Turns ON the calibration property display.
OFF or 0 (preset value)	Turns OFF the calibration property display.

Query response	{1 0}<newline><^END>
Example of use	10 OUTPUT 717;":SENS1:CORR:PROP ON" 20 OUTPUT 717;":SENS1:CORR:PROP?" 30 ENTER 717;A
Equivalent key	[Cal] - Property

:SENS{1-4}:CORR:RVEL:COAX

Syntax	:SENSe{[1] 2 3 4}:CORRection:RVELocity:COAX <numeric> :SENSe{[1] 2 3 4}:CORRection:RVELocity:COAX?
Description	For channel 1 (:SENS1) to channel 4 (:SENS4), sets the velocity factor.
Parameters	

	<numeric>
Description	Velocity factor
Range	0.01 to 10
Preset value	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":SENS1:CORR:RVEL:COAX 0.7" 20 OUTPUT 717;":SENS1:CORR:RVEL:COAX?" 30 ENTER 717;A
Equivalent key	[Cal] - Velocity Factor

:SENS{1-4}:CORR:STAT

Syntax :SENSe{[1]|2|3|4}:CORRection:STATe {ON|OFF|1|0}
 :SENSe{[1]|2|3|4}:CORRection:STATe?

Description For channel 1 (:SENS1) to channel 4 (:SENS4), turns ON/OFF the error correction.

Parameters

	Description
ON or 1	Turns ON the error correction.
OFF or 0 (preset value)	Turns OFF the error correction.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:CORR:STAT ON"
 20 OUTPUT 717;":SENS1:CORR:STAT?"
 30 ENTER 717;A

Equivalent key **[Cal] - Correction**

:SENS{1-4}:CORR:TYPE{1-4}?

Syntax :SENSe{[1]|2|3|4}:CORRection:TYPE{[1]|2|3|4}?

Description For trace 1 (:TYPE1) to trace 4 (:TYPE4) of channel 1 (:SENS1) to channel 4 (:SENS4), reads out the information (calibration type, port numbers) of the applied calibration coefficients for the actual error correction.

Query response {ERES|NONE|RESPO|RESPS|RESPT|SOLT1|SOLT2},{numeric 1},{numeric 2}<newline><^END>

{ERES|NONE|RESPO|RESPS|RESPT|SOLT1|SOLT2}:

	Description
ERES	The enhanced response calibration is applied.
NONE	Any calibration is not applied.
RESPO	The response calibration (open) is applied.
RESPS	The response calibration (short) is applied.
RESPT	The response calibration (thru) is applied.
SOLT1	The full 1-port calibration is applied.
SOLT2	The full 2-port calibration is applied.

{numeric 1}: the calibration port number
(This parameter is 0 when the first parameter is NONE.)

{numeric 2}: the calibration port number
(This parameter is 0 when the first parameter is not ERES, RESPT and SOLT2.)

Example of use
10 OUTPUT 717;":SENS1:CORR:TYPE1?"
20 ENTER 717;A\$

Equivalent key No equivalent key is available on the front panel.

:SENS{1-4}:FREQ

Syntax :SENSe{[1]|2|3|4}:FREQuency[:CW|FIXed] <numeric>
:SENSe{[1]|2|3|4}:FREQuency[:CW|FIXed]?

Description Sets the fixed frequency (CW frequency) for the power sweep for channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Fixed frequency
Range	3E5 to 3E9
Preset value	3E5
Unit	Hz (hertz)
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:FREQ 1E9"
20 OUTPUT 717;":SENS1:FREQ?"
30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TYPE on page 428

Equivalent key **[Sweep Setup] - Power - CW Freq**

:SENS{1-4}:FREQ:CENT

Syntax :SENSe{[1]|2|3|4}:FREQuency:CENTer <numeric>
:SENSe{[1]|2|3|4}:FREQuency:CENTer?

Description Sets the center value of the sweep range of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Center value
Range	3E5 to 3E9
Preset value	4.25015E9
Unit	Hz (hertz)
Resolution	0.5 or 1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SENS1:FREQ:CENT 2E9"
20 OUTPUT 717;":SENS1:FREQ:CENT?"
30 ENTER 717;A

Related commands :SENS{1-4}:FREQ:SPAN on page 417

Equivalent key **[Center]**

:SENS{1-4}:FREQ:DATA?

Syntax :SENSe{[1]|2|3|4}:FREQuency:DATA?

Description For channel 1 (:SENS1) to channel 4 (:SENS4), reads out the frequencies of all measurement point.

The data transfer format when this command is executed depends on the setting with the :FORM:DATA command. (Query only)

Query response {numeric 1},...,{numeric NOP}<newline><^END>

	Description
{numeric n}	Frequency at the n-th measurement point

Where NOP is the number of measurement points and n is an integer between 1 and NOP.

Example of use

```
10  DIM A(1:201)
20  OUTPUT 717;" :SENS1:FREQ:DATA?"
30  ENTER 717;A( *)
```

Related commands :FORM:DATA on page 338

Equivalent key No equivalent key is available on the front panel.

:SENS{1-4}:FREQ:SPAN

Syntax :SENSe{[1]|2|3|4}:FREQuency:SPAN <numeric>
:SENSe{[1]|2|3|4}:FREQuency:SPAN?

Description Sets the span value of the sweep range of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Span value
Range	0 to 2.9997E9
Preset value	2.9997E9
Unit	Hz (hertz)
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SENS1:FREQ:SPAN 1E9"
20 OUTPUT 717;":SENS1:FREQ:SPAN?"
30 ENTER 717;A

Related commands :SENS{1-4}:FREQ:CENt on page 415

Equivalent key **[Span]**

:SENS{1-4}:FREQ:STAR

Syntax :SENSe{[1]|2|3|4}:FREQuency:STARt <numeric>
:SENSe{[1]|2|3|4}:FREQuency:STARt?

Description Sets the start value of the sweep range of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Start value
Range	3E5 to 3E9
Preset value	3E5
Unit	Hz (hertz)
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:FREQ:STAR 100E6"
20 OUTPUT 717;":SENS1:FREQ:STAR?"
30 ENTER 717;A

Related commands :SENS{1-4}:FREQ:STOP on page 419

Equivalent key **[Start]**

:SENS{1-4}:FREQ:STOP

Syntax :SENSe{[1]|2|3|4}:FREQuency:STOP <numeric>
:SENSe{[1]|2|3|4}:FREQuency:STOP?

Description Sets the stop value of the sweep range of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Stop value
Range	3E5 to 3E9
Preset value	3E9
Unit	Hz (hertz)
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SENS1:FREQ:STOP 100E6"
20 OUTPUT 717;":SENS1:FREQ:STOP?"
30 ENTER 717;A

Related commands :SENS{1-4}:FREQ:STAR on page 418

Equivalent key **[Stop]**

:SENS{1-4}:ROSC:SOUR?

Syntax :SENSe{[1]|2|3|4}:ROSCillator:SOURce?

Description Reads out whether the external reference signal is inputted to the Ref In connector on the rear panel. (Query only)

Query response {INTernal|EXTernal}<newline><^END>

	Description
INTernal	The external reference signal is not inputted.
EXTernal	The external reference signal is inputted.

Example of use 10 OUTPUT 717;" :SENS1:ROSC:SOUR?"
20 ENTER 717;A\$

Equivalent key Displayed on the instrument status bar (at the bottom of the LCD display).

:SENS{1-4}:SEGM:DATA

Syntax

```
:SENSe{[1]|2|3|4}:SEGMent:DATA 5,<mode>,<ifbw>,<pow>,<del>,<time>,<segm>,  
<star 1>,<stop 1>,<nop 1>,<ifbw 1>,<pow 1>,<del 1>,<time 1>,...,  
<star n>,<stop n>,<nop n>,<ifbw n>,<pow n>,<del n>,<time n>,...,  
<star N>,<stop N>,<nop N>,<ifbw N>,<pow N>,<del N>,<time N>  
  
:SENSe{[1]|2|3|4}:SEGMent:DATA?
```

Where N is the number of segments (specified with <segm>) and n is an integer between 1 and N.

Description

Creates the segment sweep table for channel 1 (:SENS1) to channel 4 (:SENS4).

The data transfer format when this command is executed depends on the setting with the :FORM:DATA command.

Parameters

The first value is 5 and the parameters listed below follow.

	Description
<mode>	Stimulus setting mode 0: Specifies with start/stop values 1: Specifies with center/span values
<ifbw>	ON/OFF of the IF bandwidth setting for each segment 0: Off, 1: On
<pow>	ON/OFF of the power setting for each segment 0: Off, 1: On
	ON/OFF of the sweep delay time setting for each segment 0: Off, 1: On
<time>	ON/OFF of the sweep time setting for each segment 0: Off, 1: On
<segm>	Number of segments (1 to 201)
<star n>	Start value/center value of the n-th segment
<stop n>	Stop value/span value of the n-th segment
<nop n>	Number of measurement points of the n-th segment
<ifbw n>	IF bandwidth of the n-th segment Not required when the IF bandwidth setting for each segment is OFF (<ifbw> = 0)
<pow n>	Power of the n-th segment Not required when the power setting for each segment is OFF (<pow> = 0)
<del n>	Sweep delay time of the n-th segment Not required when the sweep delay time setting for each segment is OFF (= 0)

	Description
<time n>	Sweep time of the n-th segment (specify 0 If you want to set “auto setting”) Not required when the sweep time setting for each segment is OFF (<time> = 0)

Query response 5,{mode},{ifbw},{pow},{del},{time},{segm},
{star 1},{stop 1},{nop 1},{pow 1},{del 1},{time 1},...,
{star n},{stop n},{nop n},{pow n},{del n},{time n},...,
{star N},{stop N},{nop N},{pow N},{del N},{time N}<newline><^END>

Example of use 10 DIM H(1:3,1:4)
20 OUTPUT 717;" :SENS1:SEGM:DATA 5,0,1,0,0,0,3,";
30 OUTPUT 717;"1E9,3E9,11,70e3,";
40 OUTPUT 717;"3E9,4E9,51,7e3,";
50 OUTPUT 717;"4E9,6E9,11,70e3"
60 OUTPUT 717;" :SENS1:SEGM:DATA?"
70 ENTER 717;A,B,C,D,E,F,G,H(*)

Related commands :SENS{1-4}:SWE:TYPE on page 428
:FORM:DATA on page 338

Equivalent key **[Sweep Setup] - Edit Segment Table**

:SENS{1-4}:SEGM:SWE:POIN?

Syntax	:SENSe{[1] 2 3 4}:SEGMENT:SWEep:POINts?
Description	For the segment sweep table of channel 1 (:SENS1) to channel 4 (:SENS4), reads out the total number of the measurement points of all segments. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":SENS1:SEGM:SWE:POIN?" 20 ENTER 717;A
Related commands	:SENS{1-4}:SEGM:DATA on page 421
Equivalent key	No equivalent key is available on the front panel.

:SENS{1-4}:SEGM:SWE:TIME?

Syntax	:SENSe{[1] 2 3 4}:SEGMENT:SWEep:TIME?
Description	For the segment sweep table of channel 1 (:SENS1) to channel 4 (:SENS4), reads out the total sweep time of all segments. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":SENS1:SEGM:SWE:TIME?" 20 ENTER 717;A
Related commands	:SENS{1-4}:SEGM:DATA on page 421
Equivalent key	No equivalent key is available on the front panel.

:SENS{1-4}:SWE:DEL

Syntax :SENSe{[1]|2|3|4}:SWEp:DELay <numeric>
 :SENSe{[1]|2|3|4}:SWEp:DELay?

Description Sets the sweep delay time of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Sweep delay time
Range	0 to 1
Preset value	0
Unit	s (second)
Resolution	0.001

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:SWE:DEL 0.05"
 20 OUTPUT 717;":SENS1:SWE:DEL?"
 30 ENTER 717;A

Equivalent key **[Sweep Setup] - Sweep Delay**

:SENS{1-4}:SWE:POIN

Syntax :SENSe{[1]|2|3|4}:SWEep:POINts <numeric>
:SENSe{[1]|2|3|4}:SWEep:POINts?

Description Sets the number of measurement points of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	<numeric>
Description	Number of measurement points
Range	2 to 1601
Preset value	201
Resolution	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SENS1:SWE:POIN 801"
20 OUTPUT 717;":SENS1:SWE:POIN?"
30 ENTER 717;A

Equivalent key [Sweep Setup] - Points

:SENS{1-4}:SWE:TIME

Syntax :SENSe{[1]|2|3|4}:SWEp:TIME[:DATA] <numeric>
 :SENSe{[1]|2|3|4}:SWEp:TIME[:DATA]?

Description Sets the sweep time of channel 1 (:SENS1) to channel 4 (:SENS4).

When the auto setting of the sweep time is ON, even if you try to set the sweep time to any value with this command, it automatically returns to the value defined by the E5061A/E5062A. Before using this command, turns OFF the auto setting of the sweep time (specify OFF with the :SENS{1-4}:SWE:TIME:AUTO command).

Parameters

	<numeric>
Description	Sweep time
Range	Varies depending on the measurement conditions.
Preset value	Varies depending on the measurement conditions.
Unit	s (second)

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SENS1:SWE:TIME 1.5"
 20 OUTPUT 717;":SENS1:SWE:TIME?"
 30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TIME:AUTO on page 427

Equivalent key **[Sweep Setup] - Sweep Time**

:SENS{1-4}:SWE:TIME:AUTO

Syntax :SENSe{[1]|2|3|4}:SWEp:TIME:AUTO {ON|OFF|1|0}
:SENSe{[1]|2|3|4}:SWEp:TIME:AUTO?

Description Sets whether to automatically set the sweep time of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	Description
ON or 1 (preset value)	Turns ON the auto setting.
OFF or 0	Turns OFF the auto setting.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717; ":SENS1:SWE:TIME:AUTO ON"
20 OUTPUT 717; ":SENS1:SWE:TIME:AUTO?"
30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TIME on page 426

Equivalent key [Sweep Setup] - Sweep Time

:SENS{1-4}:SWE:TYPE

Syntax :SENSe{[1]|2|3|4}:SWEep:TYPE {LINear|LOGarithmic|SEGMENT|POWer}
:SENSe{[1]|2|3|4}:SWEep:TYPE?

Description Sets the sweep type of channel 1 (:SENS1) to channel 4 (:SENS4).

Parameters

	Description
LINear (preset value)	Specifies the linear sweep.
LOGarithmic	Specifies the logarithmic sweep. *1
SEGMENT	Specifies the segment sweep.
POWer	Specifies the power sweep.

*1. If you execute this command to try to specify the log sweep when the frequency span condition necessary for the log sweep is not satisfied (the stop frequency is about 4 times or more the start frequency), an error occurs and the command is ignored.

Query response {LIN|LOG|SEGMENT|POW}<newline><^END>

Example of use
10 OUTPUT 717; ":SENS1:SWE:TYPE SEGMENT"
20 OUTPUT 717; ":SENS1:SWE:TYPE?"
30 ENTER 717;A\$

Equivalent key **[Sweep Setup] - Sweep Type - Lin Freq|Log Freq|Segment**

:SERV:CHAN:ACT?

Syntax :SERVice:CHANnel:ACTive?

Description Reads out the active channel number. (Query only)

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717; ":SERV:CHAN:ACT?"
20 ENTER 717;A

Related commands :DISP:WIND{1-4}:ACT on page 318

Equivalent key No equivalent key is available on the front panel.

:SERV:CHAN:COUN?

Syntax	:SERVice:CHANnel:COUNT?
Description	Reads out the upper limit of the number of channels of the E5061A/E5062A. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":SERV:CHAN:COUN?" 20 ENTER 717;A
Equivalent key	No equivalent key is available on the front panel.

:SERV:CHAN{1-4}:TRAC:ACT?

Syntax	:SERVice:CHANnel{[1] 2 3 4}:TRACe:ACTive?
Description	Reads out the active trace number of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":SERV:CHAN1:TRAC:ACT?" 20 ENTER 717;A
Related commands	:CALC{1-4}:PAR{1-4}:SEL on page 286
Equivalent key	No equivalent key is available on the front panel.

:SERV:CHAN:TRAC:COUN?

Syntax	:SERVice:CHANnel:TRACe:COUNt?
Description	Reads out the upper limit of the number of traces per channel. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":SERV:CHAN:TRAC:COUN?" 20 ENTER 717;A
Equivalent key	No equivalent key is available on the front panel.

:SERV:PORT:COUN?

Syntax	:SERVice:PORT:COUNT?
Description	Reads out the number of ports of the E5061A/E5062A. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":SERV:PORT:COUN?" 20 ENTER 717;A
Equivalent key	No equivalent key is available on the front panel.

:SOUR{1-4}:POW

Syntax :SOURce{[1]|2|3|4}:POWer[:LEVel][:IMMediate]
[:AMPLitude] <numeric>

:SOURce{[1]|2|3|4}:POWer[:LEVel][:IMMediate]
[:AMPLitude]?

Description Sets the power level of channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	Power level
Range	Varies depending on the power range.
Preset value	0
Unit	dBm
Resolution	0.05

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SOUR1:POW -12.5"
20 OUTPUT 717;":SOUR1:POW?"
30 ENTER 717;A

Related commands :SOUR{1-4}:POW:ATT on page 432

Equivalent key [Sweep Setup] - Power

:SOUR{1-4}:POW:ATT

Syntax :SOURce{[1]|2|3|4}:POW:ATTenuation[:DATA] <numeric>
:SOURce{[1]|2|3|4}:POW:ATTenuation[:DATA]?

Description Sets the power range of channel 1 (:SOUR1) to channel 4 (:SOUR4).
The power range is selected depending on the setting of the attenuator. The following table shows the relationship between the attenuator value and the power range.

Attenuator	Power range	Attenuator	Power range
0 dB	-5 to +10 dBm	30 dB	-35 to -20 dBm
10 dB	-15 to 0 dBm	40 dB	-45 to -30 dBm
20 dB	-25 to -10 dBm		

If you execute this command when the power range extension function is not installed, an error occurs and the command is ignored.

Parameters

	<numeric>
Description	Attenuator value
Range	0 to 40
Preset value	0
Unit	dB
Resolution	10

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717; ":SOUR1:POW:ATT 10"
20 OUTPUT 717; ":SOUR1:POW:ATT?"
30 ENTER 717;A

Related commands :SOUR{1-4}:POW on page 431

Equivalent key [Sweep Setup] - Power - Power Ranges

:SOUR{1-4}:POW:CENT

Syntax :SOURce{[1]|2|3|4}:POWer:CENTer <numeric>
:SOURce{[1]|2|3|4}:POWer:CENTer?

Description Sets the center value of the sweep range for the power sweep for channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	Center value
Range	Varies depending on the power range.
Preset value	-2.5
Unit	dBm
Resolution	0.05 or 0.025

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SOUR1:POW:CENT 0"
20 OUTPUT 717;":SOUR1:POW:CENT?"
30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TYPE on page 428
:SOUR{1-4}:POW:ATT on page 432
:SOUR{1-4}:POW:SPAN on page 438

Equivalent key [Center]

:SOUR{1-4}:POW:PORT:COUP

Syntax :SOURce{[1]|2|3|4}:POWer:PORT:COUPle {ON|OFF|1|0}
 :SOURce{[1]|2|3|4}:POWer:PORT:COUPle?

Description Sets whether to output the same power level for each port of channel 1 (:SOUR1) to channel 4 (:SOUR4). When the power slope feature is on (ON specified with the :SOUR{1-4}:POW:SLOP:STAT command), the same power level is always outputted to all ports regardless of this setting because different power levels cannot be outputted for each port.

Parameters

	Description
ON or 1 (preset value)	Outputs the same power level to individual ports.
OFF or 0	Outputs different power levels to individual ports.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;" :SOUR1:POW:PORT:COUP OFF"
 20 OUTPUT 717;" :SOUR1:POW:PORT:COUP?"
 30 ENTER 717;A

Related commands :SOUR{1-4}:POW:PORT{1-2} on page 435

Equivalent key **[Sweep Setup] - Power - Port Couple**

:SOUR{1-4}:POW:PORT{1-2}

Syntax :SOURce{[1]|2|3|4}:POWer:PORT{[1]|2}[:LEVel][:IMMediate][:AMPLitude] <numeric>
:SOURce{[1]|2|3|4}:POWer:PORT{[1]|2}[:LEVel][:IMMediate][:AMPLitude]?

Description Sets the power level of port 1 (:PORT1) to port 2 (:PORT2) of channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	The power level at the specified port.
Range	Varies depending on the power range.
Preset value	0
Unit	dBm
Resolution	0.05

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;" :SOUR1:POW:PORT1 -12.5"
20 OUTPUT 717;" :SOUR1:POW:PORT1?"
30 ENTER 717;A

Related commands :SOUR{1-4}:POW:PORT:COUP on page 434
:SOUR{1-4}:POW:ATT on page 432

Equivalent key [Sweep Setup] - Power - Port Power - Port 1 Power|Port 2 Power

:SOUR{1-4}:POW:SLOP

Syntax :SOURce{[1]|2|3|4}:POWer[:LEVel]:SLOPe[:DATA] <numeric>
:SOURce{[1]|2|3|4}:POWer[:LEVel]:SLOPe[:DATA]?

Description Sets the correction value of the power slope feature of channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	The correction value of the power slope feature
Range	-2 to 2
Preset value	0
Unit	dB/GHz
Resolution	0.01

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SOUR1:POW:SLOP 0.1"
20 OUTPUT 717;":SOUR1:POW:SLOP?"
30 ENTER 717;A

Related commands :SOUR{1-4}:POW:SLOP:STAT on page 437

Equivalent key **[Sweep Setup] - Power - Slop [xxx dB/GHz]**

:SOUR{1-4}:POW:SLOP:STAT

Syntax :SOURce{[1]|2|3|4}:POWer[:LEVel]:SLOPe:STATe {ON|OFF|1|0}
:SOURce{[1]|2|3|4}:POWer[:LEVel]:SLOPe:STATe?

Description Turns on/off the power slope feature of channel 1 (:SOUR1) to channel 4 (:SOUR4). This function is a function to correct the attenuation of simple power level proportional to the frequency (attenuation due to cables and so on).

Parameters

	Description
ON or 1	Turns on the power slope feature.
OFF or 0 (preset value)	Turns off the power slope feature.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":SOUR1:POW:SLOP:STAT ON"
20 OUTPUT 717;":SOUR1:POW:SLOP:STAT?"
30 ENTER 717;A

Related commands :SOUR{1-4}:POW:SLOP on page 436

Equivalent key [Sweep Setup] - Power - Slop [ON/OFF]

:SOUR{1-4}:POW:SPAN

Syntax :SOURce{[1]|2|3|4}:POWer:SPAN <numeric>
:SOURce{[1]|2|3|4}:POWer:SPAN?

Description Sets the span value of the sweep range for the power sweep for channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	Span value
Range	Varies depending on the power range.
Preset value	5
Unit	dBm
Resolution	0.05

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;" :SOUR1:POW:SPAN 10"
20 OUTPUT 717;" :SOUR1:POW:SPAN?"
30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TYPE on page 428
:SOUR{1-4}:POW:ATT on page 432
:SOUR{1-4}:POW:CENT on page 433

Equivalent key **[Span]**

:SOUR{1-4}:POW:STAR

Syntax :SOURce{[1]|2|3|4}:POWer:STARt <numeric>
:SOURce{[1]|2|3|4}:POWer:STARt?

Description Sets the start value of the sweep range for the power sweep for channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	Start value
Range	Varies depending on the power range.
Preset value	-5
Unit	dBm
Resolution	0.05

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":SOUR1:POW:STAR -10"
20 OUTPUT 717;":SOUR1:POW:STAR?"
30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TYPE on page 428
:SOUR{1-4}:POW:ATT on page 432
:SOUR{1-4}:POW:STOP on page 440

Equivalent key **[Start]**

:SOUR{1-4}:POW:STOP

Syntax :SOURce{[1]|2|3|4}:POWer:STOP <numeric>
:SOURce{[1]|2|3|4}:POWer:STOP?

Description Sets the stop value of the sweep range for the power sweep for channel 1 (:SOUR1) to channel 4 (:SOUR4).

Parameters

	<numeric>
Description	Stop value
Range	Varies depending on the power range.
Preset value	0
Unit	dBm
Resolution	0.05

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":SOUR1:POW:STOP 10"
20 OUTPUT 717;":SOUR1:POW:STOP?"
30 ENTER 717;A

Related commands :SENS{1-4}:SWE:TYPE on page 428
:SOUR{1-4}:POW:ATT on page 432
:SOUR{1-4}:POW:STAR on page 439

Equivalent key **[Stop]**

:STAT:OPER?

Syntax	:STATus:OPERation[:EVENT]?
Description	Reads out the value of the Operation Status Event Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:OPER?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:OPER:COND?

Syntax	:STATus:OPERation:CONDition?
Description	Reads out the value of the Operation Status Condition Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:OPER:COND?" 20 ENTER 717;A
Related commands	:STAT:OPER:NTR on page 443 :STAT:OPER:PTR on page 444
Equivalent key	No equivalent key is available on the front panel.

:STAT:OPER:ENAB

Syntax :STATus:OPERation:ENABle <numeric>
 :STATus:OPERation:ENABle?

Description Sets the value of the Operation Status Enable Register.

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 0 to bit 3, bit 6 to bit 13 and bit 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:OPER:ENAB 16"
 20 OUTPUT 717;":STAT:OPER:ENAB?"
 30 ENTER 717;A

Related commands *SRE on page 200

Equivalent key No equivalent key is available on the front panel.

:STAT:OPER:NTR

Syntax :STATus:OPERation:NTRansition <numeric>
:STATus:OPERation:NTRansition?

Description Sets the value of negative transition filter of the Operation Status Register.

Parameters

	<numeric>
Description	Value of the negative transition filter
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 0 to bit 3, bit 6 to bit 13 and bit 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":STAT:OPER:NTR 16"
20 OUTPUT 717;":STAT:OPER:NTR?"
30 ENTER 717;A

Related commands :STAT:OPER? on page 441
:STAT:OPER:PTR on page 444

Equivalent key No equivalent key is available on the front panel.

:STAT:OPER:PTR

Syntax :STATus:OPERation:PTRansition <numeric>
 :STATus:OPERation:PTRansition?

Description Sets the value of positive transition filter of the Operation Status Register.

Parameters

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	16432
Resolution	1

Note that bit 0 to bit 3, bit 6 to bit 13 and bit 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:OPER:PTR 16"
 20 OUTPUT 717;":STAT:OPER:PTR?"
 30 ENTER 717;A

Related commands :STAT:OPER? on page 441
 :STAT:OPER:NTR on page 443

Equivalent key No equivalent key is available on the front panel.

:STAT:PRES

Syntax	:STATus:PRESet
Description	Initialize the Operation Status Register, Questionable Status Register, Questionable Limit Status Register, Questionable Limit Extra Status Register, Questionable Limit Channel Status Register, and Questionable Limit Channel Extra Status Register. (No query)
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES?

Syntax	:STATus:QUEStionable[:EVENT]?
Description	Reads out the value of the Questionable Status Event Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:BLIM?

Syntax	:STATus:QUEStionable:BLIMit[:EVENT]?
Description	Reads out the value of the Questionable Bandwidth Limit Status Event Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:BLIM?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:BLIM:CHAN{1-4}?

Syntax	:STATus:QUEStionable:BLIMit:CHANnel{[1] 2 3 4}[:EVENT]?
Description	Reads out the value of the Questionable Bandwidth Limit Channel Status Event Register of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:BLIM:CHAN1?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:BLIM:CHAN{1-4}:COND?

Syntax	:STATus:QUEStionable:BLIMit:CHANnel{[1] 2 3 4}:CONDition?
Description	Reads out the value of the Questionable Bandwidth Limit Channel Status Condition Register of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:BLIM:CHAN1:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:BLIM:CHAN{1-4}:NTR on page 448 :STAT:QUES:BLIM:CHAN{1-4}:PTR on page 449
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:BLIM:CHAN{1-4}:ENAB

Syntax :STATus:QUEStionable:BLIMit:CHANnel{[1]|2|3|4}:ENABle <numeric>
:STATus:QUEStionable:BLIMit:CHANnel{[1]|2|3|4}:ENABle?

Description Sets the value of the Questionable Bandwidth Limit Channel Status Enable Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":STAT:QUES:BLIM:CHAN1:ENAB 16"
20 OUTPUT 717;":STAT:QUES:BLIM:CHAN1:ENAB?"
30 ENTER 717;A

Related commands :STAT:QUES:BLIM:ENAB on page 450

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:BLIM:CHAN{1-4}:NTR

Syntax	:STATus:QUEStionable:BLIMit:CHANnel{[1] 2 3 4}:NTRansition <numeric> :STATus:QUEStionable:BLIMit:CHANnel{[1] 2 3 4}:NTRansition?										
Description	Sets the value of the negative transition filter of the Questionable Bandwidth Limit Channel Status Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).										
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Value of the negative transition filter</td></tr><tr><td>Range</td><td>0 to 65535</td></tr><tr><td>Preset value</td><td>0</td></tr><tr><td>Resolution</td><td>1</td></tr></table> Note that bit 5 to 15 cannot be set to 1.		<numeric>	Description	Value of the negative transition filter	Range	0 to 65535	Preset value	0	Resolution	1
	<numeric>										
Description	Value of the negative transition filter										
Range	0 to 65535										
Preset value	0										
Resolution	1										
Query response	{numeric}<newline><^END>										
Example of use	10 OUTPUT 717;":STAT:QUES:BLIM:CHAN1:NTR 16" 20 OUTPUT 717;":STAT:QUES:BLIM:CHAN1:NTR?" 30 ENTER 717;A										
Related commands	:STAT:QUES:BLIM:CHAN{1-4}? on page 446 :STAT:QUES:BLIM:CHAN{1-4}:PTR on page 449										
Equivalent key	No equivalent key is available on the front panel.										

:STAT:QUES:BLIM:CHAN{1-4}:PTR

Syntax	:STATus:QUEStionable:BLIMit:CHANnel{[1] 2 3 4}:PTRansition <numeric> :STATus:QUEStionable:BLIMit:CHANnel{[1] 2 3 4}:PTRansition?
Description	Sets the value of the positive transition filter of the Questionable Bandwidth Limit Channel Status Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).
Parameters	

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:BLIM:CHAN1:PTR 16" 20 OUTPUT 717;":STAT:QUES:BLIM:CHAN1:PTR?" 30 ENTER 717;A

Related commands	:STAT:QUES:BLIM:CHAN{1-4}? on page 446 :STAT:QUES:BLIM:CHAN{1-4}:NTR on page 448
------------------	---

Equivalent key	No equivalent key is available on the front panel.
----------------	--

:STAT:QUES:BLIM:COND?

Syntax	:STATus:QUEStionable:BLIMit:CONDition?
Description	Reads out the value of the Questionable Bandwidth Limit Status Condition Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:BLIM:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:BLIM:NTR on page 451 :STAT:QUES:BLIM:PTR on page 452
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:BLIM:ENAB

Syntax :STATus:QUEStionable:BLIMit:ENABle <numeric>
:STATus:QUEStionable:BLIMit:ENABle?

Description Sets the value of the Questionable Bandwidth Limit Status Enable Register.

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:BLIM:ENAB 16"
20 OUTPUT 717;":STAT:QUES:BLIM:ENAB?"
30 ENTER 717;A

Related commands :STAT:QUES:ENAB on page 454

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:BLIM:NTR

Syntax	:STATus:QUEStionable:BLIMit:NTRansition <numeric> :STATus:QUEStionable:BLIMit:NTRansition?										
Description	Sets the value of the negative transition filter of the Questionable Bandwidth Limit Status Register.										
Parameters	<table border="1"> <tr> <td></td><td><numeric></td></tr> <tr> <td>Description</td><td>Value of the negative transition filter</td></tr> <tr> <td>Range</td><td>0 to 65535</td></tr> <tr> <td>Preset value</td><td>0</td></tr> <tr> <td>Resolution</td><td>1</td></tr> </table> Note that bit 5 to 15 cannot be set to 1.		<numeric>	Description	Value of the negative transition filter	Range	0 to 65535	Preset value	0	Resolution	1
	<numeric>										
Description	Value of the negative transition filter										
Range	0 to 65535										
Preset value	0										
Resolution	1										
Query response	{numeric}<newline><^END>										
Example of use	<pre>10 OUTPUT 717;":STAT:QUES:BLIM:NTR 16" 20 OUTPUT 717;":STAT:QUES:BLIM:NTR?" 30 ENTER 717;A</pre>										
Related commands	:STAT:QUES:BLIM? on page 445 :STAT:QUES:BLIM:PTR on page 452										
Equivalent key	No equivalent key is available on the front panel.										

:STAT:QUES:BLIM:PTR

Syntax :STATus:QUEStionable:BLIMit:PTRansition <numeric>
:STATus:QUEStionable:BLIMit:PTRansition?

Description Sets the value of the positive transition filter of the Questionable Bandwidth Limit Status Register.

Parameters

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":STAT:QUES:BLIM:PTR 16"
20 OUTPUT 717;":STAT:QUES:BLIM:PTR?"
30 ENTER 717;A

Related commands :STAT:QUES:BLIM? on page 445
:STAT:QUES:BLIM:NTR on page 451

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:COND?

Syntax	:STATus:QUEStionable:CONDition?
Description	Reads out the value of the Questionable Status Condition Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:NTR on page 463 :STAT:QUES:PTR on page 464
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:ENAB

Syntax :STATus:QUEStionable:ENABle <numeric>
 :STATus:QUEStionable:ENABle?

Description Sets the value of the Questionable Status Enable Register.

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 0 to bit 9 and bit 12 to bit 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:ENAB 16"
 20 OUTPUT 717;":STAT:QUES:ENAB?"
 30 ENTER 717;A

Related commands *SRE on page 200

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:LIM?

Syntax	:STATus:QUEStionable:LIMit[:EVENT]?
Description	Reads out the value of the Questionable Limit Status Event Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:LIM?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:LIM:CHAN{1-4}?

Syntax	:STATus:QUEStionable:LIMit:CHANnel{[1] 2 3 4}[:EVENT]?
Description	Reads out the value of the Questionable Limit Channel Status Event Register of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:LIM:CHAN1?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:LIM:CHAN{1-4}:COND?

Syntax	:STATus:QUEStionable:LIMit:CHANnel{[1] 2 3 4}:CONDition?
Description	Reads out the value of the Questionable Limit Channel Status Condition Register of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:LIM:CHAN1:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:LIM:CHAN{1-4}:NTR on page 457 :STAT:QUES:LIM:CHAN{1-4}:PTR on page 458
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:LIM:CHAN{1-4}:ENAB

Syntax :STATus:QUEStionable:LIMit:CHANnel{[1]|2|3|4}:ENABle <numeric>
 :STATus:QUEStionable:LIMit:CHANnel{[1]|2|3|4}:ENABle?

Description Sets the value of the Questionable Limit Channel Status Enable Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	30
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:LIM:CHAN1:ENAB 16"
 20 OUTPUT 717;":STAT:QUES:LIM:CHAN1:ENAB?"
 30 ENTER 717;A

Related commands :STAT:QUES:LIM:ENAB on page 460

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:LIM:CHAN{1-4}:NTR

Syntax	:STATus:QUEStionable:LIMit:CHANnel{[1] 2 3 4}:NTRansition <numeric> :STATus:QUEStionable:LIMit:CHANnel{[1] 2 3 4}:NTRansition?
Description	Sets the value of the negative transition filter of the Questionable Limit Channel Status Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).
Parameters	

	<numeric>
Description	Value of the negative transition filter
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:LIM:CHAN1:NTR 16" 20 OUTPUT 717;":STAT:QUES:LIM:CHAN1:NTR?" 30 ENTER 717;A
Related commands	:STAT:QUES:LIM:CHAN{1-4}? on page 455 :STAT:QUES:LIM:CHAN{1-4}:PTR on page 458
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:LIM:CHAN{1-4}:PTR

Syntax	:STATus:QUEStionable:LIMit:CHANnel{[1] 2 3 4}:PTRansition <numeric> :STATus:QUEStionable:LIMit:CHANnel{[1] 2 3 4}:PTRansition?										
Description	Sets the value of the positive transition filter of the Questionable Limit Channel Status Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).										
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Value of the positive transition filter</td></tr><tr><td>Range</td><td>0 to 65535</td></tr><tr><td>Preset value</td><td>30</td></tr><tr><td>Resolution</td><td>1</td></tr></table> Note that bit 5 to 15 cannot be set to 1.		<numeric>	Description	Value of the positive transition filter	Range	0 to 65535	Preset value	30	Resolution	1
	<numeric>										
Description	Value of the positive transition filter										
Range	0 to 65535										
Preset value	30										
Resolution	1										
Query response	{numeric}<newline><^END>										
Example of use	10 OUTPUT 717; ":STAT:QUES:LIM:CHAN1:PTR 16" 20 OUTPUT 717; ":STAT:QUES:LIM:CHAN1:PTR?" 30 ENTER 717;A										
Related commands	:STAT:QUES:LIM:CHAN{1-4}? on page 455 :STAT:QUES:LIM:CHAN{1-4}:NTR on page 457										
Equivalent key	No equivalent key is available on the front panel.										

:STAT:QUES:LIM:COND?

Syntax	:STATus:QUEStionable:LIMit:CONDition?
Description	Reads out the value of the Questionable Limit Status Condition Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;" :STAT:QUES:LIM:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:LIM:NTR on page 461 :STAT:QUES:LIM:PTR on page 462
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:LIM:ENAB

Syntax :STATus:QUEStionable:LIMit:ENABle <numeric>
:STATus:QUEStionable:LIMit:ENABle?

Description Sets the value of the Questionable Limit Status Enable Register.

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	30
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:LIM:ENAB 16"
20 OUTPUT 717;":STAT:QUES:LIM:ENAB?"
30 ENTER 717;A

Related commands :STAT:QUES:ENAB on page 454

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:LIM:NTR

Syntax :STATus:QUEStionable:LIMit:NTRansition <numeric>
:STATus:QUEStionable:LIMit:NTRansition?

Description Sets the value of the negative transition filter of the Questionable Limit Status Register.

Parameters

	<numeric>
Description	Value of the negative transition filter
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":STAT:QUES:LIM:CHAN1:NTR 16"
20 OUTPUT 717;":STAT:QUES:LIM:CHAN1:NTR?"
30 ENTER 717;A

Related commands :STAT:QUES:LIM? on page 455
:STAT:QUES:LIM:PTR on page 462

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:LIM:PTR

Syntax :STATus:QUEStionable:LIMit:PTRansition <numeric>
 :STATus:QUEStionable:LIMit:PTRansition?

Description Sets the value of the positive transition filter of the Questionable Limit Status Register.

Parameters

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	30
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:LIM:CHAN1:PTR 16"
 20 OUTPUT 717;":STAT:QUES:LIM:CHAN1:PTR?"
 30 ENTER 717;A

Related commands :STAT:QUES:LIM? on page 455
 :STAT:QUES:LIM:NTR on page 461

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:NTR

Syntax :STATus:QUEStionable:NTRansition <numeric>
:STATus:QUEStionable:NTRansition?

Description Sets the value of negative transition filter of the Questionable Status Register.

Parameters

	<numeric>
Description	Value of the negative transition filter
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 0 to bit 9 and bit 12 to bit 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;":STAT:QUES:NTR 16"
20 OUTPUT 717;":STAT:QUES:NTR?"
30 ENTER 717;A

Related commands :STAT:QUES? on page 445
:STAT:QUES:PTR on page 464

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:PTR

Syntax :STATus:QUEStionable:PTRansition <numeric>
 :STATus:QUEStionable:PTRansition?

Description Sets the value of positive transition filter of the Questionable Status Register.

Parameters

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	3072
Resolution	1

Note that bit 0 to bit 9 and bit 12 to bit 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:PTR 16"
 20 OUTPUT 717;":STAT:QUES:PTR?"
 30 ENTER 717;A

Related commands :STAT:QUES? on page 445
 :STAT:QUES:NTR on page 463

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:RLIM?

Syntax	:STATus:QUEStionable:RLIMit[:EVENT]?
Description	Reads out the value of the Questionable Ripple Limit Status Event Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:RLIM?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:RLIM:CHAN{1-4}?

Syntax	:STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}[:EVENT]?
Description	Reads out the value of the Questionable Ripple Limit Channel Status Event Register of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:RLIM:CHAN1?" 20 ENTER 717;A
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:RLIM:CHAN{1-4}:COND?

Syntax	:STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:CONDition?
Description	Reads out the value of the Questionable Ripple Limit Channel Status Condition Register of channel 1 (:CHAN1) to channel 4 (:CHAN4). (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717; ":STAT:QUES:RLIM:CHAN1:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:RLIM:CHAN{1-4}:NTR on page 467 :STAT:QUES:RLIM:CHAN{1-4}:PTR on page 468
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:RLIM:CHAN{1-4}:ENAB

Syntax	:STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:ENABle <numeric> :STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:ENABle?										
Description	Sets the value of the Questionable Ripple Limit Channel Status Enable Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).										
Parameters	<table><tr><td></td><td><numeric></td></tr><tr><td>Description</td><td>Value of the enable register</td></tr><tr><td>Range</td><td>0 to 65535</td></tr><tr><td>Preset value</td><td>Varies depending on the upper limit setting for channel/trace number.</td></tr><tr><td>Resolution</td><td>1</td></tr></table> Note that bit 5 to 15 cannot be set to 1.		<numeric>	Description	Value of the enable register	Range	0 to 65535	Preset value	Varies depending on the upper limit setting for channel/trace number.	Resolution	1
	<numeric>										
Description	Value of the enable register										
Range	0 to 65535										
Preset value	Varies depending on the upper limit setting for channel/trace number.										
Resolution	1										
Query response	{numeric}<newline><^END>										
Example of use	10 OUTPUT 717;" :STAT:QUES:RLIM:CHAN1:ENAB 16" 20 OUTPUT 717;" :STAT:QUES:RLIM:CHAN1:ENAB?" 30 ENTER 717;A										
Related commands	:STAT:QUES:RLIM:ENAB on page 469										
Equivalent key	No equivalent key is available on the front panel.										

:STAT:QUES:RLIM:CHAN{1-4}:NTR

Syntax	:STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:NTRansition <numeric> :STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:NTRansition?
Description	Sets the value of the negative transition filter of the Questionable Ripple Limit Channel Status Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).
Parameters	

	<numeric>
Description	Value of the negative transition filter
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:RLIM:CHAN1:NTR 16" 20 OUTPUT 717;":STAT:QUES:RLIM:CHAN1:NTR?" 30 ENTER 717;A
Related commands	:STAT:QUES:RLIM:CHAN{1-4}? on page 465 :STAT:QUES:RLIM:CHAN{1-4}:PTR on page 468
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:RLIM:CHAN{1-4}:PTR

Syntax	:STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:PTRansition <numeric> :STATus:QUEStionable:RLIMit:CHANnel{[1] 2 3 4}:PTRansition?
Description	Sets the value of the positive transition filter of the Questionable Ripple Limit Channel Status Register of channel 1 (:CHAN1) to channel 4 (:CHAN4).
Parameters	

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:RLIM:CHAN1:PTR 16" 20 OUTPUT 717;":STAT:QUES:RLIM:CHAN1:PTR?" 30 ENTER 717;A

Related commands	:STAT:QUES:RLIM:CHAN{1-4}? on page 465 :STAT:QUES:RLIM:CHAN{1-4}:NTR on page 467
------------------	---

Equivalent key	No equivalent key is available on the front panel.
----------------	--

:STAT:QUES:RLIM:COND?

Syntax	:STATus:QUEStionable:RLIMit:CONDition?
Description	Reads out the value of the Questionable Ripple Limit Status Condition Register. (Query only)
Query response	{numeric}<newline><^END>
Example of use	10 OUTPUT 717;":STAT:QUES:RLIM:COND?" 20 ENTER 717;A
Related commands	:STAT:QUES:RLIM:NTR on page 470 :STAT:QUES:RLIM:PTR on page 471
Equivalent key	No equivalent key is available on the front panel.

:STAT:QUES:RLIM:ENAB

Syntax :STATus:QUEStionable:RLIMit:ENABle <numeric>
:STATus:QUEStionable:RLIMit:ENABle?

Description Sets the value of the Questionable Ripple Limit Status Enable Register.

Parameters

	<numeric>
Description	Value of the enable register
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use

```

10 OUTPUT 717;":STAT:QUES:RLIM:ENAB 16"
20 OUTPUT 717;":STAT:QUES:RLIM:ENAB?"
30 ENTER 717;A

```

Related commands :STAT:QUES:ENAB on page 454

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:RLIM:NTR

Syntax :STATus:QUEStionable:RLIMit:NTRansition <numeric>
:STATus:QUEStionable:RLIMit:NTRansition?

Description Sets the value of the negative transition filter of the Questionable Ripple Limit Status Register.

Parameters

	<numeric>
Description	Value of the negative transition filter
Range	0 to 65535
Preset value	0
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use 10 OUTPUT 717;":STAT:QUES:RLIM:NTR 16"
20 OUTPUT 717;":STAT:QUES:RLIM:NTR?"
30 ENTER 717;A

Related commands :STAT:QUES:RLIM? on page 465
:STAT:QUES:RLIM:PTR on page 471

Equivalent key No equivalent key is available on the front panel.

:STAT:QUES:RLIM:PTR

Syntax :STATus:QUEStionable:RLIMit:PTRansition <numeric>
:STATus:QUEStionable:RLIMit:PTRansition?

Description Sets the value of the positive transition filter of the Questionable Ripple Limit Status Register.

Parameters

	<numeric>
Description	Value of the positive transition filter
Range	0 to 65535
Preset value	Varies depending on the upper limit setting for channel/trace number.
Resolution	1

Note that bit 5 to 15 cannot be set to 1.

Query response {numeric}<newline><^END>

Example of use
10 OUTPUT 717;" :STAT:QUES:RLIM:PTR 16"
20 OUTPUT 717;" :STAT:QUES:RLIM:PTR?"
30 ENTER 717;A

Related commands :STAT:QUES:RLIM? on page 465
:STAT:QUES:RLIM:NTR on page 470

Equivalent key No equivalent key is available on the front panel.

:SYST:BACK

Syntax :SYSTem:BACKlight {ON|OFF|1|0}
 :SYSTem:BACKlight?

Description Turns ON/OFF the backlight of the LCD display.
 When the backlight is OFF, you cannot read the information on the display.

Parameters

	Description
ON or 1 (preset value)	Turns ON the backlight.
OFF or 0	Turns OFF the backlight.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":SYST:BACK OFF"
 20 OUTPUT 717;":SYST:BACK?"
 30 ENTER 717;A

Equivalent key **[System] - Backlight**
 To turn it ON, press any key on the front panel.

:SYST:BEEP:COMP:IMM

Syntax	:SYSTem:BEEPer:COMPLete:IMMediate
Description	Generates a beep for the notification of the completion of the operation. (No query)
Example of use	10 OUTPUT 717; ":SYST:BEEP:COMP:IMM"
Related commands	:SYST:BEEP:COMP:STAT on page 473 :SYST:BEEP:WARN:IMM on page 474
Equivalent key	[System] - Misc Setup - Beeper - Test Beep Complete

:SYST:BEEP:COMP:STAT

Syntax	:SYSTem:BEEPer:COMPLete:STATe {ON OFF 1 0} :SYSTem:BEEPer:COMPLete:STATe?
Description	Turns ON/OFF the beeper for the notification of the completion of the operation.
Parameters	

	Description
ON or 1 (preset value)	Turns ON the beeper.
OFF or 0	Turns OFF the beeper.

Query response	{1 0}<newline><^END>
Example of use	10 OUTPUT 717; ":SYST:BEEP:COMP:STAT OFF" 20 OUTPUT 717; ":SYST:BEEP:COMP:STAT?" 30 ENTER 717;A
Related commands	:SYST:BEEP:COMP:IMM on page 473 :SYST:BEEP:WARN:STAT on page 474
Equivalent key	[System] - Misc Setup - Beeper - Beep Complete

:SYST:BEEP:WARN:IMM

Syntax	:SYSTem:BEEPer:WARNing:IMMediate
Description	Generates a beep for the notification of warning/limit test result. (No query)
Example of use	10 OUTPUT 717; ":SYST:BEEP:WARN:IMM"
Related commands	:SYST:BEEP:WARN:STAT on page 474 :SYST:BEEP:COMP:IMM on page 473
Equivalent key	[System] - Misc Setup - Beeper - Test Beep Warning

:SYST:BEEP:WARN:STAT

Syntax	:SYSTem:BEEPer:WARNing:STATe {ON OFF 1 0} :SYSTem:BEEPer:WARNing:STATe?
Description	Turns ON/OFF the beeper for the notification of warning/limit test result.
Parameters	

	Description
ON or 1 (preset value)	Turns ON the beeper.
OFF or 0	Turns OFF the beeper.

Query response	{1 0}<newline><^END>
Example of use	10 OUTPUT 717; ":SYST:BEEP:WARN:STAT OFF" 20 OUTPUT 717; ":SYST:BEEP:WARN:STAT?" 30 ENTER 717;A
Related commands	:SYST:BEEP:WARN:IMM on page 474 :SYST:BEEP:COMP:STAT on page 473
Equivalent key	[System] - Misc Setup - Beeper - Beep Warning

:SYST:DATE

Syntax :SYSTem:DATE <numeric 1>,<numeric 2>,<numeric 3>
:SYSTem:DATE?

Description Sets the date of the clock built in the E5061A/E5062A.

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Year	Month	Day
Range	1980 to 2099	1 to 12	1 to 31
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use
10 OUTPUT 717;" :SYST:DATE 2002,1,1"
20 OUTPUT 717;" :SYST:DATE?"
30 ENTER 717;A,B,C

Related commands :SYST:TIME on page 482
:DISP:CLOC on page 305

Equivalent key [System] - Misc Setup - Clock Setup - Set Date and Time

:SYST:ERR?

Syntax	:SYSTem:ERRor?
Description	Reads out the oldest error of the errors stored in the error queue of the E5061A/E5062A. The read-out error is deleted from the error queue. The size of the error queue is 100. Executing the *CLS command clears the errors stored in the error queue. (Query only)
NOTE	This command can not return an error that occurs by the manual operation or the COM object used in controlling the E5061A/E5062A from the VBA Macro.
Query response	{numeric},{string}<newline><^END> {numeric}: Error number {string}: Error message (a character string with double quotation marks (")) If no error is stored in the error queue, 0 and "No error" are read out as the error number and the error message.
Example of use	<pre>10 OUTPUT 717;":SYST:ERR?" 20 ENTER 717;A,B\$</pre>
Related commands	*CLS on page 196
Equivalent key	No equivalent key is available on the front panel.

:SYST:KLOC:KBD

Syntax :SYSTem:KLOCK:KBD {ON|OFF|1|0}
:SYSTem:KLOCK:KBD?

Description Sets whether to lock the operation of the front panel (key and rotary knob) and keyboard.

Parameters

	Description
ON or 1	Specifies lock.
OFF or 0 (preset value)	Specifies unlock.

Query response {1|0}<newline><^END>

Example of use
10 OUTPUT 717;":SYST:KLOC:KBD ON"
20 OUTPUT 717;":SYST:KLOC:KBD?"
30 ENTER 717;A

Related commands :SYST:KLOC:MOUS on page 478

Equivalent key **[System] - Misc Setup - Key Lock - Front Panel & Keyboard Lock**

:SYST:KLOC:MOUS

Syntax :SYSTem:KLOCK:MOUSe {ON|OFF|1|0}
 :SYSTem:KLOCK:MOUSe?

Description Sets whether to lock the operation of the mouse and touch screen.

Parameters

	Description
ON or 1	Specifies lock.
OFF or 0 (preset value)	Specifies unlock.

Query response {1|0}<newline><^END>

Example of use 10 OUTPUT 717;":SYST:KLOC:MOUS ON"
 20 OUTPUT 717;":SYST:KLOC:MOUS?"
 30 ENTER 717;A

Related commands :SYST:KLOC:KBD on page 477

Equivalent key [System] - Misc Setup - Key Lock - Mouse Lock

:SYST:POFF

Syntax	:SYSTem:POFF
Description	Turns OFF the E5061A/E5062A. (No query)
Example of use	10 OUTPUT 717; ":SYST:POFF"
Equivalent key	Standby switch

:SYST:PRES

Syntax	:SYSTem:PRESet
Description	Performs preset. There is the following difference from the setting state preset with the *RST command. (No query) The continuous initiation mode of channel 1 is set to ON.
Example of use	10 OUTPUT 717; ":SYST:PRES"
Related commands	*RST on page 199 :SYST:UPR on page 483
Equivalent key	[Preset] - OK

:SYST:SEC:LEV

Syntax :SYSTem:SECurity[:LEVel] {NON|LOW|HIGH}
 :SYSTem:SECurity[:LEVel]?

Description Sets/Reads the security level.

Parameters

	Description
NON (preset value)	Turns OFF the security level.
LOW	Turns ON and specifies LOW level to the security level.
HIGH	Turns ON and specifies HIGH level to the security level.

When the setting of security level is LOW, it is able to change to NON or HIGH. But when this setting is HIGH, it is not able to change NON or LOW.

The setting of security level can be turned NON by executing the preset or recalling when the setting of security level is HIGH.

Even if the setting of security level is ON, the command that reads out the frequency is not influenced.

Query response {NON|LOW|HIGH}<newline><^END>

Example of use 10 OUTPUT 717;":SYST:SEC LOW"
 20 OUTPUT 717;":SYST:SEC?"
 30 ENTER 717;A\$

Equivalent key **[System] - Service Menu - Security Level - None|Low|High**

:SYST:SERV?

Syntax	:SYSTem:SERVice?
Description	Reads out whether to be in the service mode. (Query only)
Query response	{1 0}<newline><^END>

	Description
1	In the service mode.
0	Not in the service mode.

Example of use	10 OUTPUT 717;":SYST:SERV?" 30 ENTER 717;A
Equivalent key	Displayed on the instrument status bar (at the bottom of the LCD display).

:SYST:TIME

Syntax :SYSTem:TIME <numeric 1>,<numeric 2>,<numeric 3>
 :SYSTem:TIME?

Description Sets the time of the clock built in the E5061A/E5062A.

Parameters

	<numeric 1>	<numeric 2>	<numeric 3>
Description	Hour (24-hour basis)	Minute	Second
Range	0 to 23	0 to 59	0 to 59
Resolution	1	1	1

If the specified parameter is out of the allowable setup range, the minimum value (if the lower limit of the range is not reached) or the maximum value (if the upper limit of the range is exceeded) is set.

Query response {numeric 1},{numeric 2},{numeric 3}<newline><^END>

Example of use 10 OUTPUT 717;":SYST:TIME 17,30,0"
 20 OUTPUT 717;":SYST:TIME?"
 30 ENTER 717;A,B,C

Related commands :SYST:DATE on page 475
 :DISP:CLOC on page 305

Equivalent key [System] - Misc Setup - Clock Setup - Set Date and Time

:SYST:UPR

Syntax	:SYSTem:UPReset
Description	Executes the user-specified preset. The command is executed regardless of the preset operation mode. (No query) If the user-specified preset file (D:\UserPreset.sta) does not exist, a warning message is displayed, and “:SYST:PRES” is executed.
Example of use	10 OUTPUT 717; ":SYST:UPR"
Related commands	*RST on page 199 :SYST:PRES on page 479
Equivalent key	[Preset] - OK

:TRIG

Syntax	:TRIGger[:SEQuence][:IMMediate]
Description	Regardless of the setting of the trigger mode, generates a trigger immediately and executes a measurement. There is the following difference from the trigger with the :TRIG:SING command. The execution of the command finishes at the time of a trigger. If you execute this command when the trigger system is not in the trigger wait state (trigger event detection state), an error occurs and the command is ignored. For details about the trigger system, refer to “Trigger system” on page 80. (No query)
Example of use	10 OUTPUT 717; ":TRIG"
Related commands	:TRIG:SING on page 484
Equivalent key	No equivalent key is available on the front panel.

:TRIG:SING

Syntax	:TRIGger[:SEQuence]:SINGle
Description	Regardless of the setting of the trigger mode, generates a trigger immediately and executes a measurement. There is the following difference from the trigger with the :TRIG command. The execution of the command finishes when the measurement (all sweeps) initiated with this command finishes. In other words, you can wait for the end of the measurement using the *OPC? command. If you execute this command when the trigger system is not in the trigger wait state (trigger event detection state), an error occurs and the command is ignored. For details about the trigger system, refer to “Trigger system” on page 80. (No query)
Example of use	10 OUTPUT 717; ":TRIG:SING" 20 OUTPUT 717; "*OPC?" 30 ENTER 717;A
Related commands	:TRIG on page 484 *OPC? on page 198
Equivalent key	No equivalent key is available on the front panel.

:TRIG:SOUR

Syntax :TRIGger[:SEQuence]:SOURce {INTernal|EXTernal|MANual|BUS}
:TRIGger[:SEQuence]:SOURce?

Description Selects the trigger source from the following 4 types.

Internal	Uses the internal trigger to generate continuous triggers automatically.
External	Generates a trigger when the trigger signal is inputted externally via the Ext Trig connector or the handler interface.
Manual	Generates a trigger when the key operation of [Trigger] - Trigger is executed from the front panel.
Bus	Generates a trigger when the *TRG command is executed.

When you change the trigger source during sweep, the sweep is canceled.

Parameters

	Description
INTernal (preset value)	Specifies internal.
EXTernal	Specifies external.
MANual	Specifies manual.
BUS	Specifies bus.

Query response {BUS|EXT|INT|MAN}<newline><^END>

Example of use

```

10  OUTPUT 717;":TRIG:SOUR BUS"
20  OUTPUT 717;":TRIG:SOUR?"
30  ENTER 717;A$

```

Related commands *TRG on page 201

Equivalent key **[Trigger] - Trigger Source - Internal|External|Manual|Bus**

Command list

Command tree

Table 13-1 shows the SCPI command tree of the E5061A/E5062A.

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
ABORt		[No query]
CALCulate{[1] 2 3 4}		
:PARAmeter		
:COUNt	<numeric>	
:PARAmeter{[1] 2 3 4}		
:DEFine	{S11 S21 S12 S22}	
:SElect		[No query]
[:SElecte]d]		
:BLIMit		
:DB	<numeric>	
:DISPlay		
:MARKer	{ON OFF 1 0}	
:VALue	{ON OFF 1 0}	
:FAIL?		[Query only]
:MAXimum	<numeric>	
:MINimum	<numeric>	
:REPort		
[:DATA]?		[Query only]
[:STATe]	{ON OFF 1 0}	
:CONVersion		
:FUNCTion	{ZREFlection ZTRansmit YREFlection YTRansmit INVersion}	
[:STATe]	{ON OFF 1 0}	
:CORRection		
:EDELay		
:TIME	<numeric>	
:OFFSet		
:PHASe	<numeric>	
:DATA		
:FDATA	<numeric>,...,<numeric> (number of measurement points × 2 parameters)	
:FMEMory	<numeric>,...,<numeric> (number of measurement points × 2 parameters)	
:SDATA	<numeric>,...,<numeric> (number of measurement points × 2 parameters)	
:SMEMory	<numeric>,...,<numeric> (number of measurement points × 2 parameters)	
:FORMat	{MLOGarithmic PHASe GDELay SLINear SLOGarithmic SCOMplex SMITH SADMittance PLINear PLOGarithmic POLar MLINear SWR REAL IMAGinary UPHase PPHase}	

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
CALCulate{[1] 2 3 4}		
[:SELeCted]		
:FUNcTion		
:DOMain		
:COUPle	{ON OFF 1 0}	
:STARt	<numeric>	
[:STATe]	{ON OFF 1 0}	
:STOP	<numeric>	
:EXECute		[No query]
:PEXCursion	<numeric>	
:POINts?		[Query only]
:PPOLarity	{POSitive NEGative BOTH}	
:TARGet	<numeric>	
:TTRansition	{POSitive NEGative BOTH}	
:TYPE	{PTPeak STDEV MEAN MAXimum MINimum PEAK APEak ATARget}	
:LIMit		
:DATA	<numeric>,...,<numeric> (1 + number of lines × 5 parameters)	
:DISPlay		
[:STATe]	{ON OFF 1 0}	
:CLIP	{ON OFF 1 0}	
:FAIL?		[Query only]
:OFFSet		
:AMPLitude	<numeric>	
:MARKer?		[Query only]
:STIMulus	<numeric>	
:REPort		
:ALL?		[Query only]
[:DATA]?		[Query only]
:POINts?		[Query only]
[:STATe]	{ON OFF 1 0}	
:MARKer		
:BWIDth		
[:STATe]	{ON OFF 1 0}	
:COUPle	{ON OFF 1 0}	
:DISCrete	{ON OFF 1 0}	
:FUNcTion		
:DOMain		
:COUPle	{ON OFF 1 0}	
:STARt	<numeric>	
[:STATe]	{ON OFF 1 0}	
:STOP	<numeric>	
:MULTi		
:PEXCursion	<numeric>	
:PPOLarity	{POSitive NEGative BOTH}	
:TARGet	<numeric>	
:TRACking	{ON OFF 1 0}	

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
CALCulate{[1] 2 3 4}		
[:SElected]		
:MARKer		
:FUNCTion		
:MULTi		
:TTRansition	{POSitive NEGative BOTH}	
:TYPE	{OFF PEAK TARGet}	
:MATH		
:FLATness		
:DATA?		[Query only]
[:STATe]	{ON OFF 1 0}	
:FSTatistics		
:DATA?		[Query only]
[:STATe]	{ON OFF 1 0}	
:STSTistics		
:DATA?		[Query only]
[:STATe]	{ON OFF 1 0}	
:NOTCh		
[:STATe]	{ON OFF 1 0}	
:REFeRence		
[:STATe]	{ON OFF 1 0}	
:MARKer{[1] 2 3 4 5 6 7 8 9 10}		
:ACTivate		[No query]
:BWIDth		
:DATA?		[Query only]
:THReshold	<numeric>	
:FUNCTion		
:EXECute		[No query]
:PEXCursion	<numeric>	
:PPOLarity	{POSitive NEGative BOTH}	
:TARGet	<numeric>	
:TRACking	{ON OFF 1 0}	
:TTRansition	{POSitive NEGative BOTH}	
:TYPE	{MAXimum MINimum PEAK LPEak RPEak TARGet LTARget RTARget}	
:NOTCh		
:DATA?		[Query only]
:THReshold	<numeric>	
:SET	{STARt STOP CENTer RLEVel DELay}	[No query]
[:STATe]	{ON OFF 1 0}	
:X	<numeric>	
:Y?		[Query only]
:MATH		
:FUNCTion	{NORMal SUBTract DIVide ADD MULTiply}	
:MEMorize		[No query]

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
CALCulate{[1] 2 3 4}		
[:SELeCted]		
:MStatistics		
:DATA?		[Query only]
[:STATe]	{ON OFF 1 0}	
:RLIMit		
:DATA	<numeric>,...,<numeric> (1 + number of lines × 4 parameters)	
:DISPlay		
:LINE	{ON OFF 1 0}	
:SELeCt	<numeric>	
:VALue	{OFF ABSolute MARgin}	
:FAIL?		[Query only]
:REPort		
[:DATA]?		[Query only]
[:STATe]	{ON OFF 1 0}	
:SMOothing		
:APERture	<numeric>	
[:STATe]	{ON OFF 1 0}	
:TRANsform		
:TIME		
:CENTer	<numeric>	
:IMPulse		
:WIDTh	<numeric>	
:KBESsel	<numeric>	
:LPFRequency		[No query]
:SPAN	<numeric>	
:STARt	<numeric>	
:STATe	{ON OFF 1 0}	
:STEP		
:RTIME	<numeric>	
:STIMulus	{IMPulse STEP}	
:STOP	<numeric>	
[:TYPE]	{BPASs LPASs}	
CONTRol		
:HANDler		
:A		
[:DATA]	<numeric>	[No query]
:B		
[:DATA]	<numeric>	[No query]
:C		
[:DATA]	<numeric>	
:MODE	{INPut OUTPut}	
:D		
[:DATA]	<numeric>	
:MODE	{INPut OUTPut}	

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
CONTRol		
:HANDler		
:E		
[:DATA]	<numeric>	
[:EXTension]		
:INDEX		
:STATe	{ON OFF 1 0}	
:RTRigger		
:STATe	{ON OFF 1 0}	
:F		
[:DATA]	<numeric>	[No query]
:OUTPut{[1] 2}		
[:DATA]	<numeric>	
DISPlay		
:ANNotation		
:FREQuency		
[:STATe]	{ON OFF 1 0}	
:CLOCK	{ON OFF 1 0}	
:COLOr{[1] 2}		
:BACK	<numeric>,<numeric>,<numeric>	
:GRATicule{[1] 2}	<numeric>,<numeric>,<numeric>	
:LIMit{[1] 2}	<numeric>,<numeric>,<numeric>	
:RESet		[No query]
:TRACe{[1] 2 3 4}		
:DATA	<numeric>,<numeric>,<numeric>	
:MEMory	<numeric>,<numeric>,<numeric>	
:ECHO		
:CLEar		[No query]
[:DATA]	<string>	[No query]
:ENABle	{ON OFF 1 0}	
:FSIGn	{ON OFF 1 0}	
:IMAGe	{NORMal INVert}	
:MAXimize	{ON OFF 1 0}	
:SKEY		
[:STATe]	{ON OFF 1 0}	
:SPLit	{D1 D12 D1_2 D112 D1_1_2 D123 D1_2_3 D12_33 D11_23 D13_23 D12_13 D1234 D1_2_3_4 D12_34}	
:TABLE		
[:STATe]	{ON OFF 1 0}	
:TYPE	{MARKer LIMit SEGment}	
:UPDate		
[:IMMediate]		[No query]

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
DISPlay		
:WINDow{[1] 2 3 4}		
:ACTivate		[No query]
:ANNotation		
:MARKer		
:ALIGn		
[:STATe]	{ON OFF 1 0}	
:SINGle		
[:STATe]	{ON OFF 1 0}	
:LABel	{ON OFF 1 0}	
:MAXimize	{ON OFF 1 0}	
:SPLit	{D1 D12 D1_2 D112 D1_1_2 D123 D1_2_3 D12_33 D11_23 D13_23 D12_13 D1234 D1_2_3_4 D12_34}	
:TITLe		
:DATA	<string>	
[:STATe]	{ON OFF 1 0}	
:TRACe{[1] 2 3 4}		
:ANNotation		
:MARKer		
:POSition:X	<numeric>	
:POSition:Y	<numeric>	
:YAXis		
:MODE	{AUTO RELative}	
:MEMory		
[:STATe]	{ON OFF 1 0}	
:STATe	{ON OFF 1 0}	
:Y		
[:SCALe]		
:AUTO		[No query]
:PDIVision	<numeric>	
:RLEVel	<numeric>	
:RPOSition	<numeric>	
:TRACk		
:MODE	{OFF PEAK FREQuency}	
:FREQuency	<numeric>	
:X		
:SPACing	{LINear OBASe}	
:Y		
[:SCALe]		
:DIVisions	<numeric>	
FORMat		
:BORDER	{NORMal SWApped}	
:DATA	{ASCii REAL REAL32}	

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
HCOPY		
:ABORt		[No query]
:IMAGe	{NORMal INVert}	
[:IMMediate]		[No query]
INITiate{[1] 2 3 4}		
:CONTinuous	{ON OFF 1 0}	
[:IMMediate]		[No query]
MMEMory		
:CATalog?	<string>	[Query only]
:COPY	<string>,<string>	[No query]
:DELeTe	<string>	[No query]
:LOAD		
:CHANnel		
:COEFFicient	{A B C D}	[No query]
[:STATe]	{A B C D}	[No query]
:LIMit	<string>	[No query]
:PROGram	<string>	[No query]
:SEGment	<string>	[No query]
[:STATe]	<string>	[No query]
:MDIRectory	<string>	[No query]
:STORe		
:CHANnel		
:CLEar		[No query]
:COEFFicient	{A B C D}	[No query]
[:STATe]	{A B C D}	[No query]
:FDATA	<string>	[No query]
:IMAGe	<string>	[No query]
:LIMit	<string>	[No query]
:PROGram	<string>	[No query]
:SALL	{ON OFF 1 0}	
:SEGment	<string>	[No query]
[:STATe]	<string>	[No query]
:STYPe	{STATe CSTate DSTate CDSTate}	
:TRANsfer	<string>,<block>	[No query]
OUTPut		
[:STATe]	{ON OFF 1 0}	
PROGram		
:CATalog?		[Query only]
[:SELeCted]		
:NAME	<string>	
:STATe	{STOP RUN}	

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
SENSe		
:CORRection		
:COLLect		
:ECAL		
:PATH?		[Query only]
SENSe{[1] 2 3 4}		
:AVERage		
:CLEar		[No query]
:COUNt	<numeric>	
[:STATe]	{ON OFF 1 0}	
:BANDwidth		
[:RESolution]	<numeric>	
:BWIDth		
[:RESolution]	<numeric>	
:CORRection		
:CLEar		[No query]
:COEFFicient		
[:DATA]?	{ES ER ED EL ET EX}, <numeric>, <numeric>	[Query only]
:COLLect		
[:ACQuire]		
:ISOLation	<numeric>, <numeric>	
:LOAD	<numeric>	
:OPEN	<numeric>	
:SHORT	<numeric>	
:THRU	<numeric>, <numeric>	
:CKIT		
:LABel	<string>	
:ORDer		
:LOAD	<numeric>, <numeric>	
:OPEN	<numeric>, <numeric>	
:SHORT	<numeric>, <numeric>	
:THRU	<numeric>, <numeric>, <numeric>	
[:SElect]	<numeric>	
:STAN{[1] 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21}		
:ARBitrary	<numeric>	
:C0	<numeric>	
:C1	<numeric>	
:C2	<numeric>	
:C3	<numeric>	
:DELay	<numeric>	
:L0	<numeric>	
:L1	<numeric>	
:L2	<numeric>	
:L3	<numeric>	
:LABel	<string>	

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
SENSe{[1] 2 3 4}		
:CORRection		
:COLLect		
:CKIT		
:STAN{[1] 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21}		
:LOSS	<numeric>	
:TYPE	{OPEN SHORT LOAD THRU ARBI NONE}	
:Z0	<numeric>	
:ECAL		
:ERESponse	<numeric>,<numeric>	[No query]
:ISOLation		
[:STATe]	{ON OFF 1 0}	
:SOLT1	<numeric>	
:SOLT2	<numeric>,<numeric>	
:THRU	<numeric>,<numeric>	
:METHod		
:ERESponse	<numeric>,<numeric>	
[:RESPonse]		
:OPEN	<numeric>	
:SHORT	<numeric>	
:THRU	<numeric>,<numeric>	
:SOLT1	<numeric>	
:SOLT2	<numeric>,<numeric>	
:TYPE?		[Query only]
:SAVE		[No query]
:EXTension		
:PORT{[1] 2}		
[:TIME]	<numeric>	
[:STATe]	{ON OFF 1 0}	
:PROPerTy	{ON OFF 1 0}	
:RVELocity		
:COAX	<numeric>	
:STATe	{ON OFF 1 0}	
:TYPE{[1] 2 3 4}?		[Query only]
:FREQuency		
:CENTer	<numeric>	
:[CW FIXed]	<numeric>	
:DATA?		[Query only]
:SPAN	<numeric>	
:STARt	<numeric>	
:STOP	<numeric>	
:ROSCillator		
:SOURce?		[Query only]

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
SENSe{[1] 2 3 4}		
:SEGMent		
:DATA	<numeric>,...,<numeric>	
:SWEep		
:POINts?		[Query only]
:TIME		
[:DATA]?		[Query only]
:SWEep		
:DELay	<numeric>	
:POINts	<numeric>	
:TIME		
:AUTO	{ON OFF 1 0}	
[:DATA]	<numeric>	
:TYPE	{LINear LOGarithmic SEGMent POWer}	
SERVice		
:CHANnel		
:ACTive?		[Query only]
:COUNt?		[Query only]
:TRACe		
:COUNt?		[Query only]
:CHANnel{[1] 2 3 4}		
:TRACe		
:ACTive?		[Query only]
:PORT		
:COUNt?		[Query only]
SOURce{[1] 2 3 4}		
:POWer		
:ATTenuation		
[:DATA]	<numeric>	
:CENTer	<numeric>	
[:LEVel]		
[:IMMediate]		
[:AMPLitude]	<numeric>	
:SLOPe		
[:DATA]	<numeric>	
:STATe	{ON OFF 1 0}	
:PORT		
:COUPle	{ON OFF 1 0}	
:PORT{[1] 2}		
[:LEVel]		
[:IMMediate]		
[:AMPLitude]	<numeric>	
:SPAN	<numeric>	
:STARt	<numeric>	

SCPI Command Reference
Command list

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
SOURce{[1] 2 3 4}		
:POWer		
:STOP	<numeric>	
STATus		
:OPERation		
:CONDition?		[Query only]
:ENABle	<numeric>	
[::EVENTt]?		[Query only]
:NTRansition	<numeric>	
:PTRansition	<numeric>	
:PRESet		[No query]
:QUEStionable		
:CONDition?		[Query only]
:ENABle	<numeric>	
[::EVENTt]?		[Query only]
:LIMit		
:CHANnel{[1] 2 3 4}		
:CONDition?		[Query only]
:ENABle	<numeric>	
[::EVENTt]?		[Query only]
:NTRansition	<numeric>	
:PTRansition	<numeric>	
:CONDition?		[Query only]
:ENABle	<numeric>	
[::EVENTt]?		[Query only]
:NTRansition	<numeric>	
:PTRansition	<numeric>	
STATus		
:QUEStionable		
:NTRansition	<numeric>	
:PTRansition	<numeric>	
SYSTem		
:BACKlight	{ON OFF 1 0}	
:BEEPer		
:COMPlete		
:IMMediate		
:STATe	{ON OFF 1 0}	
:WARNIing		
:IMMediate		
:STATe	{ON OFF 1 0}	
:DATE	<numeric>, <numeric>, <numeric>	
:ERRor?		[Query only]
:KLOCK		

Table 13-1 E5061A/E5062A SCPI command tree

Command	Parameters	Note
SYSTem		
:KLOCK		
:KBD	{ON OFF 1 0}	
:MOUSE	{ON OFF 1 0}	
:POFF		[No query]
:PRESet		[No query]
:SECurity		
[:LELe]	{NONE LOW HIGH}	
:SERvice?		[Query only]
:TIME	<numeric>,<numeric>,<numeric>	
:UPReset		[No query]
TRIGger		
[:SEQuence]		
[:IMMediate]		[No query]
:SINGle		[No query]
:SOURce	{INTernal EXTernal MANual BUS}	

A Manual Changes

This appendix contains the information required to adapt this manual to earlier versions or configurations of the Agilent E5061A/E5062A than that indicated by the current printing date of this manual. The information in this manual applies directly to the E5061A/E5062A model that has the serial number prefix listed on the title page of this manual.

Manual Changes

To adapt this manual to your Agilent E5061A/E5062A, refer to Table A-1 and Table A-2.

Table A-1 **Manual Changes by Serial Number**

Serial Prefix or Number	Make Manual Changes


Table A-2 **Manual Changes by Firmware Version**

Version	Make Manual Changes
A.02.00 or later	Change 1
A.02.10 or later	Change 2
A.03.00 or later	Change 3

Agilent Technologies uses a two-part, ten-character serial number that is stamped on the serial number plate (Figure A-1).

Execute the ***IDN?** command on page 198 to check the firmware version.

Figure A-1 **Serial Number Plate (Example)**

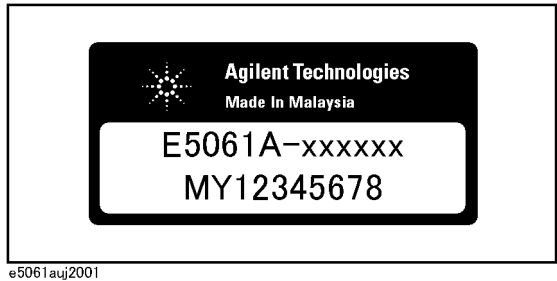

e5061auj2001

Change 3

The firmware revision A.02.10 or below does not support the following functions. Please disregard the descriptions of these functions in this manual.

- ☐ Compliant with LXI (Lan eXtensions for Instrumentation) standard Class C.*¹

Change 2

The firmware revision A.02.00 or below does not support the following functions. Please disregard the descriptions of these functions in this manual.

- ☐ Offset limit line function
- ☐ Ripple test function
- ☐ Bandwidth test function

The firmware revision A.02.00 and below does not support the following SCPI commands. Please delete their descriptions in this manual.

- **:CALC{1-4}:BLIM** on page 203
- **:CALC{1-4}:BLIM:DB** on page 204
- **:CALC{1-4}:BLIM:DISP:MARK** on page 205
- **:CALC{1-4}:BLIM:DISP:VAL** on page 206
- **:CALC{1-4}:BLIM:FAIL?** on page 207
- **:CALC{1-4}:BLIM:MAX** on page 208
- **:CALC{1-4}:BLIM:MIN** on page 209
- **:CALC{1-4}:BLIM:REP?** on page 210
- **:CALC{1-4}:LIM:OFFS:AMPL** on page 238
- **:CALC{1-4}:LIM:OFFS:MARK** on page 239
- **:CALC{1-4}:LIM:OFFS:STIM** on page 240
- **:CALC{1-4}:LIM:REP:ALL?** on page 241
- **:CALC{1-4}:RLIM** on page 286
- **:CALC{1-4}:RLIM:DATA** on page 287
- **:CALC{1-4}:RLIM:DISP:LINE** on page 288
- **:CALC{1-4}:RLIM:DISP:SEL** on page 289
- **:CALC{1-4}:RLIM:DISP:VAL** on page 290
- **:CALC{1-4}:RLIM:FAIL?** on page 291
- **:CALC{1-4}:RLIM:REP?** on page 292
- **:MMEM:LOAD:RLIM** on page 350
- **:MMEM:STOR:LIM** on page 358
- **:STAT:QUES:BLIM?** on page 445

*1. This function is available when the volume label on the hard disk is AL300 or higher.

- **:STAT:QUES:BLIM:CHAN{1-4}?** on page 446
- **:STAT:QUES:BLIM:CHAN{1-4}:COND?** on page 446
- **:STAT:QUES:BLIM:CHAN{1-4}:ENAB** on page 447
- **:STAT:QUES:BLIM:CHAN{1-4}:NTR** on page 448
- **:STAT:QUES:BLIM:CHAN{1-4}:PTR** on page 449
- **:STAT:QUES:BLIM:COND?** on page 449
- **:STAT:QUES:BLIM:ENAB** on page 450
- **:STAT:QUES:BLIM:NTR** on page 451
- **:STAT:QUES:BLIM:PTR** on page 452
- **:STAT:QUES:RLIM?** on page 465
- **:STAT:QUES:RLIM:CHAN{1-4}?** on page 465
- **:STAT:QUES:RLIM:CHAN{1-4}:COND?** on page 465
- **:STAT:QUES:RLIM:CHAN{1-4}:ENAB** on page 466
- **:STAT:QUES:RLIM:CHAN{1-4}:NTR** on page 467
- **:STAT:QUES:RLIM:CHAN{1-4}:PTR** on page 468
- **:STAT:QUES:RLIM:COND?** on page 468
- **:STAT:QUES:RLIM:ENAB** on page 469
- **:STAT:QUES:RLIM:NTR** on page 470
- **:STAT:QUES:RLIM:PTR** on page 471

Change 1

The following functions are newly integrated into the firmware version A.02.00 onward. They are not supported by firmware version A.01.0x.

- ☐ User preset function.
- ☐ Notch search function
- ☐ Function to all the marker value are displayed.
- ☐ Function to change display position where marker value are displayed.
- ☐ Function to align the marker value.
- ☐ Display the overlap limit lines.
- ☐ Reference tracking function.
- ☐ Function to change display value where Y axis are displayed.
- ☐ Frequency information appearing as asterisks.
- ☐ User recovery function.*¹
- ☐ Remote control using HTTP.*¹

*1. This function is available when the volume label on the hard disk is AL200 or higher.

The firmware version A.01.0x does not support the following SCPI commands. Please delete their descriptions in this manual.

- **:CALC{1-4}:LIM:DISP:CLIP** on page 236
- **:CALC{1-4}:MARK:NOTC** on page 261
- **:CALC{1-4}:MARK{1-10}:NOTC:DATA?** on page 276
- **:CALC{1-4}:MARK{1-10}:NOTC:THR** on page 277
- **:DISP:WIND{1-4}:ANN:MARK:ALIG** on page 319
- **:DISP:WIND{1-4}:ANN:MARK:SING** on page 320
- **:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:X** on page 325
- **:DISP:WIND{1-4}:TRAC{1-4}:ANN:MARK:POS:Y** on page 326
- **:DISP:WIND{1-4}:TRAC{1-4}:ANN:YAX:MODE** on page 327
- **:DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:FREQ** on page 333
- **:DISP:WIND{1-4}:TRAC{1-4}:Y:TRAC:MODE** on page 334
- **:SYST:SEC:LEV** on page 480
- **:SYST:UPR** on page 483

B **Status Reporting System**


This appendix describes the status reporting system of the Agilent E5061A/E5062A.

General Status Register Model

The Agilent E5061A/E5062A has a status reporting system to report the condition of the instrument.

Figure B-1

General status register model

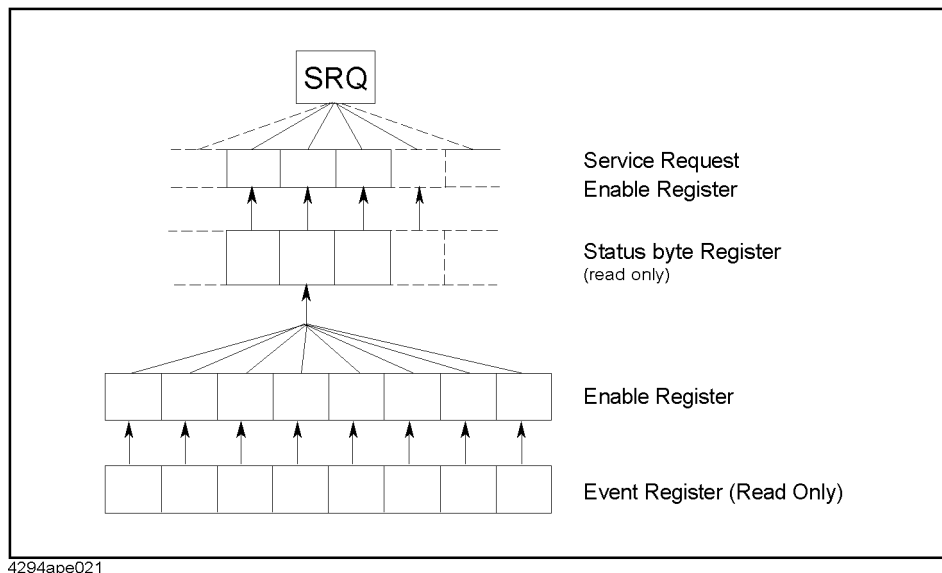

The status reporting system has a hierarchical structure as shown in Figure B-1. When the instrument satisfies a particular condition, the corresponding bit of the event register is set to 1. Therefore, you can check the instrument status by reading the event register.

When the event register bit is set to “1” and a corresponding enable register bit (a bit marked with an arrow in Figure B-1) is also “1,” the summary bit of the status byte register is set to “1.” You can read the status byte register by using the serial poll.

If the bit of the service request enable register is “1,” a service request (SRQ) is generated by the positive transition of the corresponding status byte register bit. By generating SRQ, you can notify the controller that the E5061A/E5062A is requesting service. In other words, interruption by SRQ can be programmed. For more information on using SRQ, see “Using the Status Register” on page 84 in Chapter 5, “Making a Measurement,” or “Using the status reporting system” on page 166 in Chapter 11, “Working with Automatic Test Systems.”

Event Register

Reflects the corresponding condition of the E5061A/E5062A (e.g., occurrence of an event) as a bit status. These bits continuously monitor changes in the E5061A/E5062A's state and change the bit status when the condition (e.g., change bit status to "1" if a specific event occurs) for each bit is met. You cannot change the bit status by issuing a SCPI command.

Enable Register

Setting the enable register allows you to specify event register bits that can set "1" to the summary bit of the status byte register when an event occurs. The register bits work as mask bits; setting "1" to an enable register will enable a corresponding bit in the event register.

For example, when you want to set "1" as the summary bit in the status byte register by a specific register condition, set the corresponding enable register to "1."

Status Byte Register

If the enabled event register is set to "1," a corresponding bit of the status byte register is also set to "1." This register also indicates the output queue and SRQ status.

The value of the status byte register can be read by using the ***STB?** command on page 201 command or serial poll (SPOLL statement in HTBasic) from the controller.

Reading the status byte register by using the ***STB?** command does not affect the contents of the status byte register. However, reading it with the SPOLL statement of HTBasic will clear the RQS bit in the status byte register.

Also, setting the service request enable register using the ***SRE** command on page 200 command can generate a service request synchronously with the status byte register.


Condition Register and Transition Filter

When the status register has a transition filter, there is a lower register called a condition register under the event register. The transition filter is between the event register and the condition register.

The transition filter enables you to select a positive and/or negative transition of the condition register bit in order to set a bit in the corresponding event register. For example, using the negative transition filter to set bit 3 to “1” causes bit 3 of the event register to be set to “1” when bit 3 of the condition register makes a negative transition, that is, changes from 1 to 0.

Figure B-2

Transition filter and condition register

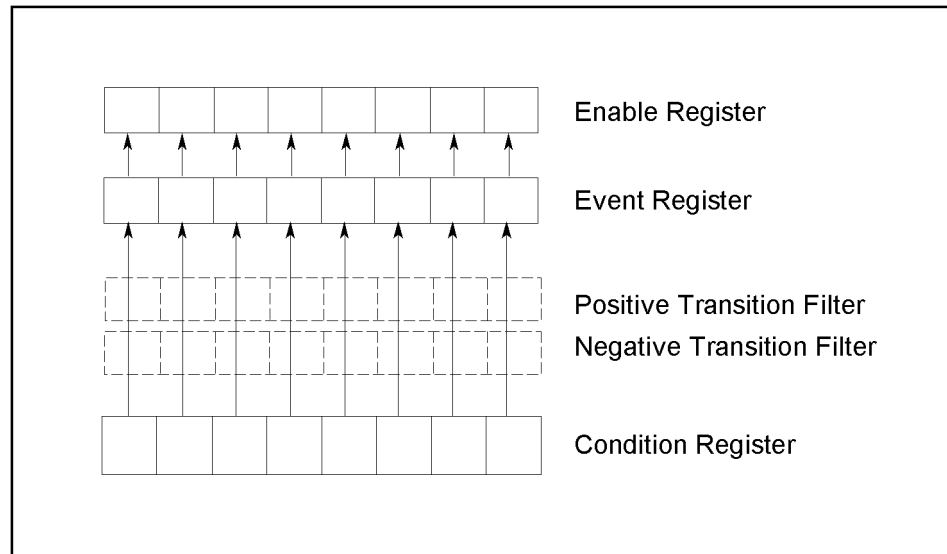

4294ape022

In the E5061A/E5062A, the following registers provide a condition register and transition filter:


- Operation status register
- Questionable status register
- Questionable limit status register
- Questionable limit extra status register
- Questionable limit channel {1-16} status register
- Questionable limit channel {1-16} extra status register

Status Register Structure

The status reporting system has a hierarchical structure as shown in Figure B-3 through Figure B-9. The status byte register is a summary of registers in the lower level. This section describes the E5061A/E5062A’s status registers in each hierarchy. Each bit of the status register is described in Table B-1 through Table B-11.


Status Reporting System
Status Register Structure

Figure B-3 Status Register Structure (1 of 7)

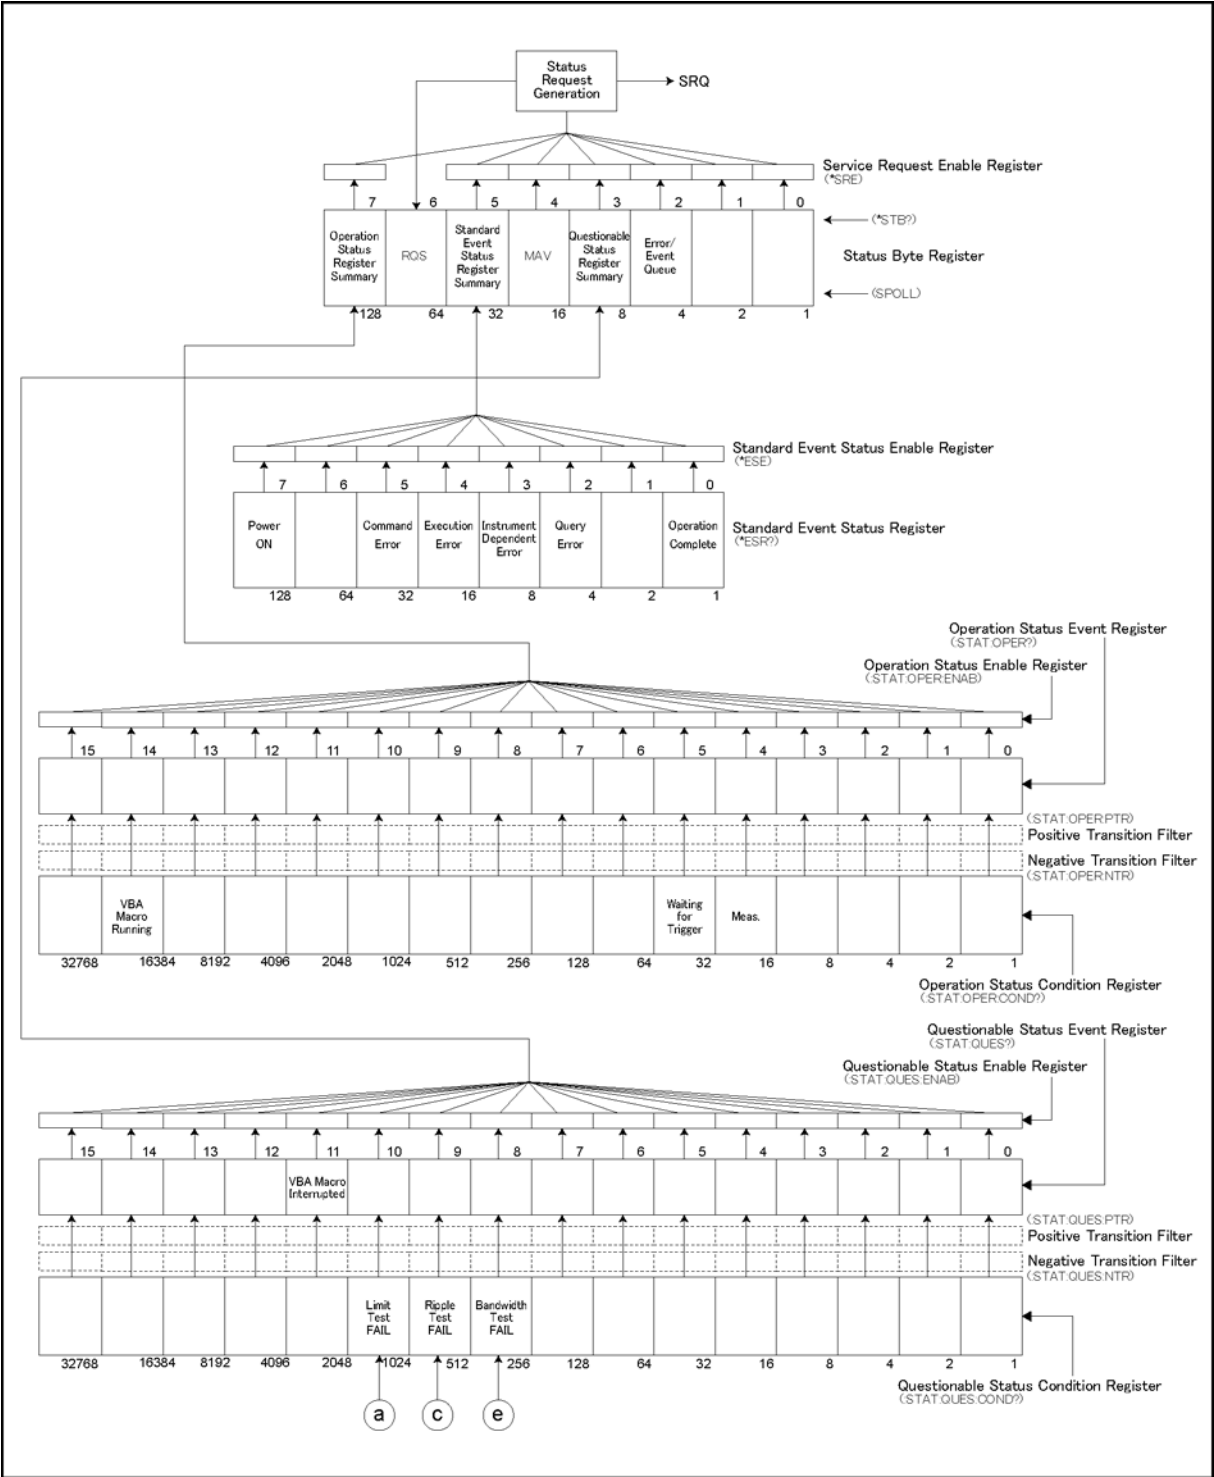


e5061ape3001

Figure B-4 Status Register Structure (2 of 7)

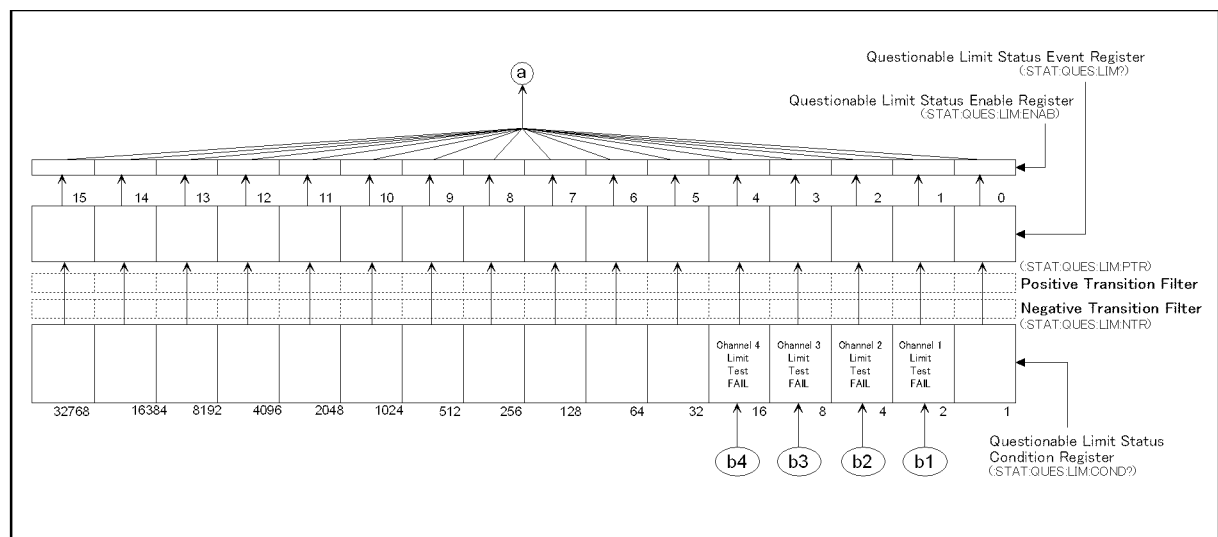

e5061ape0405


Figure B-5 Status Register Structure (3 of 7)

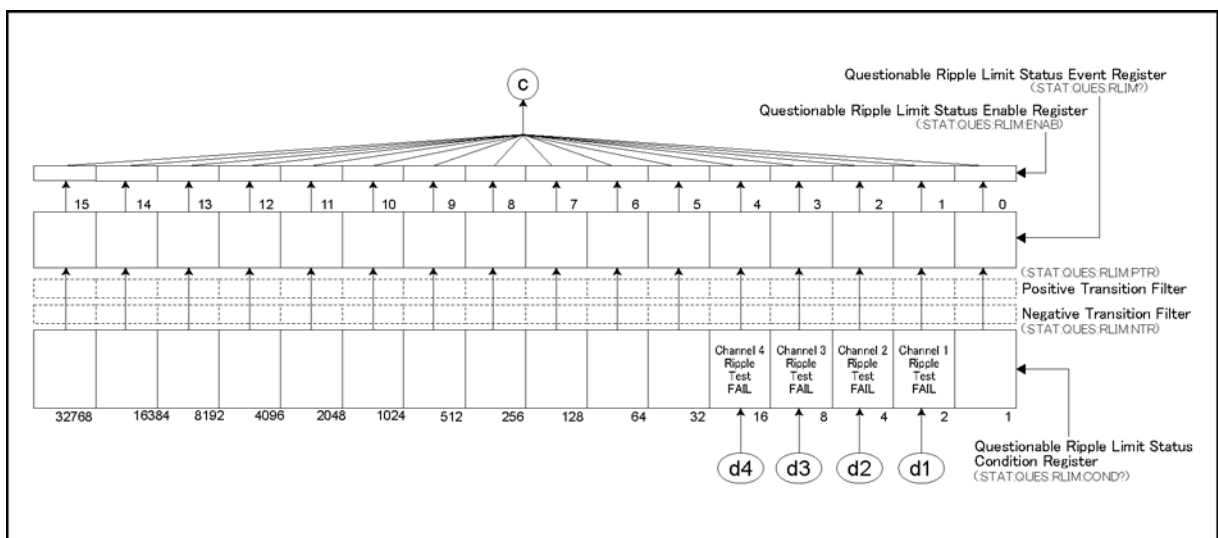

e5061ape3002


Status Reporting System
Status Register Structure

Figure B-6 Status Register Structure (4 of 7)

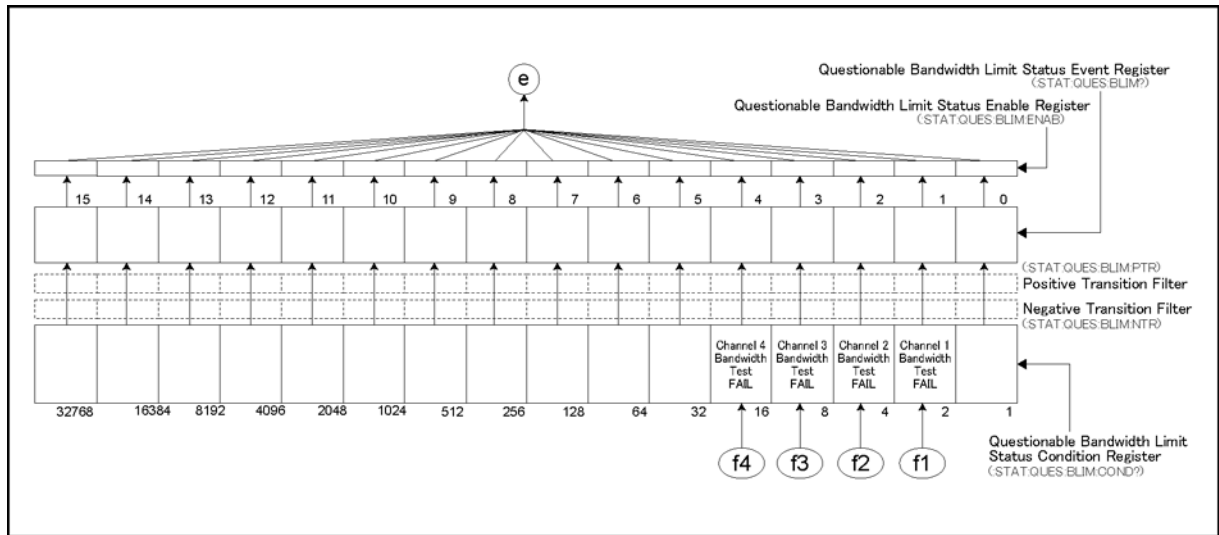

e5061ape3003


Figure B-7 Status Register Structure (5 of 7)

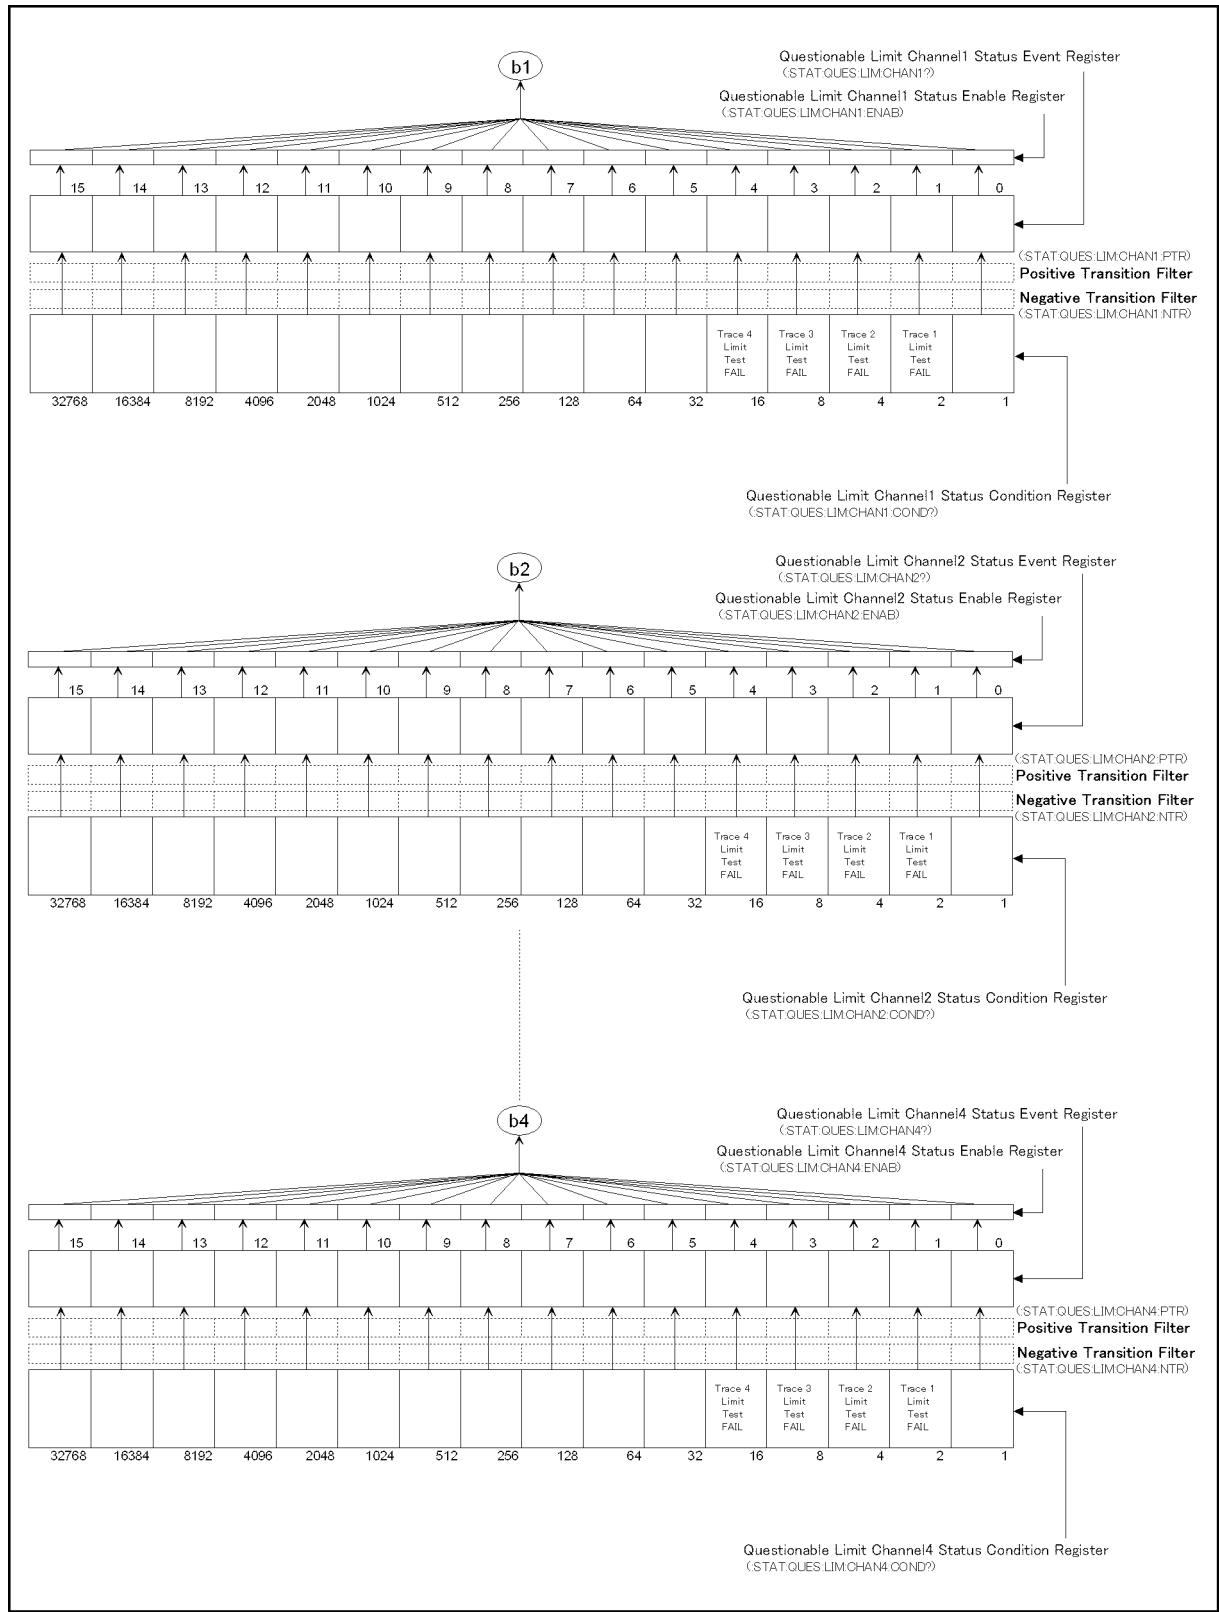

e5061ape0406


Status Reporting System
Status Register Structure

Figure B-8 Status Register Structure (6 of 7)

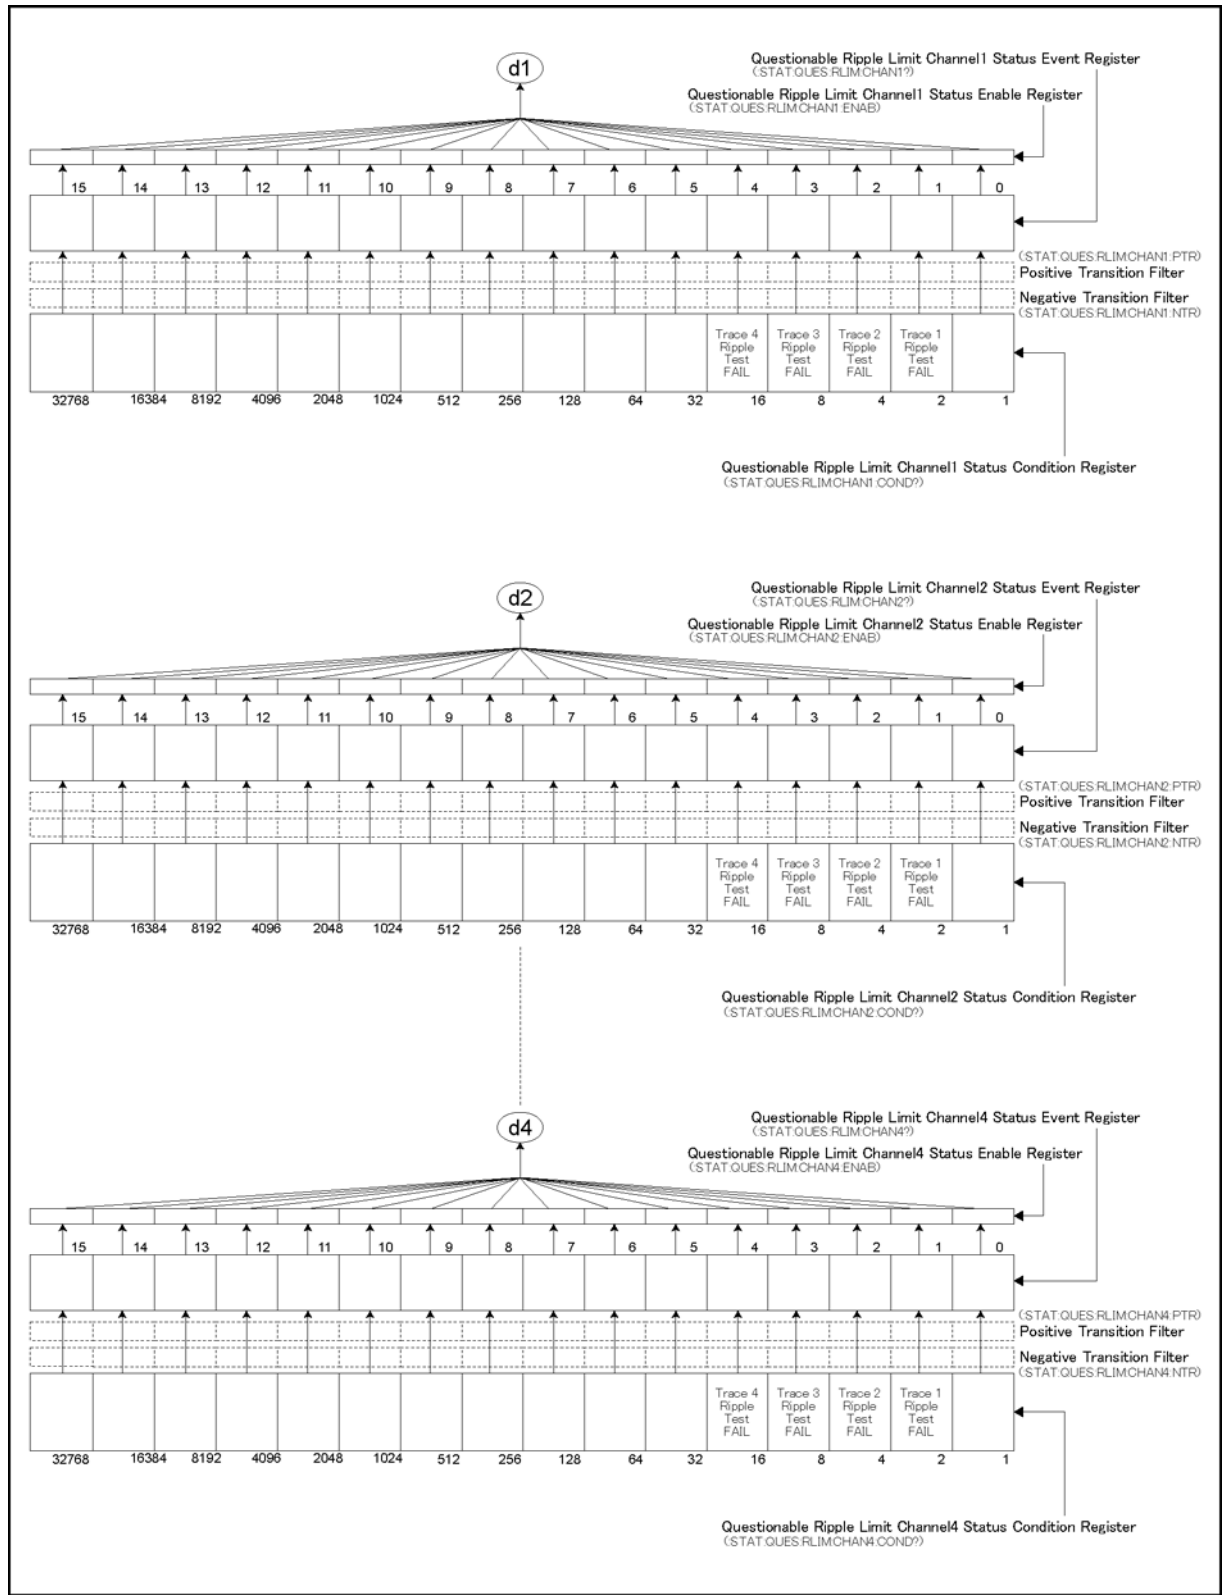

e5061ape3004

Figure B-9 Status Register Structure (7 of 7)

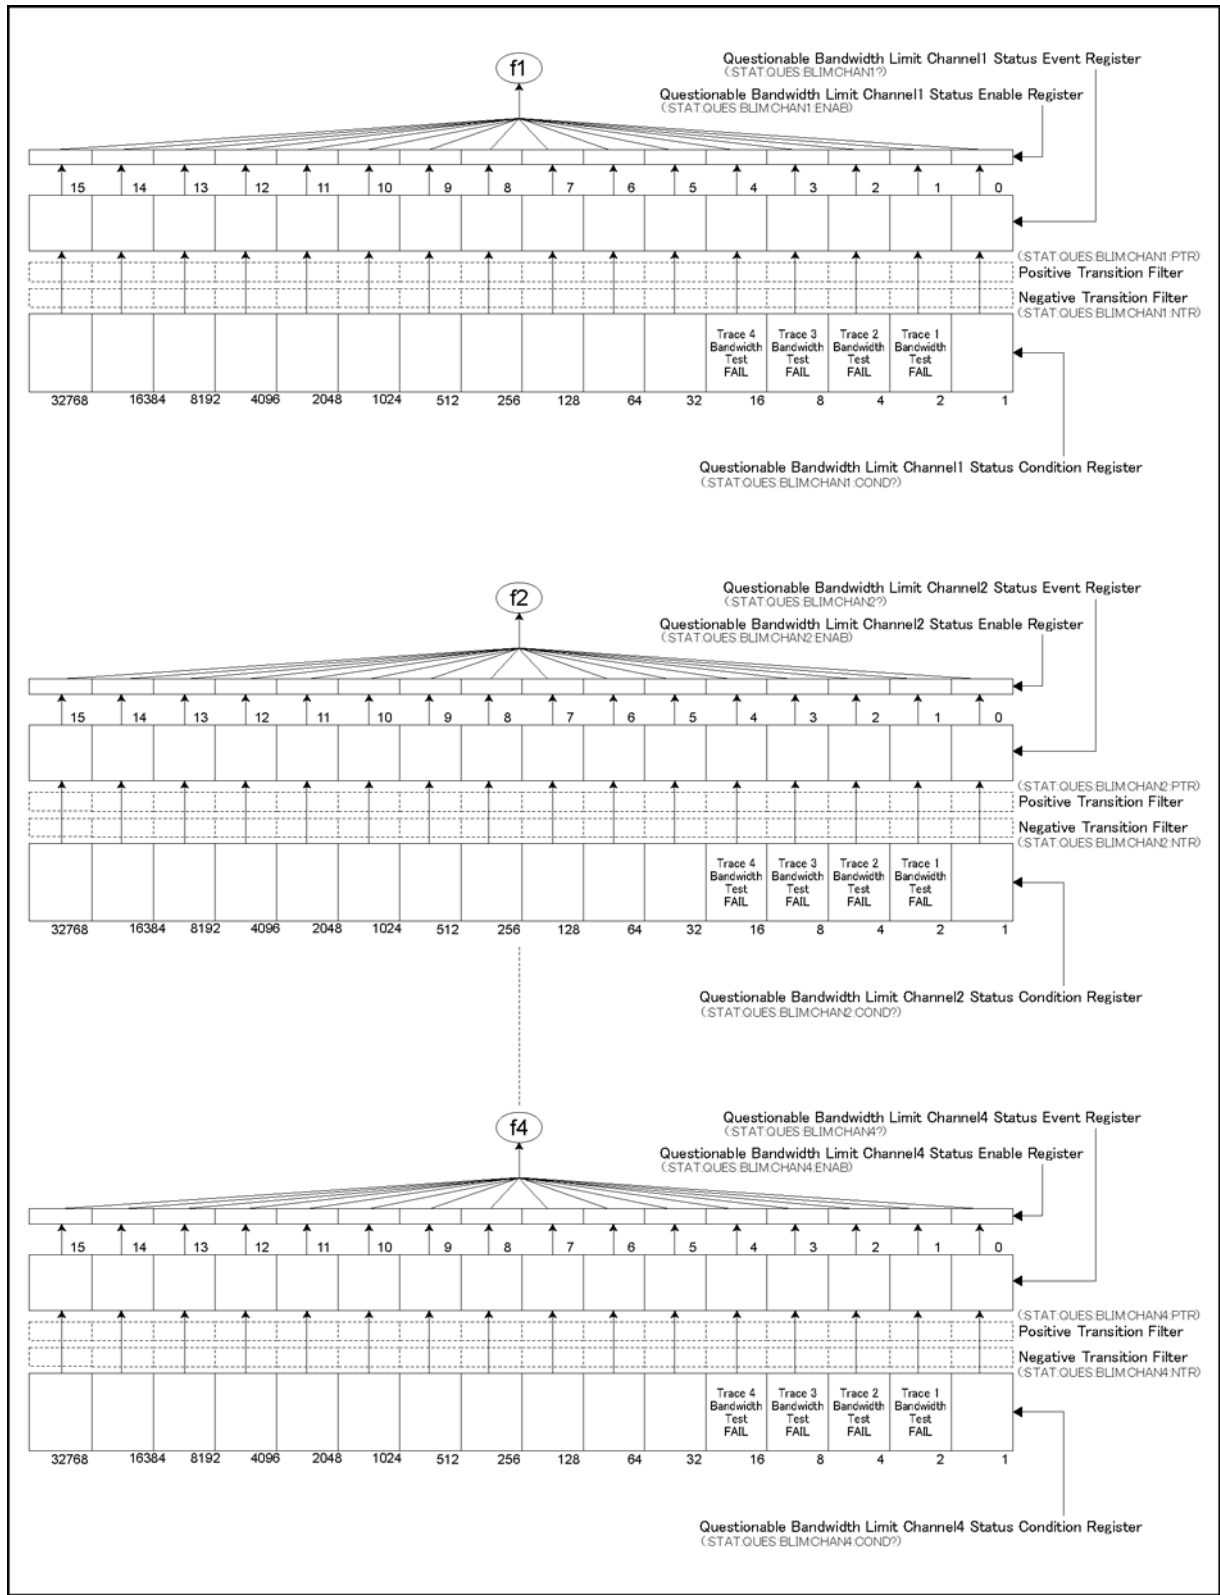

e5061ape3005

Table B-1

Status Bit Definitions of Status Byte Register

Bit Position	Name	Description
0, 1	Not used	Always 0
2	Error/Event Queue	Set to “1” if the error/event queue contains data; reset to “0” when all the data has been retrieved.
3	Questionable Status Register Summary	Set to “1” when one of the enabled bits in the status event status register is set to “1.”
4	MAV (Message Available)	Set to “1” when the output queue contains data; reset to “0” when all the data has been retrieved.
5	Standard Event Status Register Summary	Set to “1” when one of the enabled bits in the status event status register is set to “1.”
6	RQS	Set to “1” when any of the status byte register bits enabled by the service request enable register is set to “1”; reset to “0” when all the data has been retrieved through serial polling.
7	Operation Status Register Summary	Set to “1” when one of the enabled bits in the operational status register is set to “1.”

Issuing the ***CLS** command will clear all bits from the status byte register.

Table B-2

Status Bit Definitions of Event Status Register (ESR)

Bit Position	Name	Description
0	Operation Complete	Set to “1” upon completion of all operations done by commands that precede the *OPC? command on page 198 command.
1	Not used	Always 0
2	Query Error	- Set to “1” when the E5061A/E5062A receives a data output request but there is no data to output. - Set to “1” when the data of the E5061A/E5062A’s output queue has been cleared because of a new message received before the completion of data output.
3	Instrument Dependent Error	Set to “1” when an error has occurred and the error is not a command, query, or execution error.
4	Execution Error	- Set to “1” when any parameter in an SCPI command exceeds its input range or is inconsistent with the E5061A/E5062A’s capabilities. - Set to “1” when an SCPI command cannot be properly executed due to some condition of the E5061A/E5062A.
5	Command Error	- Set to “1” when an IEEE 488.2 syntax error occurs (a command sent to the E5061A/E5062A does not follow the IEEE 488.2 syntax). Possible violations include the command parameter violating the E5061A/E5062A listening formats or being unacceptable. - Set to “1” when a semantic error occurs. Possible causes include a command containing misspellings being sent to the E5061A/E5062A or an IEEE 488.2 command not supported by the E5061A/E5062A being sent. - Set to “1” when GET (Group Execution Trigger) is input while a program message is being received.
6	Not used	Always 0
7	Power ON	Set to “1” when the E5061A/E5062A is powered ON, or when the firmware is restarted.

Issuing the *CLS command will clear all bits from the standard event status register.

Table B-3

Status Bit Definitions of the Operation Status Condition Register

Bit Position	Name	Description
0 - 3	Not used	Always 0
4	Measurement	Set to “1” during measurement ^{*1} .
5	Waiting for Trigger	Set to “1” while the instrument is waiting for a trigger ^{*2} .
6 - 13	Not used	Always 0
14	VBA Macro Running	Set to “1” while a VBA macro is running.
15	Not used	Always 0

*1. This is the time from the beginning of the first sweep to the end of the last sweep when several sweeps are executed for one measurement.

*2. This is when the trigger system is in “Waiting for Trigger” state. For more information on the trigger system, refer to “Trigger system” on page 80.

Issuing the ***CLS** command will clear all bits from the operation status event register.

Table B-4

Status Bit Definitions of the Questionable Status Condition Register

Bit Position	Name	Description
0 - 7	Not used	Always 0
8	Bandwidth Test Fail (Questionable bandwidth limit status register summary)	Set to “1” while one of the enabled bits in the questionable bandwidth limit status event register is set to “1.”
9	Ripple Test Fail (Questionable ripple limit status register summary)	Set to “1” while one of the enabled bits in the questionable ripple limit status event register is set to “1.”
10	Limit Test Fail (Questionable limit status register summary)	Set to “1” while one of the enabled bits in the questionable limit status event register is set to “1.”
11 - 15	Not used	Always 0

Table B-5

Status Bit Definitions of the Questionable Status Event Register

Bit Position	Name	Description
0 - 7	Not used	Always 0
8	Bandwidth Test Fail (Questionable bandwidth limit status register summary)	Set to "1" when a transition of the condition register occurs if the transition filters are set as valid values.
9	Ripple Test Fail (Questionable ripple limit status register summary)	Set to "1" when a transition of the condition register occurs if the transition filters are set as valid values.
10	Limit Test Fail (Questionable limit status register summary)	Set to "1" when a transition of the condition register occurs if the transition filters are set as valid values.
11	VBA Macro Interrupted	Set to "1" when a VBA macro is interrupted by one of the following reasons. ^{*1} • Occurrence of an execution error • Executing "End" statement in the VBA Macro • Executing :PROG:STAT STOP • Operating [Ctrl]+[Break] using the keyboard • Operating [Macro Break] or [Macro Setup] - Stop using the front panel
12 - 15	Not used	Always 0

^{*1}. This setting is made after you click the **End** button in the dialog box displayed when the VBA macro is interrupted.

Issuing the ***CLS** command will clear all bits from the questionable status event register.

Table B-6 **Status Bit Definitions of the Questionable Limit Status Condition Register**

Bit Position	Name	Description
0	Not used	Always 0
1	Channel 1 Limit Test Fail (questionable limit channel 1 status register summary)	Set to “1” while one of the enabled bits in the questionable limit channel 1 status event register is set to “1.”
2	Channel 2 Limit Test Fail (questionable limit channel 2 status register summary)	Set to “1” while one of the enabled bits in the questionable limit channel 2 status event register is set to “1.”
3	Channel 3 Limit Test Fail (questionable limit channel 3 status register summary)	Set to “1” while one of the enabled bits in the questionable limit channel 3 status event register is set to “1.”
4	Channel 4 Limit Test Fail (questionable limit channel 4 status register summary)	Set to “1” while one of the enabled bits in the questionable limit channel 4 status event register is set to “1.”
5-15	Not used	Always 0

Issuing the ***CLS** command will clear all bits from the questionable bandwidth limit status event register.

Table B-7 **Status Bit Definitions of the Questionable Limit Channel {1-4} Status Condition Register**

Bit Position	Name	Description
0	Not used	Always 0
1	Trace 1 Limit Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the limit test result for trace 1.
2	Trace 2 Limit Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the limit test result for trace 2.
3	Trace 3 Limit Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the limit test result for trace 3.
4	Trace 4 Limit Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the limit test result for trace 4.
5-15	Not used	Always 0

Issuing the ***CLS** command will clear all the bits in the questionable limit channel {1-4} status event register.

Table B-8 **Status Bit Definitions of the Questionable Bandwidth Limit Status Condition Register**

Bit Position	Name	Description
0	Not used	Always 0
1	Channel 1 Bandwidth Test Fail (questionable bandwidth limit channel 1 status register summary)	Set to “1” while one of the enabled bits in the questionable bandwidth limit channel 1 status event register is set to “1.”
2	Channel 2 Bandwidth Test Fail (questionable bandwidth limit channel 2 status register summary)	Set to “1” while one of the enabled bits in the questionable bandwidth limit channel 2 status event register is set to “1.”
3	Channel 3 Bandwidth Test Fail (questionable bandwidth limit channel 3 status register summary)	Set to “1” while one of the enabled bits in the questionable bandwidth limit channel 3 status event register is set to “1.”
4	Channel 4 Bandwidth Test Fail (questionable bandwidth limit channel 4 status register summary)	Set to “1” while one of the enabled bits in the questionable bandwidth limit channel 4 status event register is set to “1.”
5-15	Not used	Always 0

Issuing the ***CLS** command will clear all bits from the questionable bandwidth limit status event register.

Table B-9 **Status Bit Definitions of the Questionable Bandwidth Limit Channel {1-4} Status Condition Register**

Bit Position	Name	Description
0	Not used	Always 0
1	Trace 1 Bandwidth Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the bandwidth test result for trace 1.
2	Trace 2 Bandwidth Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the bandwidth test result for trace 2.
3	Trace 3 Bandwidth Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the bandwidth test result for trace 3.
4	Trace 4 Bandwidth Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the bandwidth test result for trace 4.
5-15	Not used	Always 0

Issuing the ***CLS** command will clear all the bits in the questionable bandwidth limit channel {1-4} status event register.

Table B-10

Status Bit Definitions of the Questionable Ripple Limit Status Condition Register

Bit Position	Name	Description
0	Not used	Always 0
1	Channel 1 Ripple Test Fail (questionable ripple limit channel 1 status register summary)	Set to “1” while one of the enabled bits in the questionable ripple limit channel 1 status event register is set to “1.”
2	Channel 2 Ripple Test Fail (questionable ripple limit channel 2 status register summary)	Set to “1” while one of the enabled bits in the questionable ripple limit channel 2 status event register is set to “1.”
3	Channel 3 Ripple Test Fail (questionable ripple limit channel 3 status register summary)	Set to “1” while one of the enabled bits in the questionable ripple limit channel 3 status event register is set to “1.”
4	Channel 4 Ripple Test Fail (questionable ripple limit channel 4 status register summary)	Set to “1” while one of the enabled bits in the questionable ripple limit channel 4 status event register is set to “1.”
5-15	Not used	Always 0

Issuing the ***CLS** command will clear all bits from the questionable ripple limit status event register.

Table B-11

Status Bit Definitions of the Questionable Ripple Limit Channel {1-4} Status Condition Register

Bit Position	Name	Description
0	Not used	Always 0
1	Trace 1 Ripple Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the ripple test result for trace 1.
2	Trace 2 Ripple Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the ripple test result for trace 2.
3	Trace 3 Ripple Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the ripple test result for trace 3.
4	Trace 4 Ripple Test Fail	Set to “0” when a measurement cycle begins; set to “1” when the measurement cycle finishes and returns “fail” as the ripple test result for trace 4.
5-15	Not used	Always 0

Issuing the ***CLS** command will clear all the bits in the questionable ripple limit channel {1-4} status event register.

Using the Status Reporting System

You can manage the status report system using the following commands in any combination:

- *CLS on page 196
- *SRE on page 200
- *STB? on page 201
- *ESE on page 197
- *ESR? on page 197
- :STAT:PRES on page 445
- :STAT:OPER:ENAB on page 442
- :STAT:OPER:COND? on page 441
- :STAT:OPER? on page 441
- :STAT:OPER:PTR on page 444
- :STAT:OPER:NTR on page 443
- :STAT:QUES:ENAB on page 454
- :STAT:QUES:COND? on page 453
- :STAT:QUES? on page 445
- :STAT:QUES:PTR on page 464
- :STAT:QUES:NTR on page 463
- :STAT:QUES:LIM:ENAB on page 460
- :STAT:QUES:LIM:COND? on page 459
- :STAT:QUES:LIM? on page 455
- :STAT:QUES:LIM:PTR on page 462
- :STAT:QUES:LIM:NTR on page 461
- :STAT:QUES:LIM:CHAN{1-4}:ENAB on page 456
- :STAT:QUES:LIM:CHAN{1-4}:COND? on page 455
- :STAT:QUES:LIM:CHAN{1-4}? on page 455
- :STAT:QUES:LIM:CHAN{1-4}:PTR on page 458
- :STAT:QUES:LIM:CHAN{1-4}:NTR on page 457
- :STAT:QUES:BLIM? on page 445
- :STAT:QUES:BLIM:CHAN{1-4}? on page 446
- :STAT:QUES:BLIM:CHAN{1-4}:COND? on page 446
- :STAT:QUES:BLIM:CHAN{1-4}:ENAB on page 447
- :STAT:QUES:BLIM:CHAN{1-4}:NTR on page 448
- :STAT:QUES:BLIM:CHAN{1-4}:PTR on page 449
- :STAT:QUES:BLIM:COND? on page 449
- :STAT:QUES:BLIM:ENAB on page 450
- :STAT:QUES:BLIM:NTR on page 451
- :STAT:QUES:BLIM:PTR on page 452
- :STAT:QUES:RLIM? on page 465
- :STAT:QUES:RLIM:CHAN{1-4}? on page 465
- :STAT:QUES:RLIM:CHAN{1-4}:COND? on page 465
- :STAT:QUES:RLIM:CHAN{1-4}:ENAB on page 466
- :STAT:QUES:RLIM:CHAN{1-4}:NTR on page 467
- :STAT:QUES:RLIM:CHAN{1-4}:PTR on page 468
- :STAT:QUES:RLIM:COND? on page 468
- :STAT:QUES:RLIM:ENAB on page 469
- :STAT:QUES:RLIM:NTR on page 470
- :STAT:QUES:RLIM:PTR on page 471

Status Reporting System

Using the Status Reporting System

For sample programs that demonstrate the use of the commands listed above, refer to “Using the Status Register” on page 84 in Chapter 5 or “Obtaining Test Results” on page 121 in Chapter 8.

C Error Messages

The Agilent E5061A/E5062A provides error messages to indicate its operating status. This appendix describes the error messages of the E5061A/E5062A in order of error number.

Error Messages

An error message is displayed against a red background in the instrument message/warning area in the lower left part of the screen. Pushing a front panel key or executing **:DISP:CCL** command clears the error message. Errors caused by the operation of a front panel key simply appear on the display. They are not stored in the error queue with some exceptions.

An error with a positive error number is one uniquely defined for this instrument. On the other hand, an error with a negative error number is basically one defined for common GPIB devices in IEEE488.2

A

20

Additional standard needed

The GPIB command that turns ON the calibration function has been sent before all of the data measurements needed to calculate the calibration factor have been completed. For instance, the "SENS:CORR:COLL:SAVE" command is sent to calculate calibration coefficients and turn on error correction for 1-Port Calibration when open and short calibration are completed but load calibration is not completed. Be sure to measure all necessary calibration data before sending commands. This error is not generated by front key operations.

77

Additional test set calibration needed

Multiport test set calibration needs to be completed. This error occurs when Slef Cal (SENS:CORR:MULT:SELF:ONCE) is performed without having test set calibration completed.

B

-168

Block data not allowed

An block-data element has been received at a position where this instrument does not accept one.

C

240

Calibration data lost

This error occurs when a file containing the system calibration data is not found or in a damaged state at time of the startup of this instrument, indicating a failure of this instrument. Contact an Agilent Technology sales office or the company from which you bought the instrument.

22

Calibration method not selected

This error occurs when the command for validating the calibration, SENS:CORR:COLL:SAVE, is executed before the command for selecting a calibration type, SENS:CORR:COLL:METH:xxxx, is executed. This error is not generated by front key operations.

-148

Character data not allowed

A character data element (not violating the standard) has been received at a position where

this instrument does not accept one. Double quotes (“”) are omitted where it is necessary to place a parameter in double quotes (“”), for example.

-100

Command error

A comprehensive syntax error has occurred showing that this instrument cannot detect a more detailed error. This code simply shows that a command error defined in 11.5.1.1.4, IEEE488.2 has occurred.

D

-222

Data out of range

A data element (not violating the standard) outside the range defined by this instrument has been received. This error occurs when an integer-based command for which the parameter can be rounded exceeds the range of -65536 to +65536 or when a real-number-based command for which the parameter can be rounded exceeds the range of -9.9e37 to +9.9e37, for example.

This error occurs also when a numeric value other than a specified one is entered into a command in which the “port number” and “CalKit number” are specified as parameters and hence the parameters are not rounded. Such commands are, for example, SENS:CORR:COLL:ACQ:OPEN, SENS:CORR:COLL:ECAL:SOLT1, SENS:CORR:COLL:CKIT:ORD:LOAD, etc.

-104

Data type error

The parser has recognized a data element that must not exist. Block data has been sent instead of numeric value data or character string data that had been expected, for example.

E

32

Ecal module not in appropriate RF path

This error occurs when an ECal command, SENS:CORR:COLL:ECAL:SOLTn, is executed with the port on the ECal module not connected correctly to the instrument.

-200

Execution error

An error associated with execution has been generated for which this instrument cannot specify the error message. This code shows that an error associated with execution defined in 11.5.1.1.5, IEEE488.2 has occurred. This error occurs also when a calibration measurement is aborted.

-123

Exponent too large

The absolute value of the exponent exceeds 32,000 (see 7.7.2.4.1, IEEE488.2).

-178

Expression data not allowed

An expression-data element has been received at a position where this instrument does not accept one.

-170

Expression error

When the expression data is put to syntactic analysis, an error not corresponding to one of Error Numbers -171 through -179 occurs.

F

31	Failed to configure ECal module This error occurs when the control of the ECal module fails at time of executing an ECal command, SENS:CORR:COLL:ECAL:SOLTn. The failure results from the failure to connect the ECal module to the USB port, failure of the ECal module, etc.
76	Failed to configure multiport test set This error occurs when multiport test set control is enabled (SENS:MULT ON) and the analyzer fails to control the test set. Make sure the analyzer and the test set are connected with the parallel cable, and the test set is powered on.
102	Failed to copy file This error occurs when copying a file (MMEM:COPY command) fails.
104	Failed to create directory This error occurs when creating a directory (MMEM:MDIR command) fails.
103	Failed to delete file This error occurs when deleting a file (MMEM:DEL command) fails.
100	Failed to read file This error occurs when a 2-port touchstone file (CALC:FSIM:SEND:PMC:PORT:USER:FIL command), the formatted data array (MMEM:LOAD:FDAT command) and limit table (MMEM:STOR:LIM command) for the active trace on the active channel, segment sweep table (MMEM:LOAD:SEGM command) for the active channel, a VBA project file (MMEM:LOAD:PROG command), etc. cannot be read normally.
101	Failed to write file This error occurs when the formatted data array (MMEM:STOR:FDATcommand) and limit table (MMEM:STOR:LIM command) for the active trace on the active channel, segment sweep table (MMEM:STOR:SEGM command) for the active channel, display image (MMEM:STOR:IMAG command) for the LCD screen, a VBA project file (MMEM:STOR:PROG command), etc. cannot be written normally.
54	Fault location not allowed This error occurs when the fault location function is enabled when the sweep type is not set to linear or the number of measurement points is two. The fault location function is available only when linear sweep with more than two measurement points.
-257	File name error A file name error. This message appears when an error exists in the file name and hence a command is not executed correctly. This error occurs when you try to copy to an unsuitable file name, for example.
-256	File name not found The file name specified is not found and hence the command is not executed correctly. This error occurs when you try to read a file that does not exist in a disk or a disk is not correctly inserted into the drive to read or write a file, for example.
107	File transfer failed This error occurs when writing data into or reading data from a file (MMEM:TRAN

command) fails.

G

-105 **GET not allowed**

A group execution trigger (GET) has been received in the program message (see 7.7, IEEE488.2).

H

-114 **Header suffix out of range**

The unit of the header is outside the range. The header is invalid in the unit for numeric parameters following a SCPI command.

I

-224 **Illegal parameter value**

The parameter value is not suitable. This error occurs when the CALC:PAR:DEF command is used to specify an S-parameter that does not exist in the model.

-282 **Illegal program name**

This error occurs when a nonexistent VBA program name is specified by the PROG:SEL:NAME command.

-213 **Init ignored**

Because another measurement is in progress, the request for initiating a measurement ("INIT" command) is ignored.

-161 **Invalid block data**

Block data has been expected, but the block data that appears is invalid for some reason (see 7.7.6.2, IEEE488.2). The END message is received before the length of block data has been filled, for example.

-101 **Invalid character**

An invalid character exists in the program message character string.

-141 **Invalid character data**

An invalid character is found in the character data element, or the parameter received is not valid.

-121 **Invalid character in number**

A character that is invalid for the data type subject to syntactic analysis has been received. For example, a letter is found in a decimal numeric value or a numeric character "9" in octal data.

-171 **Invalid expression**

The expression-data element is invalid (see 7.7.7.2, IEEE488.2). Parentheses are not paired, or illegal characters are used, for example.

-103 **Invalid separator**

The parser (a syntactic analysis program) had been expecting a delimiter, but a character

Error Messages

Error number: -151

that is not a delimiter has been sent.

-151

Invalid string data

Character string data has been expected, but the character string data that appears is invalid for some reason (see 7.7.5.2, IEEE488.2). The END message is received before the ending quotation mark character appears, for example.

-131

Invalid suffix

The suffix does not comply with the syntax defined in 7.7.3.2, IEEE488.2. Or it does not suit 4294A.

L

53

Log sweep requires 2 octave minimum span

The span of sweep range is not satisfied the requirement for logarithmic sweep. The sweep type is automatically changed to linear sweep when this error occurs.

For example, this error occurs when, with the start and stop frequency are set 1 MHz and 2 MHz respectively, the sweep type is changed to logarithmic sweep.

Set the stop frequency to more than four times as many as the start frequency. And then select logarithmic sweep.

M

-109

Missing parameter

The number of parameters is less than that required for the command, or the parameter has not been entered. For example, the command SENS{1-4}:SWE:POIN requires one more parameter.

Therefore, when a message “SENS1:SWE:POIN” is sent to a correct program message “SENS1:SWE:POIN 201” this instrument receives the former message as an invalid one because all parameters have not been entered. Enter command parameters correctly.

75

Multiport test set not enabled

This error occurs when multiport test set calibration is performed while test set control is not enabled.

N

56

Not enough points for connector model

This error occurs when the connector measurement function of the SRL measurement is performed with the number of measurement points less than 101. Use at least 101 points.

52

No valid memory trace

This error occurs when there is no valide memory trace data and :DISP: WIND:TRAC:MEM ON or DISP:WIND:TRAC:STAT ON is received or parameters other than “NORM” is set with CALC:MATH:FUNC.

-120

Numeric data error

An error resulting from the numeric value data (including numeric value data having no

	decimal point representation) has occurred. A numeric value error other than Errors -121 through -129 has occurred.
-128	Numeric data not allowed An numeric-value-data element (not violating the standard) has been received at a position where this instrument does not accept one.
	O
200	Option not installed The command received has been ignored because of the mismatch between the contents of an option for this instrument and the command. For example, this error occurs when the source attenuator (power range) is set at a value other than zero (SOUR:POW:ATT command) in a model not having the extended power output option. This error is not generated by front key operations.
-225	Out of memory Insufficient memory is available in this instrument to perform the required operation.
	P
-220	Parameter error When a parameter-related error other than Errors -221 through -229 occurs, that error is displayed.
-108	Parameter not allowed The number of parameters exceeds that required for the command. For instance, when a program message “:SENS1:SWE:TYPE LIN, SEGM” is sent instead of a correct program message with a command “:SENS1:SWE:TYPE LIN” which requires a parameter, the instrument receives the message as the number of parameters is invalid. See the command reference to confirm the required number of parameters.
41	Peak not found This error occurs when, after specifying a peak and executing the CALC:MARK:FUNC:EXEC and CALC:FUNC:EXEC commands, the specified peak is not found in the marker search analysis.
220	Phase lock loop unlocked This error occurs when the PLL circuit of this instrument becomes unlocked while the measurement is in progress. The measurement value is not correct. This error may occur when an external reference out of specification is connected to this instrument. Should an error occur with an external reference not connected, this instrument is faulty. Contact an Agilent Technology sales office or the company from which you bought the instrument.
221	Port 1 receiver overload The input to Test Port 1 exceeds the maximum input level. The measurement value is not correct. When a DUT is an amplifier or the like, this error may occur, damaging the receiver in the worst case. Should this error occur with a passive part used as the DUT or with nothing connected to the test port, this instrument is faulty. Contact an Agilent

Technology sales office or the company from which you bought the instrument.

If this error occurs, the stimulus signal output is automatically turned to off.

222

Port 2 receiver overload

The input to Test Port 2 exceeds the maximum input level. The measurement value is not correct. When a DUT is an amplifier or the like, this error may occur, damaging the receiver in the worst case. Should this error occur with a passive part used as the DUT or with nothing connected to the test port, this instrument is faulty. Contact an Agilent Technology sales office or the company from which you bought the instrument.

If this error occurs, the stimulus signal output is automatically turned to off.

241

Power on test failed

This error occurs when the power-on test fails, indicating a failure of this instrument. Contact an Agilent Technology sales office or the company from which you bought the instrument.

61

Power unlevelled

The out power level exceeds available range.

For example, if the level after correction exceeds the power level that can be outputted when correcting the power level with the power slope feature, this error occurs.

Check that the power level is set correctly, and the correction value of the power slope is set correctly.

120

Printer error

This error occurs when the previous printing is still in progress or the printer fails (offline, short of paper, etc.) at time of outputting the display image on the LCD screen to the printer (HCOP:IMM command).

121

Print failed

This error occurs when printing fails for reasons other than Error 120, Printer error.

-284

Program currently running

This error occurs when the PROG:SEL:STAT RUN command is executed with the VBA program in the Run state.

-112

Program mnemonic too long

The length of the header exceeds 12 characters (see 7.6.1.4.1, IEEE488.2).

-286

Program runtime error

An error occurring when VBA is executed.

Q

-430

Query DEADLOCKED

The state that generates a “DEADLOCKED” Query error (see 6.3.1.7, IEEE488.2). This error occurs when both input and output buffers have become full, preventing the instrument from continuing processing, for example.

-400

Query error

A comprehensive query error has occurred showing that this instrument cannot detect a

	more detailed error. This code simply shows that a query error defined in 11.5.1.1.7 and 6.3, IEEE488.2 has occurred.
-410	Query INTERRUPTED The state that generates a “INTERRUPTED” Query error (see 6.3.2.3, IEEE488.1). This error occurs when data bytes (DAB) or GET are received before the transmission of the response after a query has not been completed, for example.
-420	Query UNTERMINATED The state that generates an “UNTERMINATED” Query error (see 6.3.2, IEEE488.2). This error occurs when this instrument is designated as the talker and an incomplete program message is received, for example.
-440	Query UNTERMINATED after indefinite response After a query asking for an indefinite response has been run, another query is received in the same program message (See 6.5.7.5.7, IEEE488.2).
	R
105	Recall failed This error occurs when reading an instrument status file (State01.sta, etc.) (MMEM:LOAD:STAT command) fails.
	S
106	Save failed This error occurs when writing an instrument status file (State01.sta, etc.) (MMEM:STOR:STAT command) fails.
50	Specified channel hidden This error occurs when an attempt is made to activate a channel not on display using the DISP:WIND:ACT command. This error is not generated by front key operations.
23	Specified error term dose not exist
21	Specified ports overlapped This error occurs when a port number is duplicated in a command requiring two or more port numbers as parameters. Specify port setup correctly to avoid duplication of ports. This error is not generated by front key operations.
51	Specified trace dose not exist
-150	String data error When a character-string-data element is put to syntactic analysis, an error not corresponding to one of Error Numbers -151 through -159 occurs.
-158	String data not allowed A character-string-data element has been received at a position where this instrument does not accept one.

-138	Suffix not allowed A suffix is attached to a numeric value element to which a suffix is not allowed to be attached.
-134	Suffix too long The unit is too long. The unit is expressed in 12 or more characters (see 7.7.3.4, IEEE488.2).
-102	Syntax error A command or data type that is not recognized exists.
-310	System error One of the errors designated as “system errors” in this instrument has occurred.
T	
40	Target value not found This error occurs when the target is not found during the marker search analysis after specifying the target and executing the CALC:MARK:FUNC:EXEC and CALC:FUNC:EXEC commands. This error occurs also when the bandwidth is not found after executing the bandwidth marker command, CALC:MARK:BWID:DATA?
-124	Too many digits The number of digits of the argument of the decimal numeric-value-data element exceeds 255 with the preceding 0 removed (see 7.7.2.4.1, IEEE488.2).
-223	Too much data The block-, expression-, or character-string-type program data that has been received conforms with the standard. But it exceeds the amount that can be processed under the condition of the memory or conditions specific to memory-related devices. In this instrument, this error occurs when the number of characters exceeds 254 in a character-string parameter.
-211	Trigger ignored This instrument receives and detects a trigger command (“TRIG”) or an external trigger signal. But it is ignored due to the timing condition (This instrument is not in the wait-for-trigger state, for example). Change the setup so that a trigger command or an external trigger signal can be sent after the instrument has entered the wait-for-trigger state.
U	
-113	Undefined header A command not defined in this instrument, though not illegal in the syntactic structure, has been received. For example, when a message “:DISP:WIND1:TABL:MEM ON” is sent to a correct program message “:DISP:WIND1:TRAC1:MEM ON,” the message sent is received as an undefined command by this instrument. See the command reference and use correct commands. This error occurs also when a port not existing on this model is specified in a command specifying a port number as an index. Such commands are CALC:FSIM:SEND:DEEM:PORTn:xxxx, CALC:FSIM:SEND:PMC:PORTn:xxxx,

CALC:FSIM:SEND:ZCON:PORTn:Z0:R, and SENS:CORR:EXT:PORTn:TIME; they include PORTn as a part.

Warning Message

A warning message is displayed in the instrument message/Warning area in the lower left part of the display against a gray background. Pushing a front panel key or executing **:DISP:CCL** command clears the message.

This message simply appears on the display, being not known to a remote environment such as a GPIB. This message is not displayed when another error (against a red background) has already been displayed in the instrument message/Warning area.

The warning messages for this instrument are as follows:

Cable Z out of range

This error occurs in SRL measurement function when measured average impedance is out of the tolerance (system impedance $\pm 30\%$), and the SRL calculation is not valid.

Fault location not allowed

This warning message is displayed when the gating/transform function of time domain function is turned on, number of points is set 2 or sweep type is set logarithmic/segment sweep.

The gating function and transform function are automatically turned off when this warning message is displayed.

Log sweep requires 2 octave minimum span

If you change the sweep range that does not satisfy the necessary condition of the frequency span (the stop frequency is about 4 times or more of the start frequency) when the sweep type is set to the log sweep, this message is displayed.

If this message is displayed, the sweep type is automatically set to the linear sweep.

For example, if you attempt to change the log type to the log sweep when the start frequency is set to 1 MHz and the stop frequency to 2 MHz, this error occurs.

Set the stop frequency to a value of about 4 times or more the start frequency and then set the low sweep.

Peak not found

This warning message is displayed when, with the tracking turned on, the peak specified by the marker search has not been found by the time the sweep is finished (with the tracking executed).

Segment table changed

This warning message is displayed when the setting specified segment by segment in the segment table is automatically changed by a change in the other setting.

For example, this warning message is displayed when, with the power specified segment by segment in the segment table, the power setting for a segment is adjusted by a change in the power range setting.

Target value not found

This warning message is displayed when, with the tracking turned on, the target specified by the marker search has not been found by the time the sweep is finished (with the tracking executed).

This warning message is displayed also when, with the bandwidth marker displayed, the setting for the bandwidth marker is changed at the end of the sweep, or when, with the

active marker changed or moved, the bandwidth is not found.

User Preset File not found

This warning message is displayed if no user preset file (D:\UserPreset.sta) exists when executing the **:SYST:UPR** command.

If this message is displayed, a normal preset (**:SYST:PRES**) will be performed.

Error Messages
Error number:

Numerics

24-bit I/O port, 148

A

A:, 132

Active channel, 40

Active low, 149

Active trace, 40

Address

 GPIB address, 26

 IP address, 27

 SICL-LAN address, 28

Agilent I/O Libraries, 28

Allocation, 44

Analog measurement, 150

Analysis command, 93

Analysis results, 94

Analysis(search) range, 93

Analysis(search) type

 Analysis command, 93

Aperture

 Smoothing aperture, 47

Application Programs, 169

Arbitrary impedance, 64

ASCII transfer format, 105

Auto recall, 132

Auto scale, 48

autorec.sta, 132

Average

 Analysis command, 93

 Statistical analysis, 100

Averaging, 43

B

bandwid.htb, 98

Bandwidth, 42

Bandwidth definition value, 97

Bandwidth search, 97

Basic measurement

 Sample program, 170

Beeper

 Generates a beep

 Completion of the operation, 473

 Notification of warning/limit test result, 474

 Turns on/off

 Completion of the operation, 473

 Notification of warning/limit test result, 474

Binary transfer format

 byte order, 107

 format, 106

Bit definitions

 Operation status register, 518

 Questionable limit channel{1-4} status register, 520, 521, 522

 Questionable limit status register, 520

 Questionable status register, 518

 Standard event status register, 517

 Status byte register, 516

Bitmap, 133

Bus trigger, 81

Byte order, 107

C

C0, 64

C1, 64

C2, 64

C3, 64

cal.htb, 71

Calibration

 Sample program, 67

Calibration coefficient arrays, 110

 Saving/recalling, 132

Calibration coefficients

 Calculating, 62

Calibration data, 60

Calibration Kit, 60, 64

Calibration kit name, 64

Calibration property, 411

Calibration type

 Checking the applied calibration type, 63

 Selecting, 60

Center frequency

 Bandwidth search, 97

 Notch search, 99

Center value

 Frequency sweep range, 41

 Power sweep range, 43

Channel display, 44

Characteristic impedance, 43

Class assignment, 65

Class Module

 Importing, 134

Clear

 Averaging, 43

 Echo window, 49

 Error message display, 304

 Error queue, 196

 Status registers, 196

Clock

 turning on or off screen display, 49

Command tree, 486

 Concepts, 36

Communication with external instruments, 147

Condition register, 508

cont_upd.htb, 165

Continuous initiation mode, 82

Control over SICL-LAN server, 28

Controlling over LAN

 Using SICL-LAN server, 176

 Using telnet server, 184

Copy

 File, 139

 The data trace to the memory trace, 47

Corrected data arrays, 108
 Saving/recalling, 132
Corrected memory arrays, 108
Creating directory, 139
ctrl_lan.xls, 184
ctrl_lansicl.xls, 176
CW frequency, 43

D

Data arrays
 Corrected, 108
 Formatted, 109
Data flow, 108
Data format, 47
Data math operations, 47
Data trace, 47
Data transfer format, 104
Date display
 On/off, 49
Defining a peak
 Analysis command, 93
 Marker search, 92
Defining a target
 Analysis command, 94
 Marker search, 92
Delay time
 Port extension, 410
 Sweep delay time, 42
Delete, 139
Delta marker(Reference marker), 90
Detecting Occurrence of an Error, 166
Device selector, 26
Difference between the maximum and minimum values
 Analysis command, 93
 Statistical analysis, 100
Directory
 Creating, 139
 Deleting, 139
 Retrieving file property, 139
Disabling the network function, 27
Discrete mode, 267
Display of the calibration property, 411
Display scale, 48
Display update on/off
 screen display, 49
Divisions, 48
documentation map, 4

E

ECal, 63
 Sample program, 75
ecal.htb, 77
Echo window
 printing a message, 49
 Showing/hiding, 46
Electrical Characteristics
 Input signal, 158

 Output signal, 159
 Power supply, 159
Electrical delay time, 213
Electronic calibration, 63
Enable register, 507
Enabling the network function, 27
Equivalent key to SCPI command, 195
Error correction, 62
Error detection, 166
Error message
 Clear, 304
 Reading method, 166
Error Messages, 526
Error queue, 166
 Clear, 196
Event register, 507
Ex_3_1.sta, 52
Ex_4_1.sta, 67
Ex_4_2.sta, 75
Expanded phase format, 47
Extension, 132
External reference signal, 420
External trigger, 81

F

F/W version, 198
Fail display
 Showing/hiding, 120
File
 Copying, 139
 Deleting, 139
 Retrieving file property, 139
 Saving/recalling, 132
 Transferring
 Command, 139
 Sample program, 140
file_sav.htb, 137
file_xfr.htb, 143
Firmware version, 198, 500
Fixed frequency, 43
Flexible disk, 132
Flow
 Data flow, 108
Folder
 Creating, 139
 Deleting, 139
Formatted data arrays, 109
 Saving, 133
Formatted memory arrays, 110
Frequency base, 335
Front panel key
 Equivalent key to SCPI command, 195
Full n-port calibration, 60
Full scale value, 48

G

GPIO, 25

GPIB address, 26
 GPIB remote control system, 25
 Graph
 Layout, 44
 Maximizing, 44
 Graph horizontal axis, 335
 Graticule label, 48
 Group delay format, 47

H

Handler I/O port
 Inputting/outputting data, 152
 Overview, 148
 Pin layout, 149
 Timing chart, 155
 handler.htb, 160
 Hiding frequency labels, 49
 Hold state, 81
 How to use this manual, 20

I

Idle state, 82
 IEEE 32-bit floating point format, 107
 IEEE 64-bit floating point format, 106
 IF bandwidth, 42
 Images on the LCD screen
 Saving, 133
 Imaginary format, 47
 Importing, 134
 INDEX, 150
 Information
 Product information, 198
 Property of file, 139
 Initialization
 Error queue, 196
 Instrument setting, 199, 479, 483
 Status registers, 196
 Initiate state, 82
 Inputting data
 Handler I/O port, 152
 Trace(formatted data array), 115
 Installation and Quick Start Guide, 4
 Instrument status
 Saving/recalling, 132
 Internal clock
 Turning on or off screen display, 49
 Internal data arrays, 108
 Internal data processing, 108
 Internal trigger, 81
 IP address, 27
 Isolation, 60

K

Key lock feature, 162

L

L0, 64
 L1, 64
 L2, 64
 L3, 64
 LAN remote control system, 27
 lim_test.htb, 128
 Limit Lines
 Configuring, 120
 Showing/hiding, 120
 Limit table
 Saving/recalling, 134
 Setting, 120
 Showing/hiding, 46
 Limit test, 119
 Turning on or off, 120
 Limit test result write strobe signal, 151
 Linear magnitude format, 47
 Linear sweep, 41
 List(segment) sweep, 42
 LOAD, 65
 Loading, 134
 Local key, 38
 Logarithmic magnitude format, 47
 Looking up commands, 20
 Loss
 Bandwidth search, 97
 Notch search, 99

M

Macro(VBA)
 Control, 367
 Saving/loading, 134
 Managing Files, 139
 Manual change, 500
 Manual printing history, 2
 Manual trigger, 81
 Manufacture, 198
 Marker
 How to use, 90
 List, 46
 Marker list table, 46
 Marker search, 91
 range, 91
 Math operations, 47
 Maximizing a window and a graph, 44
 Maximum value search
 Analysis command, 93
 Marker search, 91
 meas_bpf.htb, 173
 Measurement data
 Saving, 133
 Measurement parameters, 41
 Measurement state, 82
 Measuring a band pass filter, 170
 Measuring the calibration data, 60
 Memory arrays

-
- Corrected, 108
 - Formatted, 110
 - Memory trace, 47
 - Message terminator, 37
 - Minimum value search
 - Analysis command, 93
 - Marker search, 91
 - Model number, 198
 - N**
 - Name
 - Calibration kit, 64
 - Standard, 64
 - Negative logic, 149
 - Negative transition filter, 508
 - Network function
 - Enabling/disabling, 27
 - Notch search, 99
 - Notch Value, 99
 - Number of measurement points, 42
 - Reading out
 - Linear sweep, 425
 - Segment sweep, 423
 - Number of traces, 41
 - O**
 - Obtaining test results, 121
 - Each channel, 122
 - Each measurement point, 121
 - Each trace, 121
 - Overall test result, 124
 - Offset delay, 64
 - Offset loss, 64
 - Offset Z0, 64
 - OPEN, 65
 - Operation status register, 509
 - Bit definitions, 518
 - Reading out the condition register, 441
 - Reading out the event register, 441
 - Setting the enable register, 442
 - Setting the negative transition filter, 443
 - Setting the positive transition filter, 444
 - Operational Manual, 4
 - Order base, 335
 - Output port write strobe signal, 151
 - Outputting data
 - Handler I/O port, 152
 - Internal data arrays, 111
 - Overall test result, 124
 - P**
 - parameter
 - SCPI command, 195
 - PASS FAIL STROBE, 151
 - Pass/Fail test, 119
 - Peak excursion value, 92, 93
 - Peak search
 - Analysis command, 93
 - Marker search, 91
 - Performing a calibration, 60
 - Phase format, 47
 - Pin layout, 149
 - Polar format, 47
 - Polarity
 - Analysis command, 93
 - Marker search, 92
 - Port
 - Handler I/O port, 152
 - Port 23, 34
 - Port 5025, 35
 - Port extension, 409, 410
 - Positive transition filter, 508
 - Power, 42
 - Power range, 42
 - Power slope, 42
 - Power sweep, 43
 - Prefix, 500
 - Preset, 199, 479, 483
 - Primary value, 109
 - Printer
 - Aborts the print output, 339
 - Outputs the display image, 339
 - Selects the print color, 339
 - Product information, 198
 - Program (sample)
 - file name
 - bandwid.htb, 98
 - cal.htb, 71
 - cont_upd.htb, 165
 - ctrl_lan.xls, 184
 - ctrl_lansicl.xls, 176
 - ecal.htb, 77
 - file_sav.htb, 137
 - file_xfr.htb, 143
 - handler.htb, 160
 - lim_test.htb, 128
 - meas_bpf.htb, 173
 - read_asc.htb, 112
 - read_bin.htb, 114
 - search.htb, 96
 - setup.htb, 56
 - srq_err.htb, 168
 - srq_meas.htb, 86
 - trg_sing.htb, 88
 - write_a.htb, 116
 - write_b.htb, 118
 - title
 - Bandwidth Search, 98
 - Calibration, 71
 - Communicating with external instruments, 160
 - Configuring measurement conditions, 56
 - Controlling the update timing of LCD display, 165
 - Controlling using SICL-LAN server, 176

- Controlling using telnet server, 184
 - ECal, 77
 - Error detection using an SRQ, 168
 - File transfer, 143
 - Limit test, 128
 - Measurement of band pass filter, 173
 - Peak search, 96
 - Saving file, 137
 - Using an SRQ to detect the end of measurement, 86
 - Using the :TRIG:SING command to wait until end of measurement, 88
 - Using the ASCII transfer format to retrieve internal data arrays, 112
 - Using the ASCII transfer format to write formatted data arrays, 116
 - Using the binary transfer format to retrieve internal data arrays, 114
 - Using the binary transfer format to write formatted data arrays, 118
 - Program message terminator, 37
 - Program(VBA)
 - Control, 367
 - Saving/loading, 134
 - Programming Manual, 4
 - Property display
 - Calibration, 411
 - Property of file, 139
 - Pulse width, 155
- Q**
- Q value, 97, 99
 - Questionable bandwidth limit channel{1-16} status register
 - Reading out the condition register, 446
 - Reading out the event register, 446
 - Setting the enable register, 447
 - Setting the negative transition filter, 448
 - Setting the positive transition filter, 449
 - Questionable bandwidth limit status register
 - Reading out the condition register, 449
 - Reading out the event register, 445
 - Setting the enable register, 450
 - Setting the negative transition filter, 451
 - Setting the positive transition filter, 452
 - Questionable limit channel{1-4} status register
 - Bit definitions, 520, 521, 522
 - Reading out the condition register, 455
 - Reading out the event register, 455
 - Setting the enable register, 456
 - Setting the negative transition filter, 457
 - Setting the positive transition filter, 458
 - Questionable limit channel{1-9} status register, 509
 - Questionable limit status register, 509
 - Bit definitions, 520
 - Reading out the condition register, 459
 - Reading out the event register, 455
 - Setting the enable register, 460
 - Setting the negative transition filter, 461
 - Setting the positive transition filter, 462
 - Questionable ripple limit channel{1-16} status register
 - Reading out the condition register, 465
 - Reading out the event register, 465
 - Setting the enable register, 466
 - Setting the negative transition filter, 467
 - Setting the positive transition filter, 468
 - Questionable ripple limit status register
 - Reading out the condition register, 468
 - Reading out the event register, 465
 - Setting the enable register, 469
 - Setting the negative transition filter, 470
 - Setting the positive transition filter, 471
 - Questionable status register, 509
 - Bit definitions, 518
 - Reading out the condition register, 453
 - Reading out the event register, 445
 - Setting the enable register, 454
 - Setting the negative transition filter, 463
 - Setting the positive transition filter, 464
 - Quick Start Guide, 4
- R**
- read_asc.htb, 112
 - read_bin.htb, 114
 - READY FOR TRIGGER, 150
 - Real format, 47
 - Recall, 132
 - Auto recall, 132
 - Ref In connector, 420
 - Reference graticule line, 48
 - Reference marker, 90
 - Releasing key lock, 162
 - Remote control system
 - GPIB remote control system, 25
 - LAN remote control system, 27
 - Overview, 24
 - Remote mode, 38
 - Reset
 - Instrument setting, 199, 479, 483
 - Status registers, 196
 - Response calibration, 60
 - Restart, 43
 - Retrieving file property, 139
 - Retrieving measurement results
 - All measurement points, 111
 - Specified point, 90
 - Retrieving search(analysis) results, 94
 - RF Out
 - On/Off, 41
- S**
- S parameter, 41
 - Sample Application Programs, 169
 - Sample Program, 3
 - file name
 - bandwid.htb, 98

-
- cal.htb, 71
 - cont_upd.htb, 165
 - ctrl_lan.xls, 184
 - ctrl_lansicl.xls, 176
 - ecal.htb, 77
 - file_sav.htb, 137
 - file_xfr.htb, 143
 - handler.htb, 160
 - lim_test.htb, 128
 - meas_bpf.htb, 173
 - read_asc.htb, 112
 - read_bin.htb, 114
 - search.htb, 96
 - setup.htb, 56
 - srq_err.htb, 168
 - srq_meas.htb, 86
 - trg_sing.htb, 88
 - write_a.htb, 116
 - write_b.htb, 118
 - How to load, 21
 - title
 - Bandwidth Search, 98
 - Calibration, 71
 - Communicating with external instruments, 160
 - Configuring measurement conditions, 56
 - Controlling the update timing of LCD display, 165
 - Controlling using SICL-LAN server, 176
 - Controlling using telnet server, 184
 - ECal, 77
 - Error detection using an SRQ, 168
 - File transfer, 143
 - Limit test, 128
 - Measurement of band pass filter, 173
 - Peak search, 96
 - Saving file, 137
 - Using an SRQ to detect the end of measurement, 86
 - Using the :TRIG:SING command to wait until end of measurement, 88
 - Using the ASCII transfer format to retrieve internal data arrays, 112
 - Using the ASCII transfer format to write formatted data arrays, 116
 - Using the binary transfer format to retrieve internal data arrays, 114
 - Using the binary transfer format to write formatted data arrays, 118
 - Save, 132
 - Scale per division, 48
 - SCPI Command
 - :CALCulate{1-4}[:SElected]:MARKer:MATH:FLATness[:STATe], 255
 - :CALCulate{1-4}[:SElected]:MARKer:MATH:FSTatistics[:STATe], 257
 - :CALCulate{1-4}[:SElected]:MARKer:MATH:STATistics[:STATe], 259
 - SCPI command
 - *CLS, 196
 - *ESE, 197
 - *ESR?, 197
 - *IDN?, 198
 - *OPC, 198
 - *OPC?, 198
 - *OPT?, 199
 - *RST, 199
 - *SRE, 200
 - *STB?, 201
 - *TRG, 201
 - *WAI, 201
 - :ABORt, 202
 - :CALCulate{1-4}:PARAmeter:COUNt, 284
 - :CALCulate{1-4}:PARAmeter{1-4}:DEFine, 285
 - :CALCulate{1-4}:PARAmeter{1-4}:SElect, 286
 - :CALCulate{1-4}[:SElected]:BLIMit:DB, 204
 - :CALCulate{1-4}[:SElected]:BLIMit:DISPlay:MARKer, 205
 - :CALCulate{1-4}[:SElected]:BLIMit:DISPlay:VALue, 206
 - :CALCulate{1-4}[:SElected]:BLIMit:FAIL, 207
 - :CALCulate{1-4}[:SElected]:BLIMit:MAXimum, 208
 - :CALCulate{1-4}[:SElected]:BLIMit:MINimum, 209
 - :CALCulate{1-4}[:SElected]:BLIMit:REPort[:DATA]?, 210
 - :CALCulate{1-4}[:SElected]:BLIMit[:STATe], 203
 - :CALCulate{1-4}[:SElected]:CONVersion:FUNCTion, 212
 - :CALCulate{1-4}[:SElected]:CONVersion[:STATe], 211
 - :CALCulate{1-4}[:SElected]:CORRection:EDELay:TIME, 213
 - :CALCulate{1-4}[:SElected]:CORRection:OFFSet:PHASe, 214
 - :CALCulate{1-4}[:SElected]:DATA:FDATa, 215
 - :CALCulate{1-4}[:SElected]:DATA:FMEMOry, 216
 - :CALCulate{1-4}[:SElected]:DATA:SDATa, 217
 - :CALCulate{1-4}[:SElected]:DATA:SMEMOry, 218
 - :CALCulate{1-4}[:SElected]:FORMat, 219
 - :CALCulate{1-4}[:SElected]:FUNCTion:DATA?, 221
 - :CALCulate{1-4}[:SElected]:FUNCTion:DOMain:COUPl e, 223
 - :CALCulate{1-4}[:SElected]:FUNCTion:DOMain:STARt, 224, 247
 - :CALCulate{1-4}[:SElected]:FUNCTion:DOMain[:STATe], 222, 245
 - :CALCulate{1-4}[:SElected]:FUNCTion:DOMain:STOP, 225
 - :CALCulate{1-4}[:SElected]:FUNCTion:EXECute, 225
 - :CALCulate{1-4}[:SElected]:FUNCTion:PEXECursion, 226
 - :CALCulate{1-4}[:SElected]:FUNCTion:POINts?, 227
 - :CALCulate{1-4}[:SElected]:FUNCTion:PPOLarity, 228
 - :CALCulate{1-4}[:SElected]:FUNCTion:TARGet, 229
 - :CALCulate{1-4}[:SElected]:FUNCTion:TTRansition, 230
 - :CALCulate{1-4}[:SElected]:FUNCTion:TYPE, 231
 - :CALCulate{1-4}[:SElected]:LIMit:DATA, 233

- :CALCulate{1-4}[:SElected]:LIMit:DISPlay:CLIP, 236
- :CALCulate{1-4}[:SElected]:LIMit:DISPlay[:STATe], 235
- :CALCulate{1-4}[:SElected]:LIMit:FAIL, 237
- :CALCulate{1-4}[:SElected]:LIMit:OFFSet:AMPLitude, 238
- :CALCulate{1-4}[:SElected]:LIMit:OFFSet:MARKer, 239
- :CALCulate{1-4}[:SElected]:LIMit:OFFSet:STIMulus, 240
- :CALCulate{1-4}[:SElected]:LIMit:REPort POINTs?, 242
- :CALCulate{1-4}[:SElected]:LIMit:REPort:ALL?, 241
- :CALCulate{1-4}[:SElected]:LIMit:REPort[:DATA]?, 242
- :CALCulate{1-4}[:SElected]:LIMit[:STATe], 232
- :CALCulate{1-4}[:SElected]:MARKer:BWIDth[:STATe], 243
- :CALCulate{1-4}[:SElected]:MARKer:COUPle, 244
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:MULT i:TYPE, 254
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:DOMa in:COUPle, 246
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:DOMa in:STOP, 248
- :CALCulate{1-4}[:SElected]:MARKer:NOTCh[:STATe], 261
- :CALCulate{1-4}[:SElected]:MARKer:REfERENCE[:STAT e], 262
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:ACTivate, 264
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:BWIDth:D ATA?, 265
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:BWIDth:T HReshold, 266
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:DISCrete, 267
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: EXECute, 268
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: PEXCursion, 269
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: PPOLarity, 270
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: TARGet, 271
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: TRACking, 272
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: TTRansiTion, 273
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:FUNCTion: TYPE, 274
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:NOTCh:D ATA?, 276
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:NOTCh:T HReshold, 277
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:SET, 278
- :CALCulate{1-4}[:SElected]:MARKer{1-10}[:STATe], 263
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:X, 279
- :CALCulate{1-4}[:SElected]:MARKer{1-10}:Y?, 280
- :CALCulate{1-4}[:SElected]:MATH:FUNCTion, 281
- :CALCulate{1-4}[:SElected]:MATH:MEMorize, 281
- :CALCulate{1-4}[:SElected]:MSTatistics:DATA?, 283
- :CALCulate{1-4}[:SElected]:MSTatistics[:STATe], 282
- :CALCulate{1-4}[:SElected]:RLIMit:DATA, 287
- :CALCulate{1-4}[:SElected]:RLIMit:DISPlay:LINE, 288
- :CALCulate{1-4}[:SElected]:RLIMit:DISPlay:SElect, 289
- :CALCulate{1-4}[:SElected]:RLIMit:DISPlay:VALue, 290
- :CALCulate{1-4}[:SElected]:RLIMit:FAIL, 291
- :CALCulate{1-4}[:SElected]:RLIMit:REPort[:DATA], 292
- :CALCulate{1-4}[:SElected]:RLIMit[:STATe], 286
- :CALCulate{1-4}[:SElected]:SMOothing:APERture, 294
- :CALCulate{1-4}[:SElected]:SMOothing[:STATe], 293
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:MULT i:PEXCursion, 249
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:MULT i:PPOLarity, 250
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:MULT i:TARGet, 251
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:MULT i:TRACking, 252
- :CALCulate{1-4}[:SElected]:MARKer:FUNCTion:MULT i:TTRansiTion, 253
- :CALCulate{1-4}[:SElected]:MARKer:MATH:FLATness :DATA?, 256
- :CALCulate{1-4}[:SElected]:MARKer:MATH:FSTatistic s:DATA?, 258
- :CALCulate{1-4}[:SElected]:MARKer:MATH:STATistic s:DATA?, 260
- :CONTRol:HANDler:A[:DATA], 295
- :CONTRol:HANDler:B[:DATA], 295
- :CONTRol:HANDler:C[:DATA], 296
- :CONTRol:HANDler:C:MODE, 297
- :CONTRol:HANDler:D[:DATA], 298
- :CONTRol:HANDler:D:MODE, 299
- :CONTRol:HANDler:E[:DATA], 300
- :CONTRol:HANDler[:EXTension]:INDEX:STATe, 302
- :CONTRol:HANDler[:EXTension]:RTRigger:STATe, 303
- :CONTRol:HANDler:F[:DATA], 301
- :CONTRol:HANDler:OUTPut{1-2}[:DATA], 302
- :DISPlay:ANNotation:FREQuency[:STATe], 304
- :DISPlay:CCLear, 304
- :DISPlay:CLOCK, 305
- :DISPlay:COLor{1-2}:BACK, 306
- :DISPlay:COLor{1-2}:GRATicule{1-2}, 307
- :DISPlay:COLor{1-2}:LIMit{1-2}, 308
- :DISPlay:COLor{1-2}:RESet, 308
- :DISPlay:COLor{1-2}:TRAC{1-4}:DATA, 309
- :DISPlay:COLor{1-2}:TRAC{1-4}:MEMory, 310
- :DISPlay:ECHO:CLEAr, 311

:DISPlay:ECHO[:DATA], 311
:DISPlay:ENABle, 312
:DISPlay:FSIGn, 313
:DISPlay:IMAGe, 313
:DISPlay:MAXimize, 314
:DISPlay:SKEY[:STATe], 314
:DISPlay:SPLit, 315
:DISPlay:TABLE[:STATe], 316
:DISPlay:TABLE:TYPE, 317
:DISPlay:UPDate[:IMMediate], 318
:DISPlay:WINDow{1-4}:ACTivate, 318
:DISPlay:WINDow{1-4}:ANNotation:MARKer:ALIGn[:STATe], 319
:DISPlay:WINDow{1-4}:ANNotation:MARKer:SINGLE[:STATe], 320
:DISPlay:WINDow{1-4}:LABel, 321
:DISPlay:WINDow{1-4}:MAXimize, 322
:DISPlay:WINDow{1-4}:SPLit, 323
:DISPlay:WINDow{1-4}:TITLe:DATA, 324
:DISPlay:WINDow{1-4}:TITLe[:STATe], 324
:DISPlay:WINDow{1-4}:TRACe{1-4}:ANNotation:MARKer:POSition:X, 325
:DISPlay:WINDow{1-4}:TRACe{1-4}:ANNotation:MARKer:POSition:Y, 326
:DISPlay:WINDow{1-4}:TRACe{1-4}:ANNotation:YAXis:MODE, 327
:DISPlay:WINDow{1-4}:TRACe{1-4}:MEMory[:STATe], 328
:DISPlay:WINDow{1-4}:TRACe{1-4}:STATe, 329
:DISPlay:WINDow{1-4}:TRACe{1-4}:Y[:SCALE]:AUTO, 329
:DISPlay:WINDow{1-4}:TRACe{1-4}:Y[:SCALE]:PDIVisions, 330
:DISPlay:WINDow{1-4}:TRACe{1-4}:Y[:SCALE]:RLEVel, 331
:DISPlay:WINDow{1-4}:TRACe{1-4}:Y[:SCALE]:RPOSITION, 332
:DISPlay:WINDow{1-4}:TRACe{1-4}:Y:TRACk:FREQuency, 333
:DISPlay:WINDow{1-4}:TRACe{1-4}:Y:TRACk:MODE, 334
:DISPlay:WINDow{1-4}:X:SPACing, 335
:DISPlay:WINDow{1-4}:Y[:SCALE]:DIVisions, 336
:FORMat:BORDER, 337
:FORMat:DATA, 338
:HCOpy:ABORT, 339
:HCOpy:IMAGe, 339
:HCOpy[:IMMediate], 339
:INITiate{1-4}:CONTinuous, 341
:INITiate{1-4}[:IMMediate], 340
:MMEMory:CATalog?, 342
:MMEMory:COpy, 343
:MMEMory:DELeTe, 344
:MMEMory:LOAD:CHANnel:COEFficient {A|B|C|D}, 347
:MMEMory:LOAD:CHANnel[:STATe], 346
:MMEMory:LOAD:LIMit, 348
:MMEMory:LOAD:PROGram, 349
:MMEMory:LOAD:RLIMit, 350
:MMEMory:LOAD:SEGment, 351
:MMEMory:LOAD[:STATe], 345
:MMEMory:MDIRectory, 352
:MMEMory:STORE:CHANnel:COEFficient {A|B|C|D}, 355
:MMEMory:STORE:CHANnel[:STATe], 354
:MMEMory:STORE:FDATa, 356
:MMEMory:STORE:IMAGe, 357
:MMEMory:STORE:LIMit, 358
:MMEMory:STORE:PROGram, 359
:MMEMory:STORE:RLIMit, 360
:MMEMory:STORE:SALL, 361
:MMEMory:STORE:SEGment, 362
:MMEMory:STORE[:STATe], 353
:MMEMory:STORE:STYPe, 363
:MMEMory:TRANSfer, 364
:OUTPut[:STATe], 365
:PROGram:CATalog?, 365
:PROGram[:SELeCted]:NAME, 366
:PROGram[:SELeCted]:STATe, 367
:SENSe:CORRection:COLLect:ECAL:PATH?, 368
:SENSe:CORRection:IMPedance[:INPut][:MAGNitude], 369
:SENSe{1-4}:AVERage:CLEar, 370
:SENSe{1-4}:AVERage:COUNt, 371
:SENSe{1-4}:AVERage[:STATe], 370
:SENSe{1-4}:BANDwidth[:RESolution], 372
:SENSe{1-4}:BWIDth[:RESolution], 373
:SENSe{1-4}:CORRection:CLEar, 373
:SENSe{1-4}:CORRection:COEFficient[:DATA?], 374
:SENSe{1-4}:CORRection:COLLect[:ACQuire]:ISOLation, 399
:SENSe{1-4}:CORRection:COLLect[:ACQuire]:LOAD, 401
:SENSe{1-4}:CORRection:COLLect[:ACQuire]:OPEN, 406
:SENSe{1-4}:CORRection:COLLect[:ACQuire]:SHORT, 407
:SENSe{1-4}:CORRection:COLLect[:ACQuire]:THRU, 408
:SENSe{1-4}:CORRection:COLLect:CKIT:LABel, 376
:SENSe{1-4}:CORRection:COLLect:CKIT:ORDER:LOAD, 377
:SENSe{1-4}:CORRection:COLLect:CKIT:ORDER:OPEN, 378
:SENSe{1-4}:CORRection:COLLect:CKIT:ORDER:SHORT, 379
:SENSe{1-4}:CORRection:COLLect:CKIT:ORDER:THRU, 380
:SENSe{1-4}:CORRection:COLLect:CKIT:RESet, 380
:SENSe{1-4}:CORRection:COLLect:CKIT[:SELeCt], 375
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:ARBITrary, 381
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:C0, 382

:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
C1, 383
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
C2, 384
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
C3, 385
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
DELaY, 386
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
L0, 387
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
L1, 388
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
L2, 389
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
L3, 390
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
LABel, 391
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
LOSS, 392
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
TYPE, 393
:SENSe{1-4}:CORRection:COLLect:CKIT:STAN{1-21}:
Z0, 394
:SENSe{1-4}:CORRection:COLLect:ECAL:ERES, 395
:SENSe{1-4}:CORRection:COLLect:ECAL:ISOLation[:S
TATe], 395
:SENSe{1-4}:CORRection:COLLect:ECAL:SOLT1, 397
:SENSe{1-4}:CORRection:COLLect:ECAL:SOLT2, 397
:SENSe{1-4}:CORRection:COLLect:ECAL:THRU, 398
:SENSe{1-4}:CORRection:COLLect:METHod:ERES, 399
:SENSe{1-4}:CORRection:COLLect:METHod[:RESPOns
e]:OPEN, 402
:SENSe{1-4}:CORRection:COLLect:METHod[:RESPOns
e]:THRU, 404
:SENSe{1-4}:CORRection:COLLect:METHod:SOLT1,
403
:SENSe{1-4}:CORRection:COLLect:METHod:SOLT2,
403
:SENSe{1-4}:CORRection:COLLect:METHod:TYPE?,
405
:SENSe{1-4}:CORRection:COLLect:METHod[:RESPOns
e]:SHORT, 402
:SENSe{1-4}:CORRection:COLLect:SAVE, 407
:SENSe{1-4}:CORRection:EXTension:PORT{1-4}, 410
:SENSe{1-4}:CORRection:EXTension[:STATe], 409
:SENSe{1-4}:CORRection:PROPerTy, 411
:SENSe{1-4}:CORRection:RVELocity:COAX, 411
:SENSe{1-4}:CORRection:STATe, 412
:SENSe{1-4}:CORRection:TYPE{1-4}?, 413
:SENSe{1-4}:FREQuency:CENTer, 415
:SENSe{1-4}:FREQuency:DATA, 416
:SENSe{1-4}:FREQuency:SPAN, 417
:SENSe{1-4}:FREQuency:STARt, 418
:SENSe{1-4}:FREQuency:STOP, 419
:SENSe{1-4}:FREQuency[:CW], 414
:SENSe{1-4}:ROSCillator:SOURce, 420
:SENSe{1-4}:SEGMENT:DATA, 421
:SENSe{1-4}:SEGMENT:SWEep:POINTS?, 423
:SENSe{1-4}:SEGMENT:SWEep:TIME?, 423
:SENSe{1-4}:SWEep:DELaY, 424
:SENSe{1-4}:SWEep:POINTS, 425
:SENSe{1-4}:SWEep:TIME:AUTO, 427
:SENSe{1-4}:SWEep:TIME[:DATA], 426
:SENSe{1-4}:SWEep:TYPE, 428
:SERVice:CHANnel:ACTivE?, 428
:SERVice:CHANnel:COUNt?, 429
:SERVice:CHANnel:TRACe:COUNt?, 429
:SERVice:CHANnel{1-4}:TRACe:ACTivE?, 429
:SERVice:PORT:COUNt?, 430
:SOURce{1-4}:POWer:ATTenuation[:DATA], 432
:SOURce{1-4}:POWer:CENTer, 433
:SOURce{1-4}:POWer[:LEVel][:IMMediate][:AMPLitude
], 431
:SOURce{1-4}:POWer[:LEVel]:SLOPe:STATe, 436, 437
:SOURce{1-4}:POWer:PORT:COUPle, 434
:SOURce{1-4}:POWer:PORT{1-4}[:LEVel][:IMMediate][:
AMPLitude], 435
:SOURce{1-4}:POWer:SPAN, 438
:SOURce{1-4}:POWer:STARt, 439
:SOURce{1-4}:POWer:STOP, 440
:STATus:OPERation:CONDition?, 441
:STATus:OPERation:ENABle, 442
:STATus:OPERation[:EVENT]?, 441
:STATus:OPERation:NTRansition, 443
:STATus:OPERation:PTRansition, 444
:STATus:PRESet, 445
:STATus:QUEStionable:BLIMit:CHANnel{1-4}:CONDiti
on?, 446
:STATus:QUEStionable:BLIMit:CHANnel{1-4}:ENABle,
447
:STATus:QUEStionable:BLIMit:CHANnel{1-4}[:EVENT]
?, 446
:STATus:QUEStionable:BLIMit:CHANnel{1-4}:NTRansit
ion, 448
:STATus:QUEStionable:BLIMit:CHANnel{1-4}:PTRansiti
on, 449
:STATus:QUEStionable:BLIMit:CONDition?, 449
:STATus:QUEStionable:BLIMit:ENABle, 450
:STATus:QUEStionable:BLIMit[:EVENT]?, 445
:STATus:QUEStionable:BLIMit:NTRansition, 451
:STATus:QUEStionable:BLIMit:PTRansition, 452
:STATus:QUEStionable:CONDition?, 453
:STATus:QUEStionable:ENABle, 454
:STATus:QUEStionable[:EVENT]?, 445
:STATus:QUEStionable:LIMit:CHANnel{1-4}:CONDitio
n?, 455
:STATus:QUEStionable:LIMit:CHANnel{1-4}:ENABle,
456
:STATus:QUEStionable:LIMit:CHANnel{1-4}[:EVENT]?,
455
:STATus:QUEStionable:LIMit:CHANnel{1-4}:NTRansiti
on, 457

- :STATus:QUEStionable:LIMit:CHANnel{1-4}:PTRansition, 458
- :STATus:QUEStionable:LIMit:CONDition?, 459
- :STATus:QUEStionable:LIMit:ENABLE, 460
- :STATus:QUEStionable:LIMit[:EVENT]?, 455
- :STATus:QUEStionable:LIMit:NTRansition, 461
- :STATus:QUEStionable:LIMit:PTRansition, 462
- :STATus:QUEStionable:NTRansition, 463
- :STATus:QUEStionable:PTRansition, 464
- :STATus:QUEStionable:RLIMit:CHANnel{1-4}:CONDition?, 465
- :STATus:QUEStionable:RLIMit:CHANnel{1-4}:ENABLE, 466
- :STATus:QUEStionable:RLIMit:CHANnel{1-4}[:EVENT]?, 465
- :STATus:QUEStionable:RLIMit:CHANnel{1-4}:NTRansition, 467
- :STATus:QUEStionable:RLIMit:CHANnel{1-4}:PTRansition, 468
- :STATus:QUEStionable:RLIMit:CONDition?, 468
- :STATus:QUEStionable:RLIMit:ENABLE, 469
- :STATus:QUEStionable:RLIMit[:EVENT]?, 465
- :STATus:QUEStionable:RLIMit:NTRansition, 470
- :STATus:QUEStionable:RLIMit:PTRansition, 471
- :SYSTem:BACKlight, 472
- :SYSTem:BEEPer:COMPLet:IMMEDIATE, 473
- :SYSTem:BEEPer:COMPLet:STATe, 473
- :SYSTem:BEEPer:WARNIng:IMMEDIATE, 474
- :SYSTem:BEEPer:WARNIng:STATe, 474
- :SYSTem:DATE, 475
- :SYSTem:ERRor, 476
- :SYSTem:KLOCK:KBD, 477
- :SYSTem:KLOCK:MOUSE, 478
- :SYSTem:POFF, 479
- :SYSTem:PRESet, 479
- :SYSTem:SECurity:LEVel, 480
- :SYSTem:SERvice, 481
- :SYSTem:TIME, 482
- :SYSTem:UPReset, 483
- :TRIGger[:SEQuence][:IMMEDIATE], 484
- :TRIGger[:SEQuence]:SINGle, 484
- :TRIGger[:SEQuence]:SOURce, 485
- Command reference
 - E5061A/E5062A commands, 202
 - IEEE common commands, 196
 - Notational conventions, 194
- Command tree, 486
- Lookup, 20
- Screen display
 - update on/off, 49
- Search
 - Analysis command, 93
 - Marker search, 91
- Search range
 - Analysis command, 93
 - Marker search, 91
- Search tracking, 92
- Search type
 - Analysis command, 93
 - Marker search, 91
- search.htb, 96
- Secondary value, 109
- Segment sweep, 42
 - Total number of measurement points, 423
 - Total sweep time, 423
- Segment sweep table
 - Saving/recalling, 134
 - Setting, 42
 - Showing/hiding, 46
- Sending several commands, 37
- Serial number, 500
 - Plate, 500
 - Reading out, 198
- Service mode, 481
- Service request, 506
 - Example of use
 - Error detection, 166
 - Waiting for the end of measurement, 84
- Service request enable register, 509
 - Setting, 200
- Setting the delay time, 410
- Setting the title display area, 49
- setup.htb, 56
- SHORT, 65
- Shutdown, 479
- SICL-LAN, 28
 - Example of use, 176
- SICL-LAN address, 28
- SICL-LAN server
 - Turning on/off, 28
- Smith chart format, 47
- Smoothing, 47
- Softkey Labels
 - Showing/hiding, 46
- Source power, 42
- Span value
 - Frequency sweep range, 41
 - Power sweep range, 43
- Specifying file, 132
- SRQ, 506
 - Example of use
 - Error detection, 166
 - Waiting for the end of measurement, 84
- srq_err.htb, 168
- srq_meas.htb, 86
- Standard class assignment, 65
- Standard deviation
 - Analysis command, 93
 - Statistical analysis, 100
- Standard event status register, 509
 - Bit definitions, 517
 - Reading out the event register, 197
 - Setting the enable register, 197
- Standard module

-
- Importing, 134
 - Standard name, 64
 - Standard type, 64
 - Standard value, 64
 - Start value
 - Frequency sweep range, 41
 - Marker search range, 91
 - Power sweep range, 43
 - Search(analysis) range, 93
 - Starting a measurement, 83
 - Statistical analysis results
 - Analysis command, 94
 - Statistical analysis, 100
 - Status byte register, 507
 - Bit definitions, 516
 - Reading out, 201
 - Status register
 - Example of use
 - Error detection, 166
 - Obtaining test results, 121
 - Waiting for the end of measurement, 84
 - Register structure, 509
 - Status reporting system, 506
 - Stimulus, 41
 - Stimulus data arrays, 110
 - Stimulus signal output
 - On/Off, 41
 - Stop value
 - Frequency sweep range, 41
 - Marker search range, 91
 - Power sweep range, 43
 - Search(analysis) range, 93
 - Sweep condition, 41
 - Sweep delay time, 42
 - Sweep range, 41
 - Power sweep, 43
 - Sweep time, 42
 - Reading out
 - Linear sweep, 426
 - Segment sweep, 423
 - Sweep type, 41
 - SWR format, 47
 - System Z0, 43
- T**
- Table
 - Limit table
 - Showing/hiding, 46
 - Marker list table, 46
 - Segment sweep table
 - Setting, 42
 - Showing/hiding, 46
 - Target search
 - Analysis command, 93
 - Marker search, 91
 - telnet, 34
 - Telnet server
 - Example of use, 184
 - Turning on/off, 27
 - telnet server
 - Turning on/off, 33
 - Test results, 121
 - Each channel, 122
 - Each measurement point, 121
 - Each trace, 121
 - Overall test result, 124
 - THRU, 65
 - Time
 - Show or hide, 49
 - Timing chart, 155
 - Total number of measurement points of all segments, 423
 - Total sweep time of all segments, 423
 - Trace display, 44
 - Tracking, 92
 - Transferring files
 - Command, 139
 - Sample program, 140
 - Transition filter, 508
 - Transitional direction
 - Analysis command, 94
 - Marker search, 92
 - trg_sing.htb, 88
 - Trigger source, 81
 - Trigger system, 80
 - Triggering a measurement, 83
 - Turning on or off error correction, 62
 - Turning on or off the backlight, 49
 - Turning on or off the port extension, 409
 - Turns off the analyzer, 479
 - Typeface conventions, 3
 - Types of remote control system, 24
- U**
- Update of the LCD display, 163
 - Turning on or off, 163
 - Update once, 163
 - Update on/off
 - Screen display, 49
 - User form
 - Importing, 134
- V**
- VBA, 24
 - VBA macro
 - Control, 367
 - VBA project
 - Saving/loading, 134
 - VEE, 35
 - Velocity factor, 411
- W**
- Waiting for the end of measurement
 - Inserting wait time, 88

- Using the :TRIG:SING command, 87
- Using the status register, 84
- Waiting for trigger state, 81
- Warning Message, 536
- Window
 - Layout, 44
 - Maximizing, 44
- WinSock API
 - Example of use, 184
 - Overview, 35
- WRITE STROBE, 151
- Write strobe signal
 - Limit test result, 151
 - Output port, 151
- write_a.htb, 116
- write_b.htb, 118

Z

- Z0, 43

REGIONAL SALES AND SUPPORT OFFICES

For more information about Agilent Technologies test and measurement products, applications, services, and for a current sales office listing, visit our web site: <http://www.agilent.com/find/tmdir>. You can also contact one of the following centers and ask for a test and measurement sales representative.

21/01/2004

United States:

Test and Measurement Call Center
(tel) 1 800 452-4844
(fax) 1 888 900-8921

Australia/New Zealand:

(tel) (61 3) 9210-5555 (Australia)
(fax) (61 3) 9210-5899
(tel) (64 4) 939-0636 (New Zealand)
(fax) (64 4) 972-5364

Canada:

Test and Measurement Call Center
(tel) 1 877 894-4414
(fax) 1 888 900-8921

Asia Pacific:

(tel) (65) 6375-8100
(fax) (65) 6836-0252
Email: tm_asia@agilent.com

China:

(tel) 800 810-0189
(fax) 800 820-2816

Europe:

(tel) (31 20) 547-2323
(fax) (31 20) 547-2390

Japan:

Call Center
(tel) 0120 421-345
(tel) (81) 426 56-7832
(fax) (81) 426 56-7840

Korea:

(tel) (82 2) 2004-5004
(fax) (82 2) 2004-5115

Latin America:

(tel) (305) 269-7500
(fax) (305) 269-7599

Taiwan:

(tel) 0800 047 866
(fax) 0800 286 331